

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011024\
 Data File : BG060295.D
 Acq On : 10 Jan 2024 10:47
 Operator : MA/JU
 Sample : PB158316BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB158316BL

Quant Time: Jan 10 11:35:25 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 09 04:07:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	271165	20.000	ng	0.00
21) Naphthalene-d8	10.737	136	1021291	20.000	ng	0.00
39) Acenaphthene-d10	14.568	164	783845	20.000	ng	0.00
64) Phenanthrene-d10	17.317	188	2038251	20.000	ng	0.00
76) Chrysene-d12	21.583	240	2038607	20.000	ng	0.00
86) Perylene-d12	24.756	264	2219512	20.000	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.508	112	2746259	166.578	ng	0.00
7) Phenol-d6	7.100	99	3375345	138.263	ng	0.00
23) Nitrobenzene-d5	9.098	82	2340183	108.200	ng	0.00
42) 2,4,6-Tribromophenol	16.060	330	1516252	131.475	ng	0.00
45) 2-Fluorobiphenyl	13.193	172	4671981	82.868	ng	0.00
79) Terphenyl-d14	19.944	244	6626504	80.293	ng	0.01
Target Compounds						Qvalue
19) n-Nitroso-di-n-propyla...	9.098	70	277425	16.420	ng	# 85
32) Benzoic acid	10.061	122	72	10.207	ng	# 1
51) 2,6-Dinitrotoluene	14.568	165	102745	8.039	ng	# 33
54) 2,4-Dinitrophenol	14.574	184	97	8.598	ng	# 1
57) 2,4-Dinitrotoluene	14.568	165	102745	5.862	ng	# 26
67) 4-Bromophenyl-phenylether	16.060	248	94961	4.240	ng	# 1
77) Benzidine	19.944	184	150193	3.391	ng	# 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011024\
Data File : BG060295.D
Acq On : 10 Jan 2024 10:47
Operator : MA/JU
Sample : PB158316BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB158316BL

Quant Time: Jan 10 11:35:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration




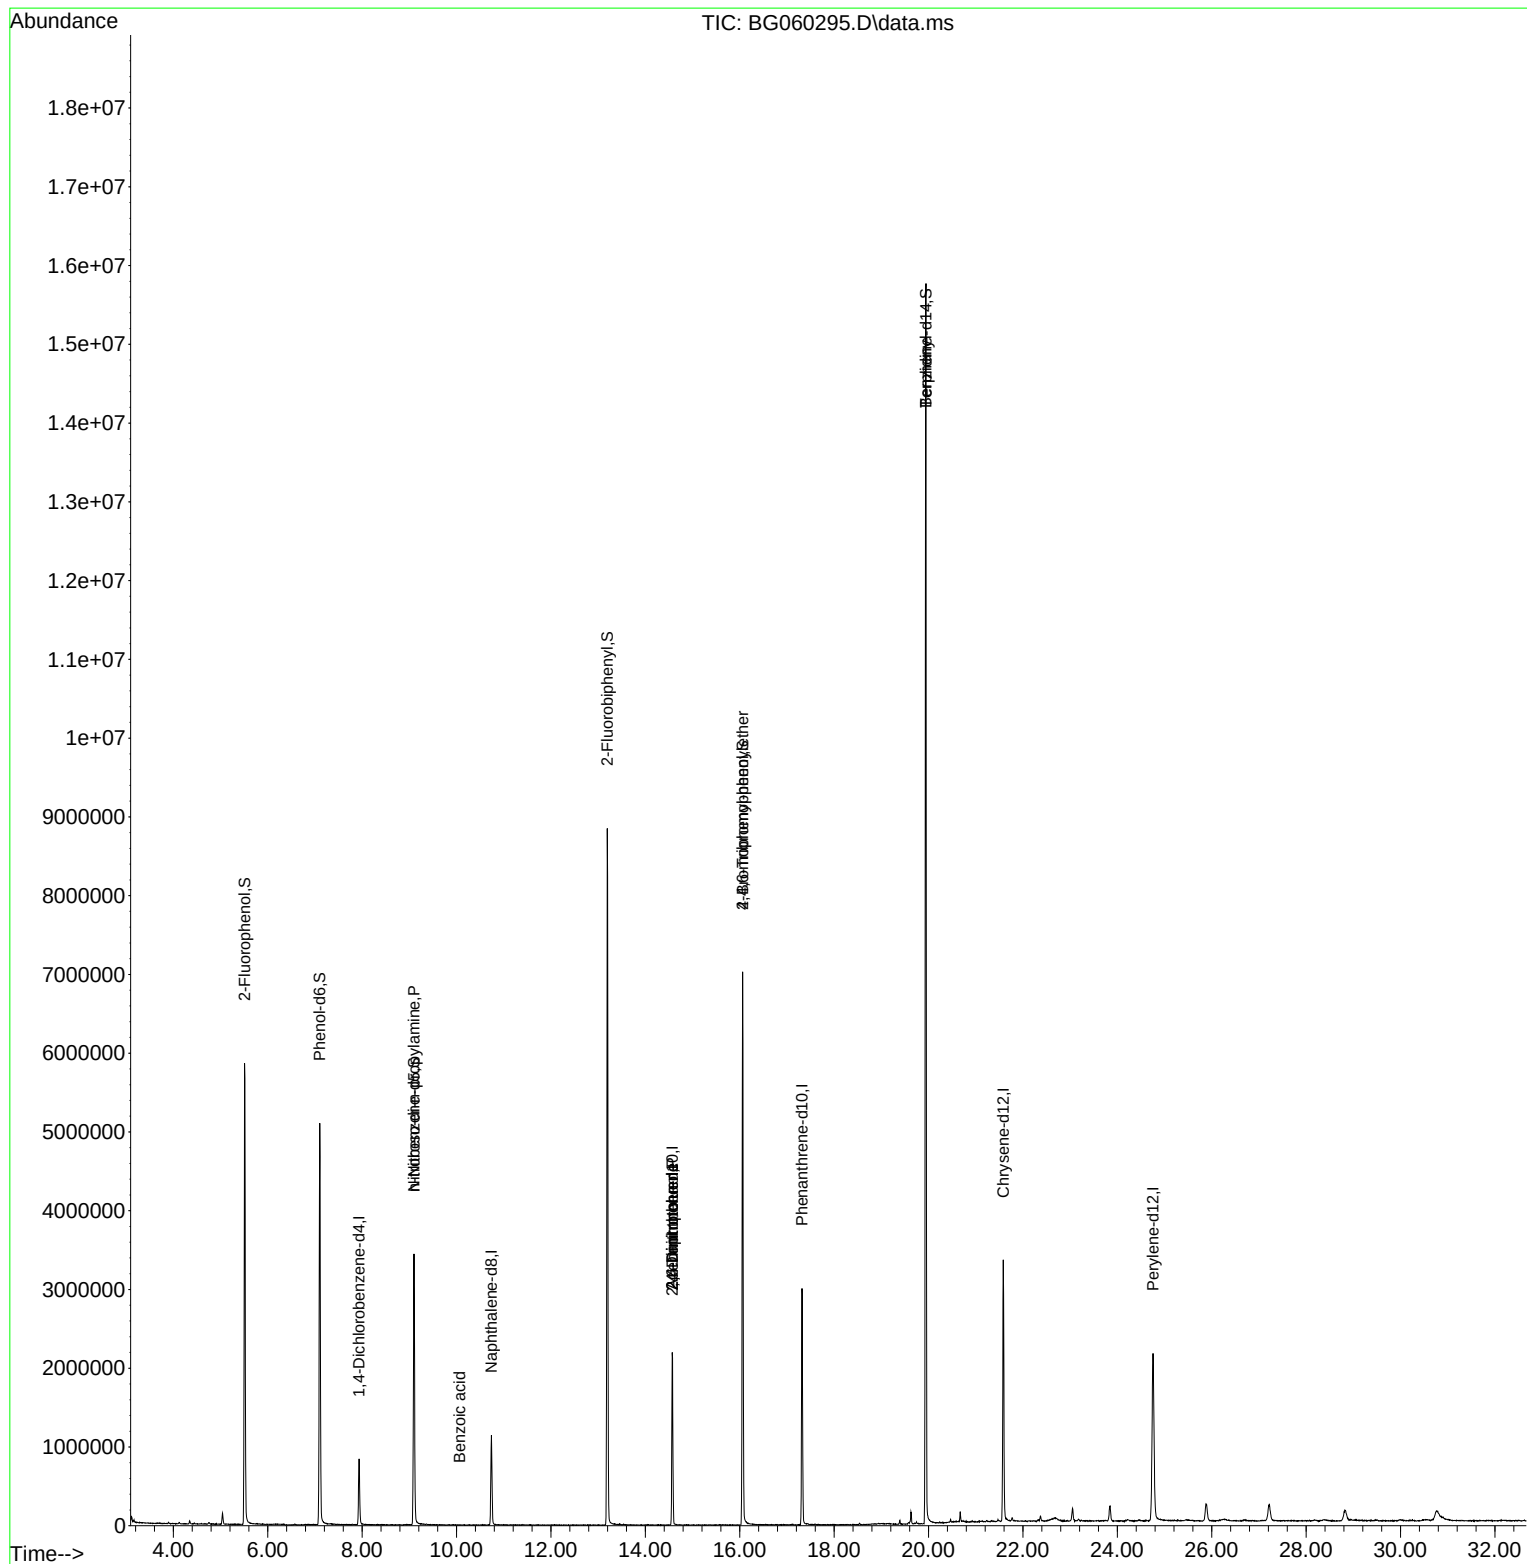




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.934 min Scan# 81
Delta R.T. 0.004 min
Lab File: BG060295.D
Acq: 10 Jan 2024 10:47




Instrument :
BNA_G
ClientSampleId :
PB158316BL


Tgt Ion:152 Resp: 271165
Ion Ratio Lower Upper
152 100
150 153.3 114.5 171.7
115 54.0 43.0 64.6



#5
2-Fluorophenol
Concen: 166.578 ng
RT: 5.508 min Scan# 412
Delta R.T. 0.005 min
Lab File: BG060295.D
Acq: 10 Jan 2024 10:47

Tgt Ion:112 Resp: 2746259
Ion Ratio Lower Upper
112 100
64 66.0 49.8 74.6
63 34.1 24.4 36.6


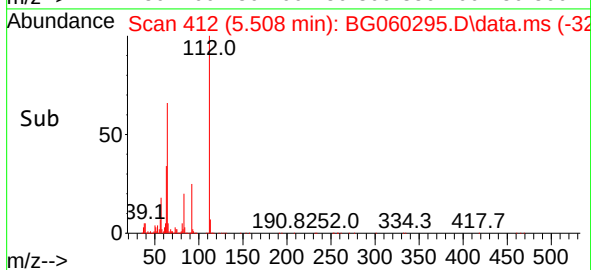






#7
Phenol-d6
Concen: 138.263 ng
RT: 7.100 min Scan# 61
Delta R.T. 0.005 min
Lab File: BG060295.D
Acq: 10 Jan 2024 10:47




Instrument :
BNA_G
ClientSampleId :
PB158316BL


Tgt Ion: 99 Resp: 3375345
Ion Ratio Lower Upper
99 100
42 15.5 10.9 16.3
71 31.9 21.5 32.3



#19
n-Nitroso-di-n-propylamine
Concen: 16.420 ng
RT: 9.098 min Scan# 1023
Delta R.T. 0.363 min
Lab File: BG060295.D
Acq: 10 Jan 2024 10:47

Tgt Ion: 70 Resp: 277425
Ion Ratio Lower Upper
70 100
42 38.0 34.3 51.5
101 0.0 6.2 9.2#
130 1.8 12.2 18.2#

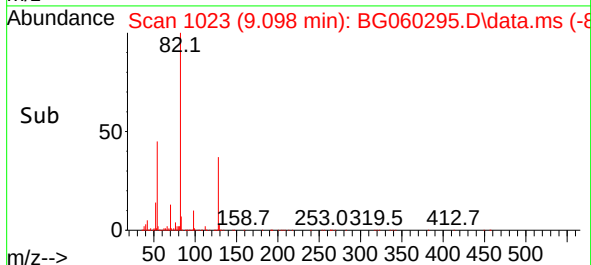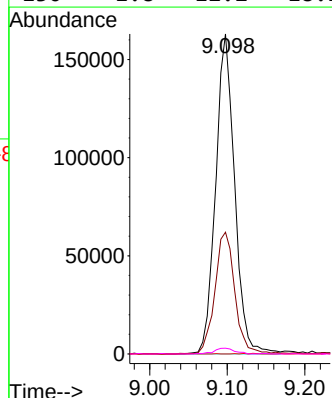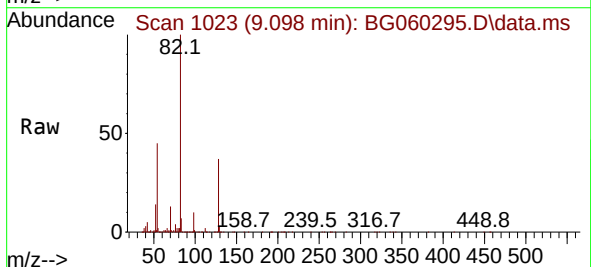







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.737 min Scan# 11
Delta R.T. 0.005 min
Lab File: BG060295.D
Acq: 10 Jan 2024 10:47

Instrument :
BNA_G
ClientSampleId :
PB158316BL

Tgt Ion:136 Resp: 1021291




Ion	Ratio	Lower	Upper
136	100		
137	10.9	8.2	12.4
54	8.1	6.2	9.2
68	8.6	6.3	9.5

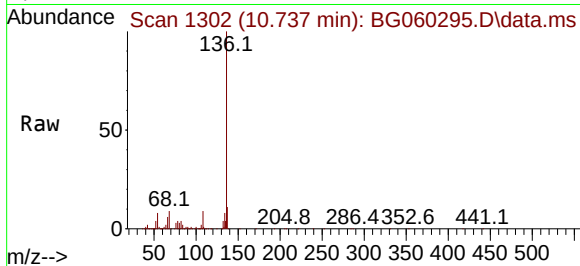


#23
Nitrobenzene-d5
Concen: 108.200 ng
RT: 9.098 min Scan# 1023
Delta R.T. 0.005 min
Lab File: BG060295.D
Acq: 10 Jan 2024 10:47

Tgt Ion: 82 Resp: 2340183

Ion	Ratio	Lower	Upper
82	100		
128	37.2	29.6	44.4
54	44.6	33.6	50.4


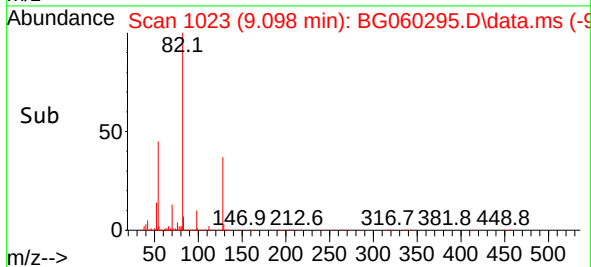

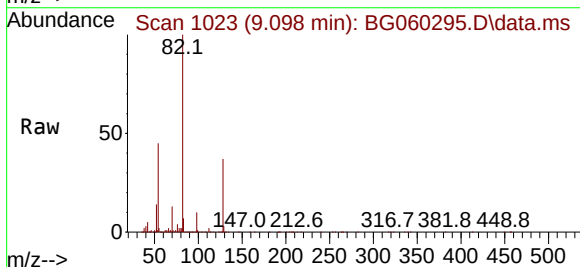




#32
Benzoic acid
Concen: 10.207 ng
RT: 10.061 min Scan# 1187
Delta R.T. 0.016 min
Lab File: BG060295.D
Acq: 10 Jan 2024 10:47




Instrument :
BNA_G
ClientSampleId :
PB158316BL


Tgt Ion:122 Resp: 72
Ion Ratio Lower Upper
122 100
105 0.0 96.0 136.0#
77 0.0 80.1 120.1#

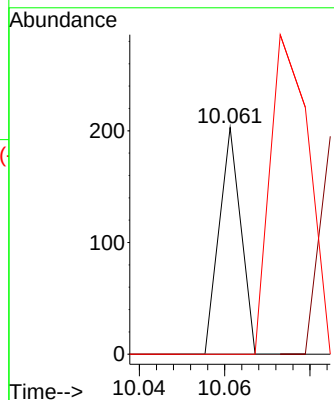

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.568 min Scan# 1954
Delta R.T. -0.001 min
Lab File: BG060295.D
Acq: 10 Jan 2024 10:47

Tgt Ion:164 Resp: 783845
Ion Ratio Lower Upper
164 100
162 103.9 84.4 126.6
160 46.7 34.6 52.0


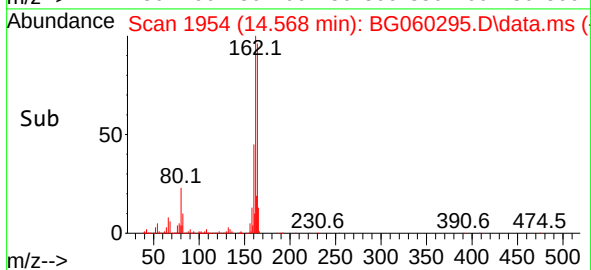
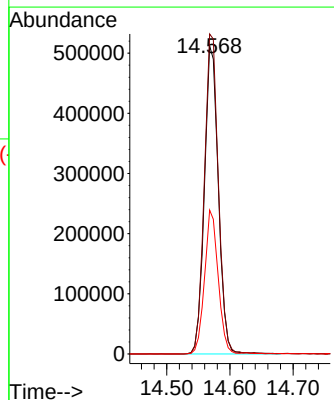





#42
2,4,6-Tribromophenol
Concen: 131.475 ng
RT: 16.060 min Scan# 21
Delta R.T. 0.005 min
Lab File: BG060295.D
Acq: 10 Jan 2024 10:47




Instrument :
BNA_G
ClientSampleId :
PB158316BL


Tgt Ion:330 Resp: 1516252
Ion Ratio Lower Upper
330 100
332 95.9 76.7 115.1
141 24.4 18.6 28.0



#45
2-Fluorobiphenyl
Concen: 82.868 ng
RT: 13.193 min Scan# 1720
Delta R.T. 0.005 min
Lab File: BG060295.D
Acq: 10 Jan 2024 10:47

Tgt Ion:172 Resp: 4671981
Ion Ratio Lower Upper
172 100
171 45.6 34.6 51.8
170 31.5 24.4 36.6


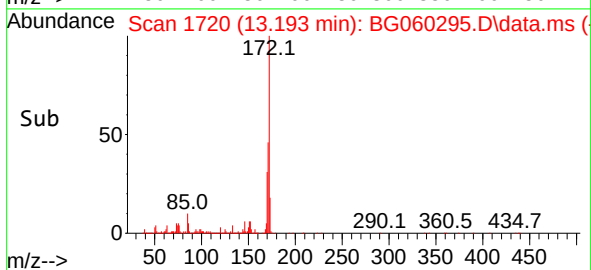




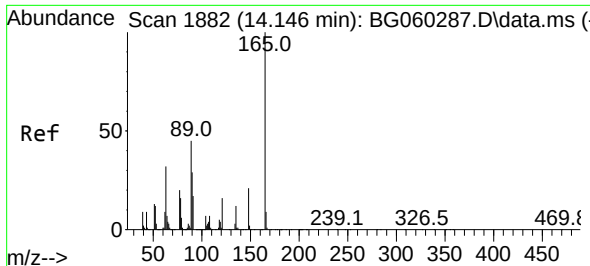

#51
2,6-Dinitrotoluene
Concen: 8.039 ng
RT: 14.568 min Scan# 1954
Delta R.T. 0.422 min
Lab File: BG060295.D
Acq: 10 Jan 2024 10:47




Instrument :
BNA_G
ClientSampleId :
PB158316BL


Tgt Ion:165 Resp: 102745
Ion Ratio Lower Upper
165 100
63 0.9 35.0 52.4#
89 1.1 36.2 54.2#

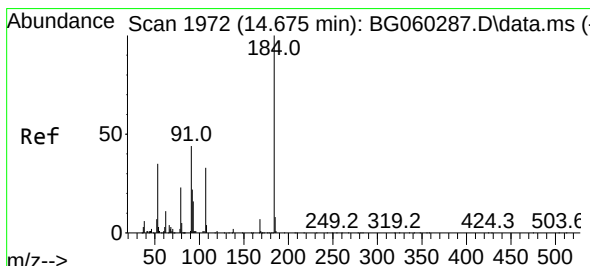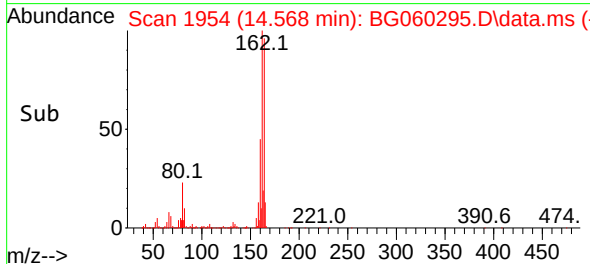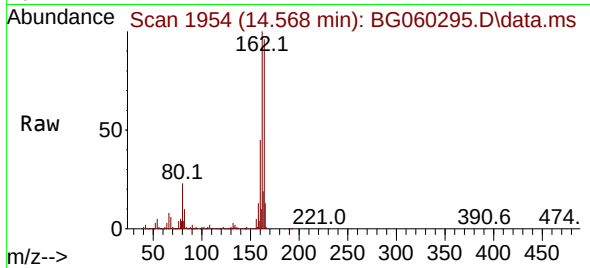

#54
2,4-Dinitrophenol
Concen: 8.598 ng
RT: 14.574 min Scan# 1955
Delta R.T. -0.101 min
Lab File: BG060295.D
Acq: 10 Jan 2024 10:47

Tgt Ion:184 Resp: 97
Ion Ratio Lower Upper
184 100
63 394.2 41.0 61.4#
154 531.8 39.2 58.8#


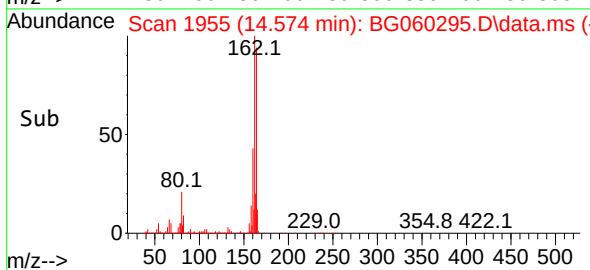

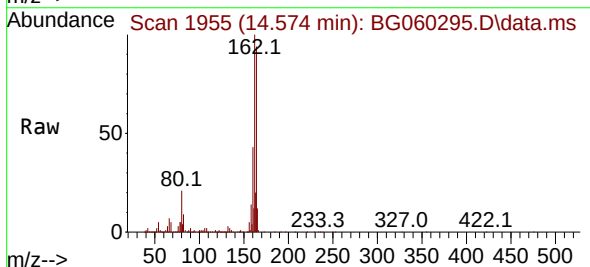




#57
2,4-Dinitrotoluene
Concen: 5.862 ng
RT: 14.568 min Scan# 1954
Delta R.T. -0.360 min
Lab File: BG060295.D
Acq: 10 Jan 2024 10:47




Instrument :
BNA_G
ClientSampleId :
PB158316BL


Tgt Ion:165 Resp: 102745
Ion Ratio Lower Upper
165 100
63 0.9 30.4 45.6#
89 1.1 55.4 83.0#
182 0.0 1.6 2.4#

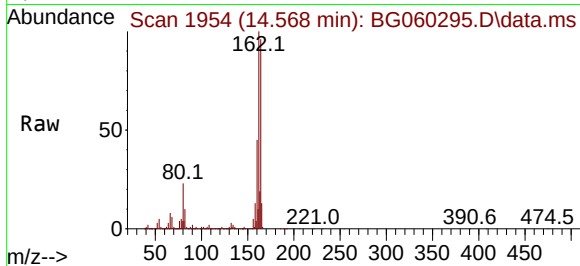

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.317 min Scan# 2422
Delta R.T. 0.005 min
Lab File: BG060295.D
Acq: 10 Jan 2024 10:47

Tgt Ion:188 Resp: 2038251
Ion Ratio Lower Upper
188 100
94 10.2 7.1 10.7
80 10.4 8.5 12.7


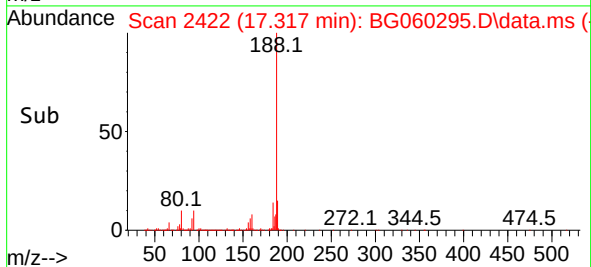

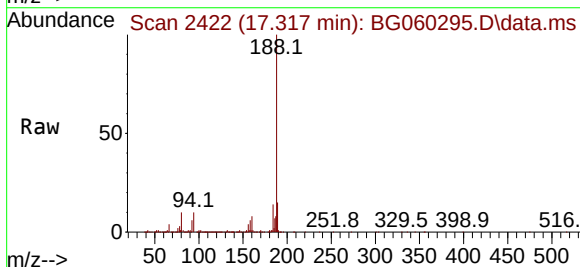




#67
4-Bromophenyl-phenylether
Concen: 4.240 ng
RT: 16.060 min Scan# 21
Delta R.T. -0.442 min
Lab File: BG060295.D
Acq: 10 Jan 2024 10:47




Instrument :
BNA_G
ClientSampleId :
PB158316BL


Tgt Ion:248 Resp: 94961
Ion Ratio Lower Upper
248 100
250 197.9 77.6 116.4#
141 409.7 34.2 51.4#



#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.583 min Scan# 3148
Delta R.T. 0.005 min
Lab File: BG060295.D
Acq: 10 Jan 2024 10:47

Tgt Ion:240 Resp: 2038607
Ion Ratio Lower Upper
240 100
120 9.6 7.3 10.9
236 26.1 20.3 30.5

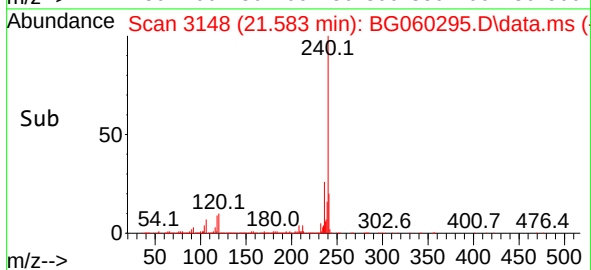

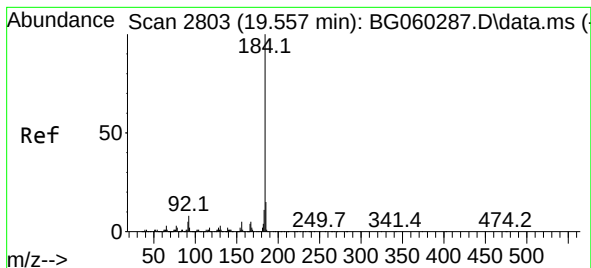

#77

Benzidine

Concen: 3.391 ng

RT: 19.944 min Scan# 2869

Delta R.T. 0.387 min

Lab File: BG060295.D

Acq: 10 Jan 2024 10:47

Instrument :

BNA_G

ClientSampleId :

PB158316BL





Tgt Ion:184 Resp: 150193

Ion Ratio Lower Upper

184 100

185 15.3 12.2 18.4

183 5.4 9.0 13.4#

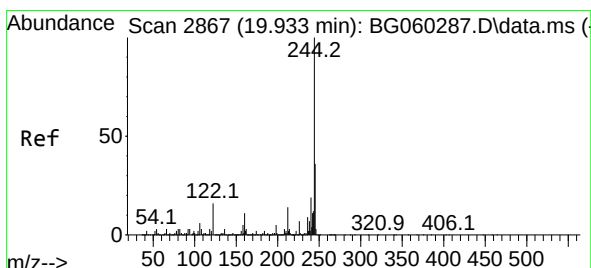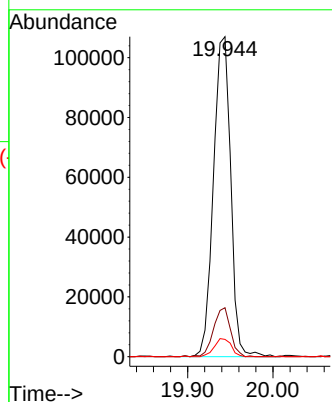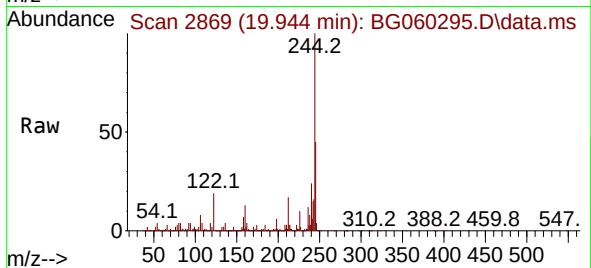

#79

Terphenyl-d14

Concen: 80.293 ng

RT: 19.944 min Scan# 2869

Delta R.T. 0.011 min

Lab File: BG060295.D

Acq: 10 Jan 2024 10:47




Tgt Ion:244 Resp: 6626504


Ion Ratio Lower Upper

244 100

212 17.1 10.9 16.3#

122 18.7 12.6 18.8

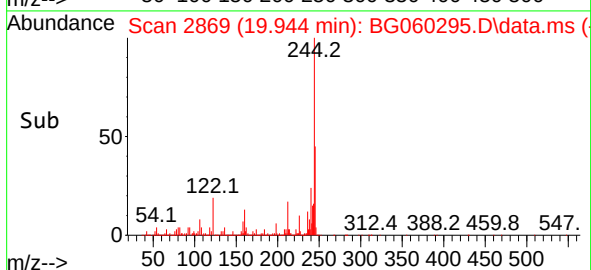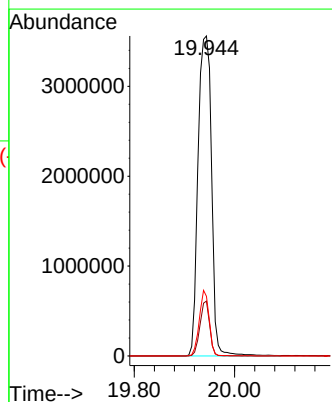



#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.756 min Scan# 30
 Delta R.T. 0.017 min
 Lab File: BG060295.D
 Acq: 10 Jan 2024 10:47

Instrument :
 BNA_G
 ClientSampleId :
 PB158316BL

Tgt Ion:264 Resp: 2219512
 Ion Ratio Lower Upper
 264 100
 260 22.8 17.8 26.6
 265 21.6 16.8 25.2

