
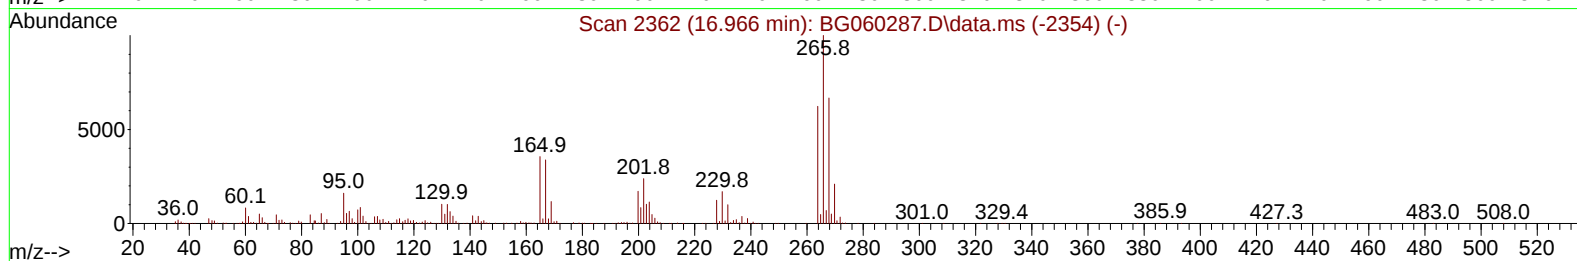
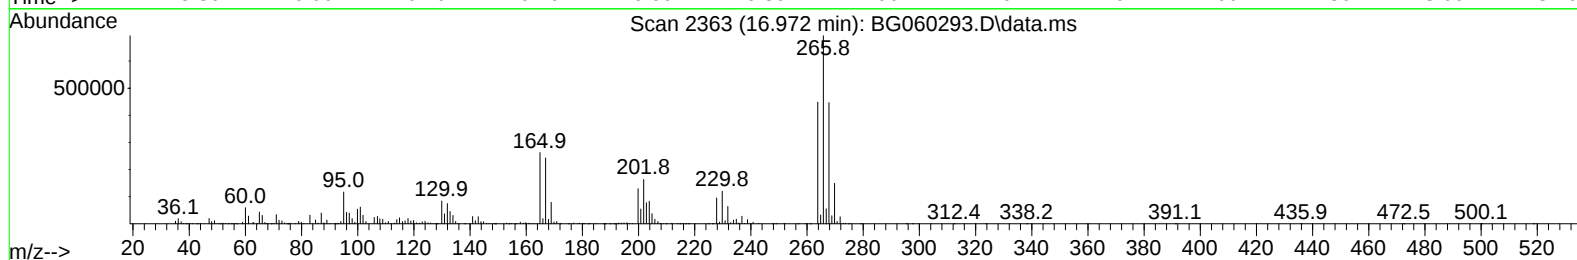


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011024\
Data File : BG060293.D
Acq On : 10 Jan 2024 9:26
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 10 11:29:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

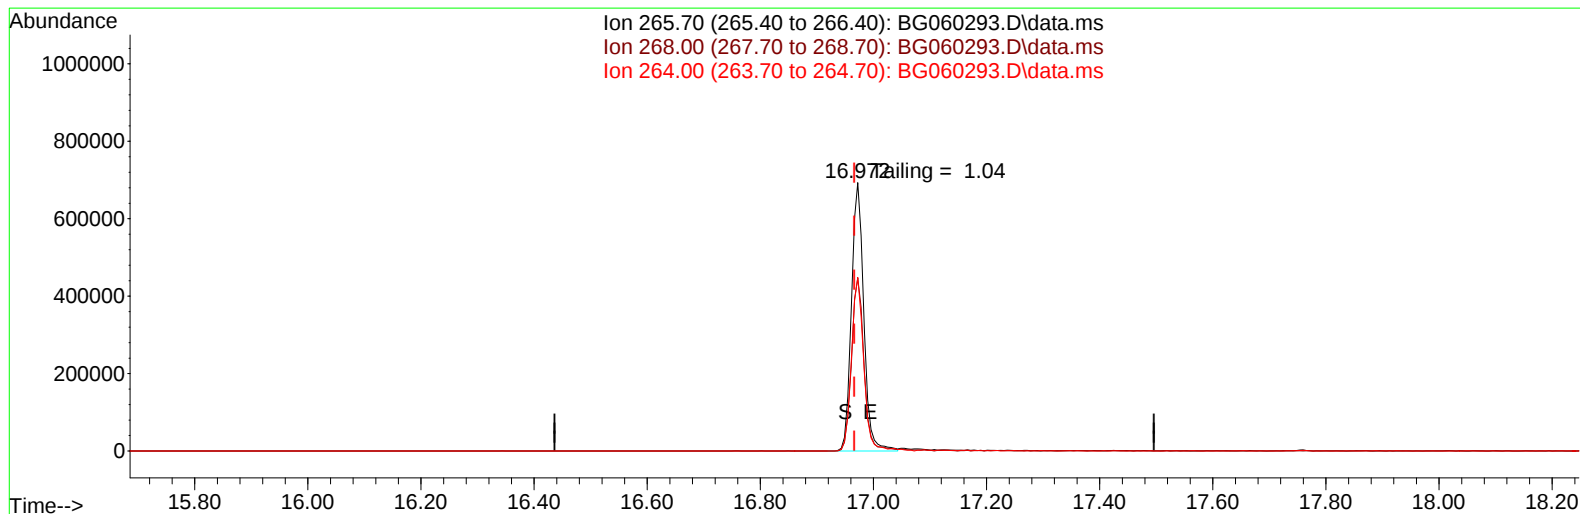

TIC: BG060293.D\data.ms

(70) Pentachlorophenol (C)




16.972min (+ 0.006) 26088.32 ng

response 1055887

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	71.80	64.43
264.00	62.30	64.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011024\
Data File : BG060293.D
Acq On : 10 Jan 2024 9:26
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 10 11:29:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

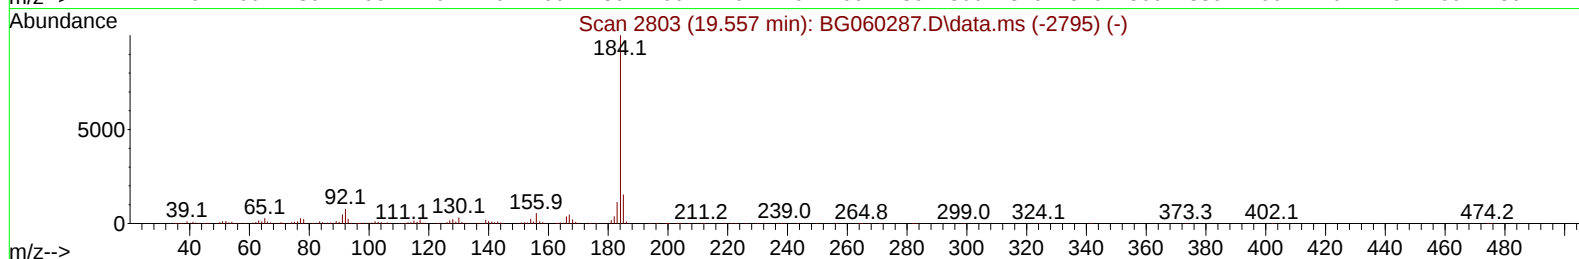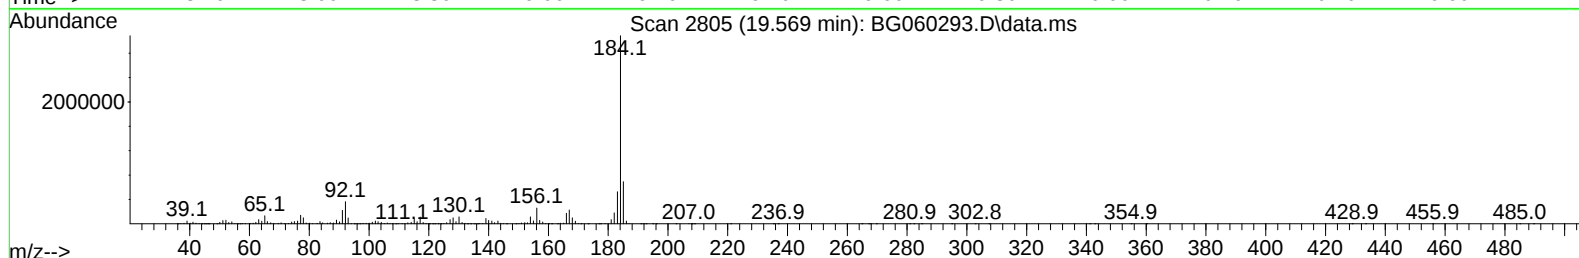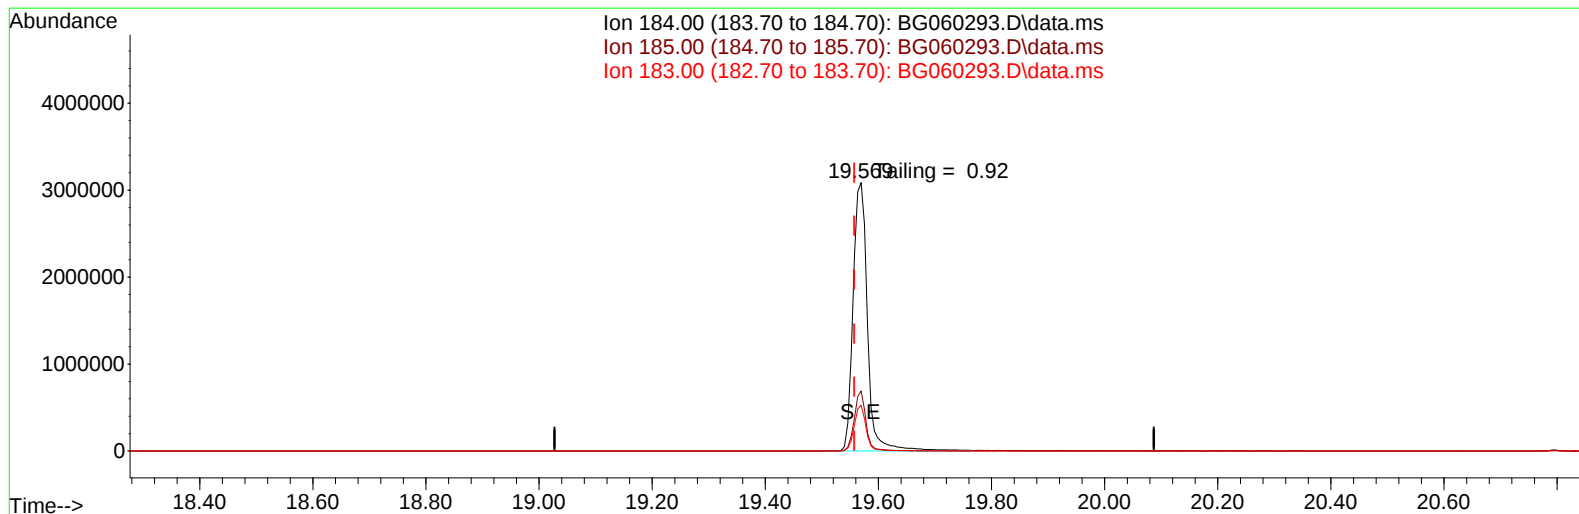

TIC: BG060293.D\data.ms

(77) Benzidine**19.569min (+ 0.012) 380245.77 ng m****response 5493510**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	22.37#
183.00	11.20	17.07#
0.00	0.00	0.00