
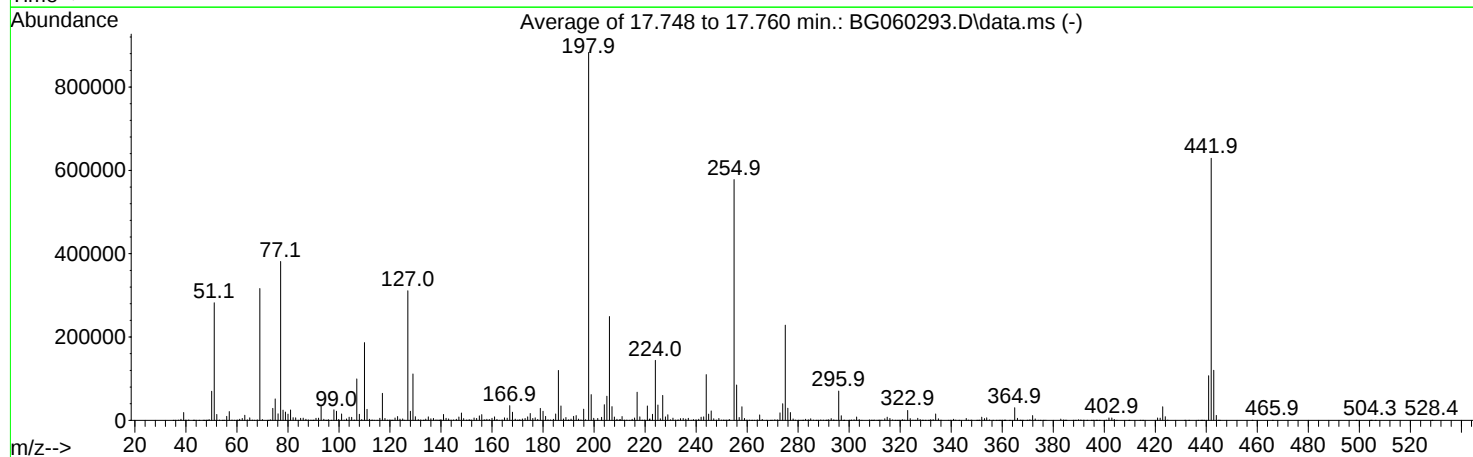


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011024\
Data File : BG060293.D
Acq On : 10 Jan 2024 9:26
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jan 09 04:07:12 2024

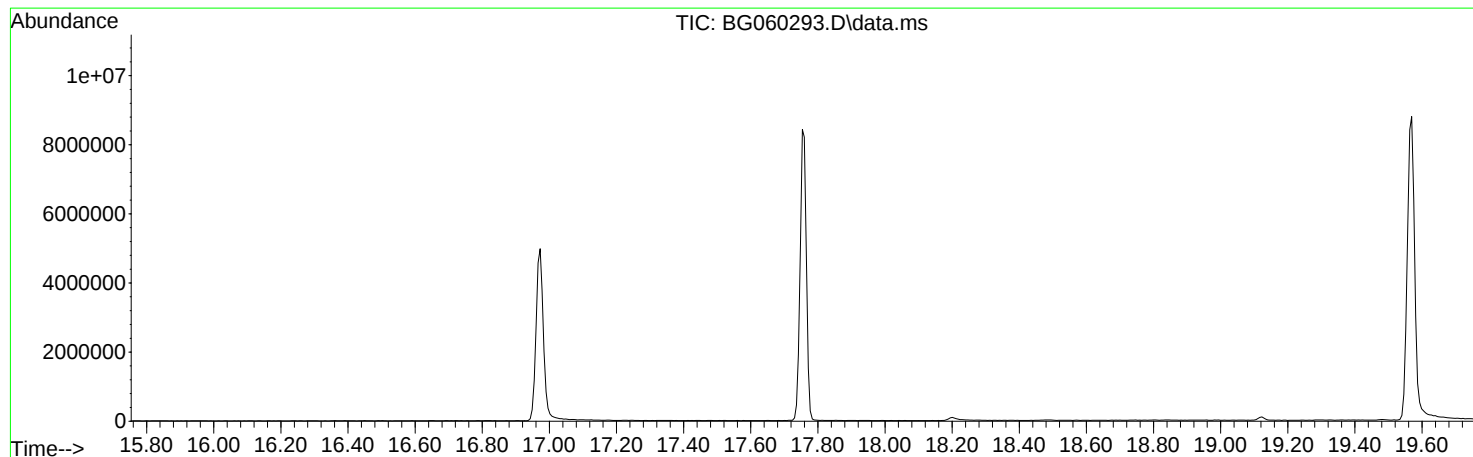




AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.0	282453	PASS
68	69	0.00	2	0.4	1360	PASS
69	198	0.00	100	35.8	316464	PASS
70	69	0.00	2	0.6	1822	PASS
127	198	10	80	35.3	311253	PASS
197	198	0.00	2	0.2	1376	PASS
198	198	100	100	100.0	882837	PASS
199	198	5	9	7.0	61987	PASS
275	198	10	60	25.9	228565	PASS
365	198	1	100	3.4	30440	PASS
441	198	0.01	100	12.1	107051	PASS
442	442	50	100	100.0	629184	PASS
443	442	15	24	19.1	120136	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011024\
Data File : BG060293.D
Acq On : 10 Jan 2024 9:26
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 10 11:29:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

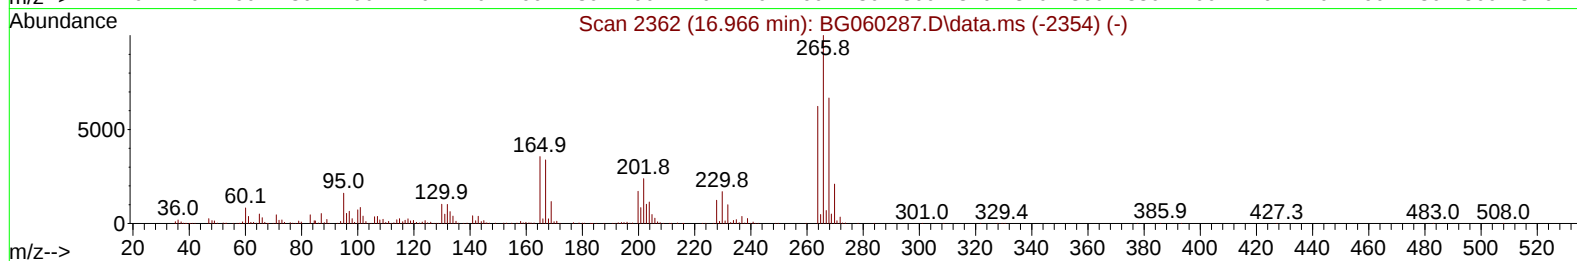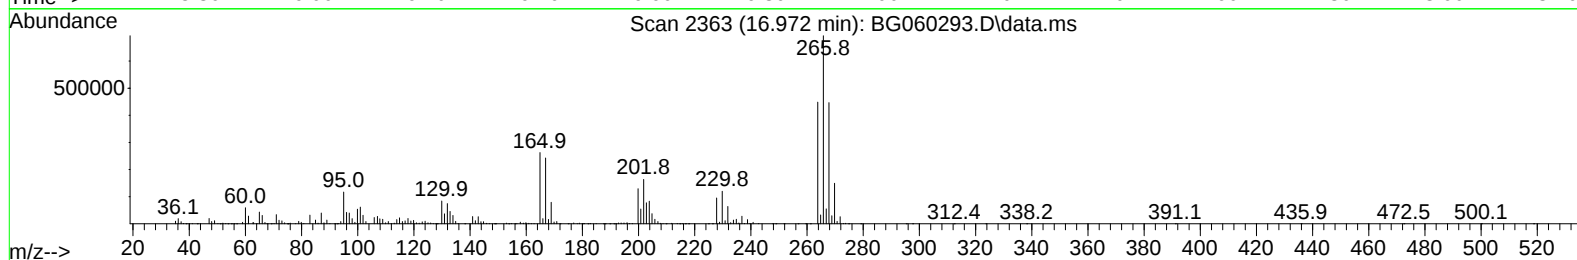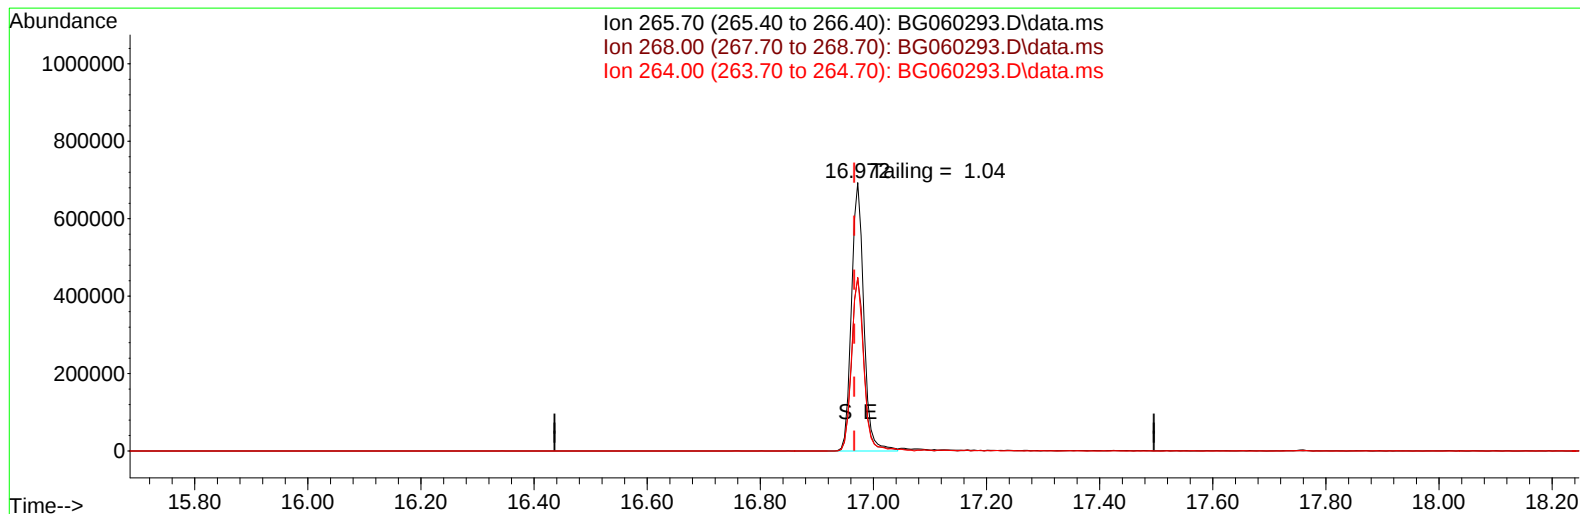

TIC: BG060293.D\data.ms

(70) Pentachlorophenol (C)

16.972min (+ 0.006) 26088.32 ng




response 1055887

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	71.80	64.43
264.00	62.30	64.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011024\
Data File : BG060293.D
Acq On : 10 Jan 2024 9:26
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 10 11:29:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

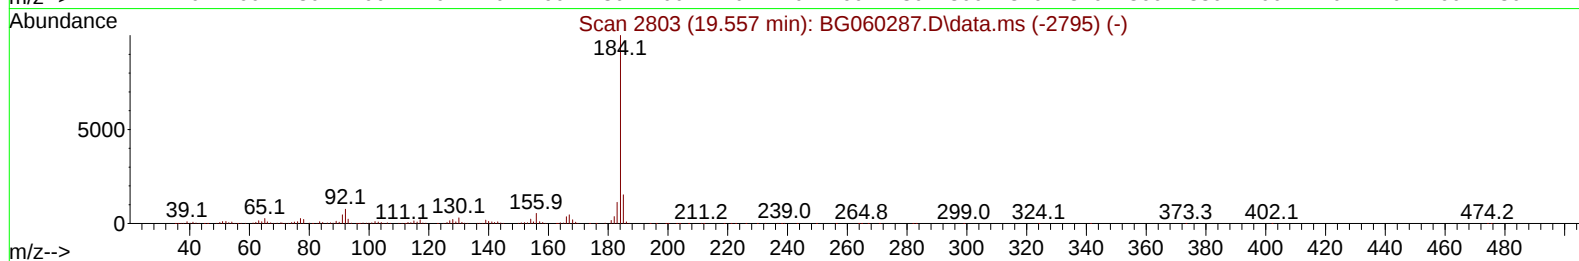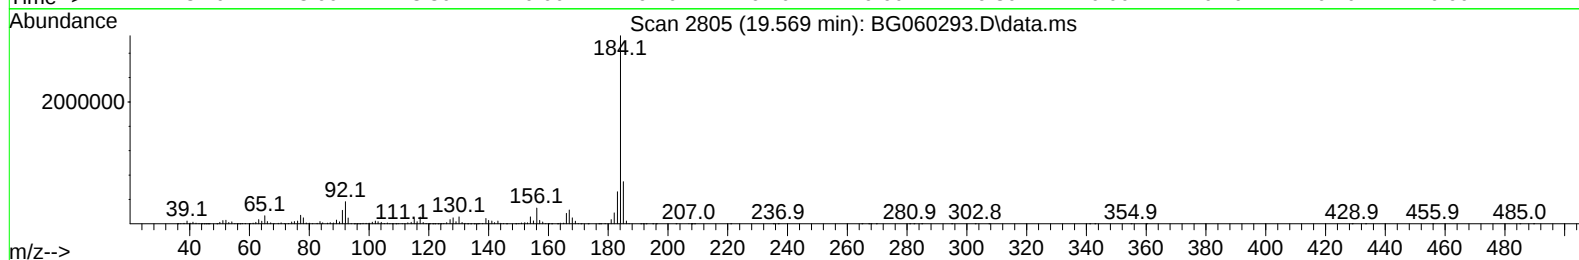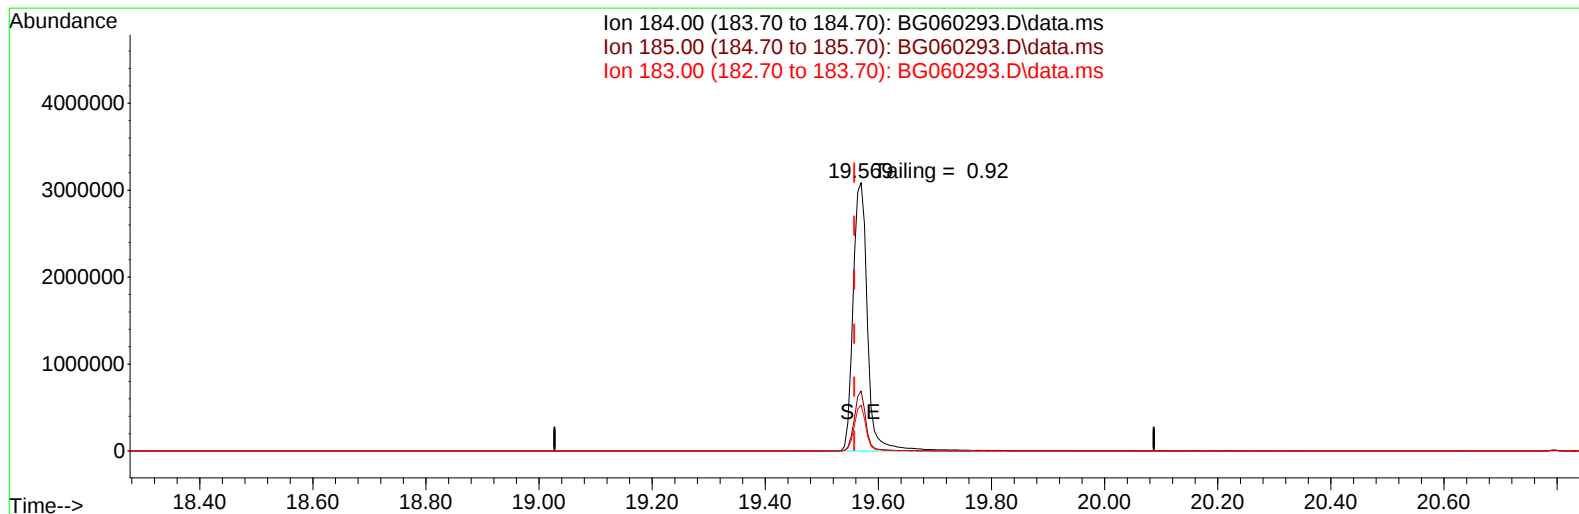

TIC: BG060293.D\data.ms

(77) Benzidine

19.569min (+ 0.012) 380245.77 ng m

response 5493510

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	22.37#
183.00	11.20	17.07#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/10/2024	BNA_G	<u>BG060293.D</u>
Compound Name	Response	Retention Time
DDT	2843958	20.797
DDD	47770	20.404
DDE	841	19.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
48611	2892569	1.68

Instrument :
BNA_G
ClientSampleId :
DFTPP