
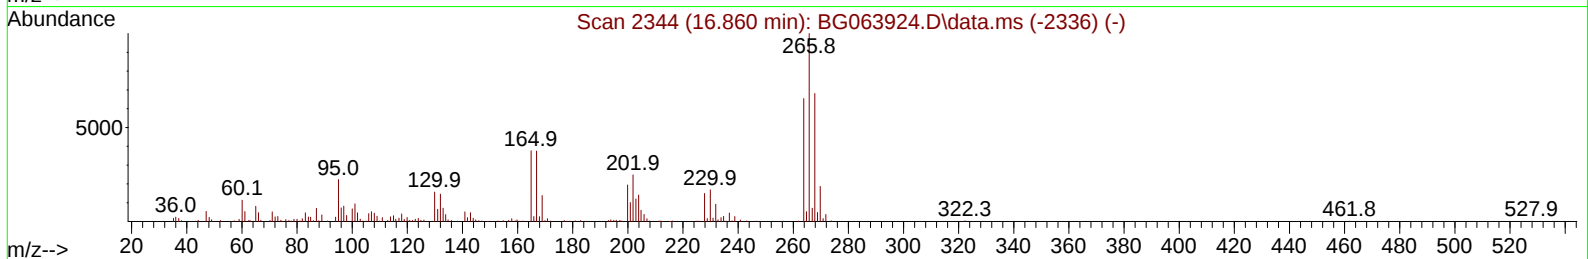
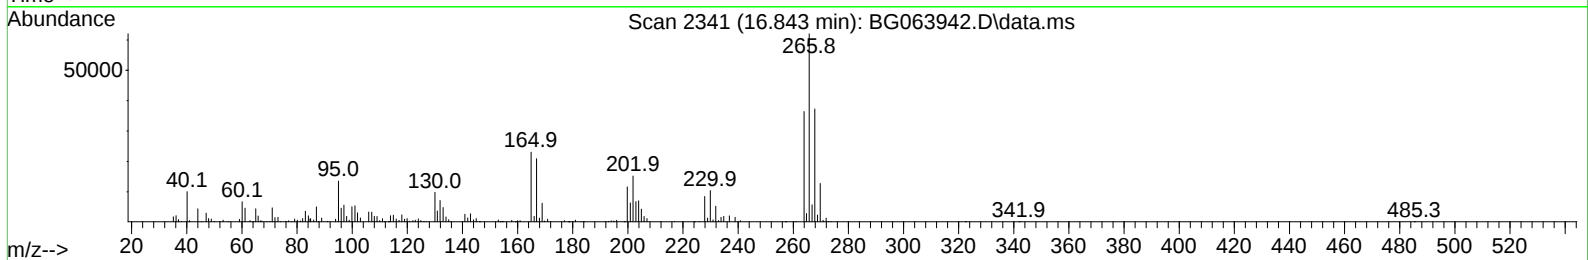


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011025\
Data File : BG063942.D
Acq On : 10 Jan 2025 8:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 10 09:22:37 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 03 23:17:54 2025
Response via : Initial Calibration

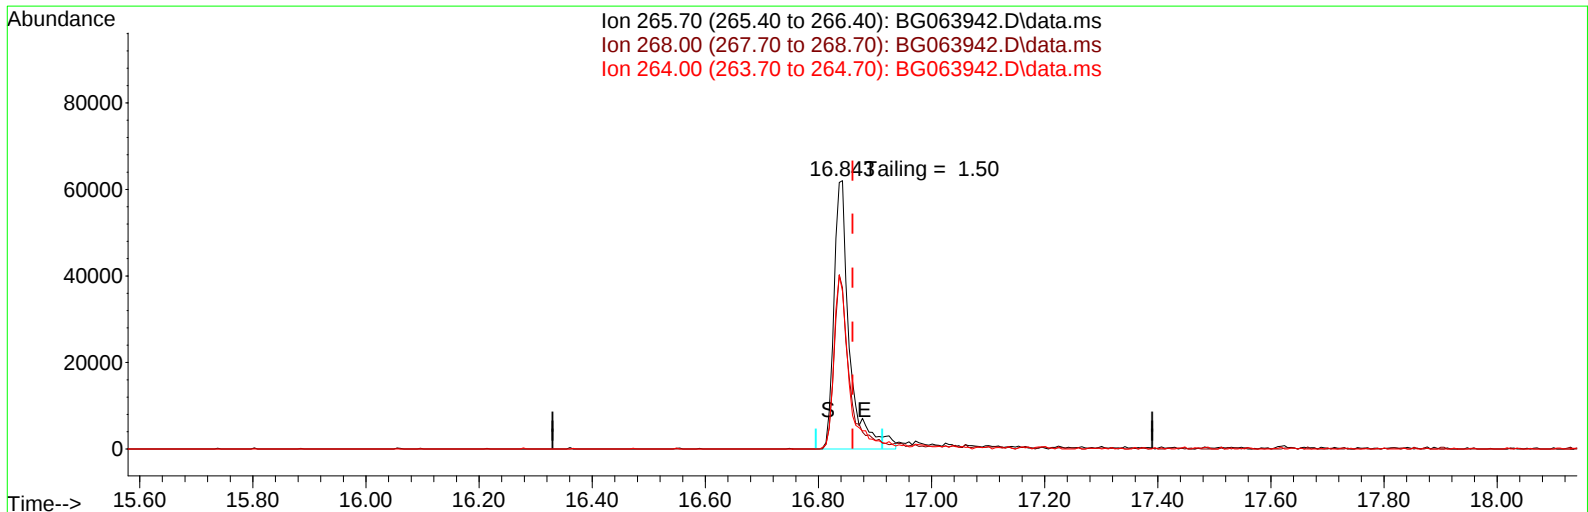

TIC: BG063942.D\data.ms

(70) Pentachlorophenol (C)




16.843min (-0.017) 170132.47 ng

response 115803

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.10	60.12
264.00	65.30	58.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011025\
Data File : BG063942.D
Acq On : 10 Jan 2025 8:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 10 09:22:37 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 03 23:17:54 2025
Response via : Initial Calibration

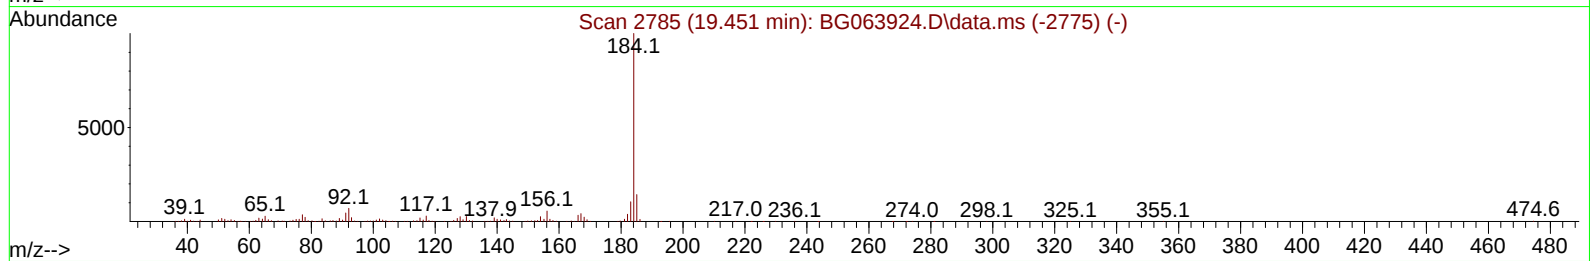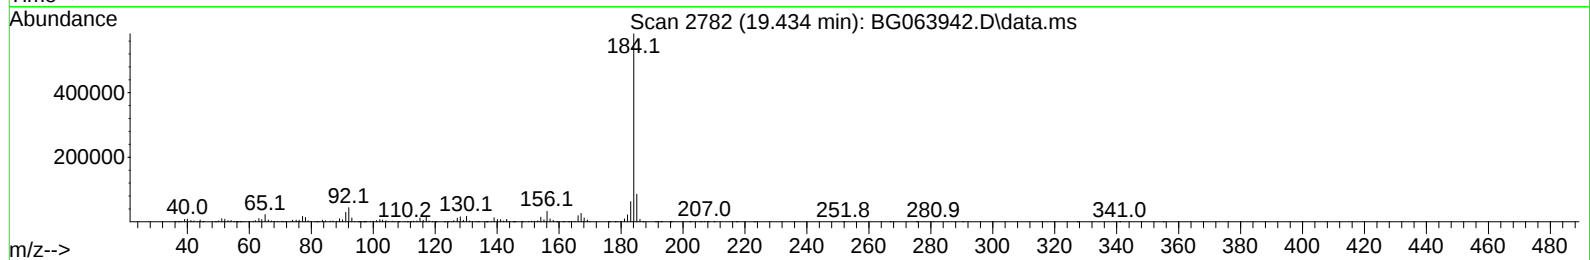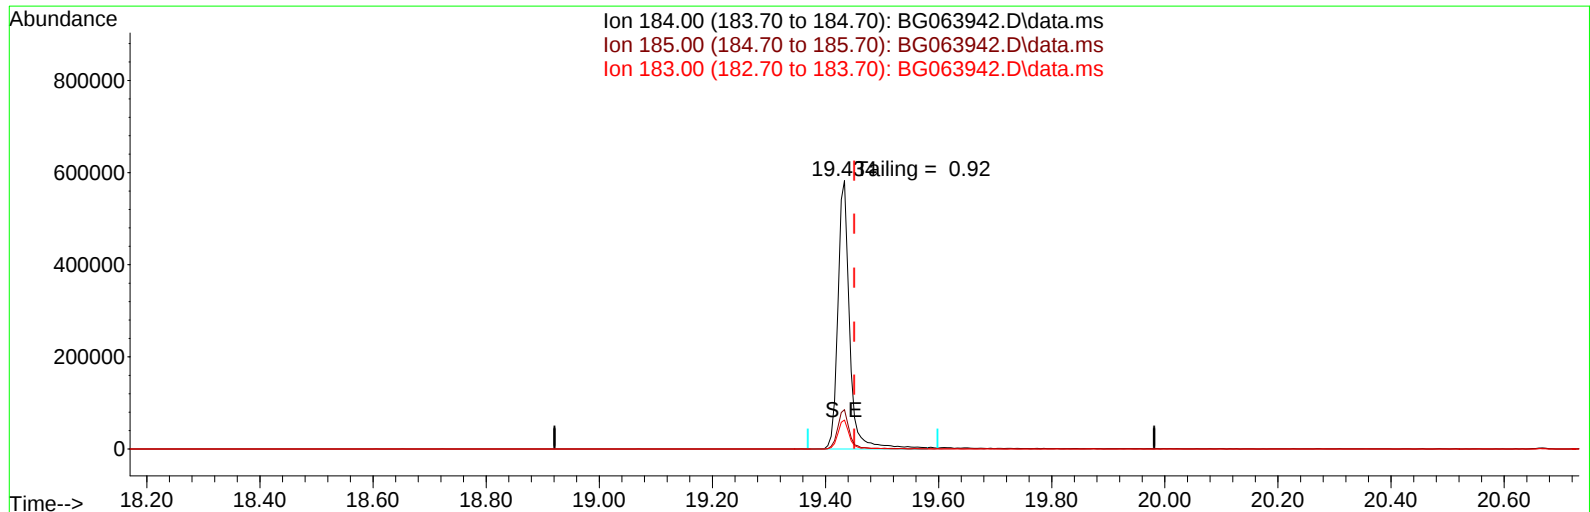

TIC: BG063942.D\data.ms

(77) Benzidine**19.434min (-0.017) 416967.61 ng****response 845968**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.67
183.00	10.50	10.79
0.00	0.00	0.00