
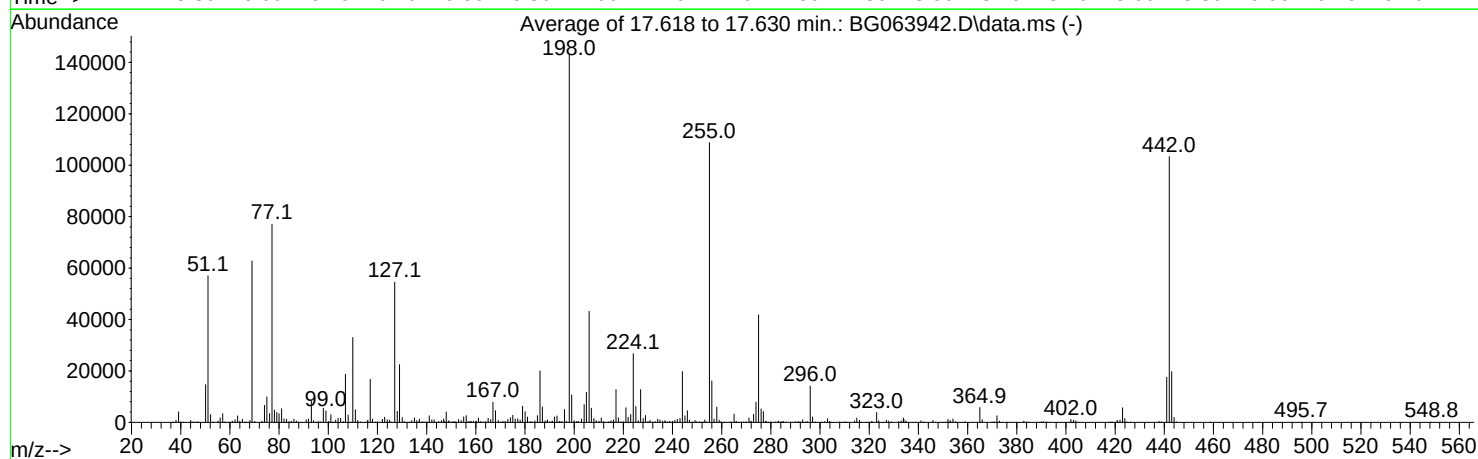


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG011025\  
Data File : BG063942.D  
Acq On : 10 Jan 2025 8:41  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG010325.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Fri Jan 03 23:17:54 2025

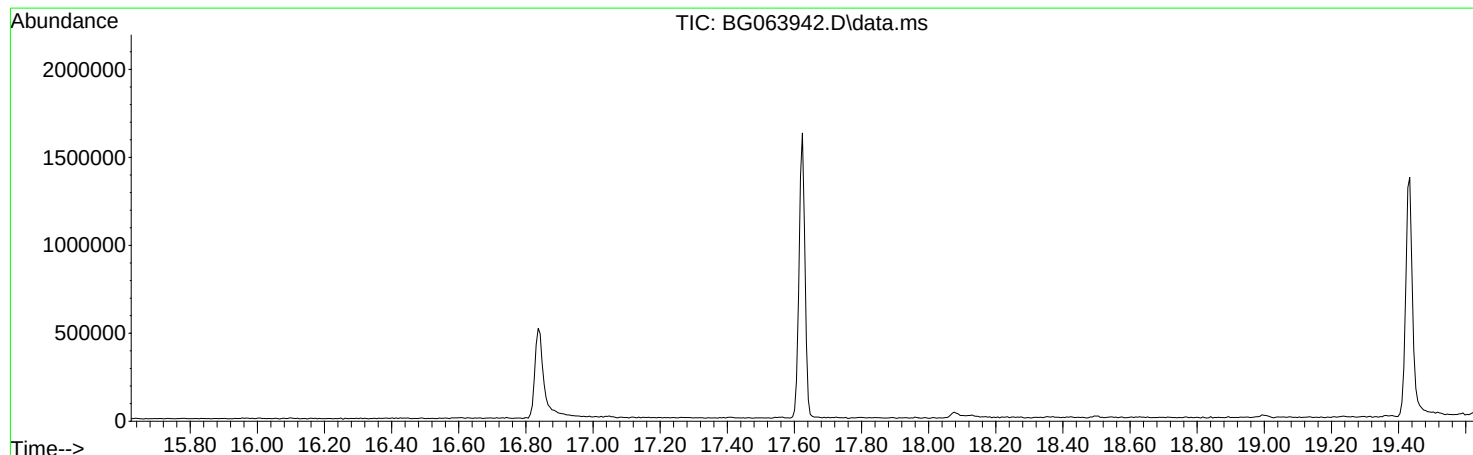

AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2466

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 39.8         | 57008      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.2          | 764        | PASS                |
| 69             | 198             | 0.00            | 100             | 43.9         | 62800      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.6          | 405        | PASS                |
| 127            | 198             | 10              | 80              | 38.1         | 54528      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.3          | 459        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 143067     | PASS                |
| 199            | 198             | 5               | 9               | 7.5          | 10733      | PASS                |
| 275            | 198             | 10              | 60              | 29.2         | 41811      | PASS                |
| 365            | 198             | 1               | 100             | 4.1          | 5805       | PASS                |
| 441            | 198             | 0.01            | 100             | 12.3         | 17574      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 103365     | PASS                |
| 443            | 442             | 15              | 24              | 19.1         | 19741      | PASS                |

### DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 1/10/2025     | BNA_G            | <u>BG063942.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 482354           | 20.667             |
| DDD           | 47943            | 20.233             |
| DDE           | 1292             | 19.721             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 49235         | 531589           | 9.26               |
|               |                  |                    |

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG011025\  
Data File : BG063942.D  
Acq On : 10 Jan 2025 8:41  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: Jan 10 09:22:37 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG010325.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Jan 03 23:17:54 2025  
Response via : Initial Calibration

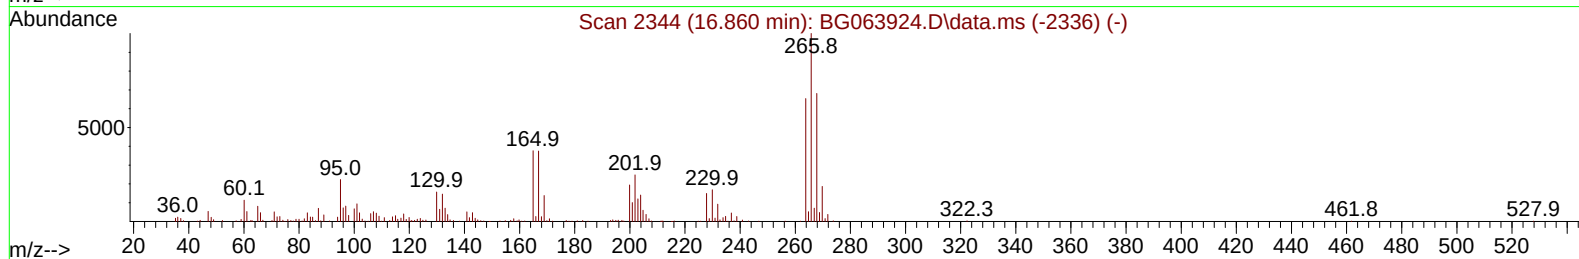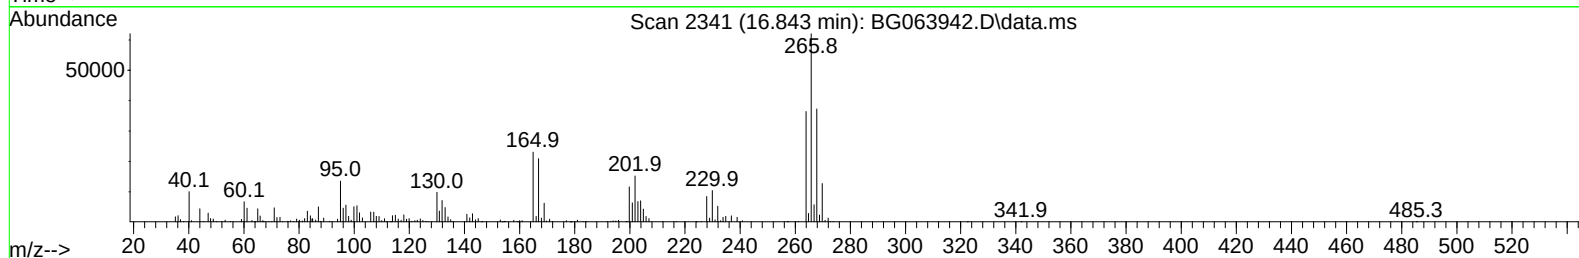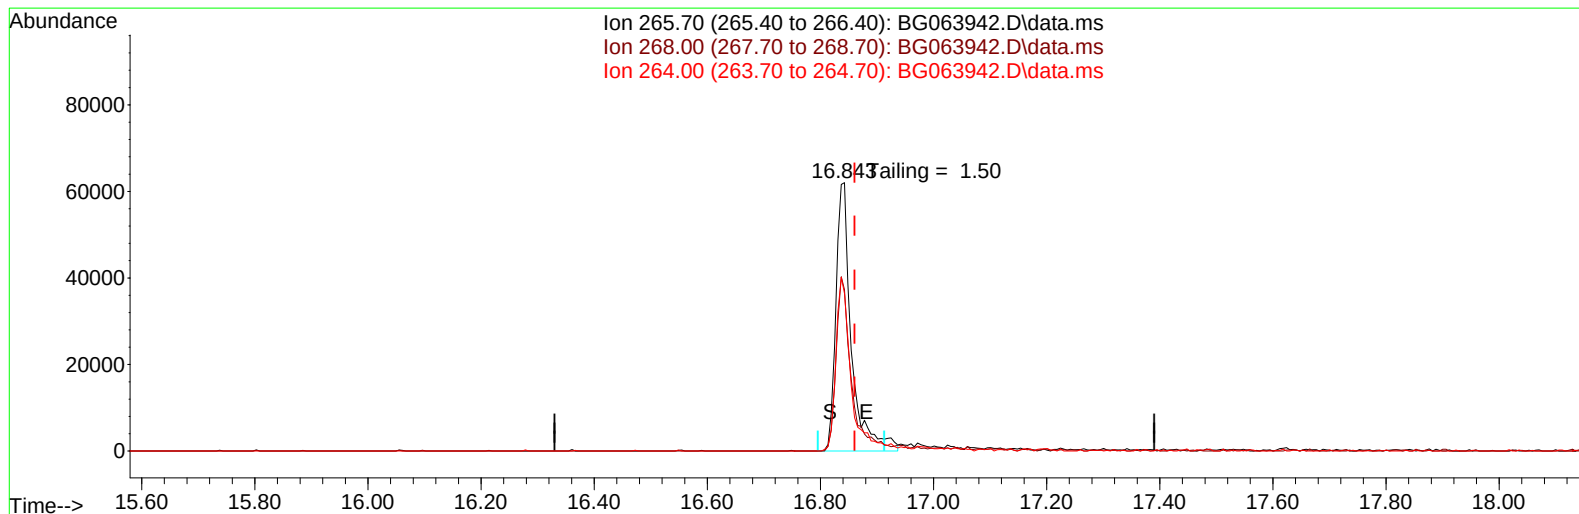

TIC: BG063942.D\data.ms

**(70) Pentachlorophenol (C)**

**16.843min (-0.017) 170132.47 ng**




**response 115803**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 68.10  | 60.12  |
| 264.00 | 65.30  | 58.76  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG011025\  
Data File : BG063942.D  
Acq On : 10 Jan 2025 8:41  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
DFTPP

Quant Time: Jan 10 09:22:37 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG010325.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Jan 03 23:17:54 2025  
Response via : Initial Calibration

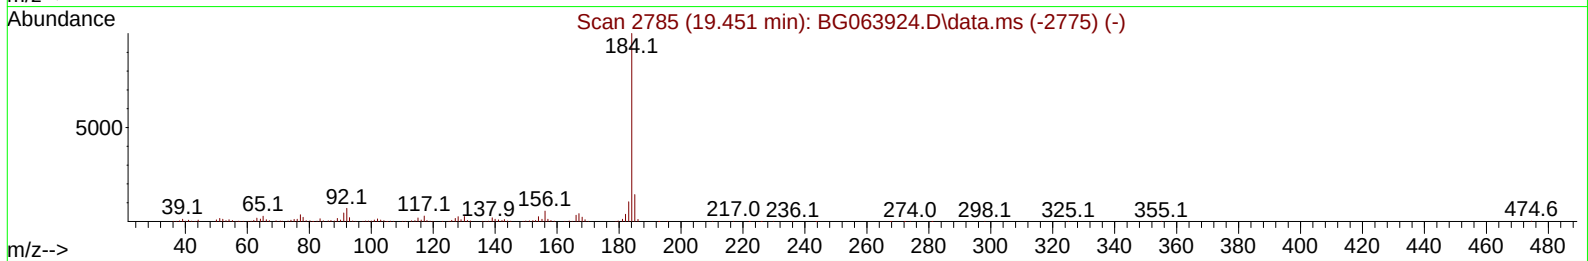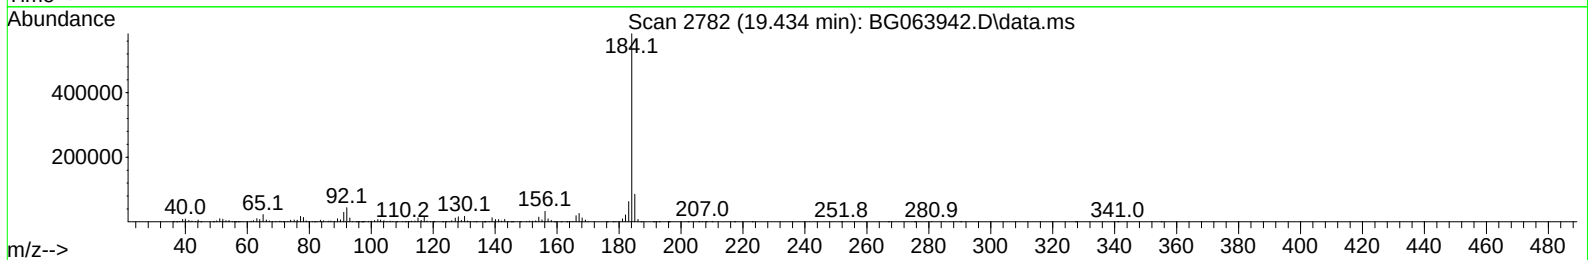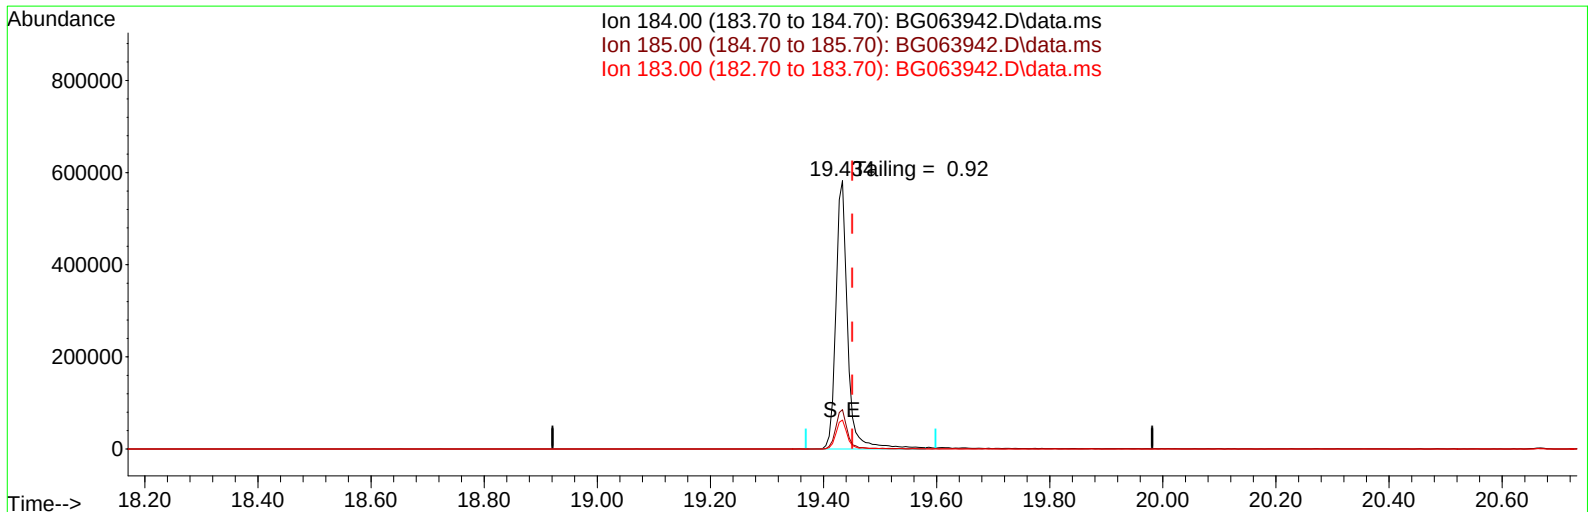

TIC: BG063942.D\data.ms

**(77) Benzidine**

**19.434min (-0.017) 416967.61 ng**

**response 845968**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.30  | 14.67  |
| 183.00 | 10.50  | 10.79  |
| 0.00   | 0.00   | 0.00   |