
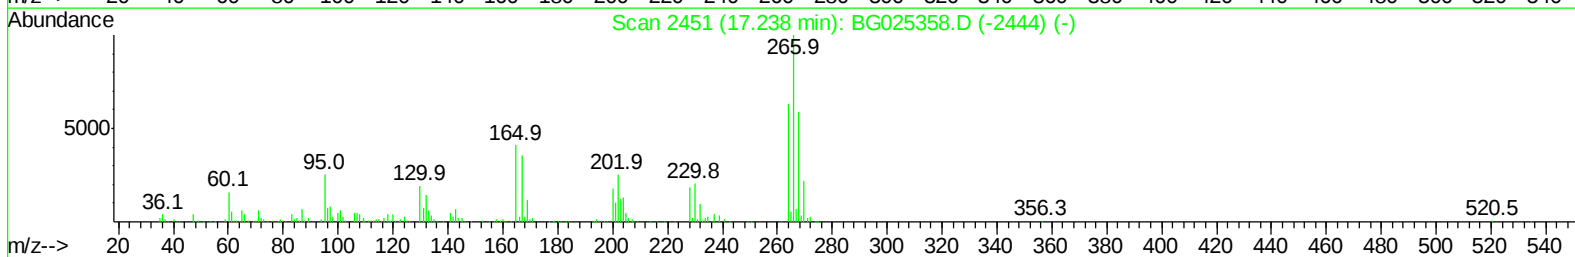
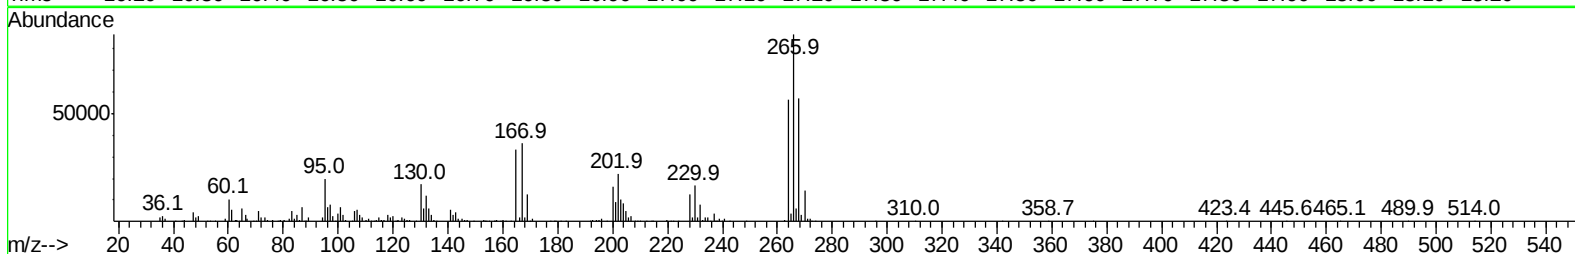


Data Path : Z:\HPCHEM1\BNA G\Data\BG011117\
Data File : BG025470.D
Acq On : 11 Jan 2017 12:42
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 12 13:49:04 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 10 11:26:22 2017
Response via : Initial Calibration

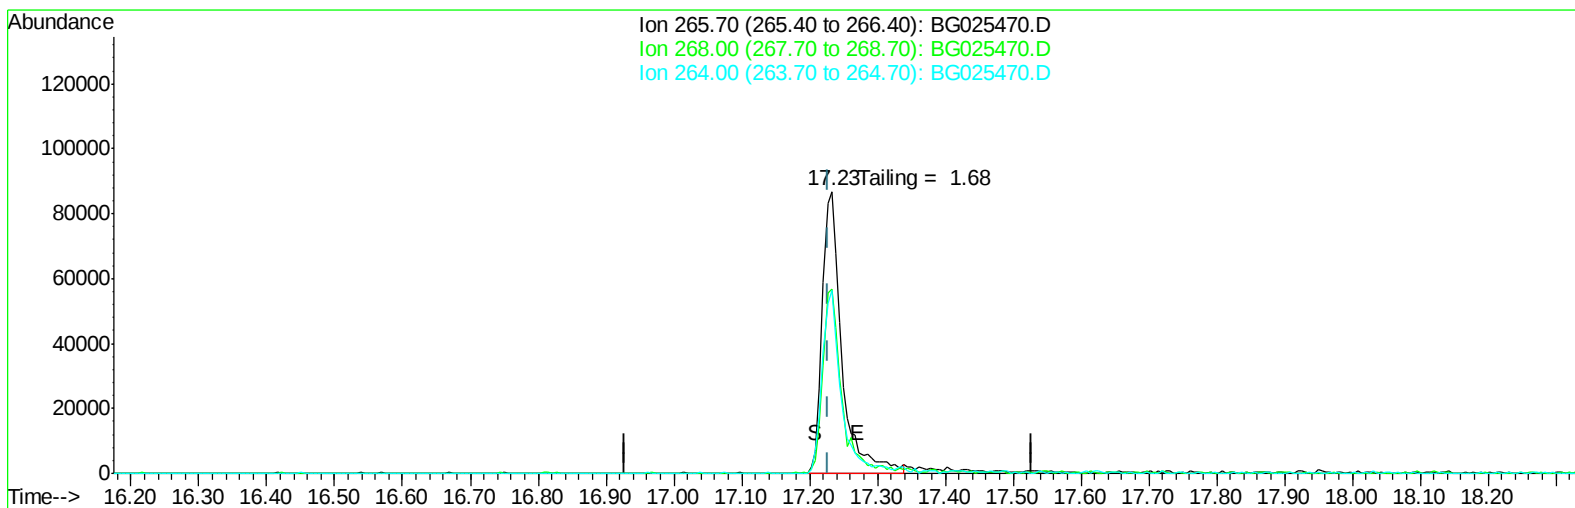

TIC: BG025470.D

(69) Pentachlorophenol (C)




17.232min (+0.005) 435754.60ng

response 172699

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	65.58
264.00	62.60	65.23
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG011117\
Data File : BG025470.D
Acq On : 11 Jan 2017 12:42
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 12 13:49:04 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 10 11:26:22 2017
Response via : Initial Calibration

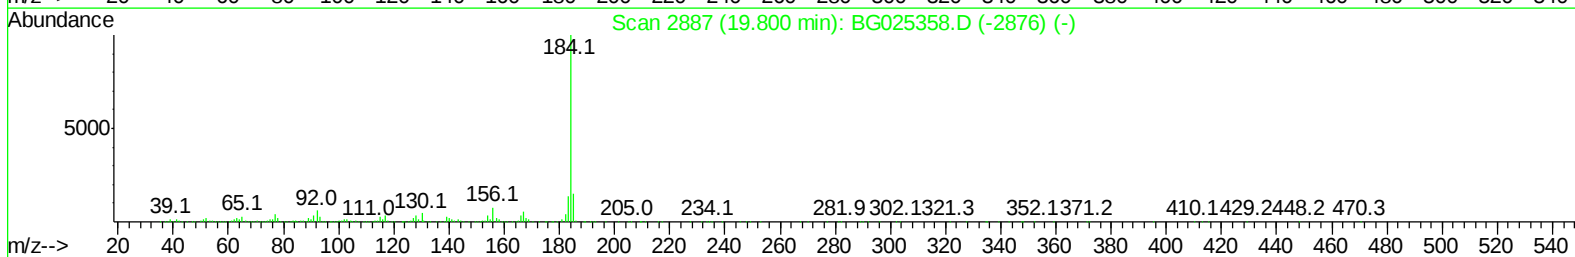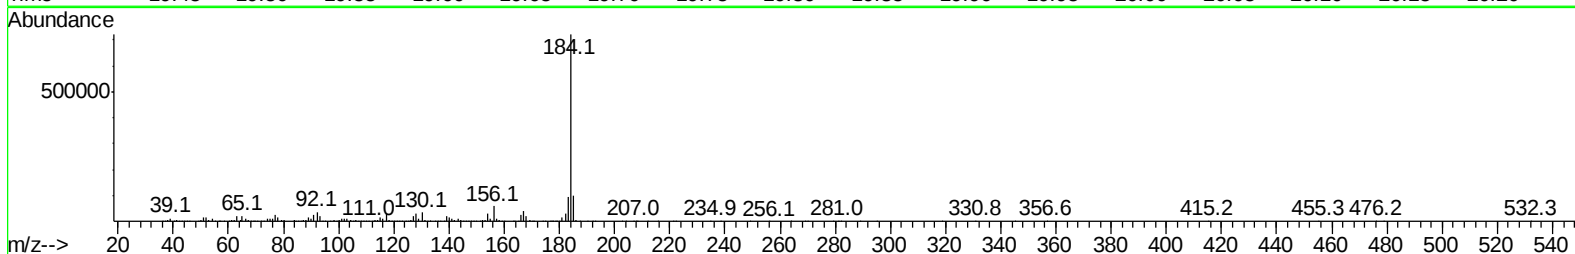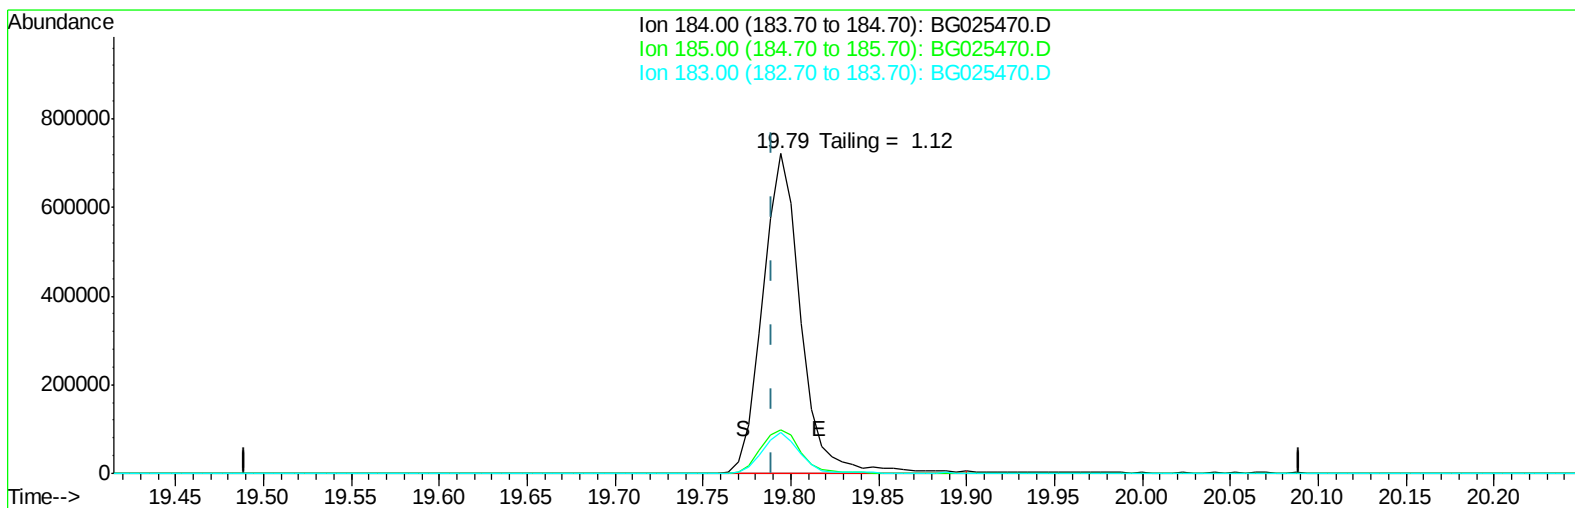

TIC: BG025470.D

(76) Benzidine

19.794min (+0.005) 641900.99ng

response 1088813

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	13.75
183.00	13.80	12.78
0.00	0.00	0.00