
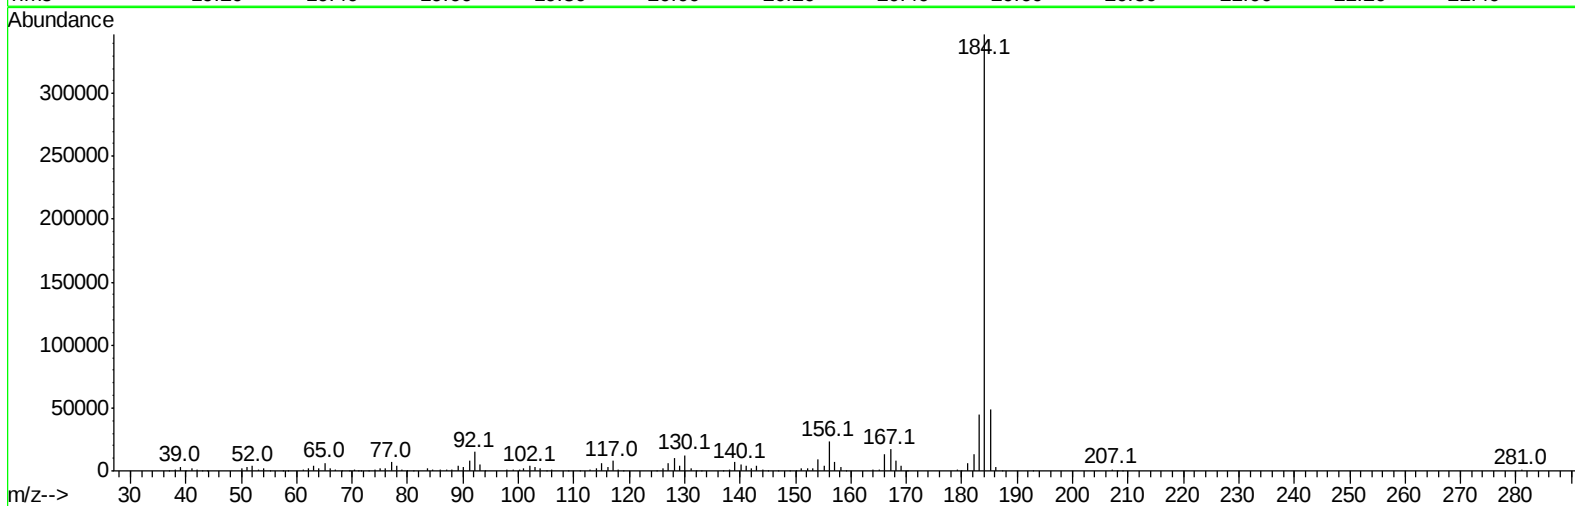


Data Path : U:\HPCHEM1\BNA G\DATA\BG011118\
Data File : BG031982.D
Acq On : 11 Jan 2018 13:53
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 12 06:29:33 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 11 15:23:30 2018
Response via : Initial Calibration

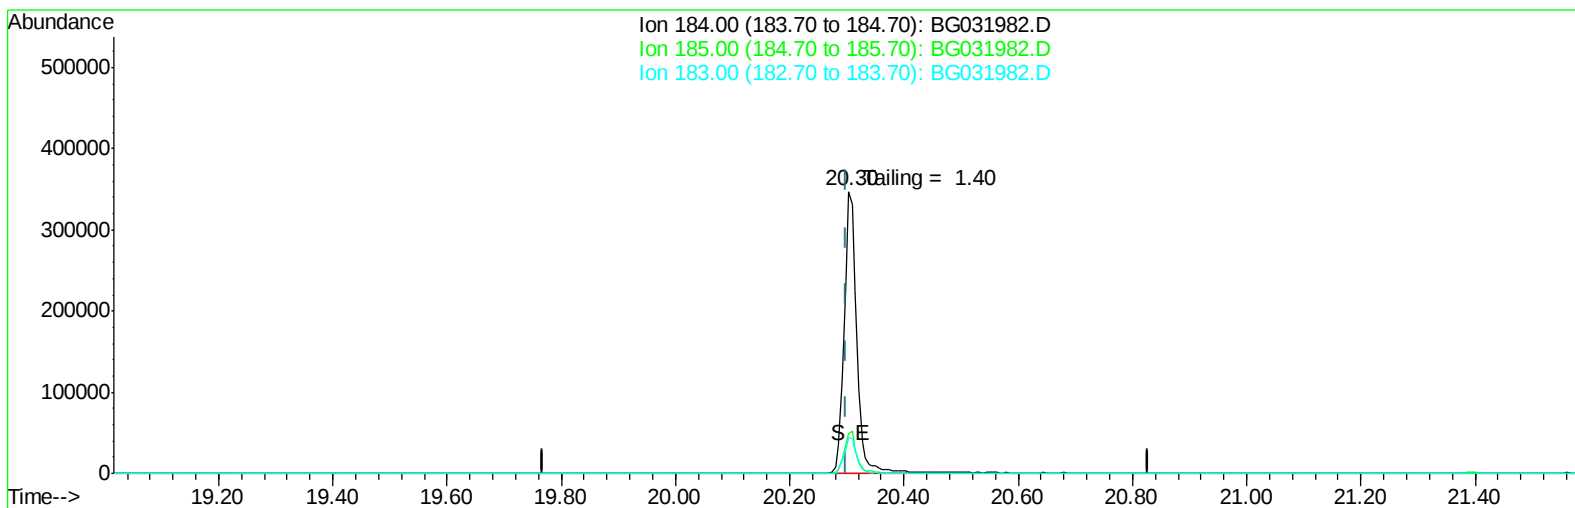

TIC: BG031982.D

(76) Benzidine



20.303min (+0.004) 320246.36ng

response 543649

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.13
183.00	13.30	12.80
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA G\DATA\BG011118\
Data File : BG031982.D
Acq On : 11 Jan 2018 13:53
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 12 06:29:33 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 11 15:23:30 2018
Response via : Initial Calibration

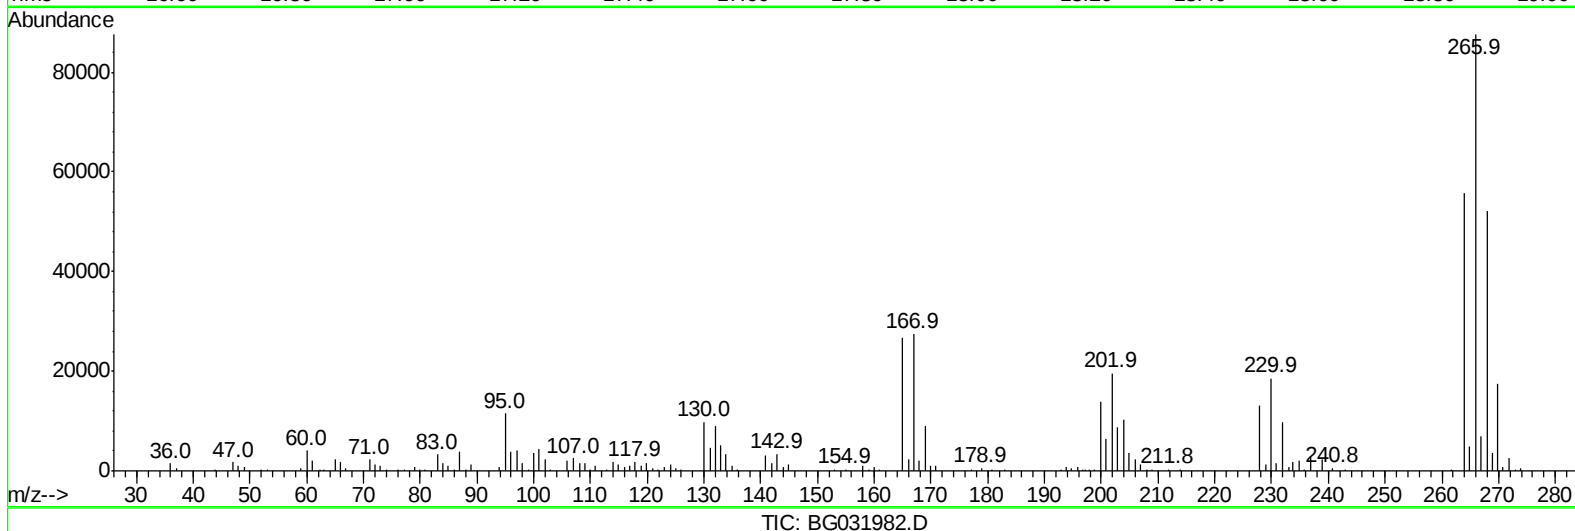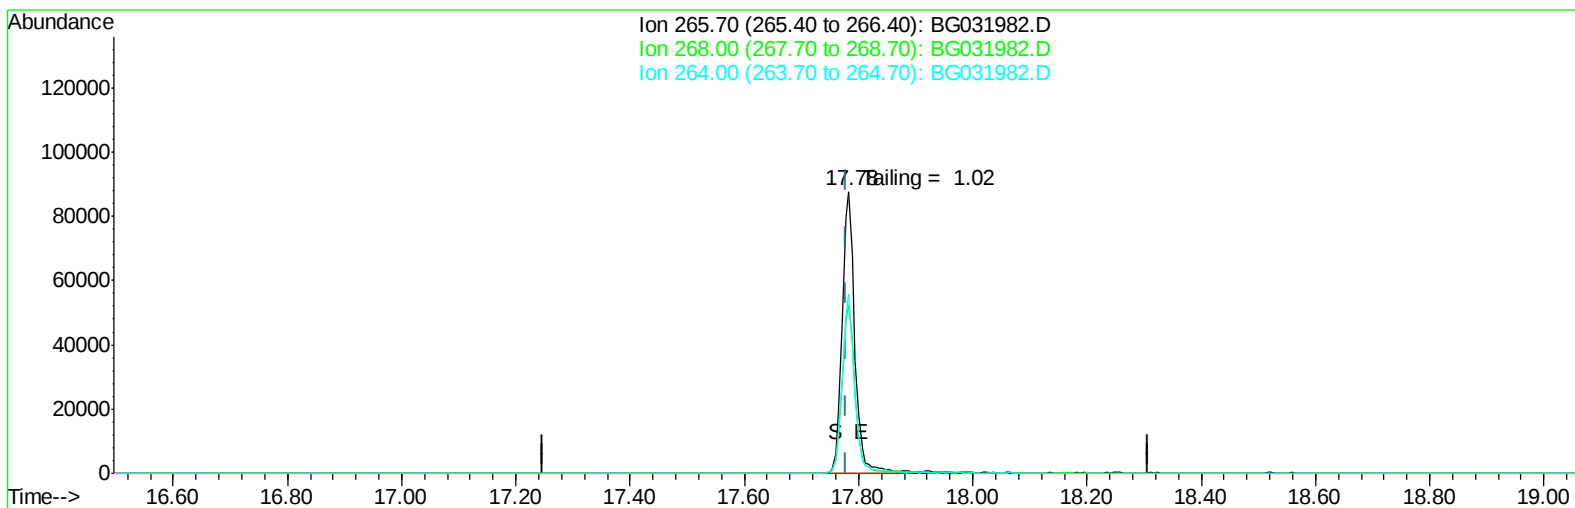

(69) Pentachlorophenol (C)

17.783min (+0.004) 216178.83ng

response 136279

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	59.42
264.00	62.00	63.56
0.00	0.00	0.00