


Data Path : U:\HPCHEM1\BNA G\DATA\BG011118\
 Data File : BG031982.D
 Acq On : 11 Jan 2018 13:53
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 11 15:23:30 2018

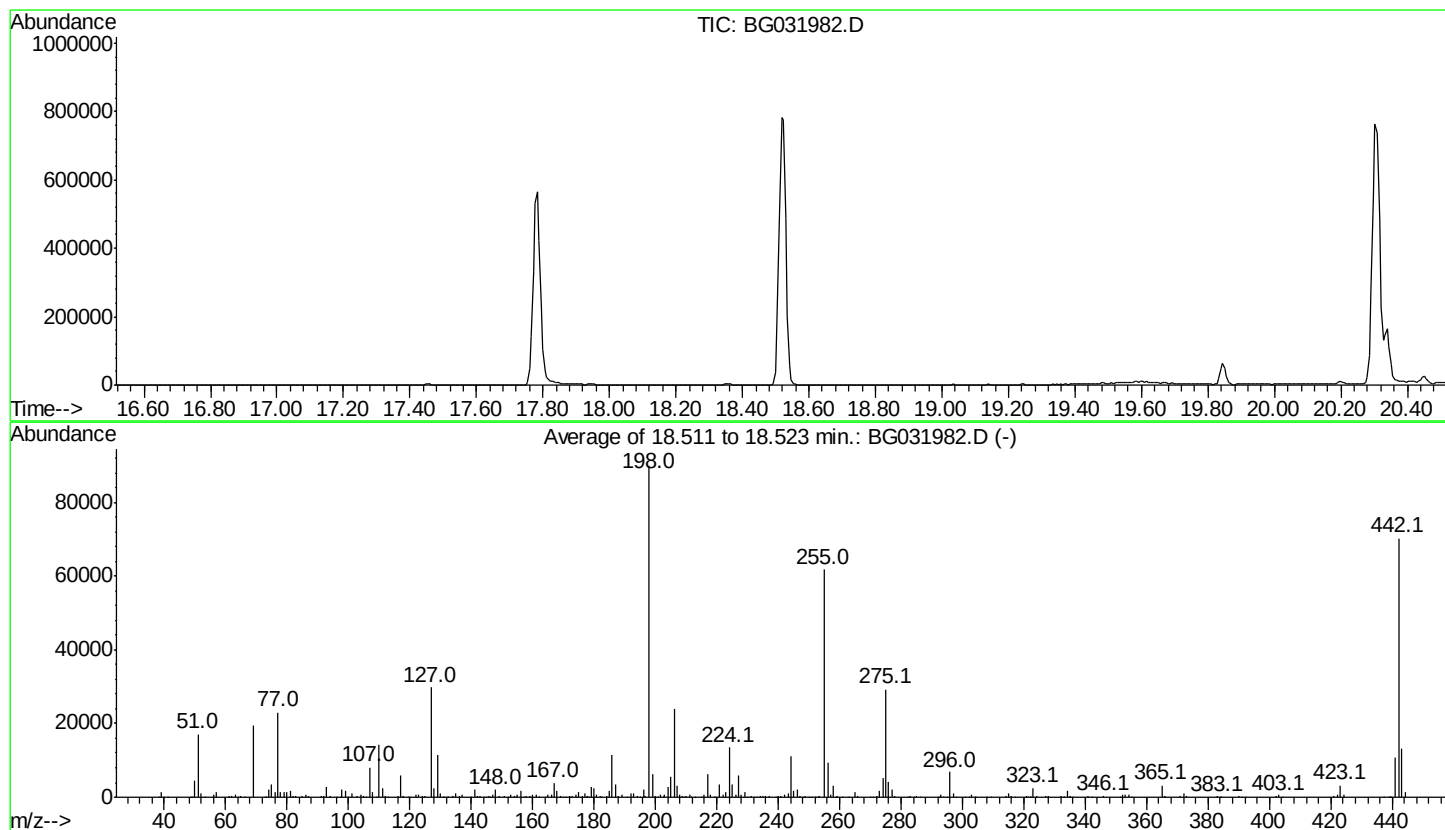

AutoFind: Scans 2591, 2592, 2593; Background Corrected with Scan 2585

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.0	17084	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	21.5	19367	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	33.1	29738	PASS
197	198	0.00	2	0.3	252	PASS
198	198	100	100	100.0	89941	PASS
199	198	5	9	7.1	6354	PASS
275	198	10	60	32.5	29250	PASS
365	198	1	100	3.5	3191	PASS
441	442	0.01	24	15.2	10696	PASS
442	198	50	100	78.1	70264	PASS
443	442	15	24	19.0	13316	PASS