
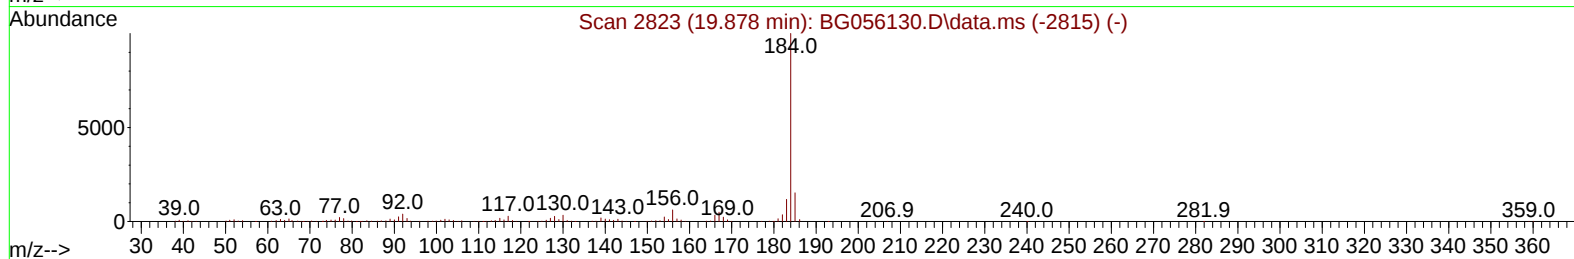
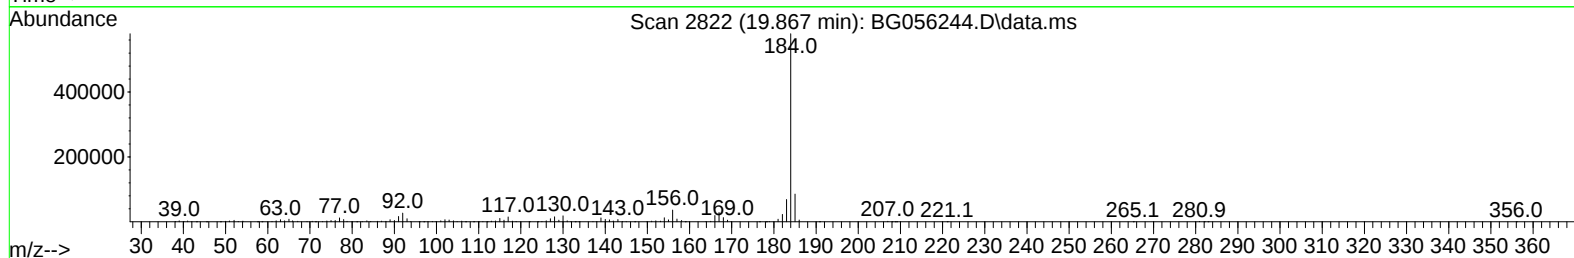


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011123\
Data File : BG056244.D
Acq On : 11 Jan 2023 10:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 12 06:52:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 12 03:38:40 2023
Response via : Initial Calibration

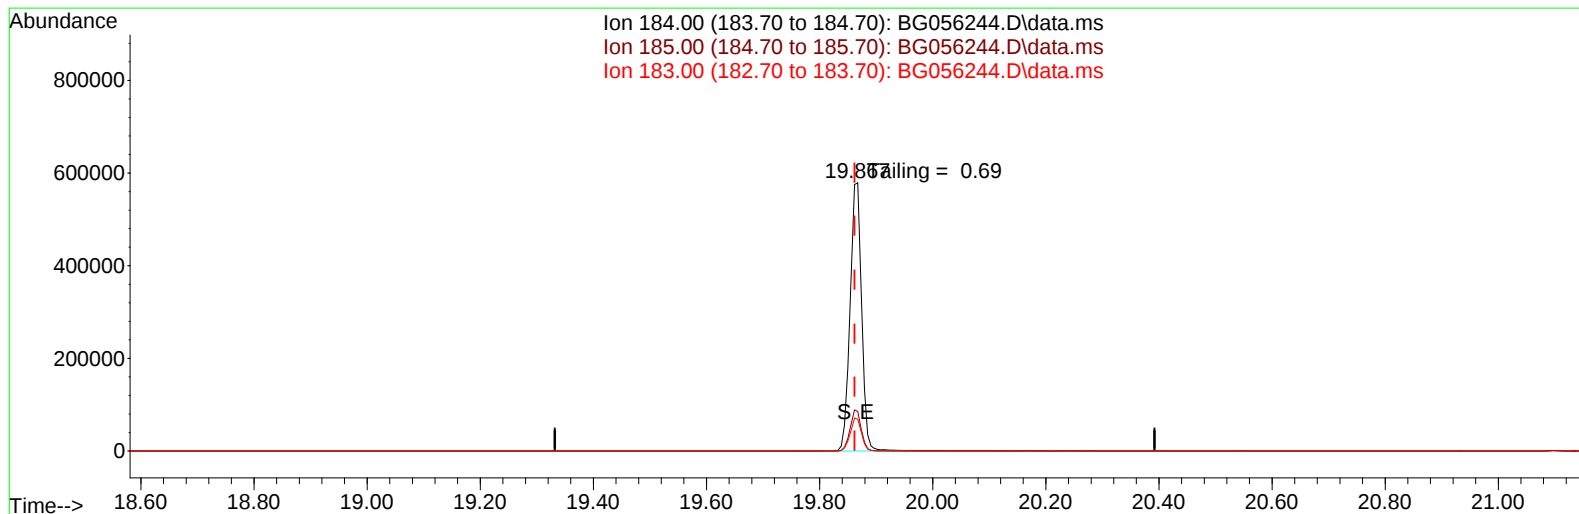




TIC: BG056244.D\data.ms

(77) Benzidine**19.867min (+ 0.005) 0.00 ng****response 825387**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.71
183.00	11.70	11.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011123\
 Data File : BG056244.D
 Acq On : 11 Jan 2023 10:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 12 06:52:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 12 03:38:40 2023
 Response via : Initial Calibration

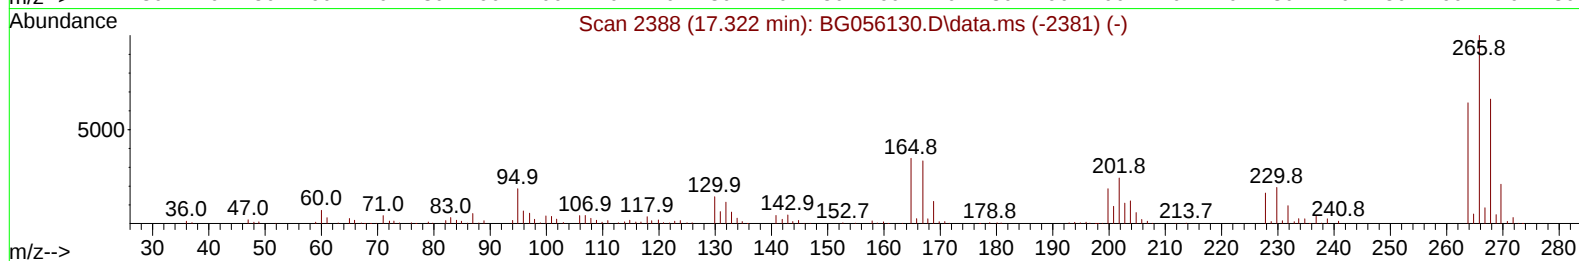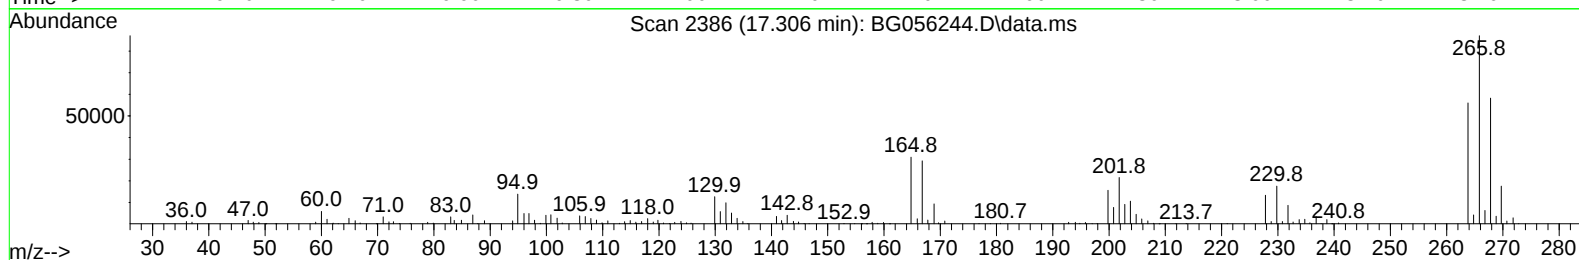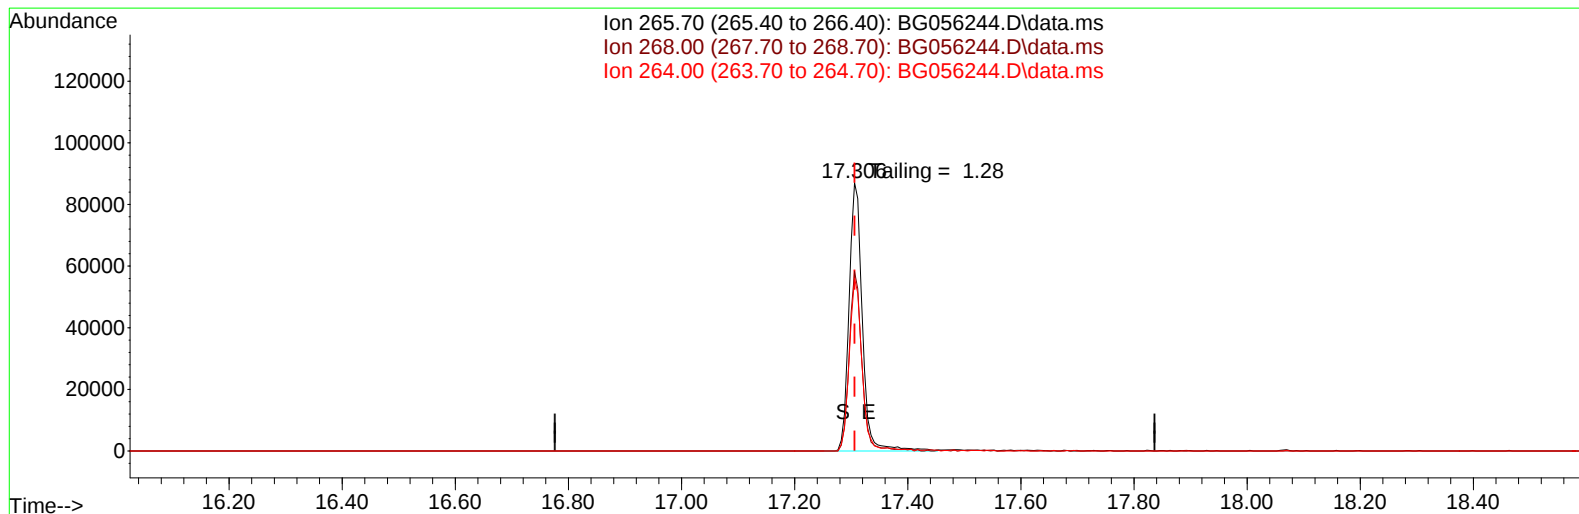

TIC: BG056244.D\data.ms

(70) Pentachlorophenol (C)

17.306min (-0.000) 24942.78 ng

response 142499

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	66.84
264.00	64.30	64.34
0.00	0.00	0.00