
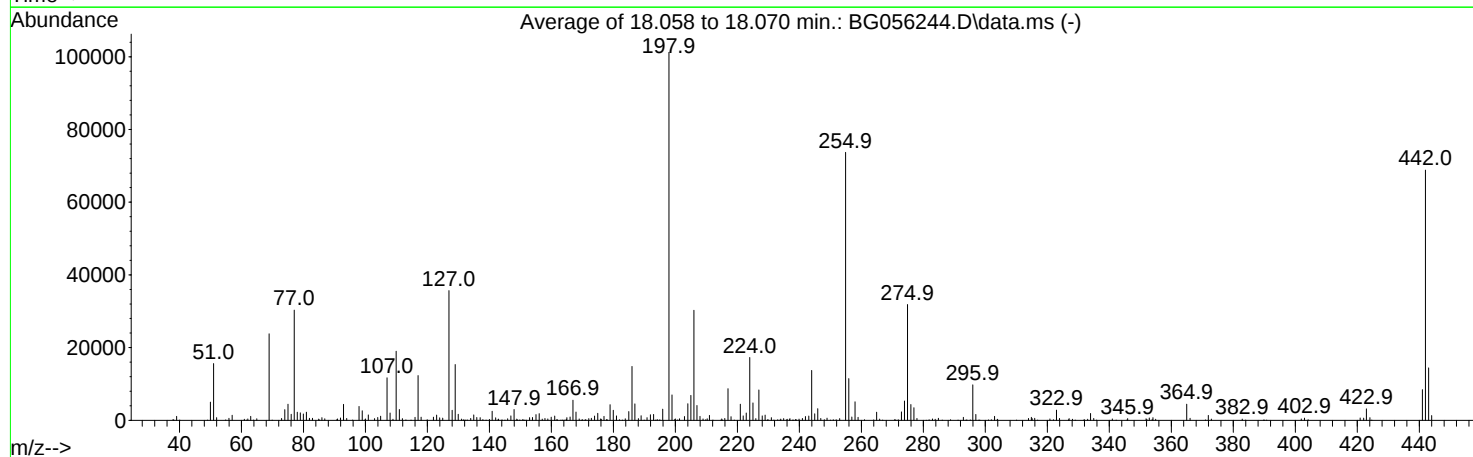


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011123\
 Data File : BG056244.D
 Acq On : 11 Jan 2023 10:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 12 03:38:40 2023

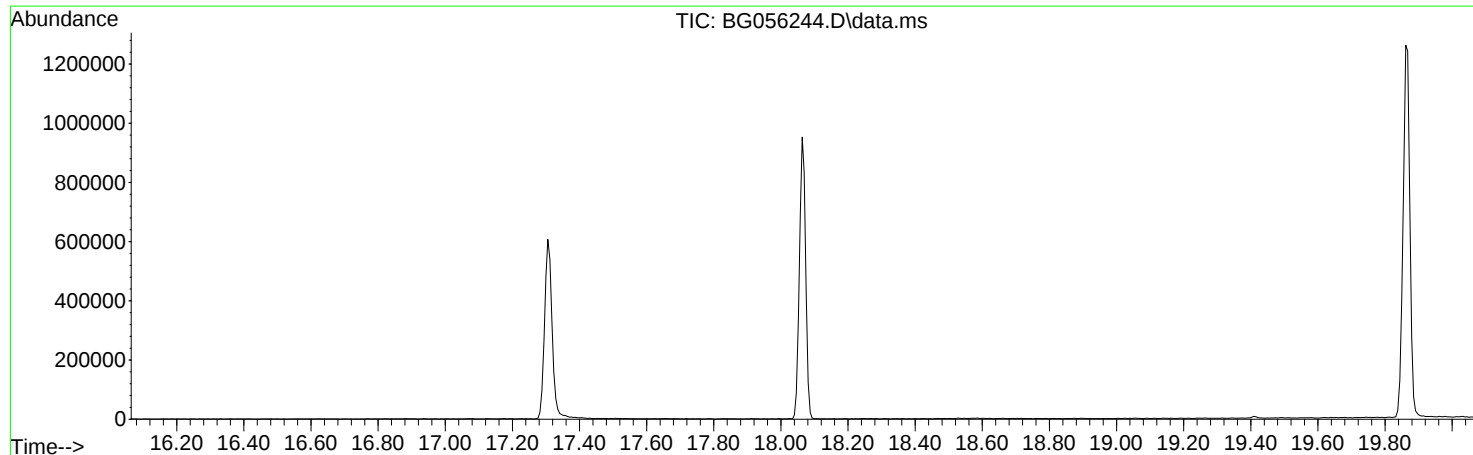




AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	15.4	15600	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	23.5	23779	PASS
70	69	0.00	2	0.2	57	PASS
127	198	10	80	35.3	35680	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	101195	PASS
199	198	5	9	6.9	6956	PASS
275	198	10	60	31.5	31845	PASS
365	198	1	100	4.4	4405	PASS
441	198	0.01	100	8.3	8419	PASS
442	442	50	100	100.0	68813	PASS
443	442	15	24	20.9	14401	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011123\
Data File : BG056244.D
Acq On : 11 Jan 2023 10:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 12 06:52:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 12 03:38:40 2023
Response via : Initial Calibration

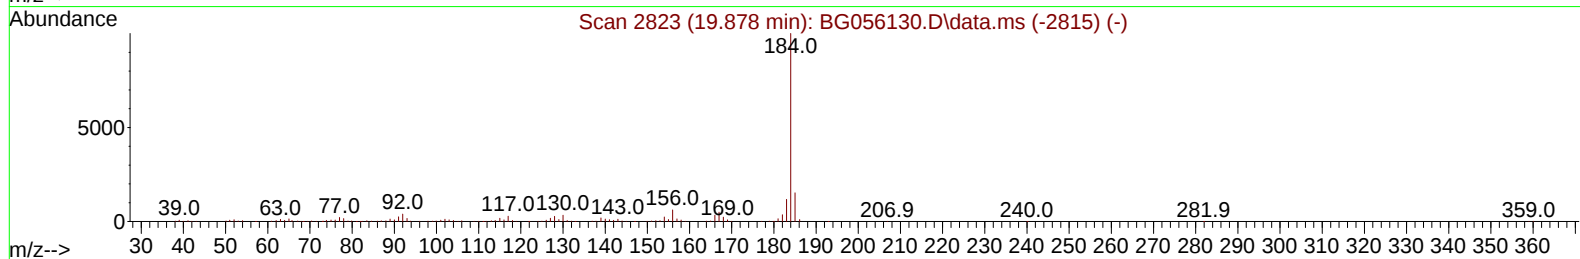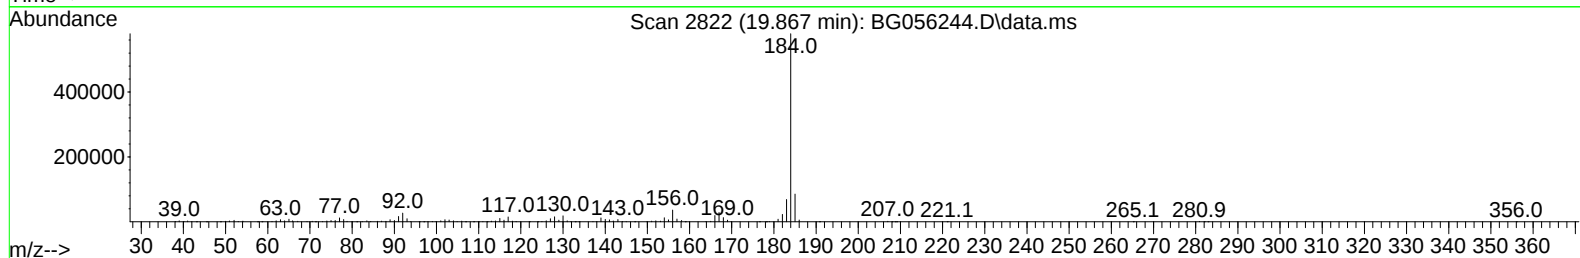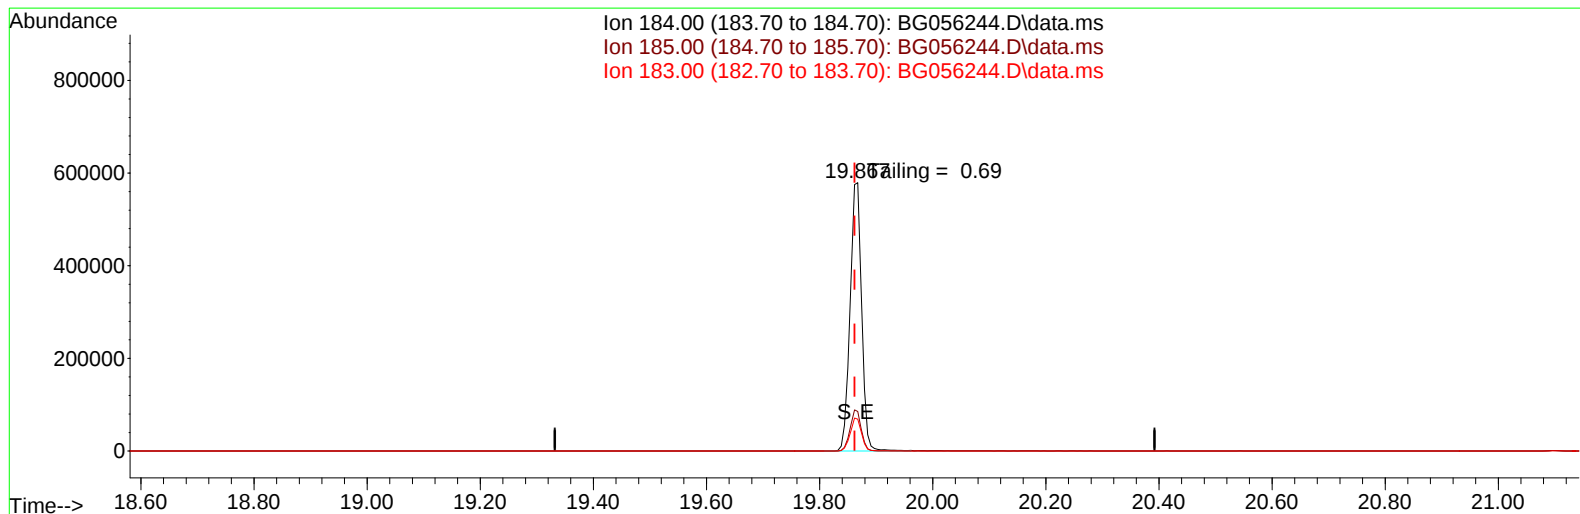

TIC: BG056244.D\data.ms

(77) Benzidine

19.867min (+ 0.005) 0.00 ng




response 825387

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.71
183.00	11.70	11.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011123\
 Data File : BG056244.D
 Acq On : 11 Jan 2023 10:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jan 12 06:52:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 12 03:38:40 2023
 Response via : Initial Calibration

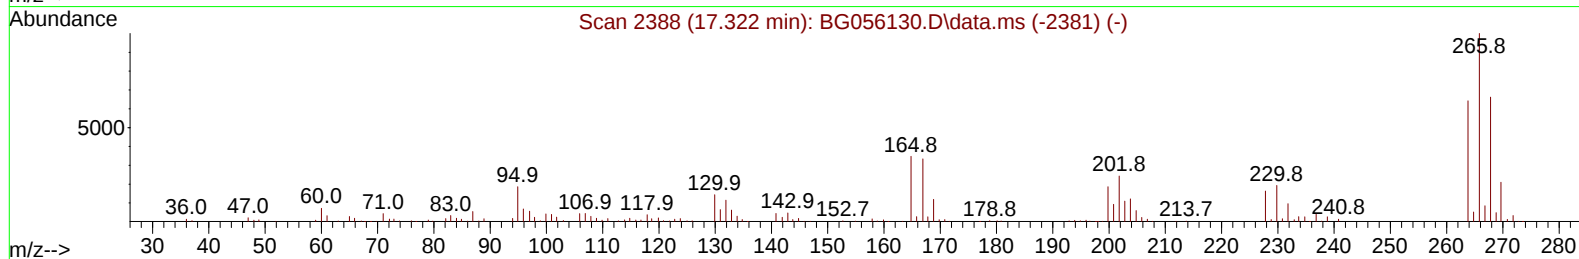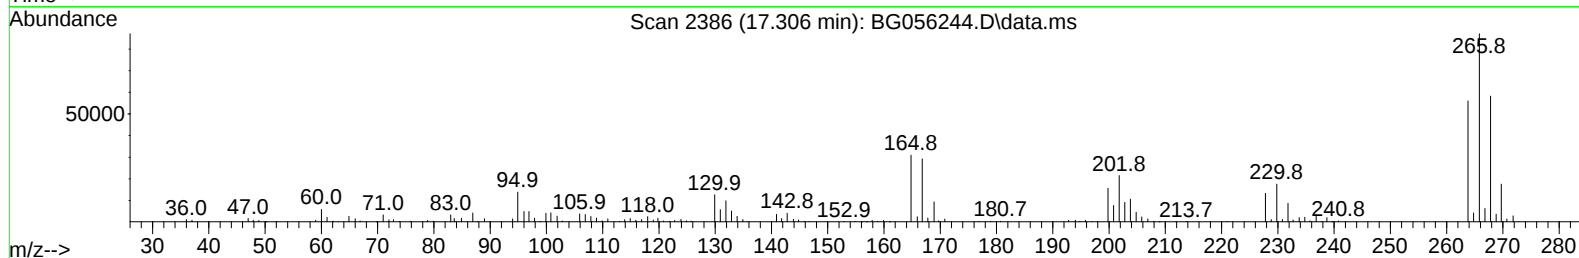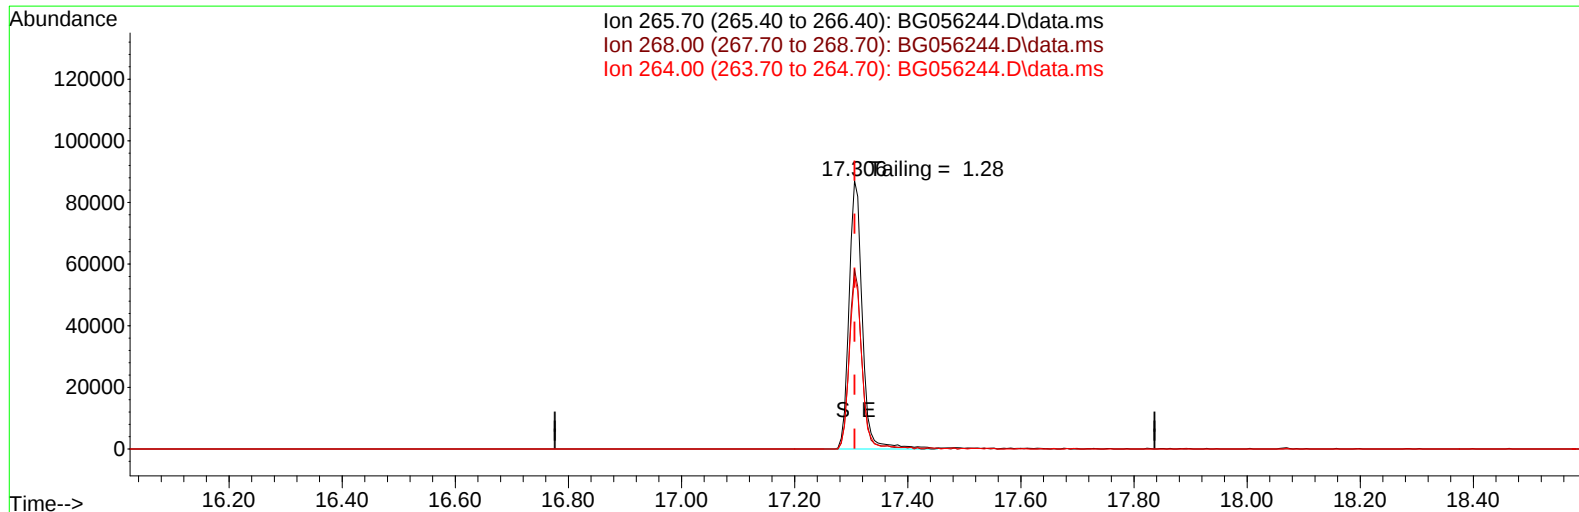

TIC: BG056244.D\data.ms

(70) Pentachlorophenol (C)

17.306min (-0.000) 24942.78 ng

response 142499

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	66.84
264.00	64.30	64.34
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/11/2023	BNA_G	BG056244.D
Compound Name	Response	Retention Time
DDT	395834	21.101
DDD	10050	20.643
DDE	372	20.144
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10422	406256	2.57

Instrument :
BNA_G
ClientSampleId :
DFTPP