
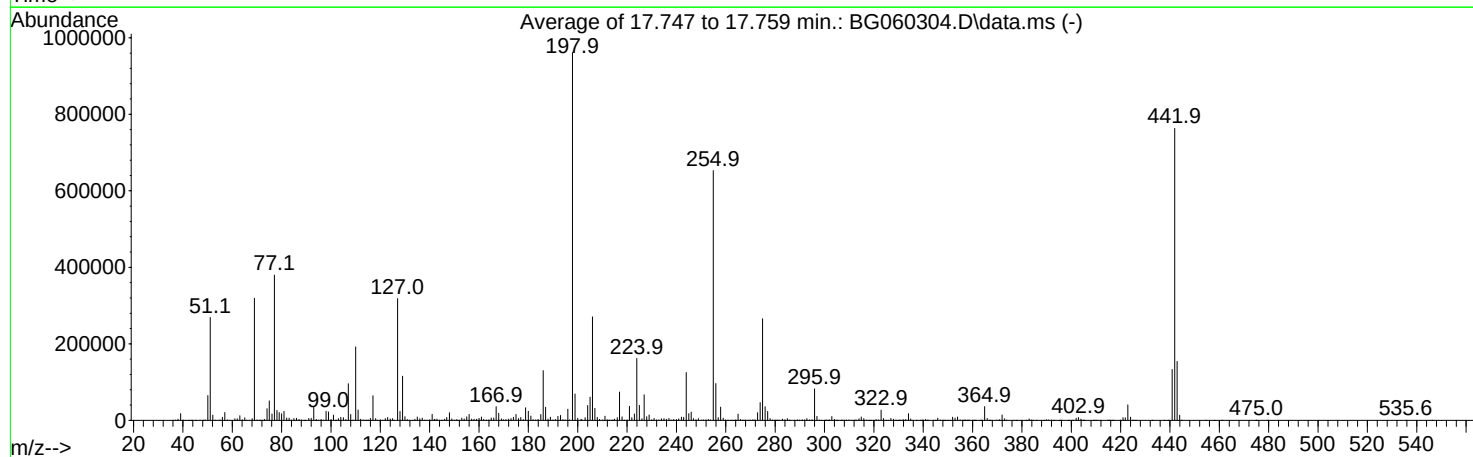


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011124\
Data File : BG060304.D
Acq On : 11 Jan 2024 11:07
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jan 09 04:07:12 2024

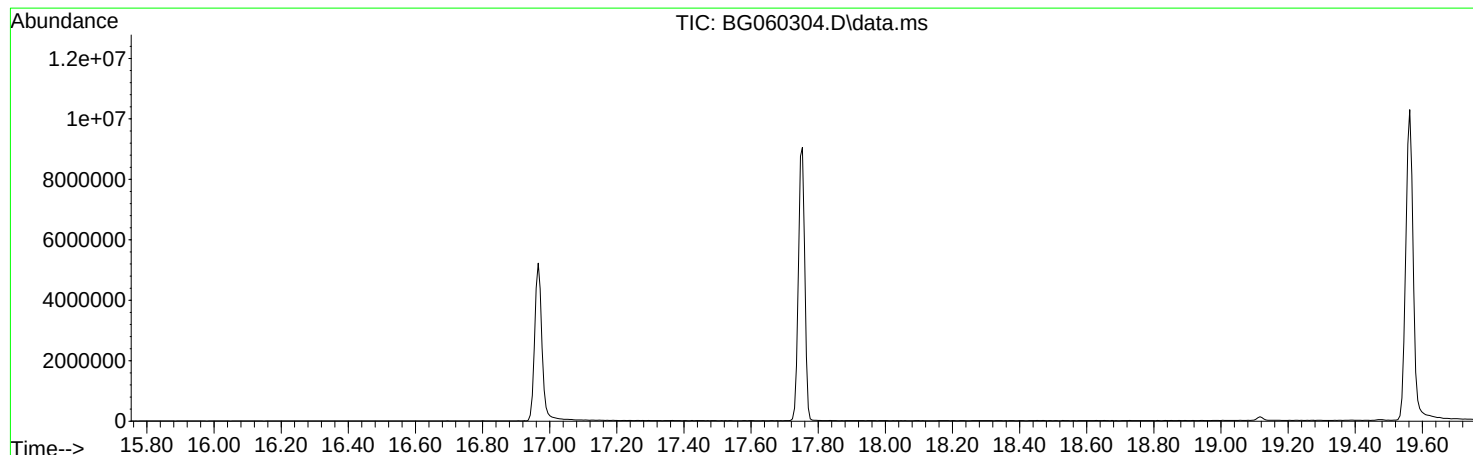




AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2488

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	28.0	268949	PASS
68	69	0.00	2	1.4	4530	PASS
69	198	0.00	100	33.2	319006	PASS
70	69	0.00	2	0.4	1214	PASS
127	198	10	80	33.1	318478	PASS
197	198	0.00	2	0.2	1453	PASS
198	198	100	100	100.0	961493	PASS
199	198	5	9	7.2	69051	PASS
275	198	10	60	27.6	265515	PASS
365	198	1	100	3.7	35861	PASS
441	198	0.01	100	13.8	132995	PASS
442	442	50	100	100.0	763307	PASS
443	442	15	24	20.1	153792	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011124\
Data File : BG060304.D
Acq On : 11 Jan 2024 11:07
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 11 12:08:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

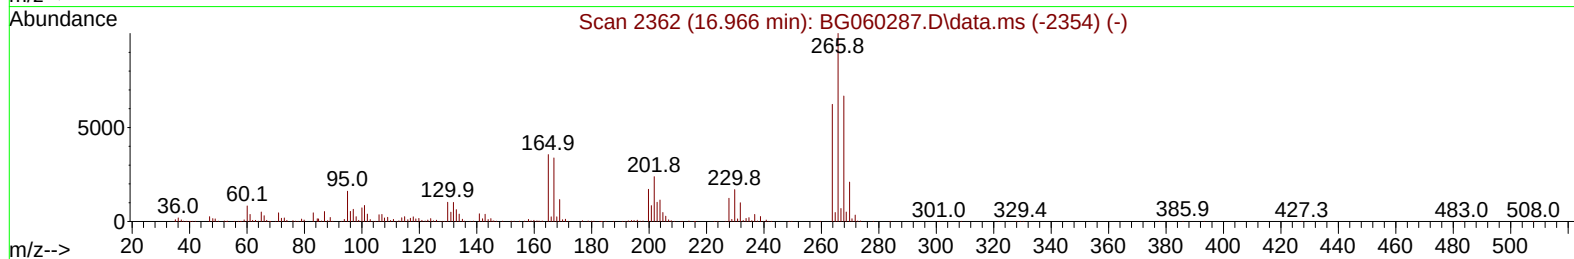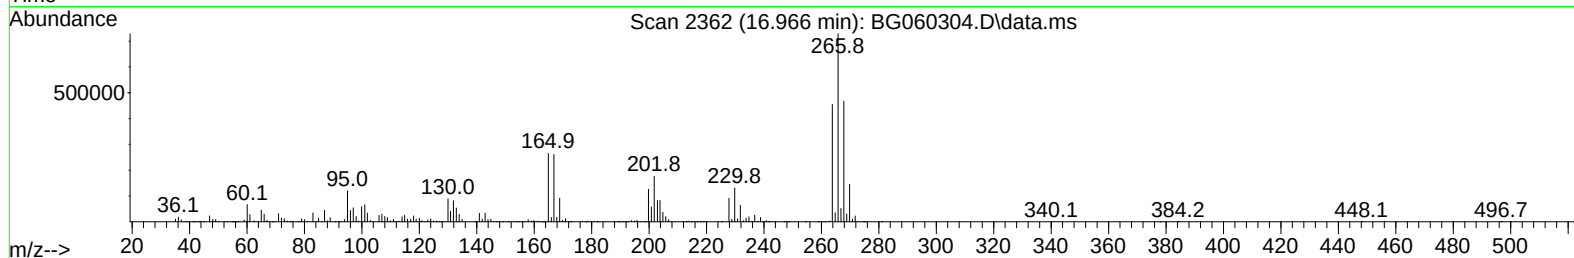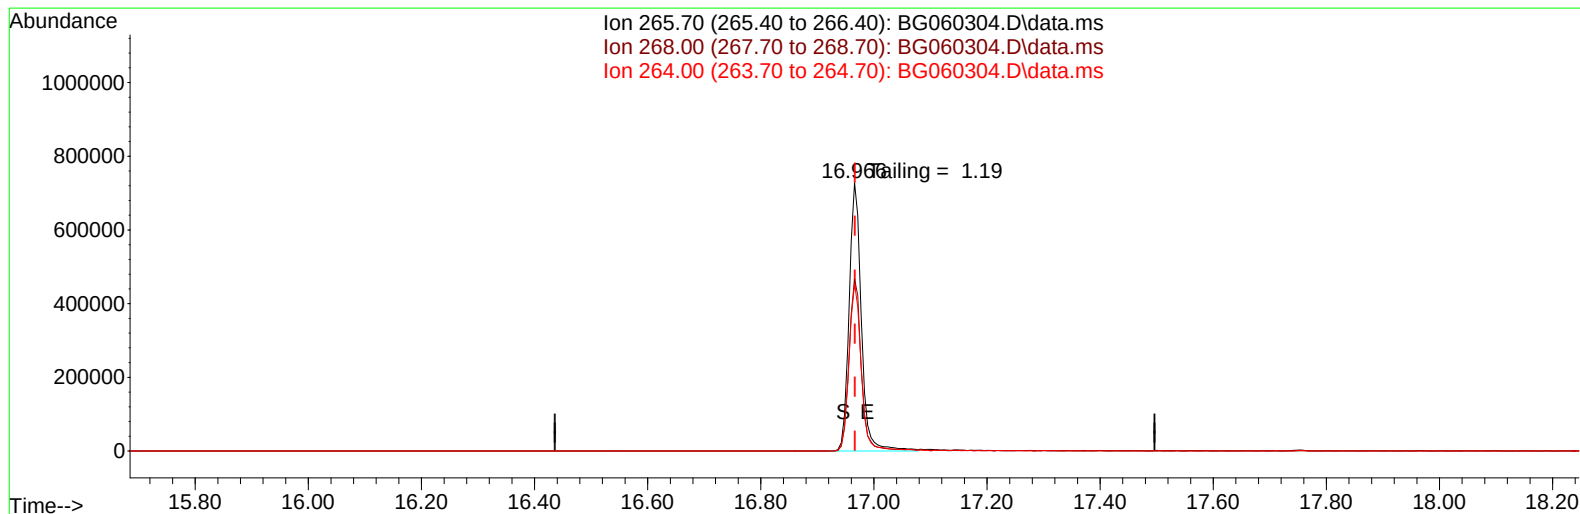

TIC: BG060304.D\data.ms

(70) Pentachlorophenol (C)

16.966min (-0.000) 513607.87 ng




response 1098250

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	71.80	64.09
264.00	62.30	62.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011124\
Data File : BG060304.D
Acq On : 11 Jan 2024 11:07
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 11 12:08:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

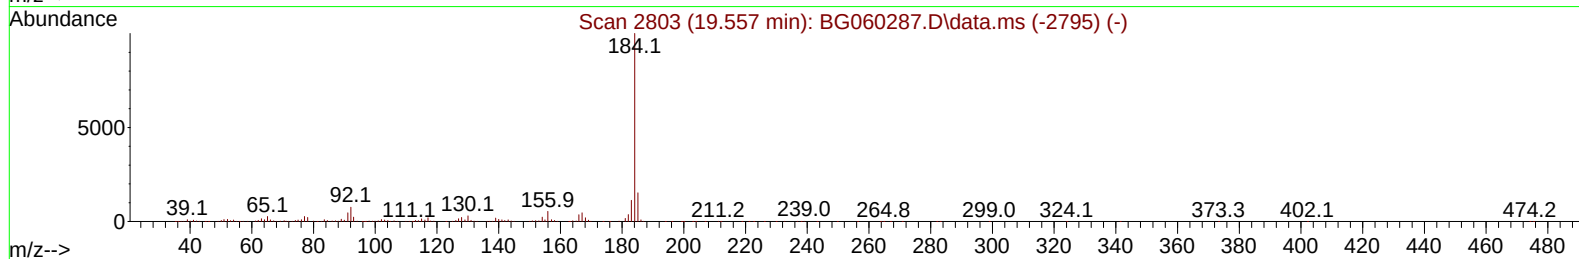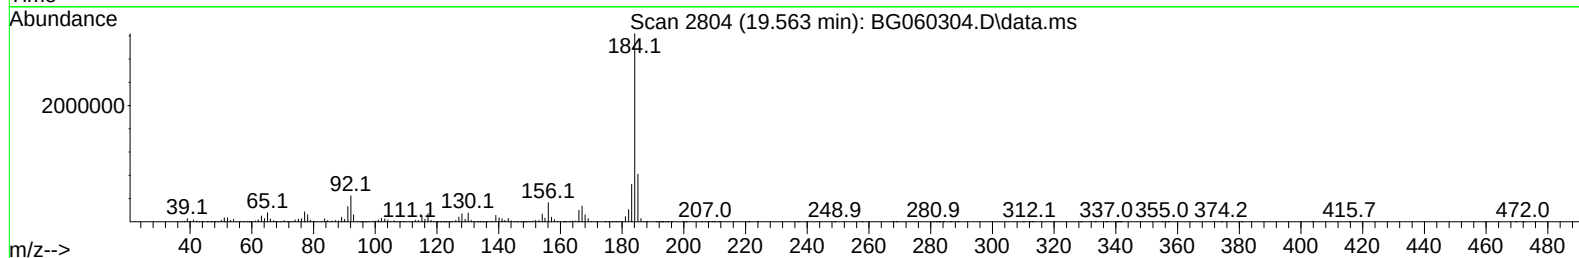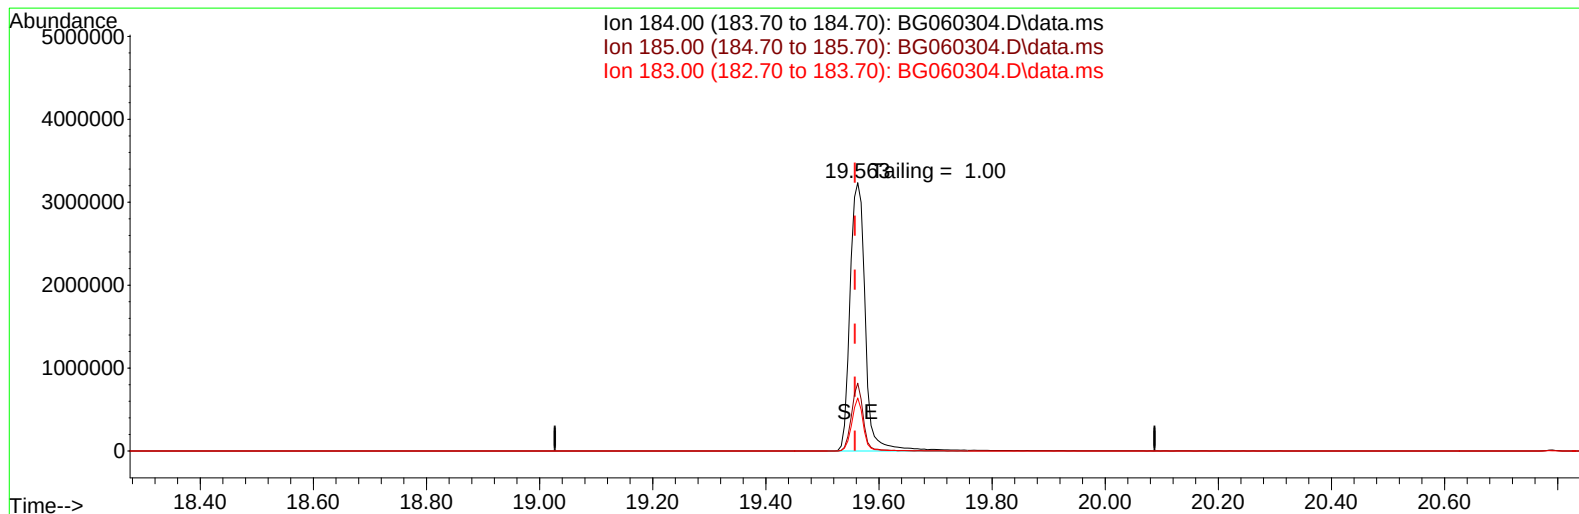

TIC: BG060304.D\data.ms

(77) Benzidine

19.563min (+ 0.005) 3018728.98 ng

response 6099173

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	25.30#
183.00	11.20	19.81#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/11/2024	BNA_G	<u>BG060304.D</u>
Compound Name	Response	Retention Time
DDT	3288610	20.791
DDD	62009	20.397
DDE	1304	19.845
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
63313	3351923	1.89

Instrument :
BNA_G
ClientSampleId :
DFTPP