

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG011216\
 Data File : BG020680.D
 Acq On : 12 Jan 2016 16:31
 Operator : SJ/IZ
 Sample : H1094-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BC952

Quant Time: Jan 13 02:44:55 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG011216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 13 02:39:33 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.04	152	15400	20.00	ng/ul	0.00
18) Naphthalene-d8	10.86	136	65927	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.68	164	47598	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.43	188	127604	20.00	ng/ul	0.00
78) Chrysene-d12	21.70	240	157676	20.00	ng/ul	0.00
86) Perylene-d12	24.96	264	150127	20.00	ng/ul	0.00

System Monitoring Compounds


3) 1,4-Dioxane-d8	3.41	96	1085	3.44	ng/uL	0.00
5) Phenol-d5	7.21	99	23615	17.90	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.36	67	16951	21.36	ng/ul	0.00
9) 2-Chlorophenol-d4	7.57	132	20681	19.98	ng/ul	0.00
13) 4-Methylphenol-d8	8.75	113	19451	17.47	ng/ul	0.00
19) Nitrobenzene-d5	9.22	128	10924	21.00	ng/ul	0.00
22) 2-Nitrophenol-d4	9.94	143	12463	20.62	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.49	165	22211	19.30	ng/ul	0.00
29) 4-Chloroaniline-d4	11.01	131	24695	21.68	ng/ul	0.00
44) Dimethylphthalate-d6	14.08	166	91915	22.13	ng/ul	0.00
47) Acenaphthylene-d8	14.38	160	100332	21.51	ng/ul	0.00
52) 4-Nitrophenol-d4	14.89	143	7947	14.25	ng/ul	0.00
58) Fluorene-d10	15.68	176	81131	21.91	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.80	200	11927	17.19	ng/ul	0.00
71) Anthracene-d10	17.53	188	139094	22.24	ng/ul	0.00
79) Pyrene-d10	19.81	212	180250	24.03	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.73	264	188419	23.55	ng/ul	0.00

Target Compounds

						Qvalue
45) Dimethylphthalate	14.13	163	36323	8.14	ng/ul	99
70) Phenanthrene	17.47	178	13133	1.73	ng/ul	97
72) Anthracene	17.47	178	13133	1.71	ng/ul	97
77) Fluoranthene	19.48	202	27344	2.96	ng/ul#	96
80) Pyrene	19.84	202	31218	3.12	ng/ul	98
83) Benzo(a)anthracene	21.68	228	15222	1.55	ng/ul	95
85) Chrysene	21.75	228	14605	1.57	ng/ul	99
88) Benzo(b)fluoranthene	23.93	252	17294	1.79	ng/ul#	98
89) Benzo(k)fluoranthene	23.93	252	17294	1.81	ng/ul	99
91) Benzo(a)pyrene	24.79	252	14199	1.53	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed





```
Data Path : Z:\HPCHEM1\BNA_G\DATA\BG011216\  
Data File : BG020680.D  
Acq On    : 12 Jan 2016   16:31  
Operator  : SJ/IZ  
Sample    : H1094-01  
Misc      :  
ALS Vial  : 9      Sample Multiplier: 1
```

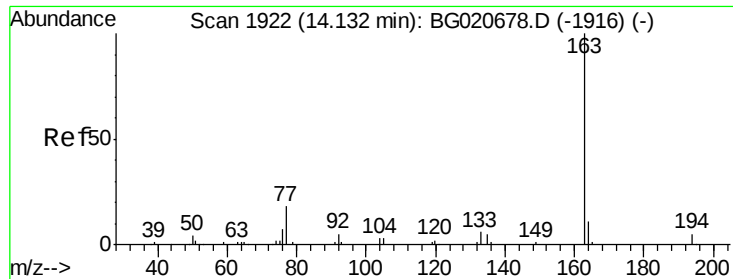

#45
Dimethylphthalate
Concen: 8.14 ng/ul
RT: 14.13 min Scan# 1922
Delta R.T. -0.00 min
Lab File: BG020680.D
Acq: 12 Jan 2016 16:31




Instrument :
BNA_G
ClientSampleId :
BC952


Tgt Ion:163 Resp: 36323
Ion Ratio Lower Upper
163 100
194 4.7 4.0 6.0
164 10.1 8.4 12.6

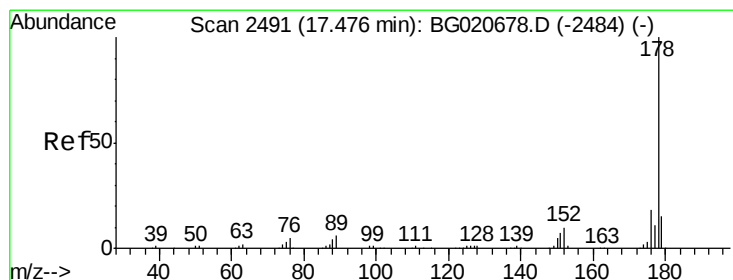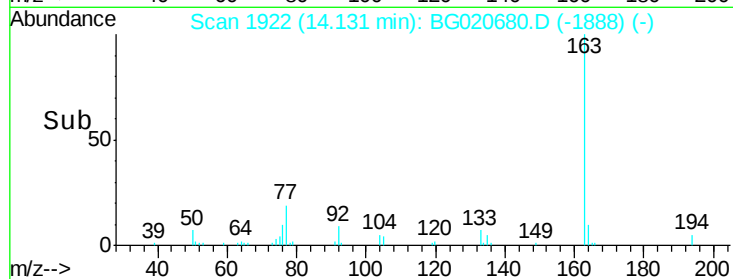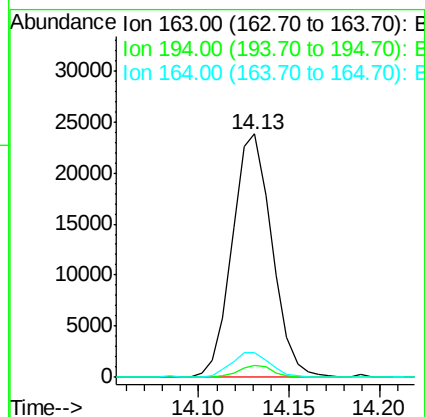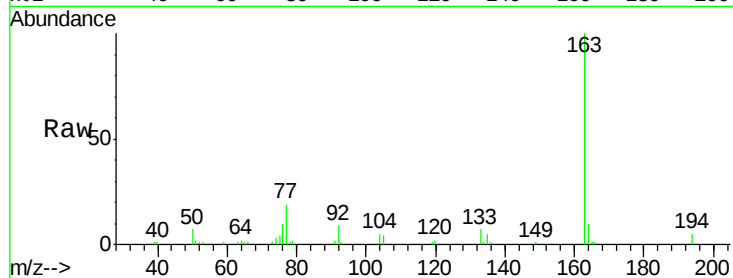

#70
Phenanthrene
Concen: 1.73 ng/ul
RT: 17.47 min Scan# 2491
Delta R.T. -0.00 min
Lab File: BG020680.D
Acq: 12 Jan 2016 16:31

Tgt Ion:178 Resp: 13133
Ion Ratio Lower Upper
178 100
179 16.2 12.3 18.5
176 21.2 15.4 23.0

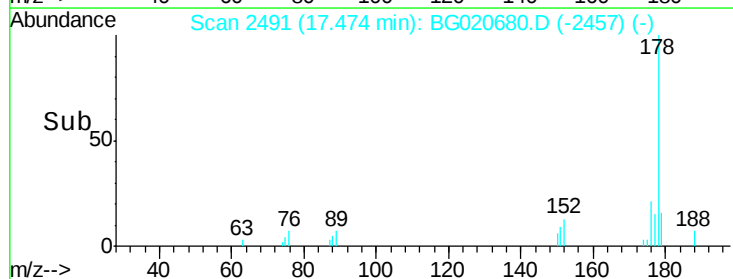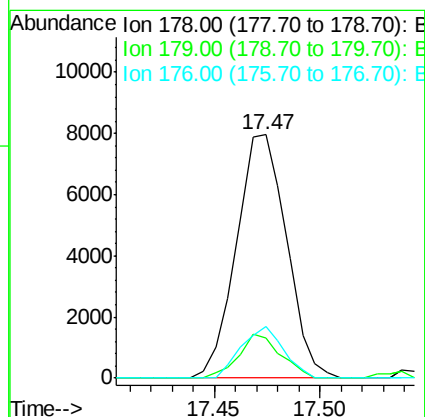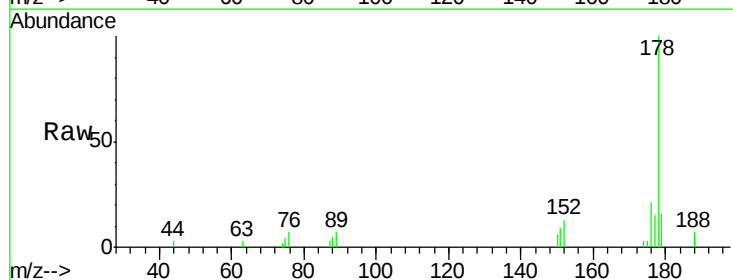

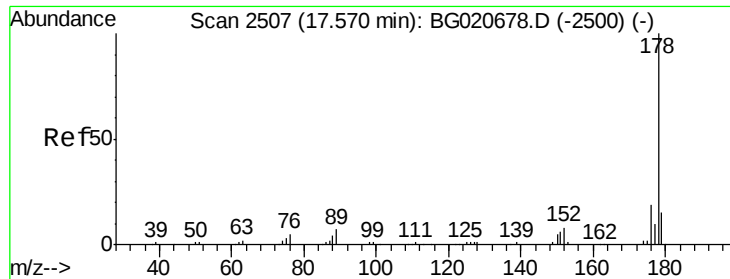

#72

Anthracene

Concen: 1.71 ng/ul

RT: 17.47 min Scan# 2491

Delta R.T. -0.10 min

Lab File: BG020680.D

Acq: 12 Jan 2016 16:31

Instrument :

BNA_G

ClientSampleId :

BC952


Tgt Ion:178 Resp: 13133

Ion Ratio Lower Upper

178 100

179 16.2 13.4 20.2




176 21.2 15.4 23.0

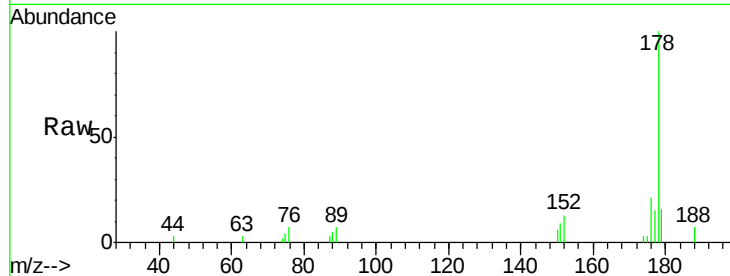

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

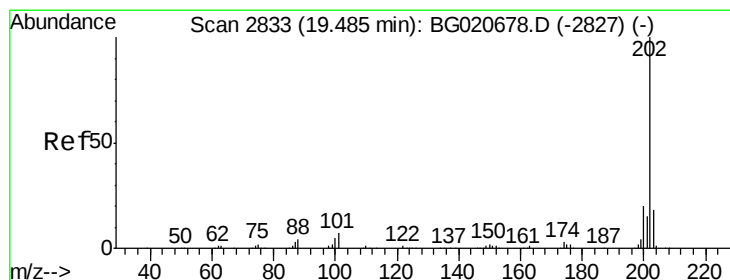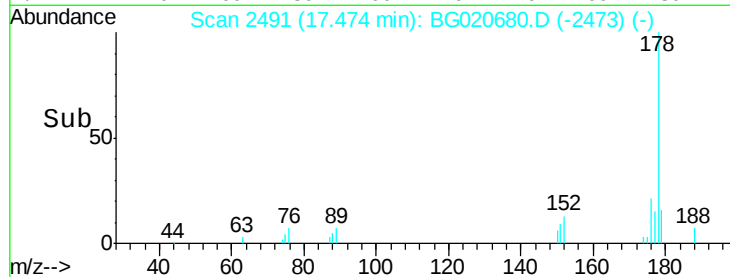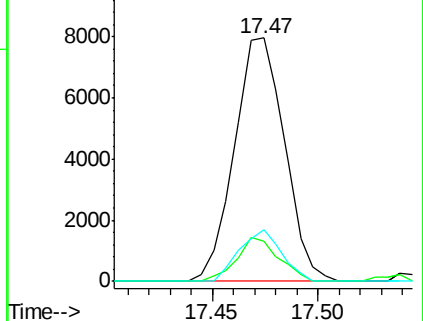

#77

Fluoranthene

Concen: 2.96 ng/ul

RT: 19.48 min Scan# 2833

Delta R.T. -0.00 min

Lab File: BG020680.D

Acq: 12 Jan 2016 16:31


Tgt Ion:202 Resp: 27344

Ion Ratio Lower Upper

202 100

101 5.1 6.1 9.1#



100 5.6 4.6 7.0

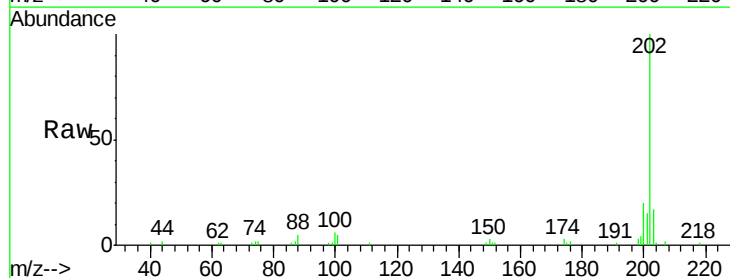


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B



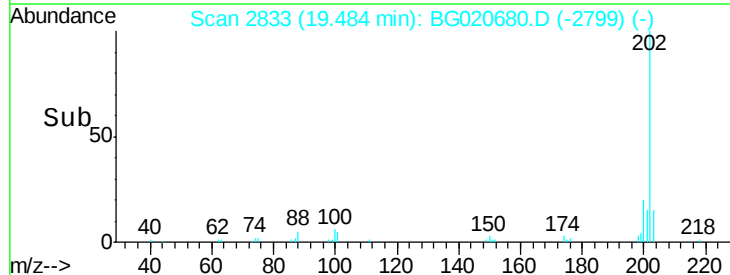
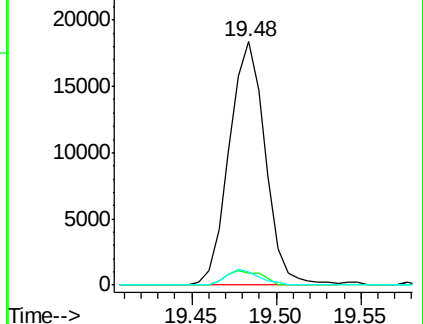


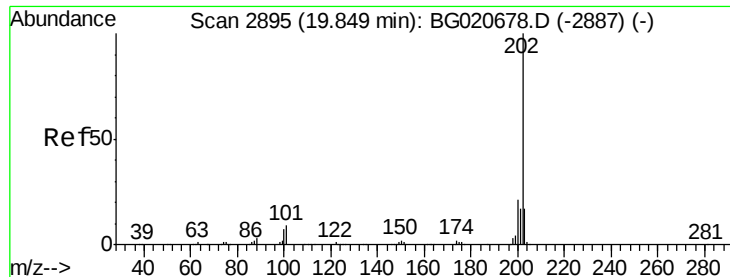

#80
 Pyrene
 Concen: 3.12 ng/ul
 RT: 19.84 min Scan# 2894
 Delta R.T. -0.01 min
 Lab File: BG020680.D
 Acq: 12 Jan 2016 16:31




Instrument :
 BNA_G
 ClientSampled :
 BC952


Tgt Ion:202 Resp: 31218
 Ion Ratio Lower Upper
 202 100
 101 7.8 6.9 10.3
 100 7.7 5.6 8.4

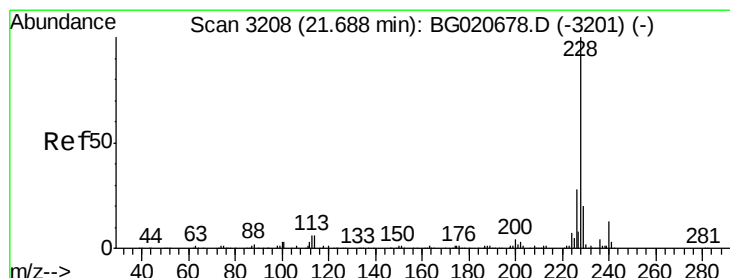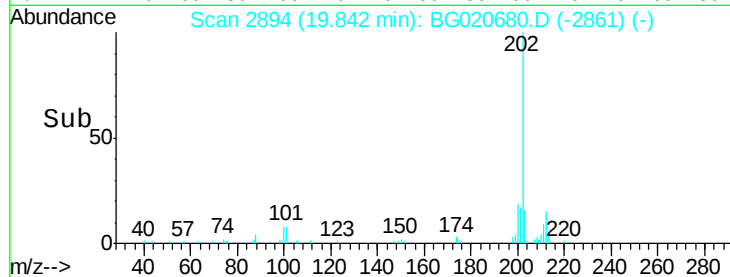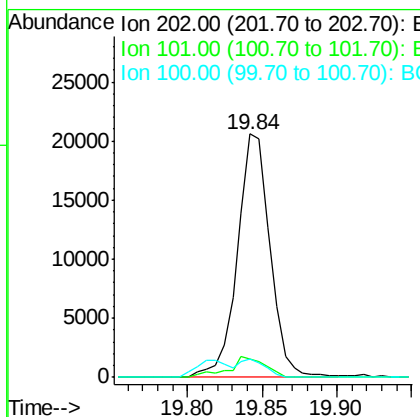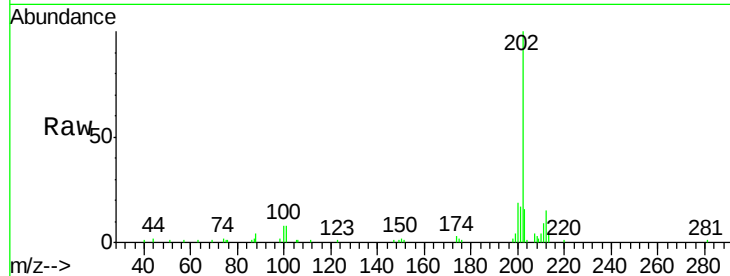

#83
 Benzo(a)anthracene
 Concen: 1.55 ng/ul
 RT: 21.68 min Scan# 3207
 Delta R.T. -0.01 min
 Lab File: BG020680.D
 Acq: 12 Jan 2016 16:31

Tgt Ion:228 Resp: 15222
 Ion Ratio Lower Upper
 228 100
 229 20.2 16.0 24.0
 226 23.2 21.8 32.8

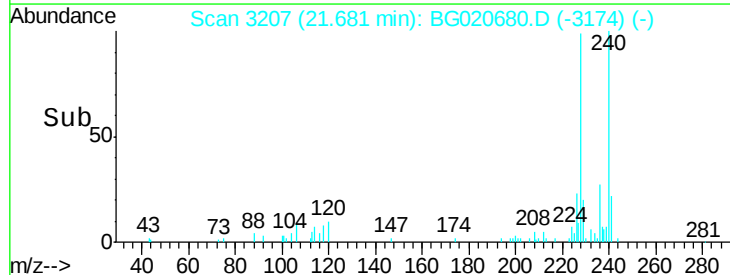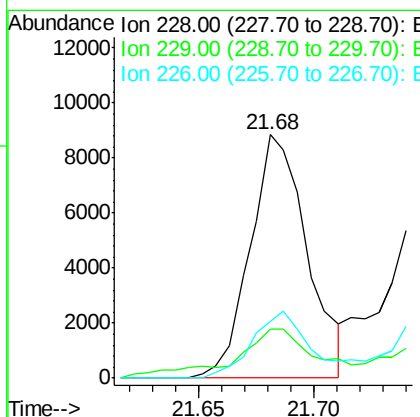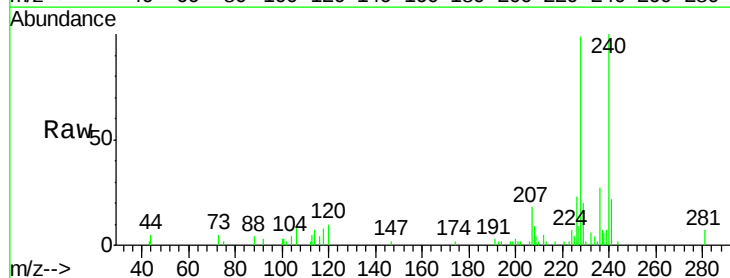

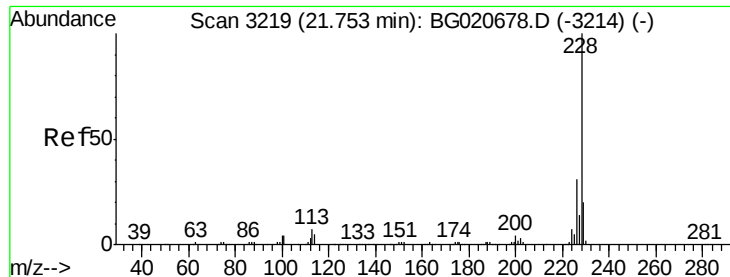

#85

Chrysene

Concen: 1.57 ng/ul

RT: 21.75 min Scan# 3219

Delta R.T. -0.00 min

Lab File: BG020680.D

Acq: 12 Jan 2016 16:31

Instrument :

BNA_G

ClientSampleId :

BC952


Tgt Ion:228 Resp: 14605

Ion Ratio Lower Upper

228 100

226 31.1 24.1 36.1




229 19.8 16.0 24.0

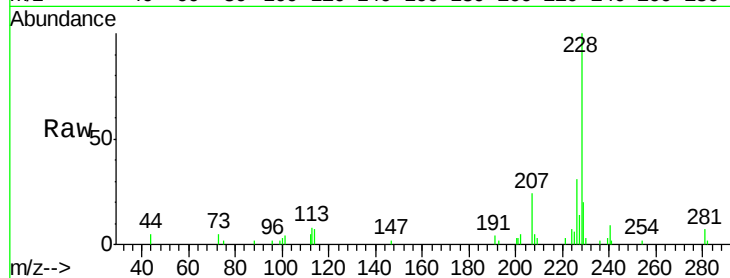

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

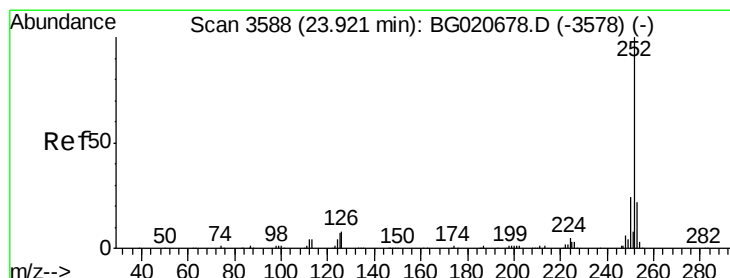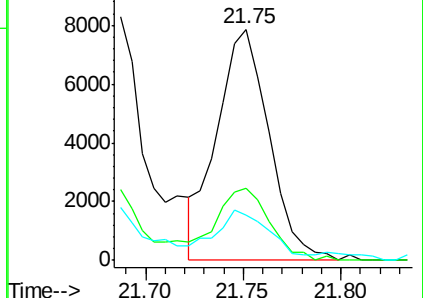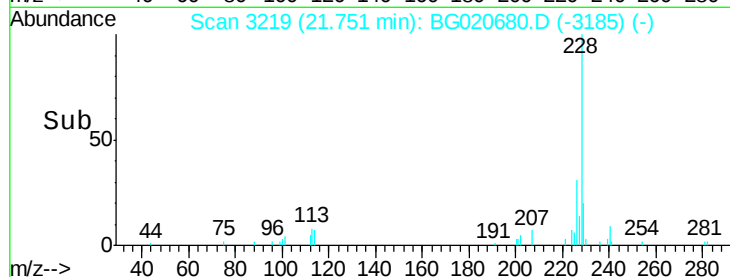

#88

Benzo(b)fluoranthene

Concen: 1.79 ng/ul

RT: 23.93 min Scan# 3590

Delta R.T. 0.01 min

Lab File: BG020680.D

Acq: 12 Jan 2016 16:31


Tgt Ion:252 Resp: 17294

Ion Ratio Lower Upper

252 100

253 21.3 17.4 26.0



125 7.4 4.9 7.3#

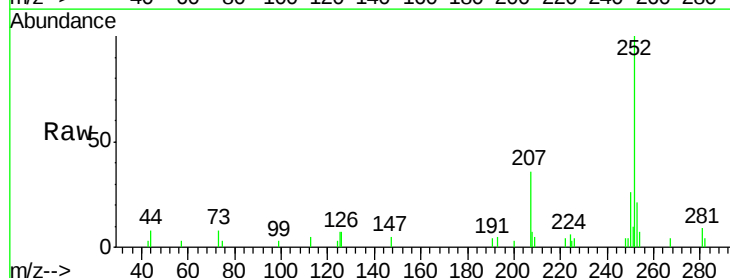


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

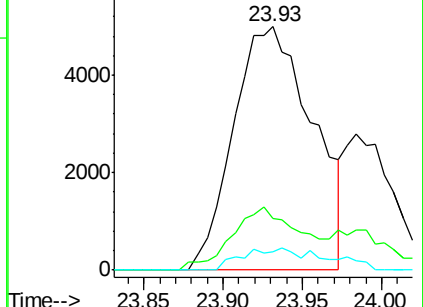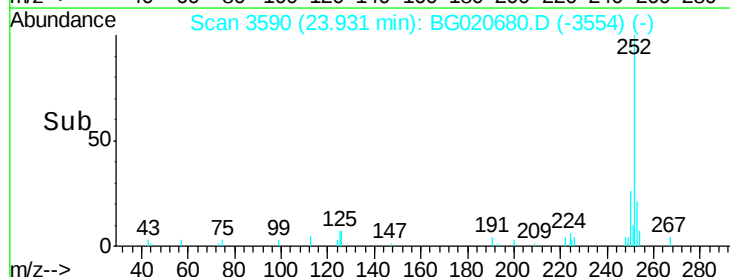

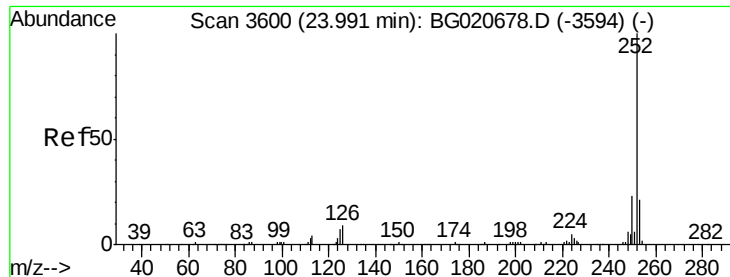

#89

Benzo(k)fluoranthene

Concen: 1.81 ng/ul

RT: 23.93 min Scan# 3590

Delta R.T. -0.06 min

Lab File: BG020680.D

Acq: 12 Jan 2016 16:31

Instrument :

BNA_G

ClientSampleId :

BC952


Tgt Ion:252 Resp: 17294

Ion Ratio Lower Upper

252 100

253 21.3 17.1 25.7




125 7.4 5.4 8.0

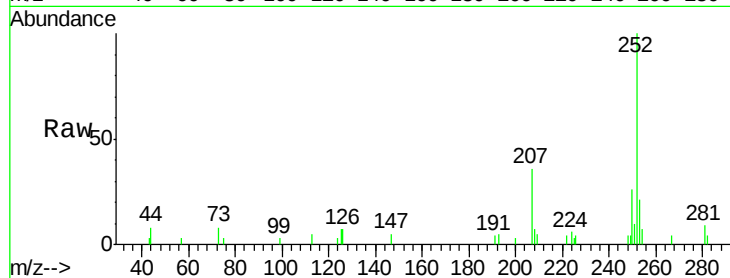

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

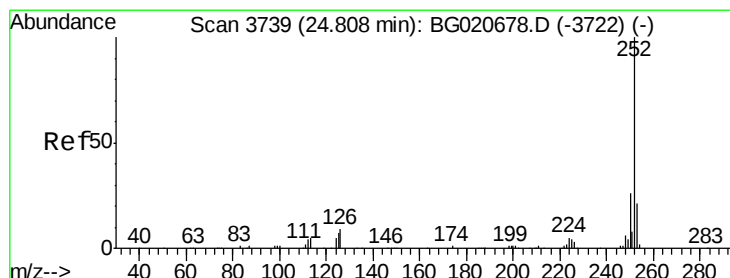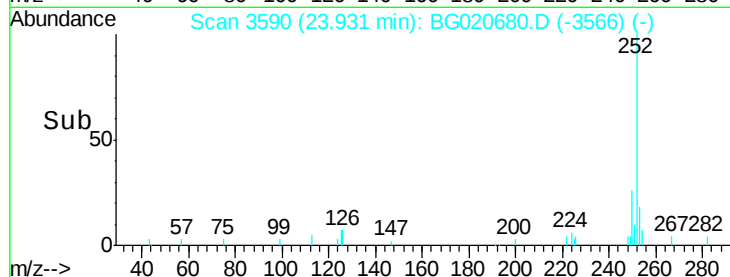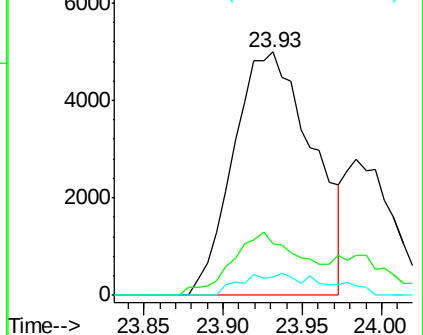

#91

Benzo(a)pyrene

Concen: 1.53 ng/ul

RT: 24.79 min Scan# 3737

Delta R.T. -0.01 min

Lab File: BG020680.D

Acq: 12 Jan 2016 16:31


Tgt Ion:252 Resp: 14199

Ion Ratio Lower Upper

252 100

253 21.2 17.2 25.8

125 6.6 5.8 8.6

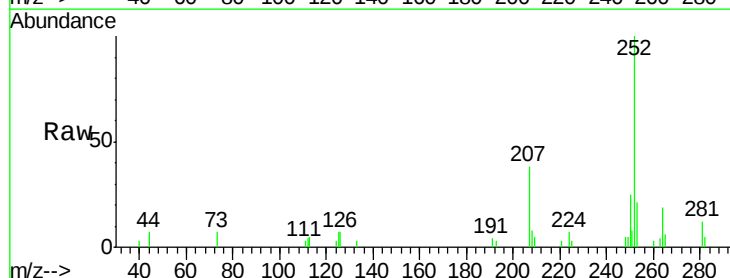

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

