

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG011216\
 Data File : BG020695.D
 Acq On : 13 Jan 2016 6:58
 Operator : SJ/IZ
 Sample : H1094-04
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BC955

Quant Time: Jan 13 07:59:26 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG011216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 13 07:56:00 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.04	152	14210	20.00	ng/ul	0.00
18) Naphthalene-d8	10.86	136	62752	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.68	164	47551	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.43	188	129209	20.00	ng/ul	0.00
78) Chrysene-d12	21.70	240	152923	20.00	ng/ul	0.00
86) Perylene-d12	24.95	264	141871	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.41	96	1878	6.46	ng/uL	0.00
5) Phenol-d5	7.20	99	46512	38.20	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.37	67	29364	40.09	ng/ul	0.00
9) 2-Chlorophenol-d4	7.57	132	37553	39.32	ng/ul	0.00
13) 4-Methylphenol-d8	8.75	113	38785	37.76	ng/ul	0.00
19) Nitrobenzene-d5	9.22	128	20049	40.50	ng/ul	0.00
22) 2-Nitrophenol-d4	9.94	143	23331	40.56	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.48	165	41585	37.97	ng/ul	0.00
29) 4-Chloroaniline-d4	11.00	131	54402	50.19	ng/ul	0.00
44) Dimethylphthalate-d6	14.08	166	163191	39.33	ng/ul	0.00
47) Acenaphthylene-d8	14.37	160	183962	39.48	ng/ul	0.00
52) 4-Nitrophenol-d4	14.89	143	19569	35.12	ng/ul	0.00
58) Fluorene-d10	15.67	176	146736	39.67	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.80	200	24698	35.15	ng/ul	0.00
71) Anthracene-d10	17.53	188	254082	40.12	ng/ul	0.00
79) Pyrene-d10	19.82	212	308134	42.35	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.73	264	318527	42.12	ng/ul	0.00


Target Compounds						Qvalue
15) N-Nitroso-di-n-propylamine	8.76	70	1025	1.19	ng/ul#	1
45) Dimethylphthalate	14.13	163	66697	14.96	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG011216\
Data File : BG020695.D
Acq On : 13 Jan 2016 6:58
Operator : SJ/IZ
Sample : H1094-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BC955

Quant Time: Jan 13 07:59:26 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG011216.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 13 07:56:00 2016
Response via : Initial Calibration




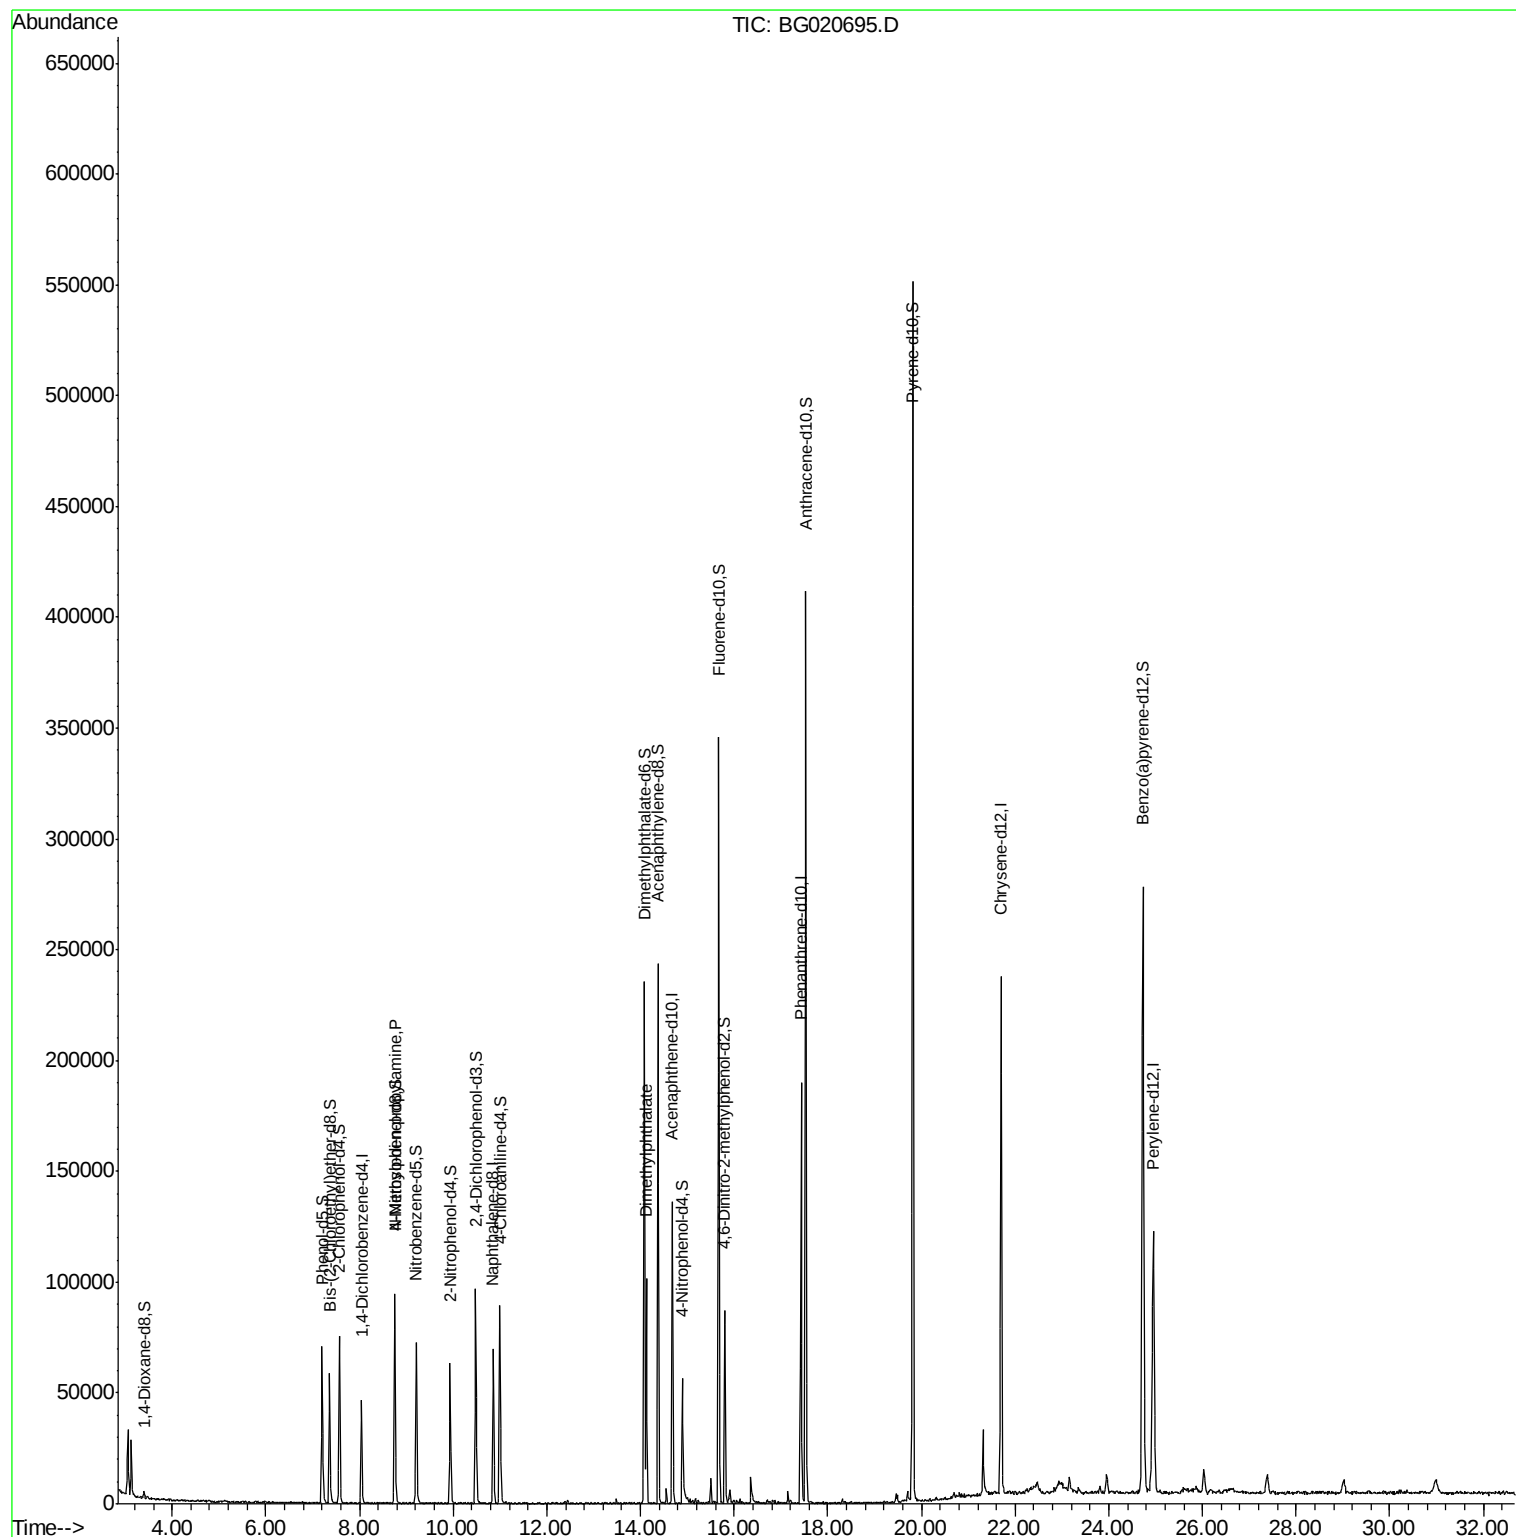


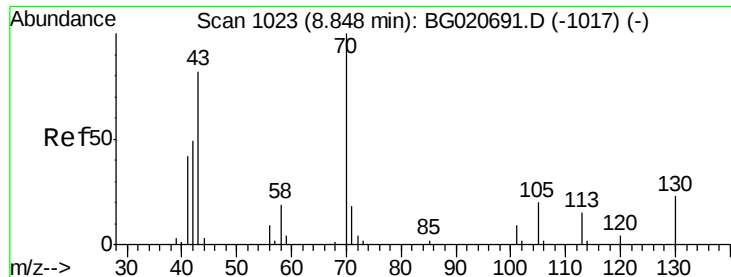

#15
N-Nitroso-di-n-propylamine
Concen: 1.19 ng/ul
RT: 8.76 min Scan# 1007
Delta R.T. -0.09 min
Lab File: BG020695.D
Acq: 13 Jan 2016 6:58

Instrument :
BNA_G
ClientSampleId :
BC955

Tgt Ion: 70 Resp: 1025
Ion Ratio Lower Upper
70 100
42 242.3 40.2 60.4#
101 0.0 7.7 11.5#
130 0.0 17.8 26.6#

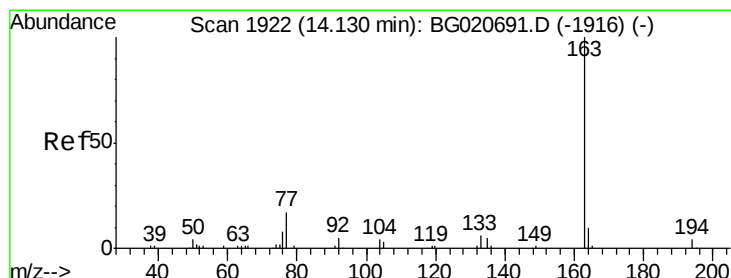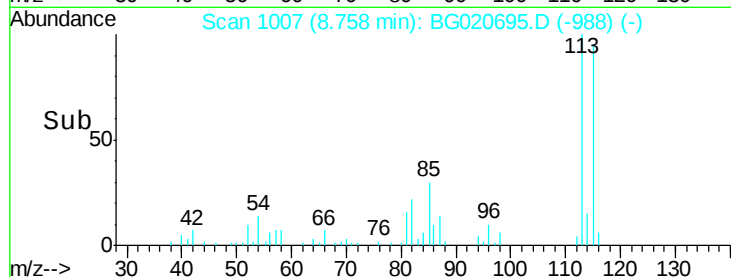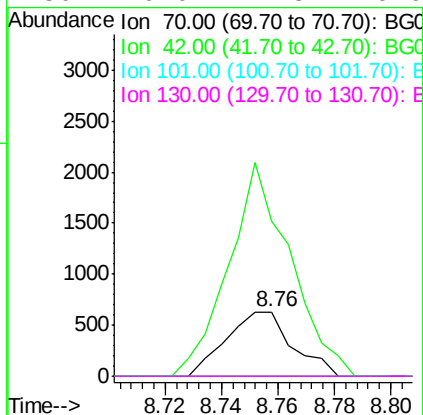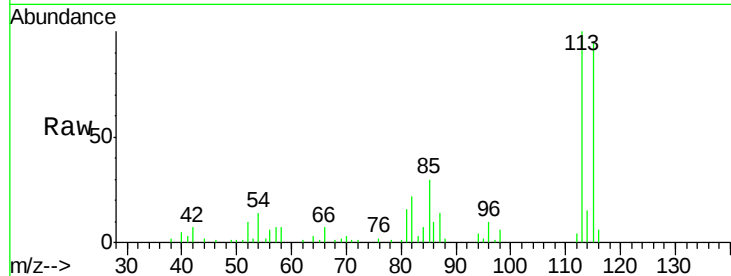

#45
Dimethylphthalate
Concen: 14.96 ng/ul
RT: 14.13 min Scan# 1921
Delta R.T. -0.00 min
Lab File: BG020695.D
Acq: 13 Jan 2016 6:58

Tgt Ion: 163 Resp: 66697
Ion Ratio Lower Upper
163 100
194 4.4 4.0 6.0
164 9.6 8.4 12.6

