

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG011216\
 Data File : BG020683.D
 Acq On : 12 Jan 2016 18:29
 Operator : SJ/IZ
 Sample : H1094-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BC956

Manual Integrations
 APPROVED

MMdadoda
 1/13/2016 3:30:56 PM

Quant Time: Jan 13 03:21:57 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG011216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 13 02:39:33 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	12651	20.00	ng/ul	0.00
18) Naphthalene-d8	10.86	136	58087	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.68	164	43002	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.43	188	119417	20.00	ng/ul	0.00
78) Chrysene-d12	21.70	240	157712	20.00	ng/ul	0.00
86) Perylene-d12	24.95	264	148126	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.41	96	1878	7.25	ng/uL	0.00
5) Phenol-d5	7.20	99	38149	35.19	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.37	67	25791	39.56	ng/ul	0.00
9) 2-Chlorophenol-d4	7.57	132	33133	38.96	ng/ul	0.00
13) 4-Methylphenol-d8	8.75	113	33364	36.49	ng/ul	0.00
19) Nitrobenzene-d5	9.22	128	16873	36.82	ng/ul	0.00
22) 2-Nitrophenol-d4	9.94	143	19297	36.24	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.49	165	34568	34.10	ng/ul	0.00
29) 4-Chloroaniline-d4	11.00	131	43831	43.68	ng/ul	0.00
44) Dimethylphthalate-d6	14.08	166	138418	36.89	ng/ul	0.00
47) Acenaphthylene-d8	14.38	160	150190	35.64	ng/ul	0.00
52) 4-Nitrophenol-d4	14.89	143	17885m	35.49	ng/ul	0.00
58) Fluorene-d10	15.68	176	123008	36.77	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.80	200	21722m	33.45	ng/ul	0.00
71) Anthracene-d10	17.53	188	218025	37.25	ng/ul	0.00
79) Pyrene-d10	19.81	212	281849	37.57	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.73	264	299694	37.96	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.13	163	52270	12.96	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG011216\
Data File : BG020683.D
Acq On : 12 Jan 2016 18:29
Operator : SJ/IZ
Sample : H1094-05
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
BC956

Manual Integrations
APPROVED

MMdadoda
1/13/2016 3:30:56 PM


Quant Time: Jan 13 03:21:57 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG011216.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 13 02:39:33 2016
Response via : Initial Calibration

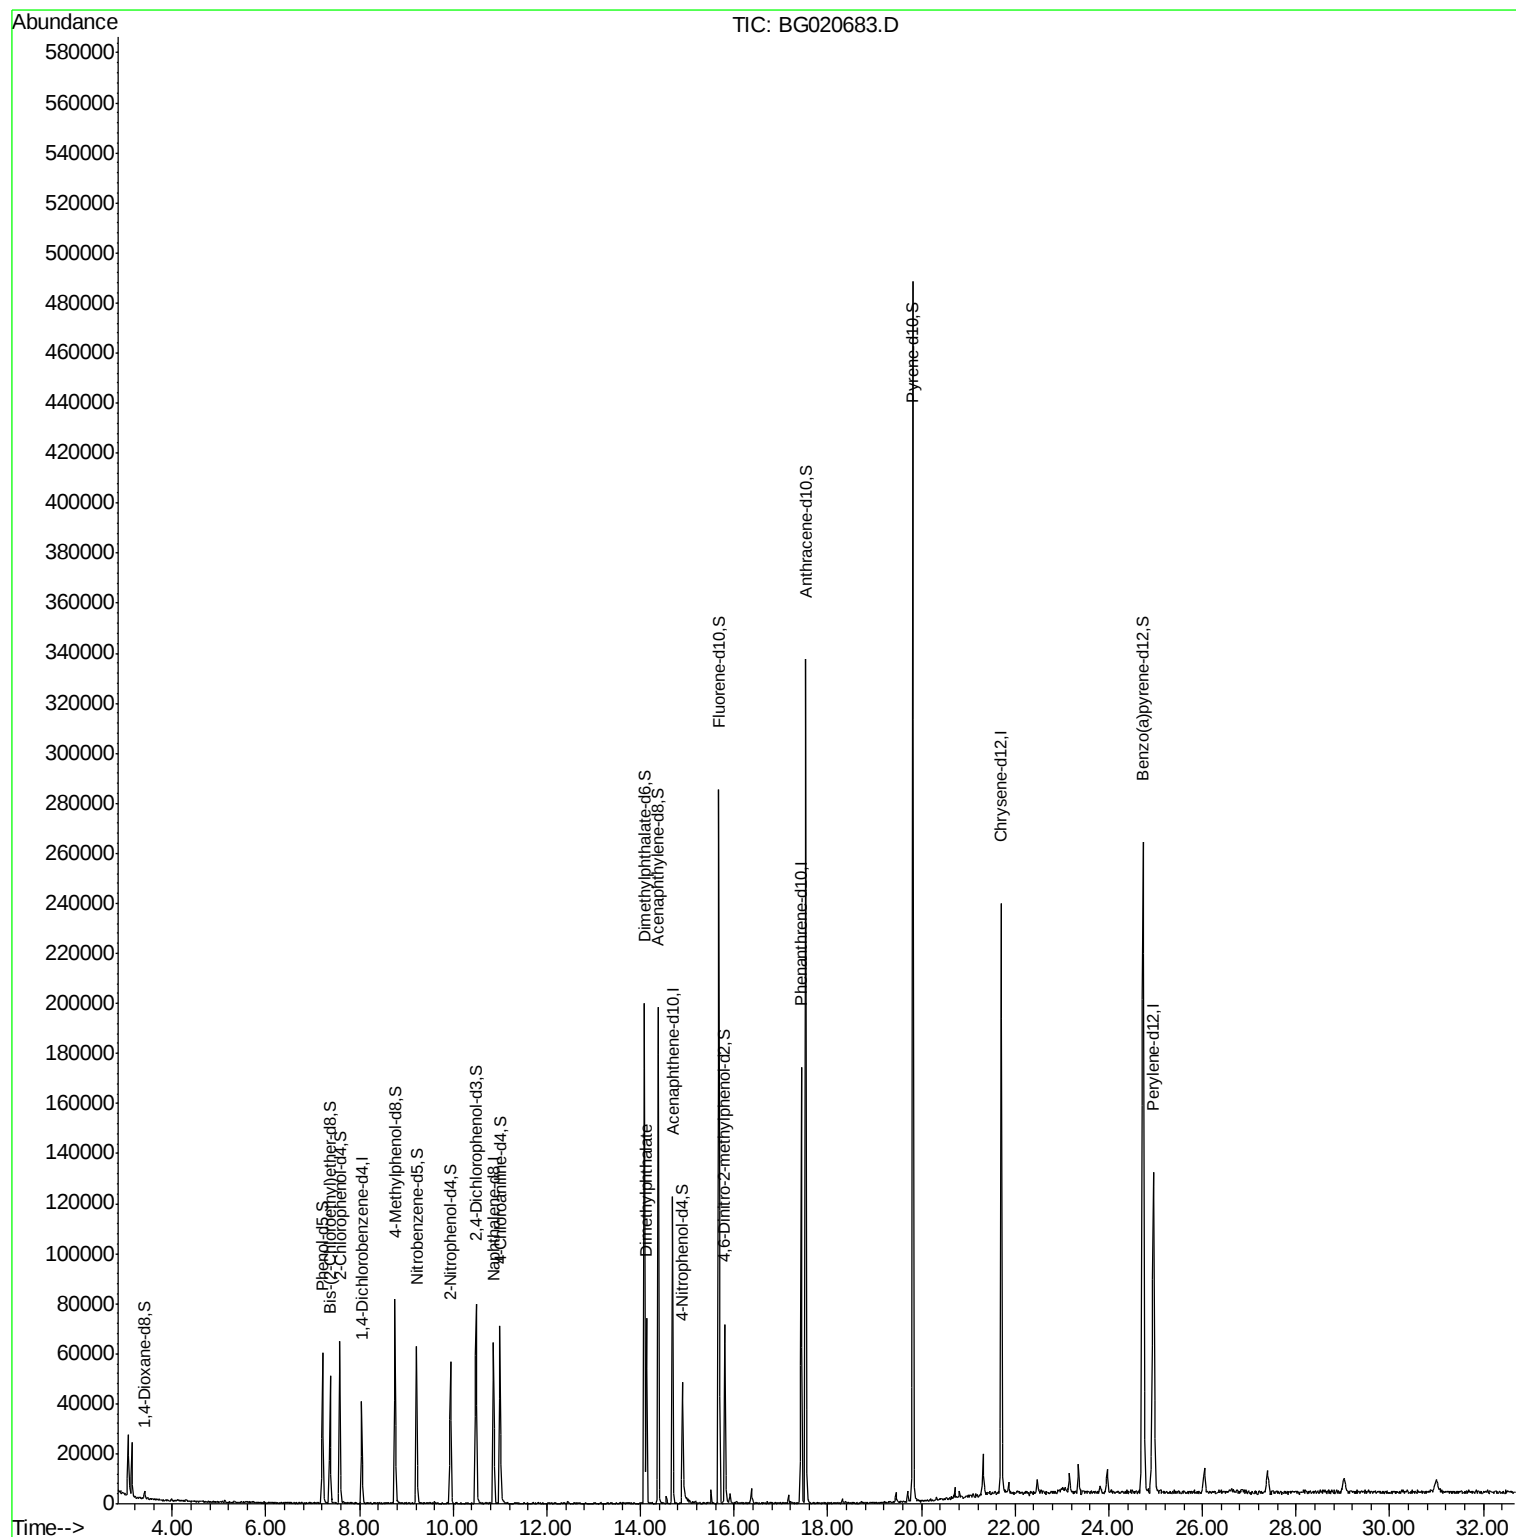

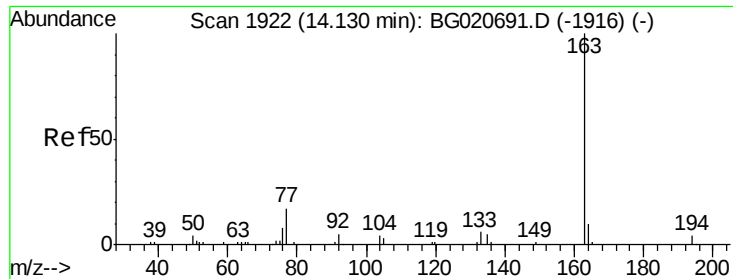

#45
 Dimethylphthalate
 Concen: 12.96 ng/ul
 RT: 14.13 min Scan# 1922
 Delta R.T. -0.00 min
 Lab File: BG020683.D
 Acq: 12 Jan 2016 18:29

Instrument :
 BNA_G
 ClientSampleId :
 BC956

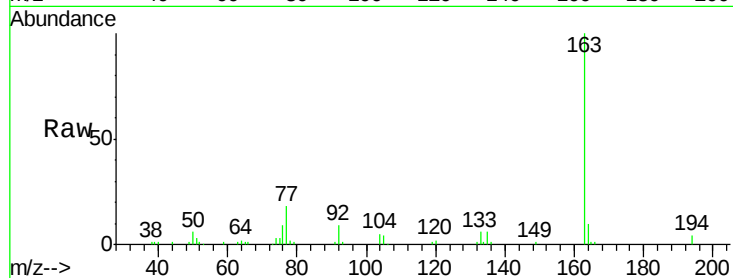

Tgt Ion:	163	Resp:	52270
Ion Ratio	Lower	Upper	
163	100		
194	4.1	4.0	6.0
164	10.3	8.4	12.6

Manual Integrations
 APPROVED

MMdadoda
 1/13/2016 3:30:56 PM

