

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG011216\
 Data File : BG020690.D
 Acq On : 12 Jan 2016 23:04
 Operator : SJ/IZ
 Sample : H1094-14
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BC9G0

Manual Integrations
 APPROVED

MMdadoda
 1/13/2016 3:32:08 PM

Quant Time: Jan 13 03:51:24 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG011216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 13 02:39:33 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.04	152	13843	20.00	ng/ul	0.00
18) Naphthalene-d8	10.86	136	60012	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.68	164	43519	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.43	188	119516	20.00	ng/ul	0.00
78) Chrysene-d12	21.70	240	154119	20.00	ng/ul	0.00
86) Perylene-d12	24.95	264	145461	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.41	96	1709	6.03	ng/uL	0.00
5) Phenol-d5	7.20	99	35273	29.74	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.36	67	23762	33.31	ng/ul	0.00
9) 2-Chlorophenol-d4	7.58	132	29721	31.94	ng/ul	0.00
13) 4-Methylphenol-d8	8.75	113	31113	31.09	ng/ul	0.00
19) Nitrobenzene-d5	9.22	128	15827	33.43	ng/ul	0.00
22) 2-Nitrophenol-d4	9.94	143	18658	33.91	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.49	165	32191	30.74	ng/ul	0.00
29) 4-Chloroaniline-d4	11.00	131	41203	39.75	ng/ul	0.00
44) Dimethylphthalate-d6	14.08	166	132423	34.87	ng/ul	0.00
47) Acenaphthylene-d8	14.38	160	145257	34.06	ng/ul	0.00
52) 4-Nitrophenol-d4	14.89	143	16590m	32.53	ng/ul	0.00
58) Fluorene-d10	15.68	176	118217	34.92	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.80	200	19031m	29.28	ng/ul	0.00
71) Anthracene-d10	17.53	188	204883	34.97	ng/ul	0.00
79) Pyrene-d10	19.81	212	261292	35.64	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.73	264	276516	35.66	ng/ul	0.00

Target Compounds					Qvalue
45) Dimethylphthalate	14.13	163	36723	9.00 ng/ul#	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG011216\
Data File : BG020690.D
Acq On : 12 Jan 2016 23:04
Operator : SJ/IZ
Sample : H1094-14
Misc :
ALS Vial : 19 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
BC9G0

Manual Integrations
APPROVED

MMdadoda
1/13/2016 3:32:08 PM

Quant Time: Jan 13 03:51:24 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG011216.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 13 02:39:33 2016
Response via : Initial Calibration

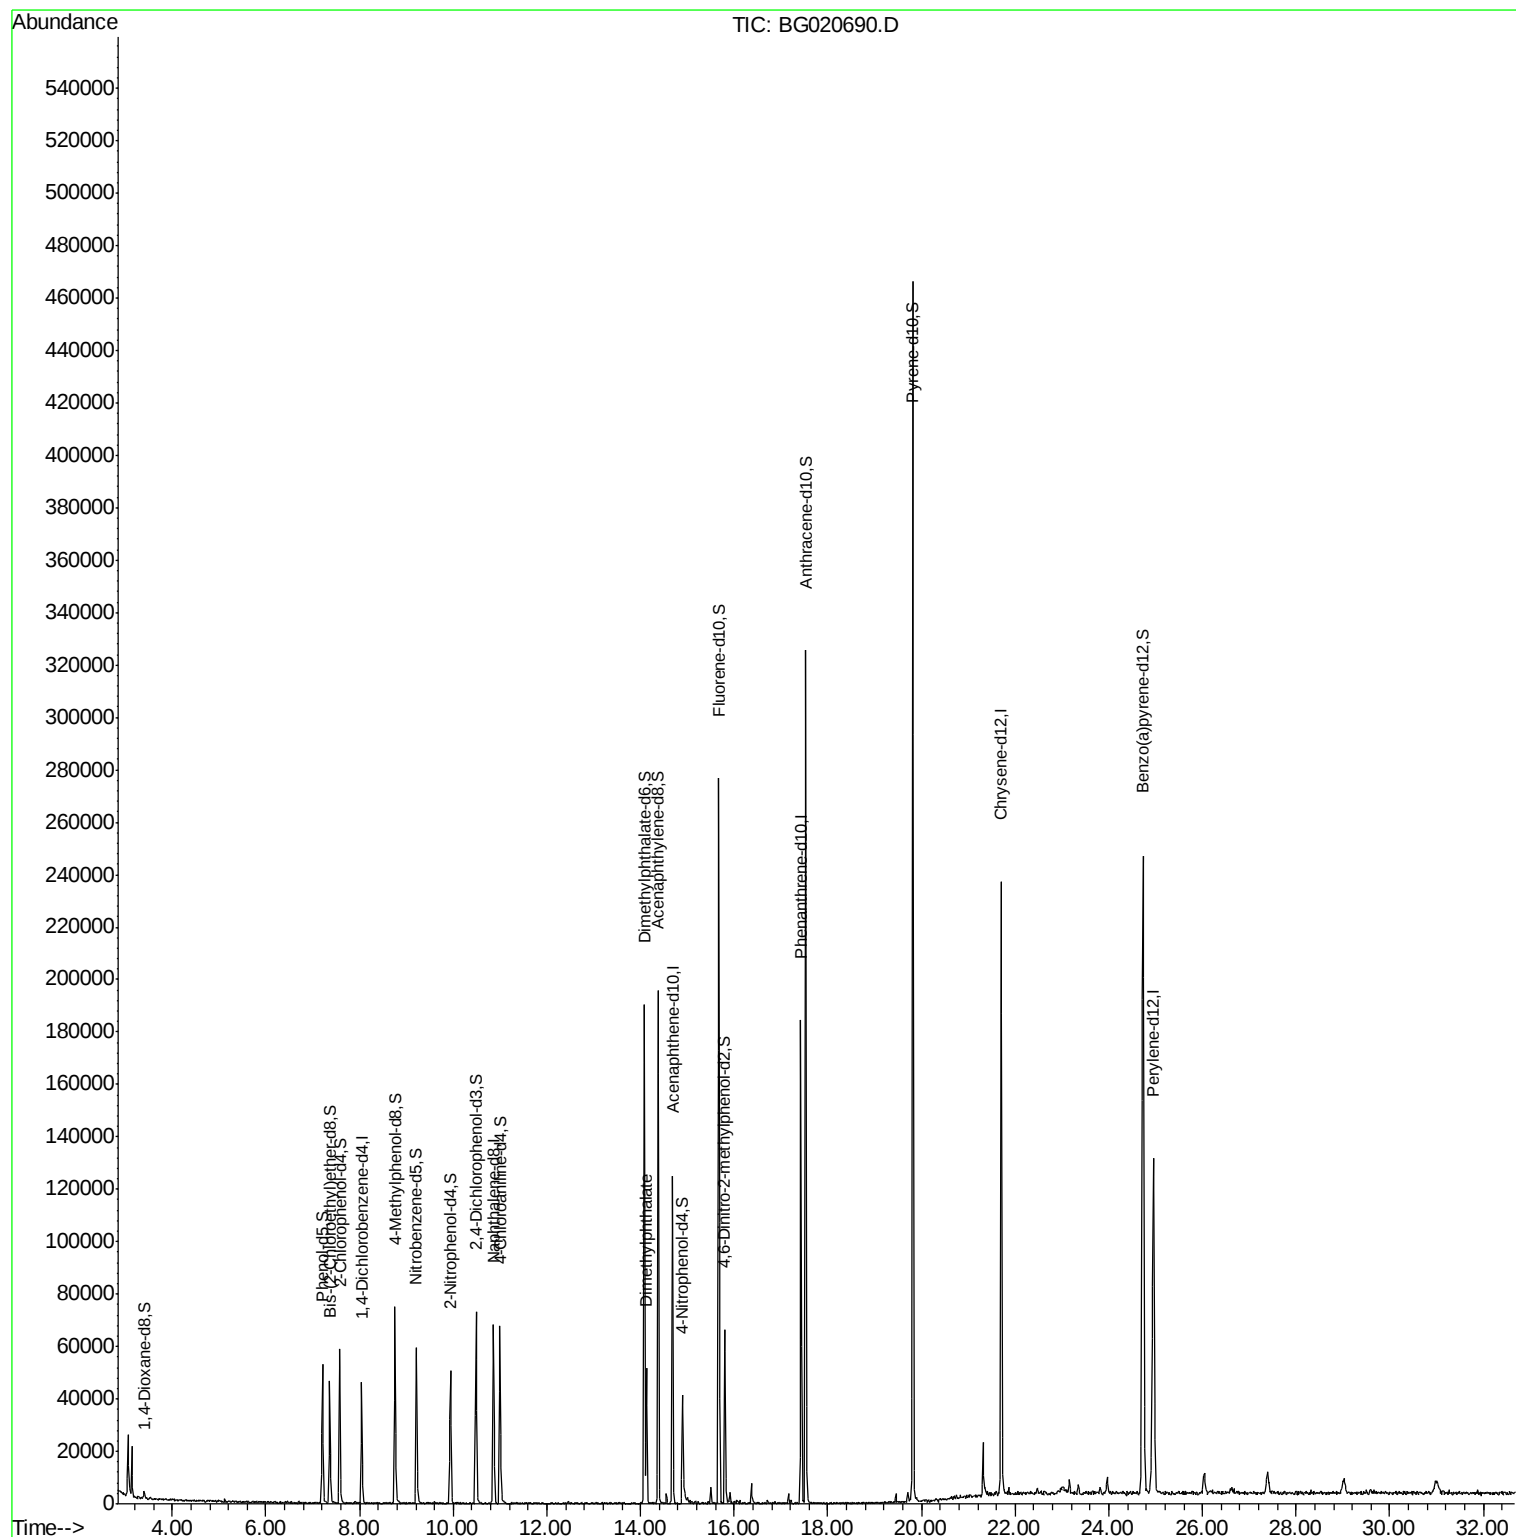

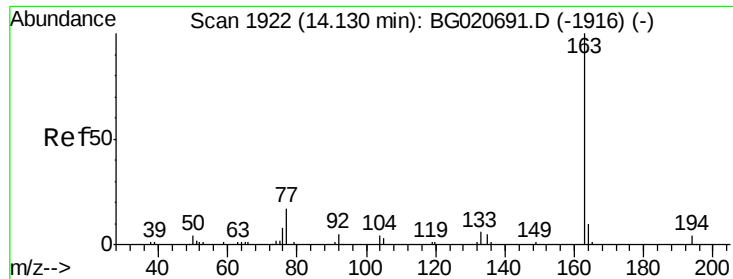

#45
 Dimethylphthalate
 Concen: 9.00 ng/ul
 RT: 14.13 min Scan# 1922
 Delta R.T. -0.00 min
 Lab File: BG020690.D
 Acq: 12 Jan 2016 23:04

Instrument :
 BNA_G
 ClientSampleId :
 BC9G0

Tgt Ion:	163	Resp:	36723
Ion Ratio	Lower	Upper	
163	100		
194	3.8	4.0	6.0#
164	10.8	8.4	12.6

Manual Integrations
 APPROVED

MMdadoda
 1/13/2016 3:32:08 PM

