


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG011216\
Data File : BG020671.D
Acq On : 12 Jan 2016 8:51
Operator : SJ/IZ
Sample : DFTPP21
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP21

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG011216.M
Title : SVOA CALIBRATION
Last Update : Wed Jan 13 07:56:00 2016

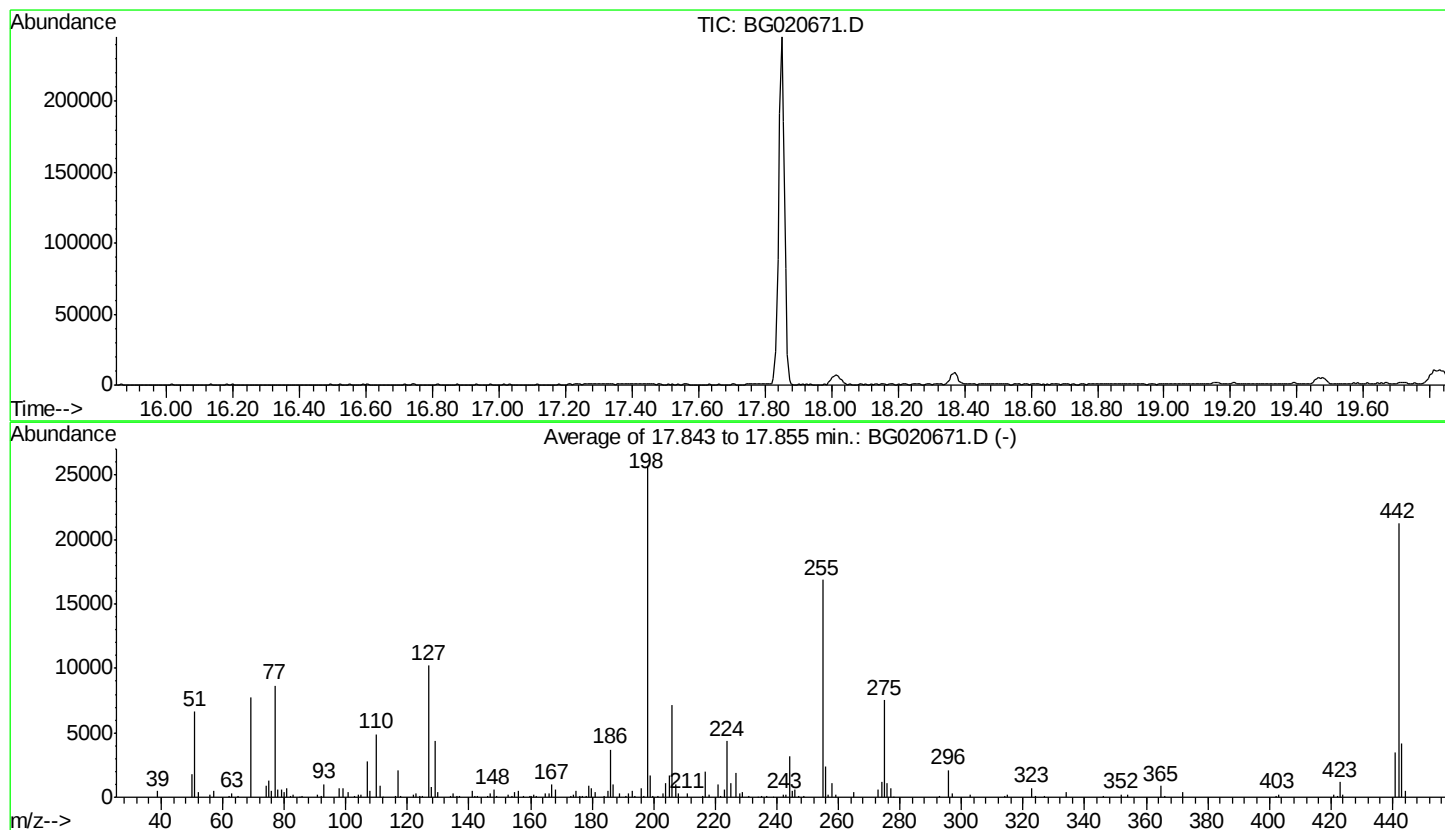

AutoFind: Scans 2554, 2555, 2556; Background Corrected with Scan 2549

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.7	6620	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	30.2	7768	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	39.6	10194	PASS
197	198	0.00	2	0.4	95	PASS
198	198	100	100	100.0	25746	PASS
199	198	5	9	6.5	1664	PASS
275	198	10	60	29.2	7512	PASS
365	198	1	100	3.4	881	PASS
441	442	0.01	100	16.3	3459	PASS
442	198	50	100	82.6	21261	PASS
443	442	15	24	19.9	4227	PASS

m/z	Abundance
39.00	565.0
44.00	262.0
50.00	1898.0
51.00	7164.0
52.00	372.0
56.00	238.0
57.00	472.0
62.00	158.0
63.00	353.0
65.00	161.0
69.00	8044.0
74.00	990.0
75.00	1317.0
75.90	551.0
77.00	8817.0
78.00	713.0
79.00	564.0
79.90	573.0
80.90	737.0
81.90	249.0
83.00	158.0
84.90	150.0
91.00	153.0
93.00	899.0
98.00	750.0
99.00	629.0
100.90	412.0
104.00	172.0
105.00	277.0
107.00	2895.0
108.00	416.0
110.00	4717.0
111.00	1005.0
117.00	2206.0
117.90	247.0
121.90	165.0
123.00	376.0
125.00	186.0
127.00	10765.0
128.00	772.0
129.00	4516.0
129.90	455.0
135.00	235.0
136.00	175.0
137.00	237.0
140.90	490.0
141.90	169.0
147.00	264.0
148.00	612.0
155.00	337.0
156.00	574.0
160.10	153.0
161.00	240.0
165.00	255.0
165.90	228.0
167.00	1528.0
168.00	679.0
173.00	176.0
173.90	252.0
174.90	479.0
176.00	210.0
179.00	833.0
179.90	682.0
181.00	323.0
185.10	440.0
186.00	3583.0
186.90	972.0
189.00	245.0
190.90	183.0
191.90	329.0
192.90	456.0
194.00	169.0
196.00	684.0
196.90	287.0
197.90	24024.0
198.90	1673.0
201.40	162.0
203.00	193.0
204.00	997.0
205.00	1568.0
206.00	6632.0
207.00	976.0
207.90	361.0
211.00	269.0
216.90	1843.0
217.90	229.0
220.90	631.0
222.90	495.0
224.00	3805.0
224.90	837.0
226.90	1765.0

Instrument :
BNA_G
ClientSampleId :
DFTPP21

227.90	245.0
228.90	402.0
236.90	185.0
238.90	151.0
242.00	165.0
242.90	189.0
244.00	3015.0
245.00	495.0
245.90	541.0
255.00	14715.0
256.00	2070.0
256.90	151.0
257.90	999.0
259.00	164.0
264.90	308.0
273.00	498.0
274.00	1054.0
275.00	6977.0
275.90	987.0
277.00	694.0
293.00	156.0
296.00	1962.0
296.90	230.0
303.00	189.0
315.00	175.0
323.00	580.0
333.90	398.0
352.00	155.0
354.00	224.0
364.90	775.0
372.00	377.0
402.90	251.0
421.00	163.0
423.00	828.0
424.00	183.0
441.00	2560.0
442.00	15271.0
443.00	3123.0
444.00	377.0

Instrument :
BNA_G
ClientSampleId :
DFTPP21

m/z	Abundance
39.00	493.0
43.90	282.0
50.00	2002.0
51.00	7281.0
52.00	525.0
56.00	284.0
57.00	602.0
63.00	348.0
65.00	192.0
69.00	9148.0
73.90	870.0
75.00	1543.0
76.00	438.0
77.00	10164.0
78.00	660.0
79.00	812.0
80.00	550.0
80.90	877.0
82.00	173.0
83.10	233.0
85.90	220.0
90.80	160.0
91.90	245.0
93.00	1203.0
98.00	754.0
98.90	731.0
100.90	545.0
102.90	163.0
104.00	163.0
105.00	226.0
107.00	3256.0
108.00	626.0
110.00	6131.0
111.00	944.0
111.90	152.0
116.10	209.0
117.00	2335.0
121.90	249.0
122.90	458.0
123.90	188.0
124.90	182.0
127.00	11859.0
127.90	927.0
129.00	5022.0
129.90	368.0
133.90	242.0
134.90	440.0
136.90	182.0
141.00	620.0
142.00	218.0
142.90	179.0
145.90	176.0
146.90	338.0
148.00	599.0
149.00	195.0
152.90	299.0
153.90	167.0
155.00	497.0
155.90	442.0
157.90	186.0
160.00	169.0
161.00	233.0
161.90	164.0
164.90	218.0
166.00	405.0
167.00	1759.0
168.00	653.0
172.90	261.0
173.90	215.0
175.00	444.0
176.00	184.0
176.90	174.0
177.90	161.0
178.90	1083.0
179.90	680.0
180.90	381.0
184.00	209.0
184.90	675.0
186.00	4147.0
186.90	1078.0
188.90	363.0
191.90	332.0
192.90	584.0
195.90	830.0
197.90	31080.0
198.90	2028.0
199.80	167.0
202.90	326.0
204.00	1280.0
205.00	1977.0
206.00	8519.0

Instrument :
BNA_G
ClientSampleId :
DFTPP21

207.00	1214.0
208.00	327.0
210.90	300.0
216.90	2437.0
218.00	247.0
220.90	1289.0
221.90	297.0
222.90	569.0
224.00	5184.0
224.90	1287.0
226.90	2001.0
228.00	266.0
228.90	491.0
230.90	156.0
233.90	153.0
235.00	171.0
236.90	170.0
241.90	295.0
243.00	279.0
244.00	3729.0
245.00	525.0
246.00	705.0
246.90	255.0
248.90	161.0
254.90	19824.0
255.90	2797.0
256.90	220.0
258.00	1203.0
258.90	161.0
264.90	368.0
272.90	672.0
274.00	1507.0
275.00	8583.0
275.90	1267.0
277.00	812.0
278.00	151.0
292.90	210.0
295.90	2199.0
296.90	360.0
303.00	205.0
314.00	176.0
315.10	252.0
323.00	984.0
324.00	165.0
326.90	249.0
334.00	419.0
345.90	209.0
352.00	382.0
354.00	300.0
365.00	1060.0
365.90	211.0
372.00	422.0
402.00	194.0
403.00	223.0
420.90	185.0
421.90	233.0
423.00	1375.0
424.00	252.0
441.00	4066.0
442.00	25296.0
443.00	4939.0
444.00	558.0

Instrument :
BNA_G
ClientSampleId :
DFTPP21

m/z	Abundance
39.00	389.0
39.90	164.0
43.90	212.0
50.00	1360.0
51.00	5416.0
52.00	258.0
56.90	527.0
62.00	151.0
62.90	304.0
69.00	6112.0
74.00	727.0
75.00	882.0
76.00	382.0
77.00	6960.0
78.00	470.0
79.00	565.0
79.90	203.0
81.00	548.0
82.90	156.0
86.00	221.0
91.00	152.0
91.90	173.0
93.00	1022.0
98.00	649.0
98.90	708.0
100.90	315.0
103.00	155.0
103.80	241.0
105.00	186.0
107.00	2292.0
107.90	439.0
109.90	3849.0
111.00	619.0
117.00	1873.0
122.00	169.0
122.90	214.0
123.90	176.0
127.00	7960.0
128.00	669.0
128.90	3555.0
129.90	235.0
135.00	336.0
135.90	219.0
141.00	454.0
147.00	255.0
147.90	486.0
152.90	162.0
154.00	161.0
154.90	368.0
156.00	457.0
159.80	171.0
160.80	279.0
164.90	298.0
166.00	209.0
167.00	1278.0
168.00	585.0
175.00	457.0
176.90	210.0
178.90	794.0
179.90	631.0
181.00	407.0
185.00	354.0
186.00	3317.0
187.00	893.0
188.90	279.0
192.00	224.0
192.90	363.0
195.90	492.0
197.90	22136.0
198.90	1291.0
201.50	160.0
203.00	274.0
204.00	894.0
205.00	1527.0
206.00	6433.0
207.00	938.0
208.00	177.0
211.10	278.0
215.90	172.0
216.90	1747.0
217.80	247.0
220.90	978.0
223.00	610.0
224.00	4023.0
225.00	1116.0
226.90	1809.0
227.80	246.0
228.90	256.0
231.00	202.0
234.90	184.0
242.00	180.0

Instrument :
BNA_G
ClientSampleId :
DFTPP21

242.90	220.0
244.00	2733.0
245.00	562.0
246.00	599.0
255.00	16022.0
256.00	2236.0
256.80	177.0
258.00	951.0
258.90	175.0
265.00	533.0
272.90	501.0
273.90	1092.0
275.00	6978.0
275.90	998.0
277.00	562.0
295.90	2184.0
296.90	395.0
302.90	174.0
314.00	164.0
314.90	218.0
322.90	537.0
334.00	492.0
351.90	193.0
353.90	182.0
365.00	809.0
365.90	185.0
371.90	404.0
402.90	236.0
421.00	157.0
422.00	159.0
423.00	1241.0
424.00	295.0
441.00	3753.0
442.00	23216.0
443.00	4619.0
444.00	508.0

Instrument :
BNA_G
ClientSampleId :
DFTPP21

Scan 2549 (17.814 min): BG020671.D
DFTPP21

m/z	Abundance
39.90	201.0
44.00	307.0
167.00	565.0

Instrument :
BNA_G
ClientSampleId :
DFTPP21