

Data Path : Z:\HPCHEM1\BNA_G\Data\BG011217\
 Data File : BG025507.D
 Acq On : 13 Jan 2017 7:36
 Operator : UM/SJ
 Sample : I1138-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-2

Quant Time: Jan 13 12:50:03 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 10 11:26:22 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.20	152	59341	20.00	ng	0.00
21) Naphthalene-d8	11.03	136	245578	20.00	ng	0.00
38) Acenaphthene-d10	14.83	164	197401	20.00	ng	0.00
63) Phenanthrene-d10	17.57	188	457216	20.00	ng	0.00
75) Chrysene-d12	21.86	240	664113	20.00	ng	0.00
86) Perylene-d12	25.26	264	693741	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.74	112	266588	81.66	ng	0.00
7) Phenol-d6	7.36	99	226571	49.28	ng	0.00
23) Nitrobenzene-d5	9.38	82	605900	108.99	ng	0.00
41) 2,4,6-Tribromophenol	16.32	330	481791	151.60	ng	0.00
44) 2-Fluorobiphenyl	13.45	172	1285353	105.42	ng	0.00
78) Terphenyl-d14	20.15	244	2168457	86.57	ng	0.00
Target Compounds						
15) Benzyl Alcohol	8.53	79	11073	2.52	ng	# 45
40) Hexachlorocyclopentadiene	13.09	237	94	8.55	ng	# 29
53) 2,4-Dinitrophenol	14.95	184	107	5.13	ng	# 15


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\Data\BG011217\
Data File : BG025507.D
Acq On : 13 Jan 2017 7:36
Operator : UM/SJ
Sample : I1138-02
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-2

Quant Time: Jan 13 12:50:03 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 10 11:26:22 2017
Response via : Initial Calibration

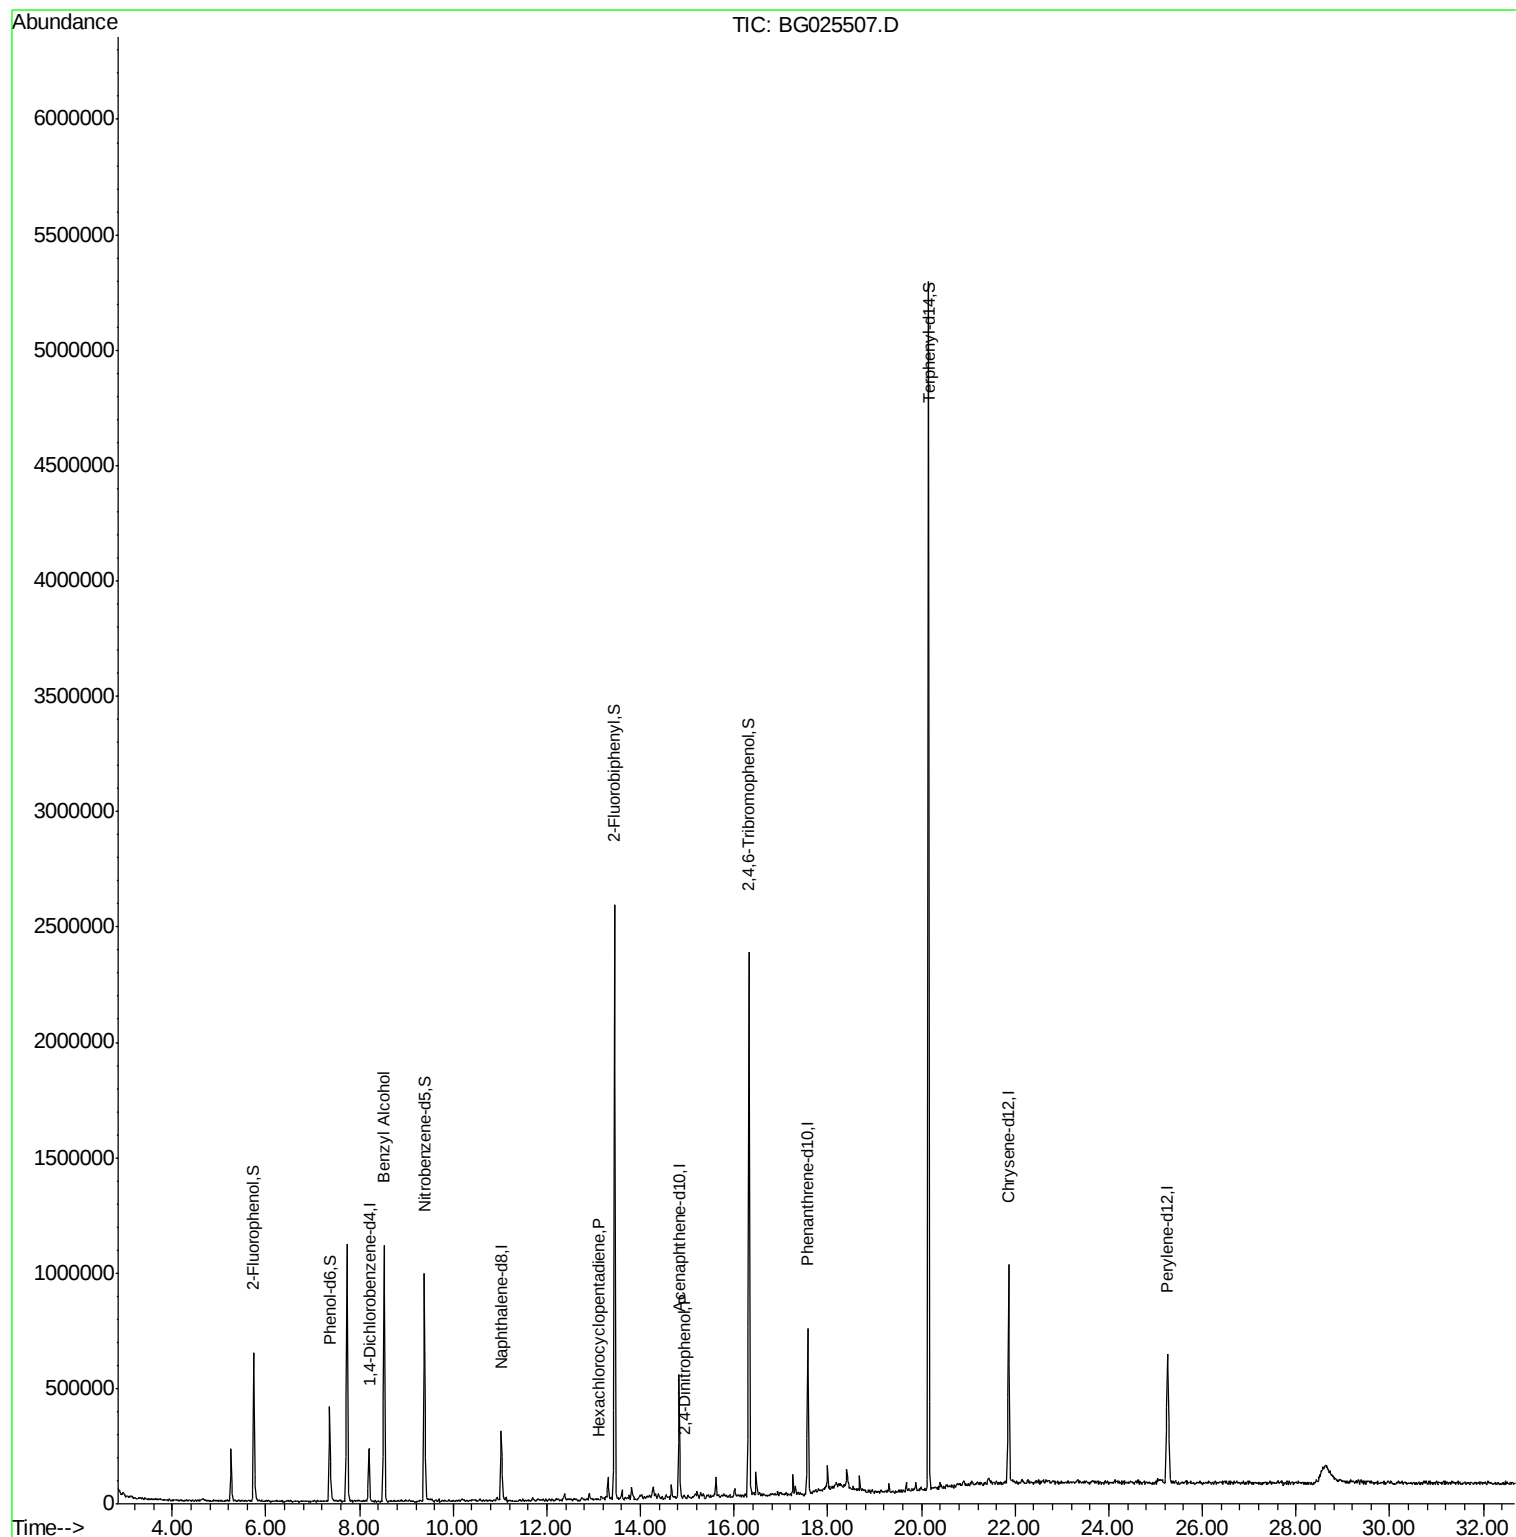

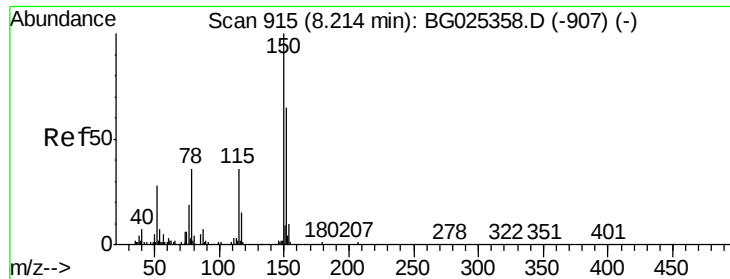


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.20 min Scan# 913
Delta R.T. 0.01 min
Lab File: BG025507.D
Acq: 13 Jan 2017 7:36

Instrument :
BNA_G
ClientSampleId :
MW-2

Tgt Ion:152 Resp: 59341
Ion Ratio Lower Upper
152 100
150 153.0 114.0 171.0
115 65.3 48.1 72.1

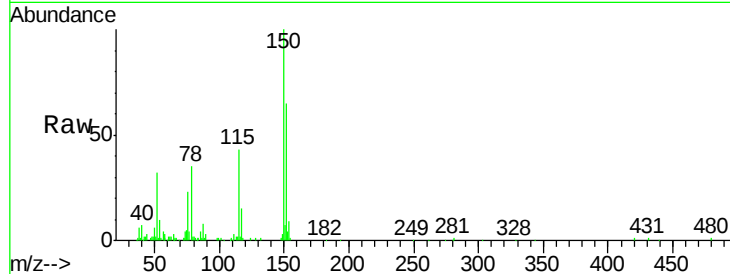


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

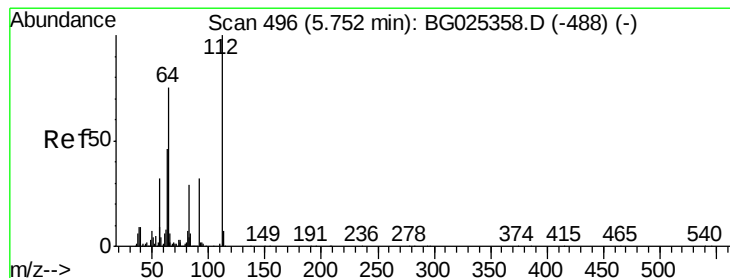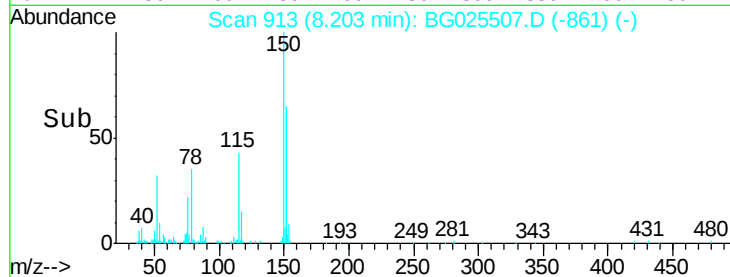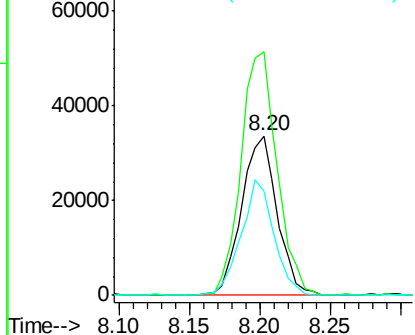



#5


2-Fluorophenol
Concen: 81.66 ng
RT: 5.74 min Scan# 494
Delta R.T. 0.01 min
Lab File: BG025507.D
Acq: 13 Jan 2017 7:36

Tgt Ion:112 Resp: 266588
Ion Ratio Lower Upper
112 100
64 70.6 61.8 92.6
63 42.0 37.2 55.8

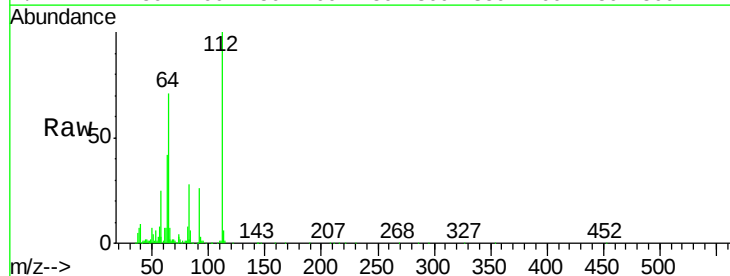

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

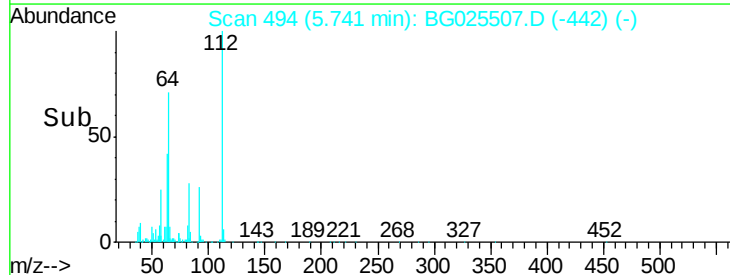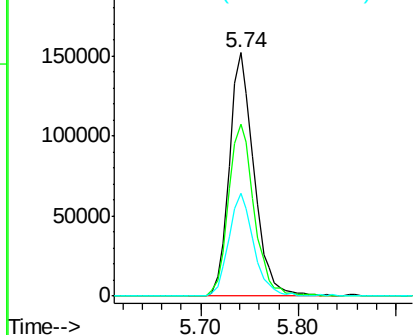

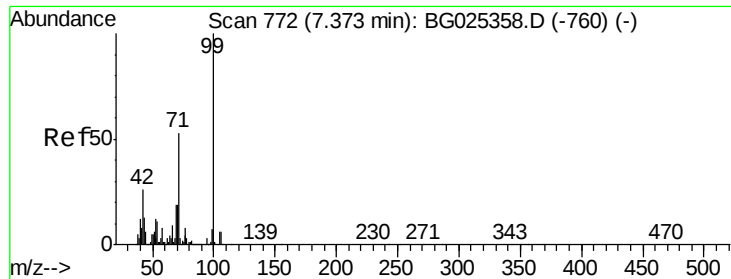

#7

Phenol-d6

Concen: 49.28 ng

RT: 7.36 min Scan# 770

Delta R.T. 0.01 min

Lab File: BG025507.D

Acq: 13 Jan 2017 7:36

Instrument :

BNA_G

ClientSampleId :

MW-2


Tgt Ion: 99 Resp: 226571

Ion Ratio Lower Upper




99 100

42 25.7 20.5 30.7

71 48.3 37.6 56.4

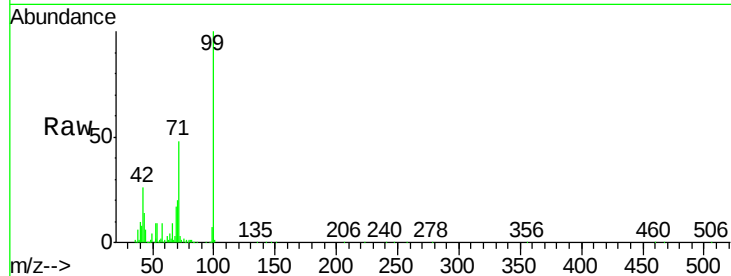

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

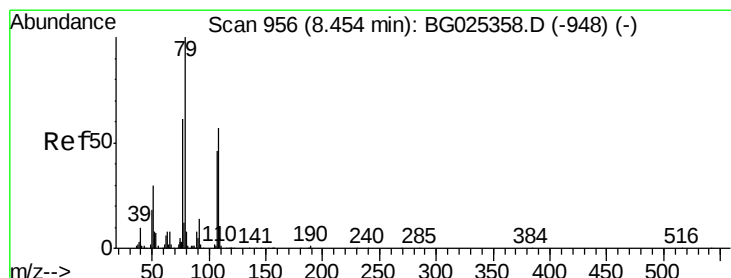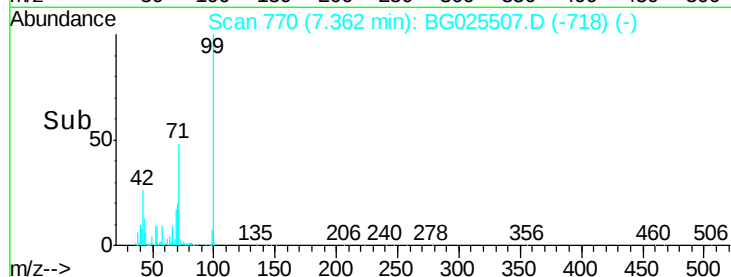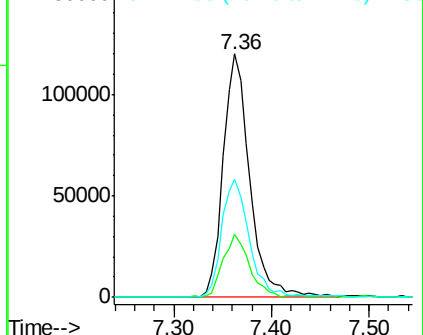

#15

Benzyl Alcohol

Concen: 2.52 ng

RT: 8.53 min Scan# 968

Delta R.T. 0.08 min

Lab File: BG025507.D

Acq: 13 Jan 2017 7:36


Tgt Ion: 79 Resp: 11073

Ion Ratio Lower Upper



79 100


108 44.5 45.5 68.3#

77 138.7 54.3 81.5#

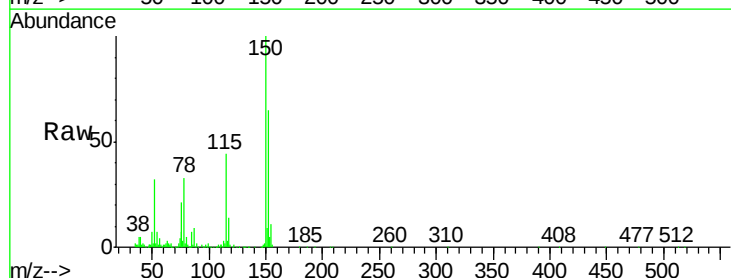

Abundance Ion 79.00 (78.70 to 79.70): BGC
Ion 108.00 (107.70 to 108.70): BGC
Ion 77.00 (76.70 to 77.70): BGC

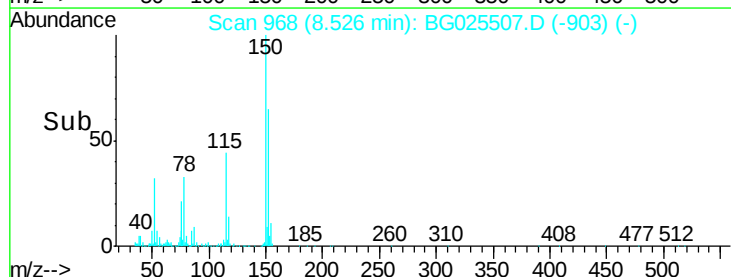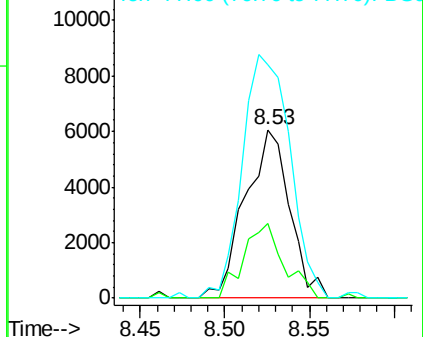


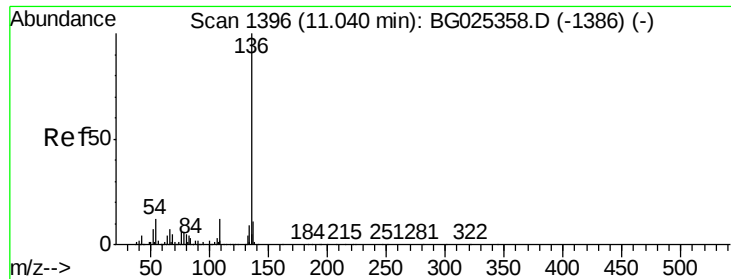




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 11.03 min Scan# 1394
Delta R.T. -0.00 min
Lab File: BG025507.D
Acq: 13 Jan 2017 7:36

Instrument :
BNA_G
ClientSampleId :
MW-2

Tgt Ion:	136	Resp:	245578
Ion	Ratio	Lower	Upper
136	100		
137	7.8	8.9	13.3#
54	11.1	9.3	13.9
68	5.1	5.1	7.7

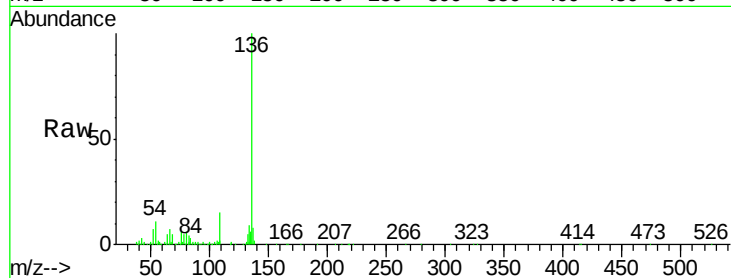


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

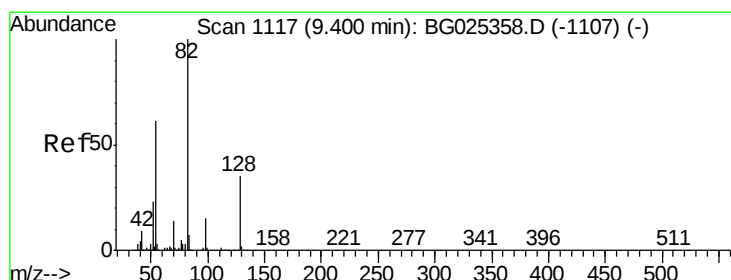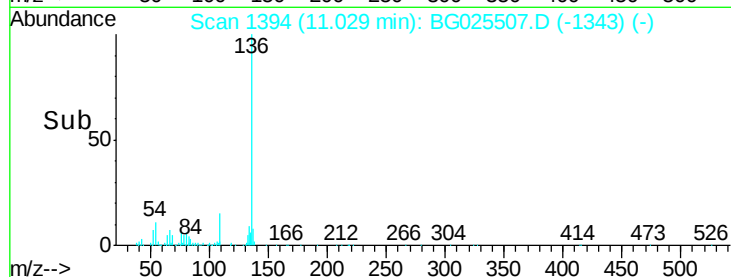
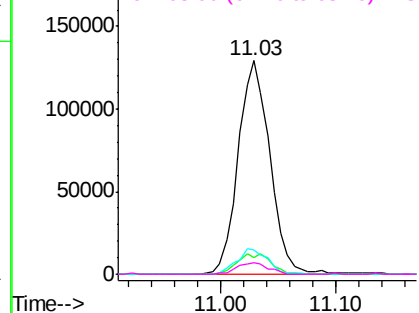



#23
Nitrobenzene-d5
Concen: 108.99 ng
RT: 9.38 min Scan# 1114
Delta R.T. -0.00 min
Lab File: BG025507.D
Acq: 13 Jan 2017 7:36

Tgt Ion:	82	Resp:	605900
Ion	Ratio	Lower	Upper
82	100		
128	34.3	26.4	39.6
54	61.1	49.4	74.2

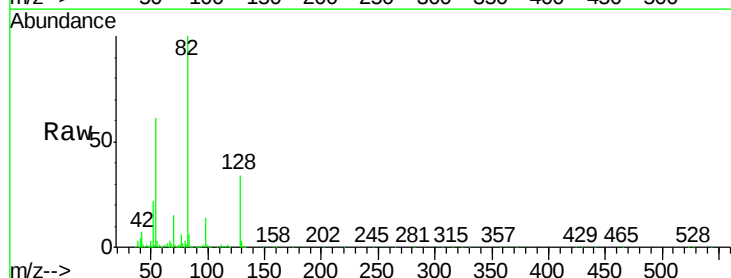

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BGC

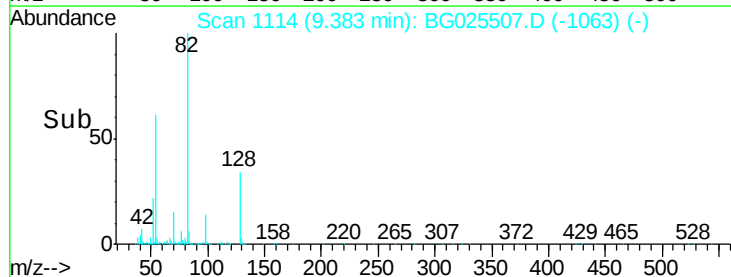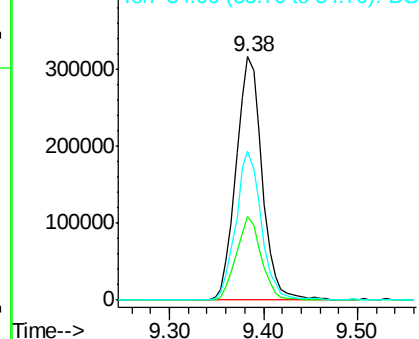

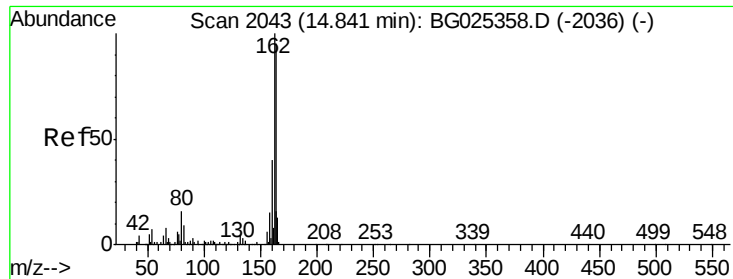

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 14.83 min Scan# 2041

Delta R.T. 0.01 min

Lab File: BG025507.D

Acq: 13 Jan 2017 7:36

Instrument :

BNA_G

ClientSampleId :

MW-2


Tgt Ion:164 Resp: 197401

Ion Ratio Lower Upper

164 100

162 101.5 85.1 127.7




160 42.2 34.7 52.1

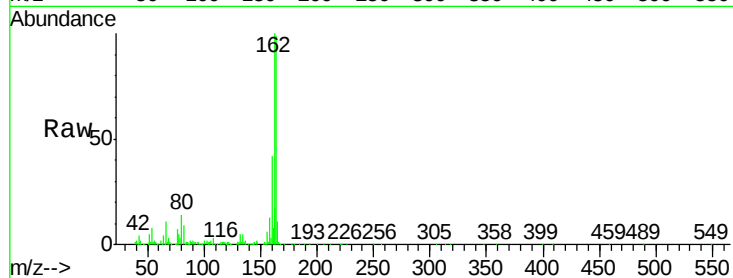

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

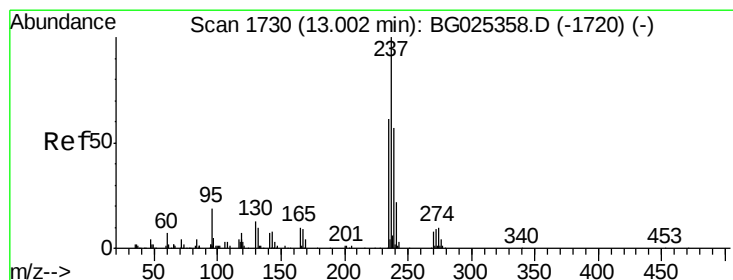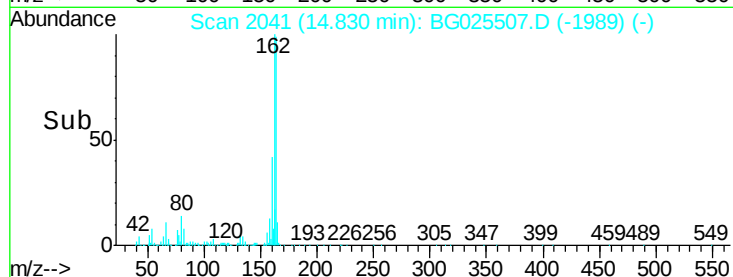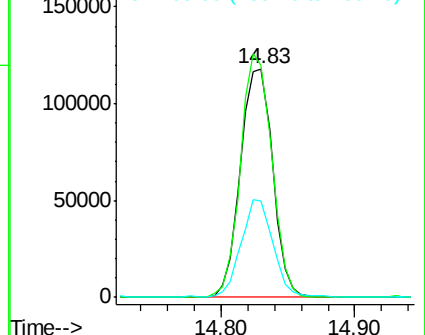

#40

Hexachlorocyclopentadiene

Concen: 8.55 ng

RT: 13.09 min Scan# 1745

Delta R.T. 0.10 min

Lab File: BG025507.D

Acq: 13 Jan 2017 7:36


Tgt Ion:237 Resp: 94

Ion Ratio Lower Upper

237 100

235 0.0 39.4 79.4#



272 0.0 0.0 32.0

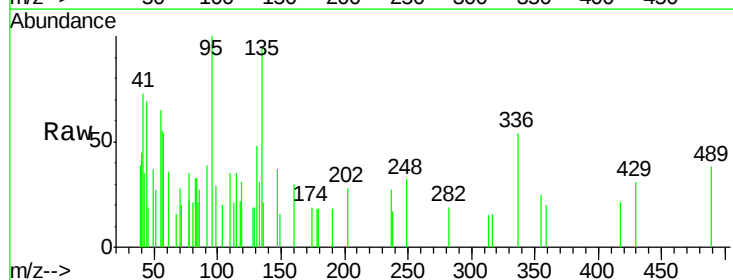

Abundance Ion 236.80 (236.50 to 237.50): E

Ion 234.90 (234.60 to 235.60): E

Ion 271.75 (271.45 to 272.45): E



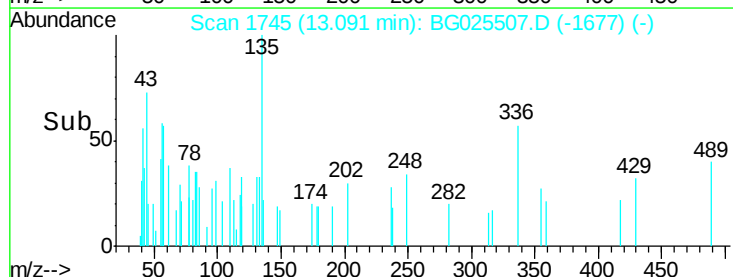
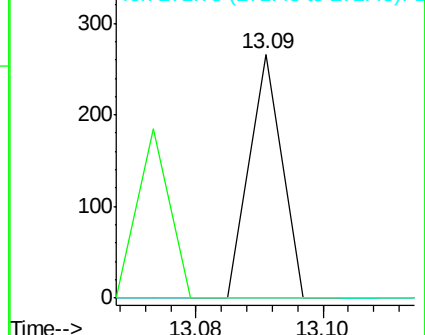




#41
2,4,6-Tribromophenol
Concen: 151.60 ng
RT: 16.32 min Scan# 2294
Delta R.T. -0.00 min
Lab File: BG025507.D
Acq: 13 Jan 2017 7:36




Instrument :
BNA_G
ClientSampleId :
MW-2


Tgt Ion:330 Resp: 481791
Ion Ratio Lower Upper
330 100
332 97.8 77.3 115.9
141 33.9 32.1 48.1

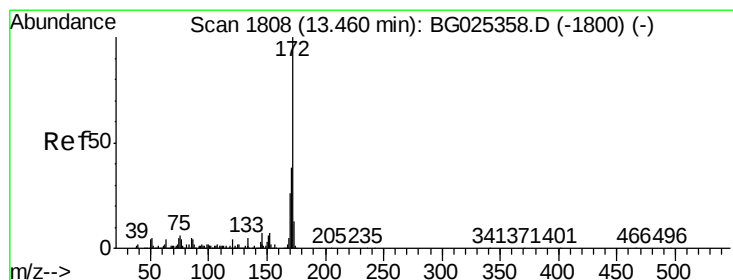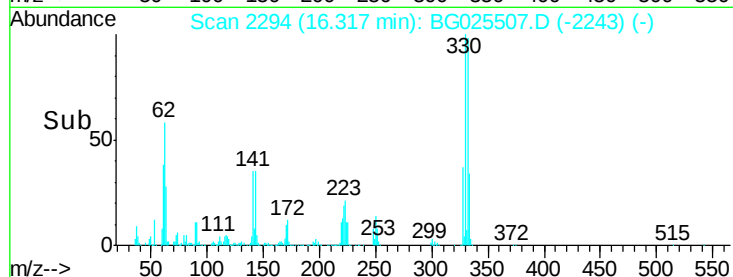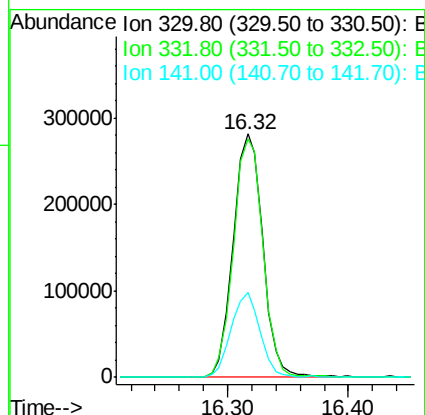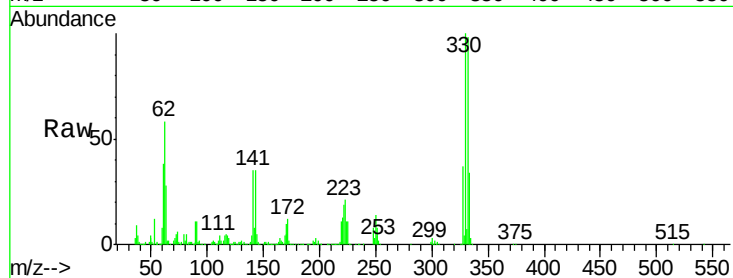

#44
2-Fluorobiphenyl
Concen: 105.42 ng
RT: 13.45 min Scan# 1806
Delta R.T. -0.00 min
Lab File: BG025507.D
Acq: 13 Jan 2017 7:36

Tgt Ion:172 Resp: 1285353
Ion Ratio Lower Upper
172 100
171 38.1 32.2 48.2
170 26.7 21.8 32.6

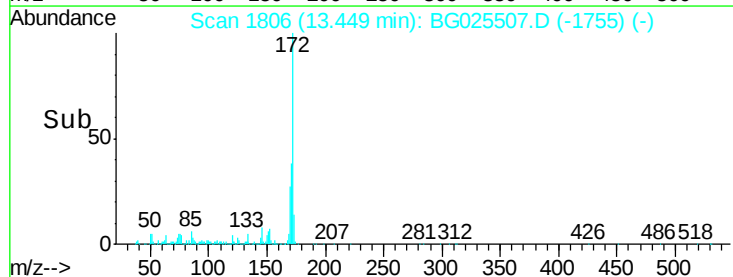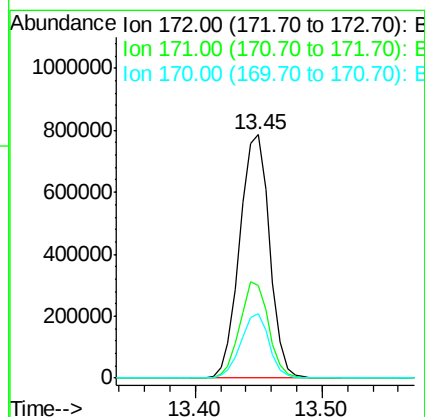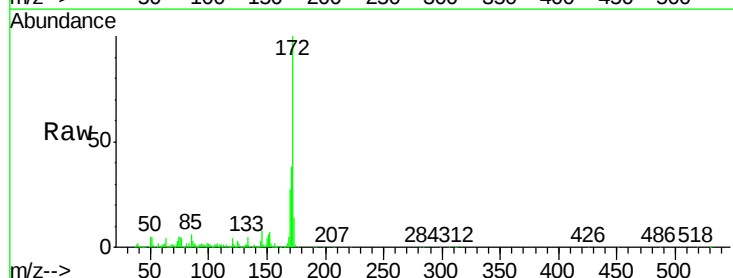

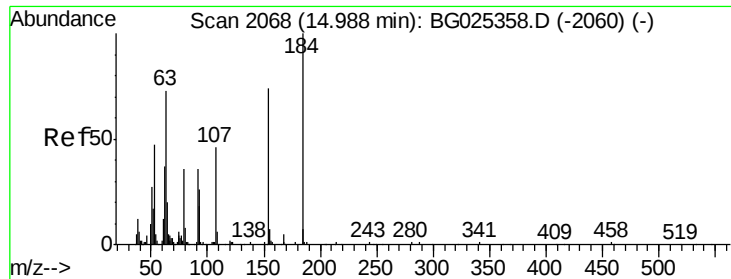

#53

2,4-Dinitrophenol

Concen: 5.13 ng

RT: 14.95 min Scan# 2062

Delta R.T. -0.02 min

Lab File: BG025507.D

Acq: 13 Jan 2017 7:36

Instrument :





BNA_G

ClientSampleId :

MW-2

Tgt Ion:184 Resp: 107

Ion	Ratio	Lower	Upper
184	100		
63	0.0	52.7	79.1#
154	0.0	57.3	85.9#

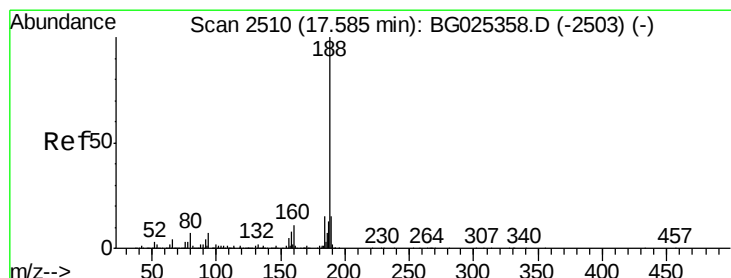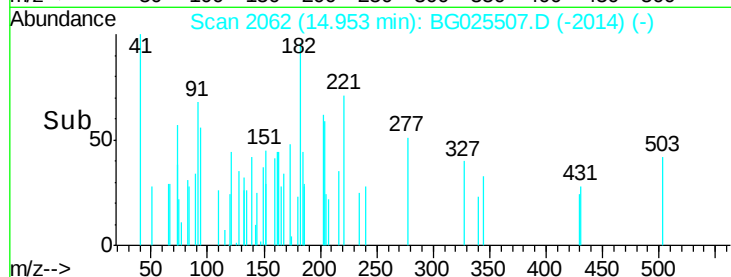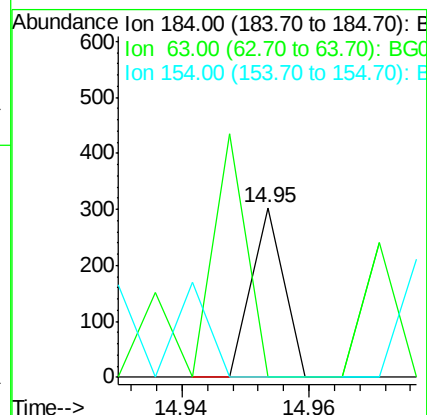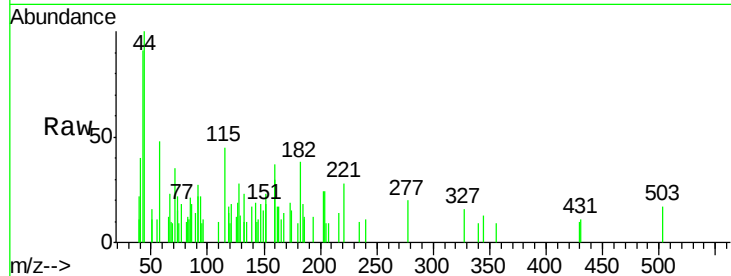

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.57 min Scan# 2507




Delta R.T. -0.01 min


Lab File: BG025507.D

Acq: 13 Jan 2017 7:36

Tgt Ion:188 Resp: 457216

Ion	Ratio	Lower	Upper
188	100		
94	5.4	5.8	8.8#
80	8.5	7.5	11.3


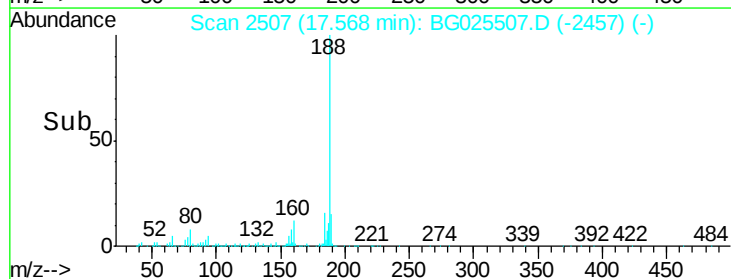
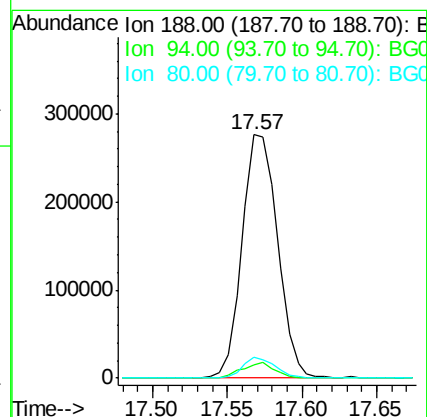
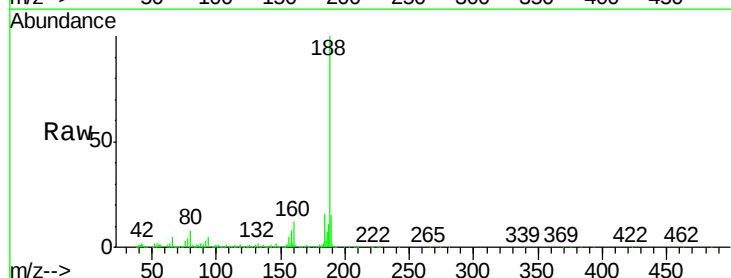


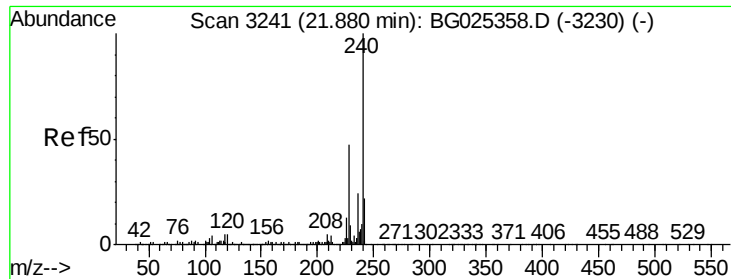

#75
 Chrysene-d12
 Concen: 20.00 ng
 RT: 21.86 min Scan# 3238
 Delta R.T. -0.00 min
 Lab File: BG025507.D
 Acq: 13 Jan 2017 7:36




Instrument :
 BNA_G
 ClientSampleId :
 MW-2


Tgt Ion:240 Resp: 664113
 Ion Ratio Lower Upper
 240 100
 120 4.7 5.7 8.5#
 236 26.4 22.2 33.4

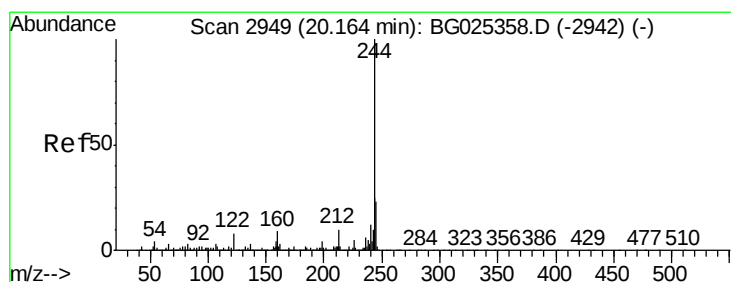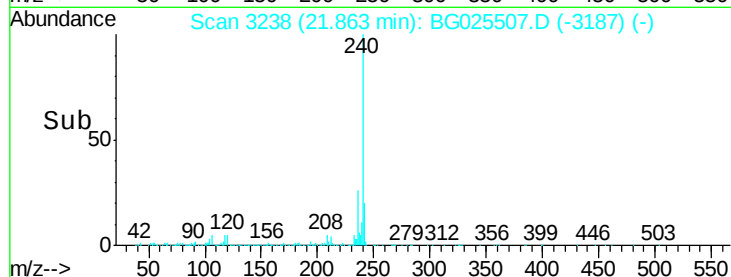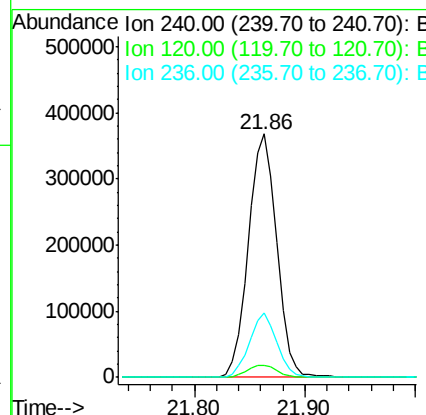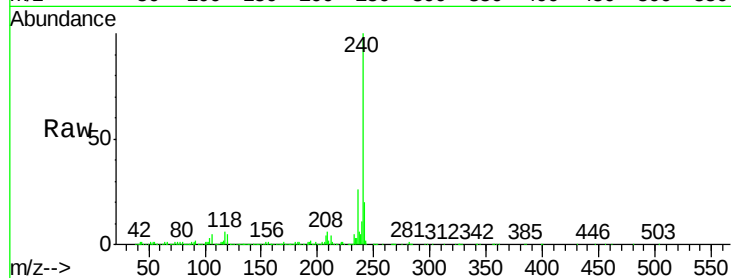

#78
 Terphenyl-d14
 Concen: 86.57 ng
 RT: 20.15 min Scan# 2947
 Delta R.T. -0.00 min
 Lab File: BG025507.D
 Acq: 13 Jan 2017 7:36

Tgt Ion:244 Resp: 2168457
 Ion Ratio Lower Upper
 244 100
 212 10.2 10.0 15.0
 122 7.2 8.6 12.8#

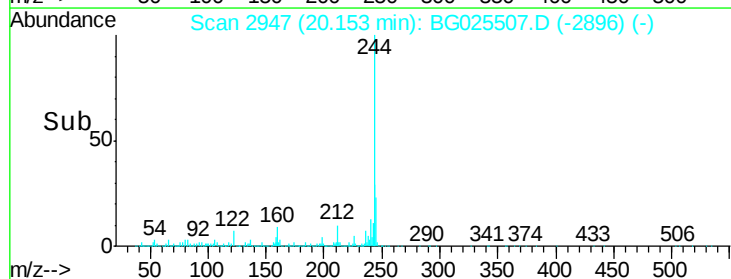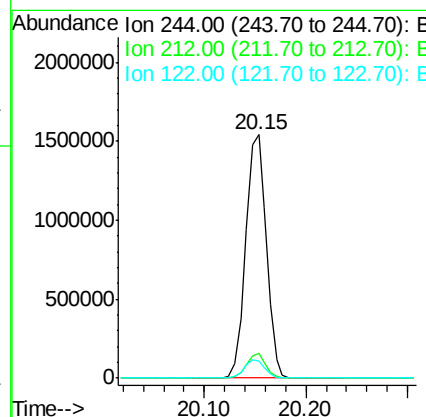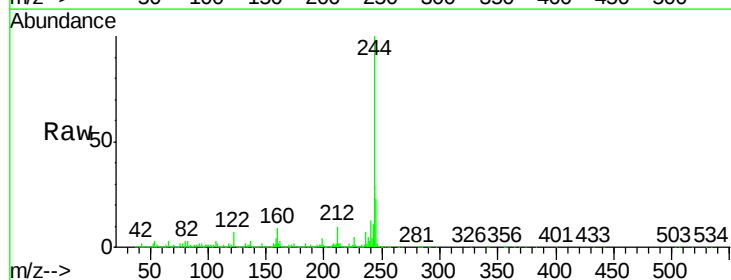

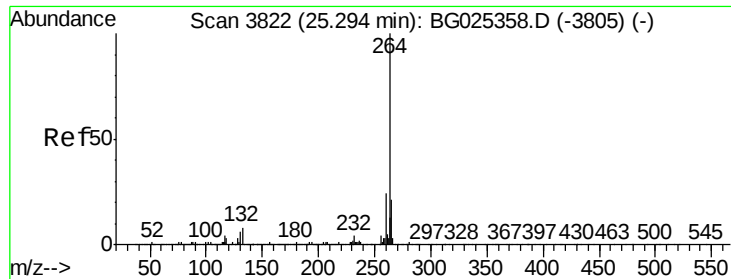

#86
Perylene-d12
Concen: 20.00 ng
RT: 25.26 min Scan# 3816
Delta R.T. -0.01 min
Lab File: BG025507.D
Acq: 13 Jan 2017 7:36

Instrument :
BNA_G
ClientSampleId :
MW-2

Tgt Ion	Ratio	Lower	Upper
264	100		
260	23.1	21.8	32.8
265	21.1	18.2	27.4

