


Data Path : Z:\HPCHEM1\BNA G\DATA\BG011217\
 Data File : BG025495.D
 Acq On : 12 Jan 2017 23:34
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 10 11:26:22 2017

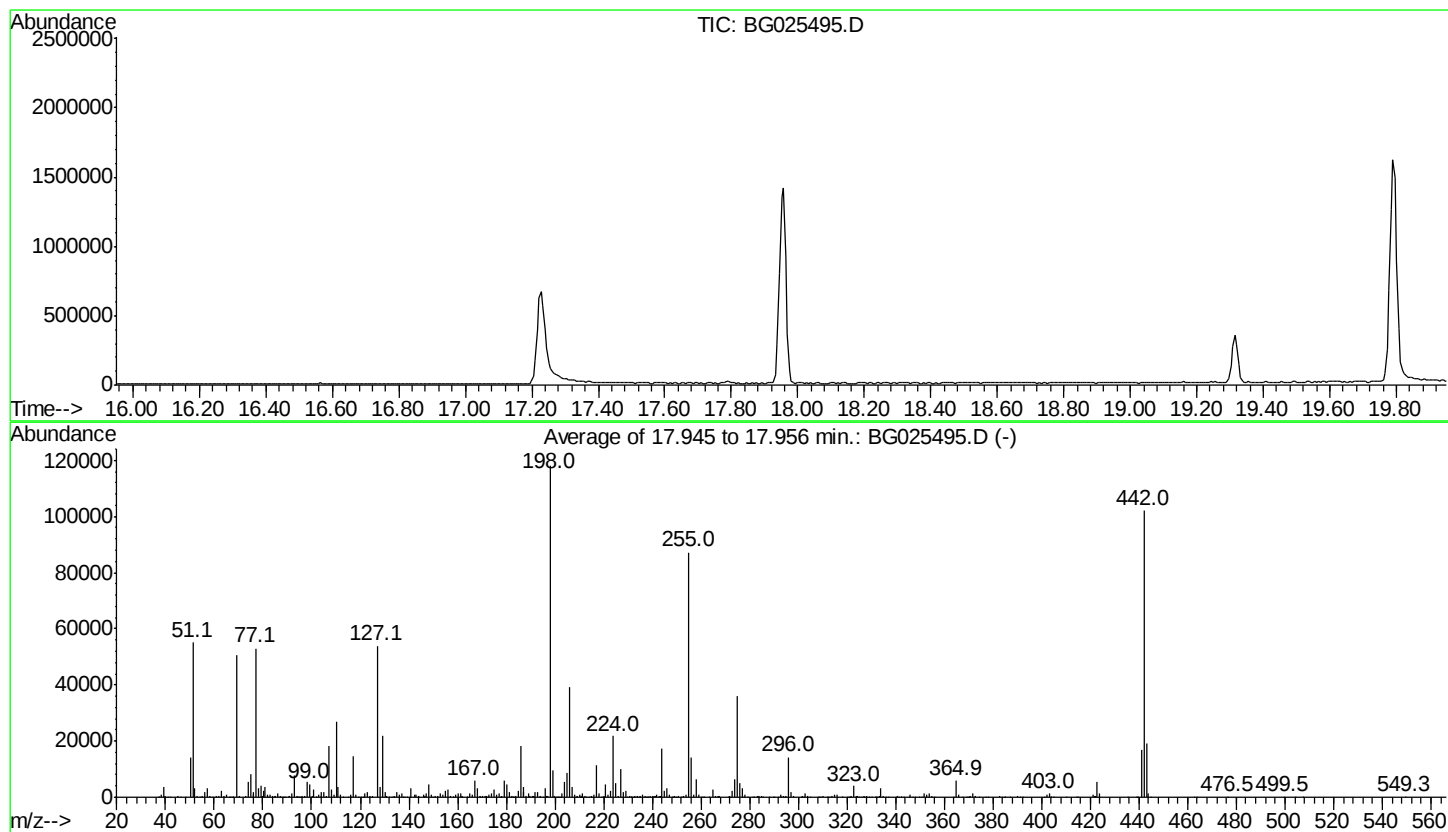

AutoFind: Scans 2571, 2572, 2573; Background Corrected with Scan 2565

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.6	55045	PASS
68	69	0.00	2	0.4	220	PASS
69	198	0.00	100	43.0	50816	PASS
70	69	0.00	2	0.5	260	PASS
127	198	10	80	45.7	53976	PASS
197	198	0.00	2	0.4	489	PASS
198	198	100	100	100.0	118112	PASS
199	198	5	9	8.0	9444	PASS
275	198	10	60	30.4	35925	PASS
365	198	1	100	4.9	5814	PASS
441	442	0.01	24	16.4	16766	PASS
442	198	50	100	86.4	102061	PASS
443	442	15	24	18.8	19154	PASS