
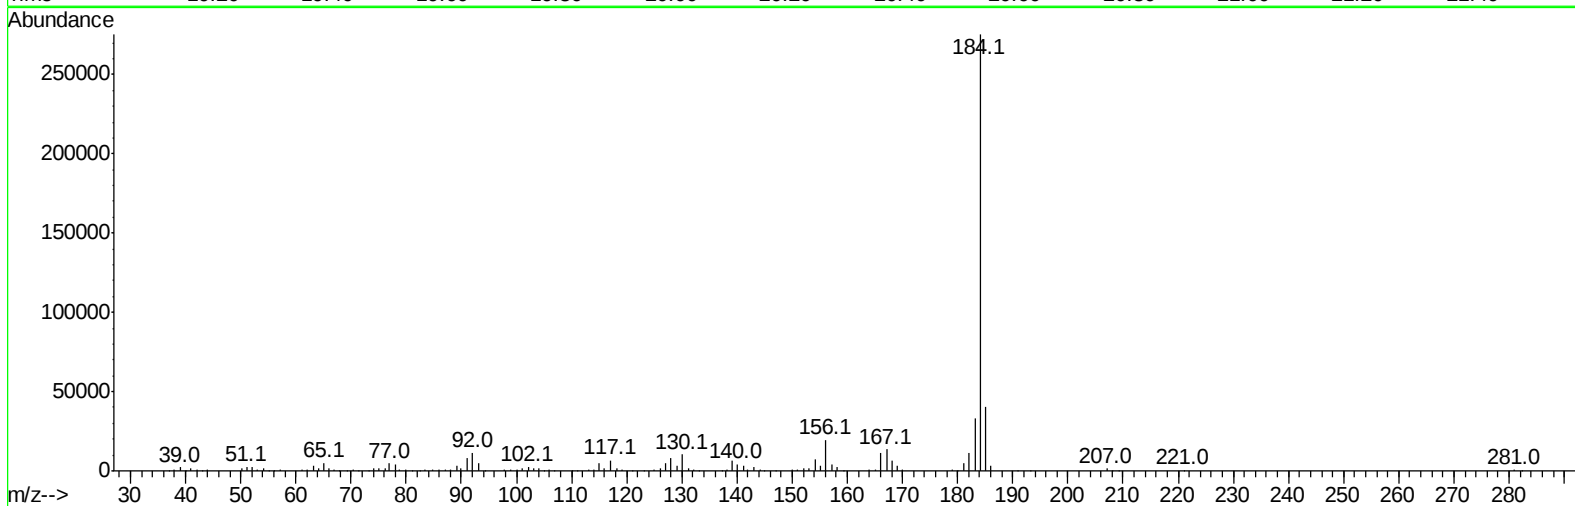


Data Path : U:\HPCHEM1\BNA G\DATA\BG011218\
Data File : BG031995.D
Acq On : 12 Jan 2018 10:34
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 13 05:49:25 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 12 17:27:17 2018
Response via : Initial Calibration

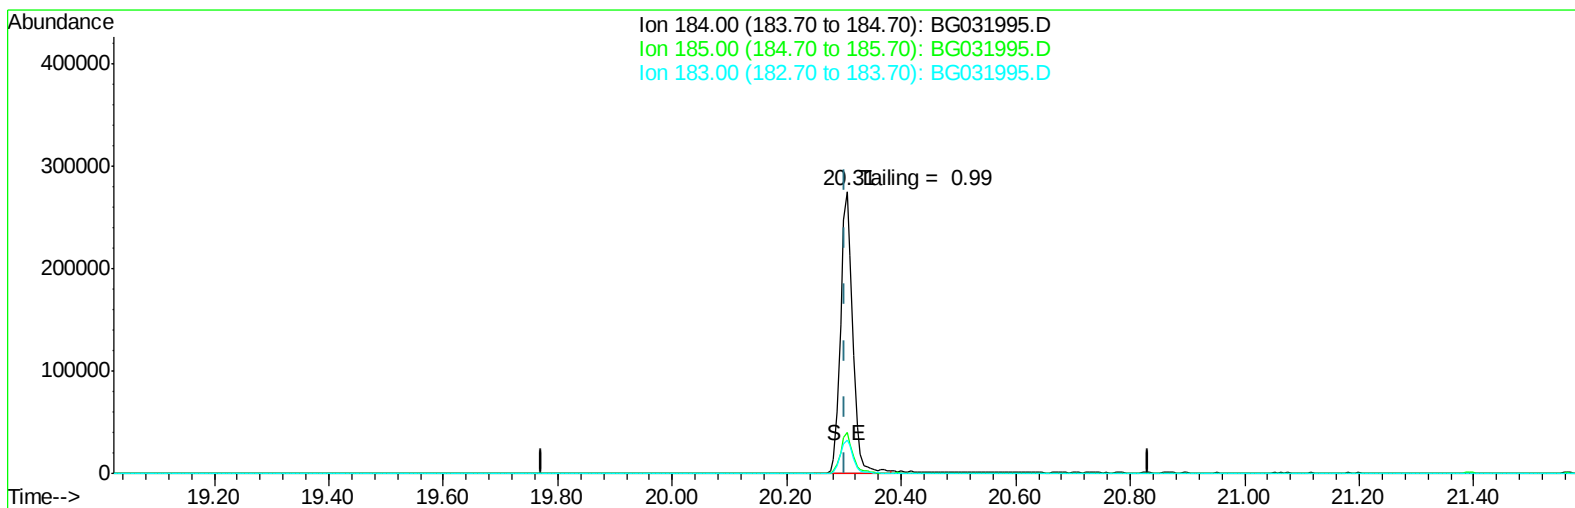

TIC: BG031995.D

(76) Benzidine



20.305min (+0.003) 5939.96ng

response 417237

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.65
183.00	13.30	12.02
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA G\DATA\BG011218\
Data File : BG031995.D
Acq On : 12 Jan 2018 10:34
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 13 05:49:25 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 12 17:27:17 2018
Response via : Initial Calibration

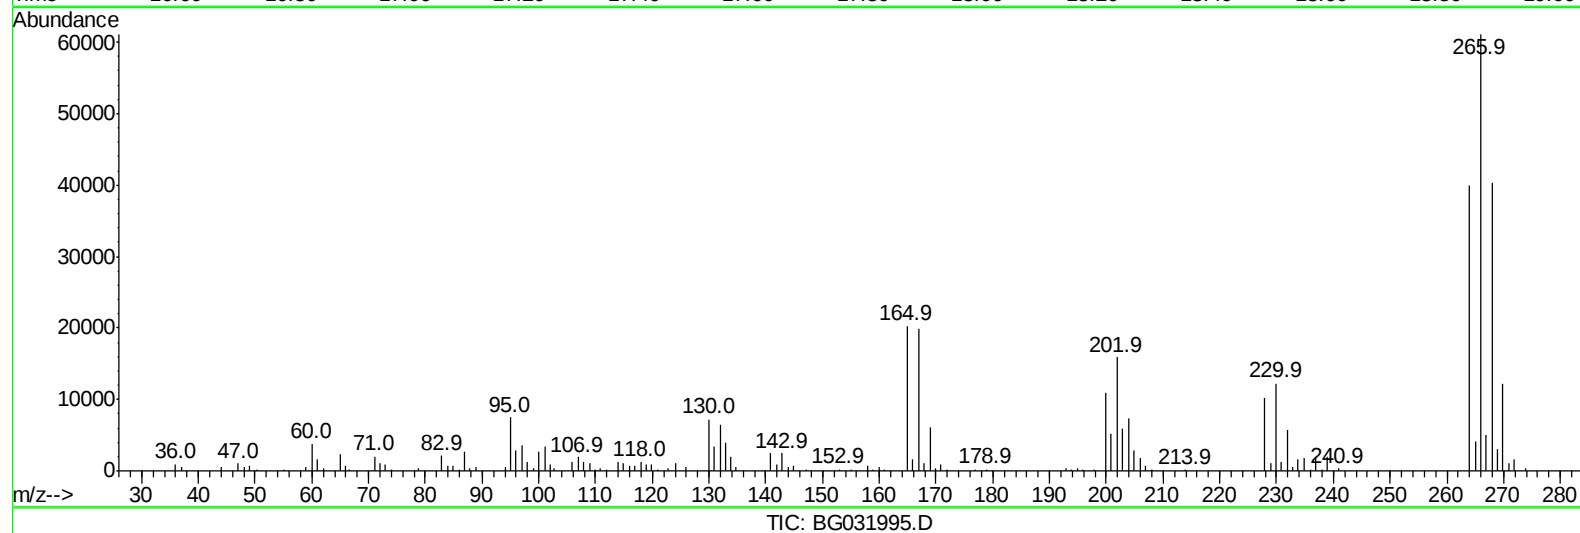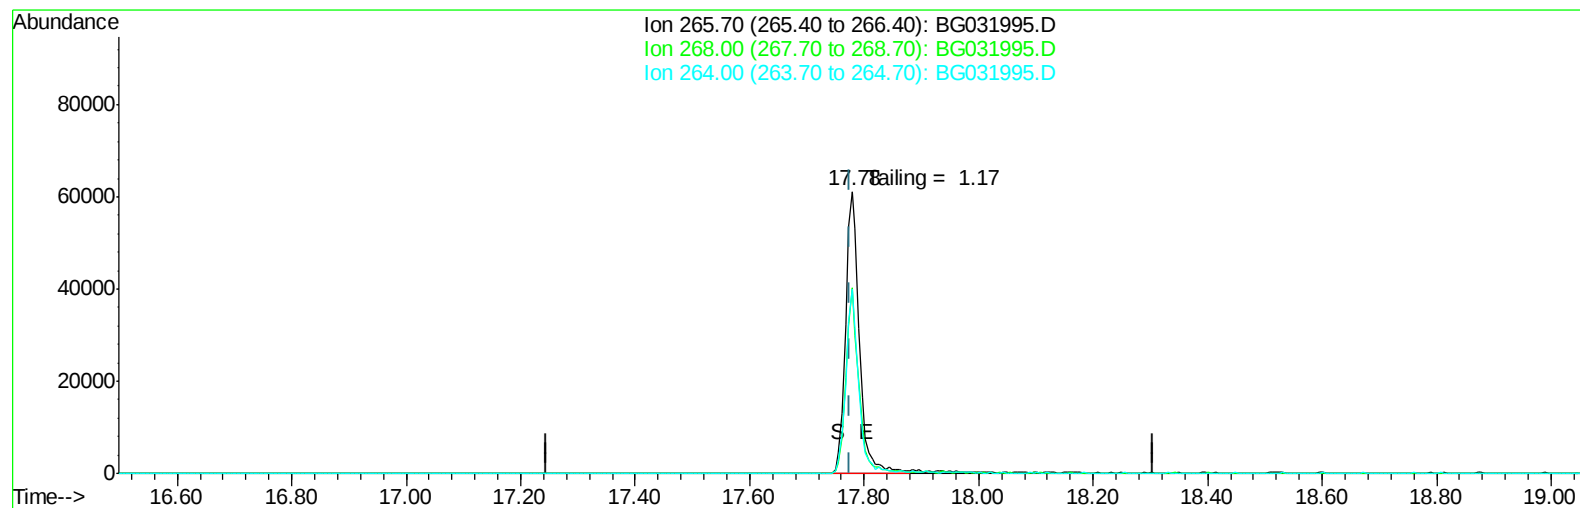

(69) Pentachlorophenol (C)

17.779min (+0.003) 25724.97ng

response 103275

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.12
264.00	62.00	65.49
0.00	0.00	0.00