
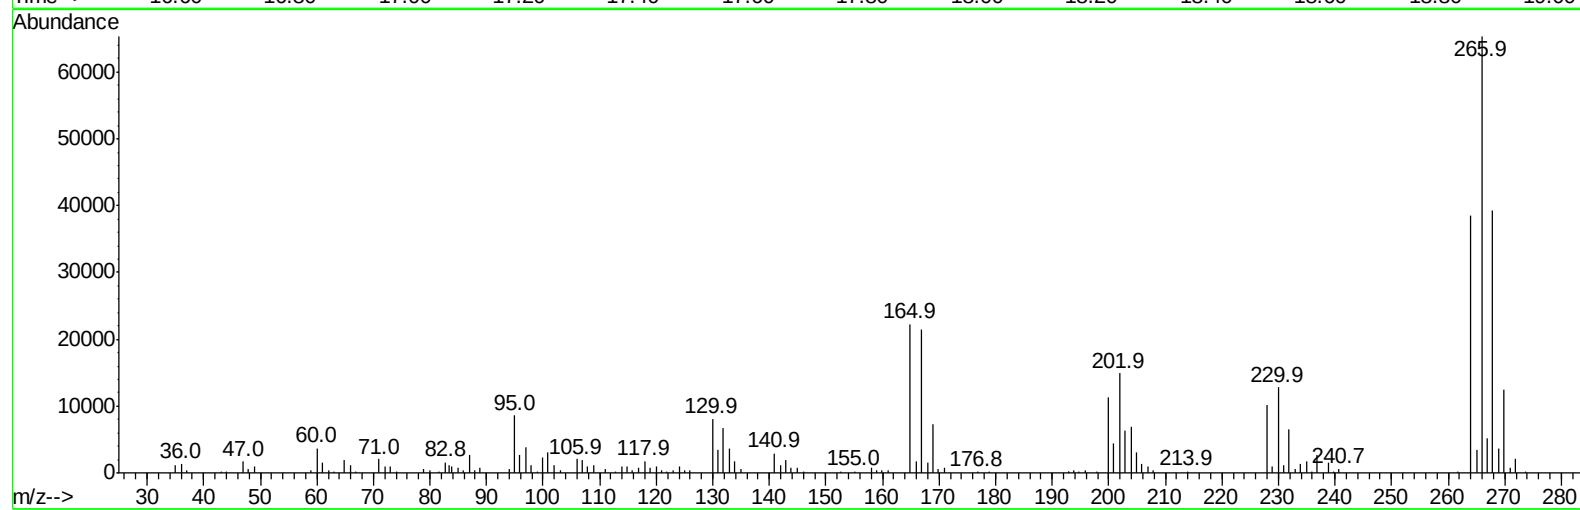


Data Path : U:\HPCHEM1\BNA G\DATA\BG011218\
Data File : BG032023.D
Acq On : 13 Jan 2018 4:11
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 13 05:52:54 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 12 17:27:17 2018
Response via : Initial Calibration

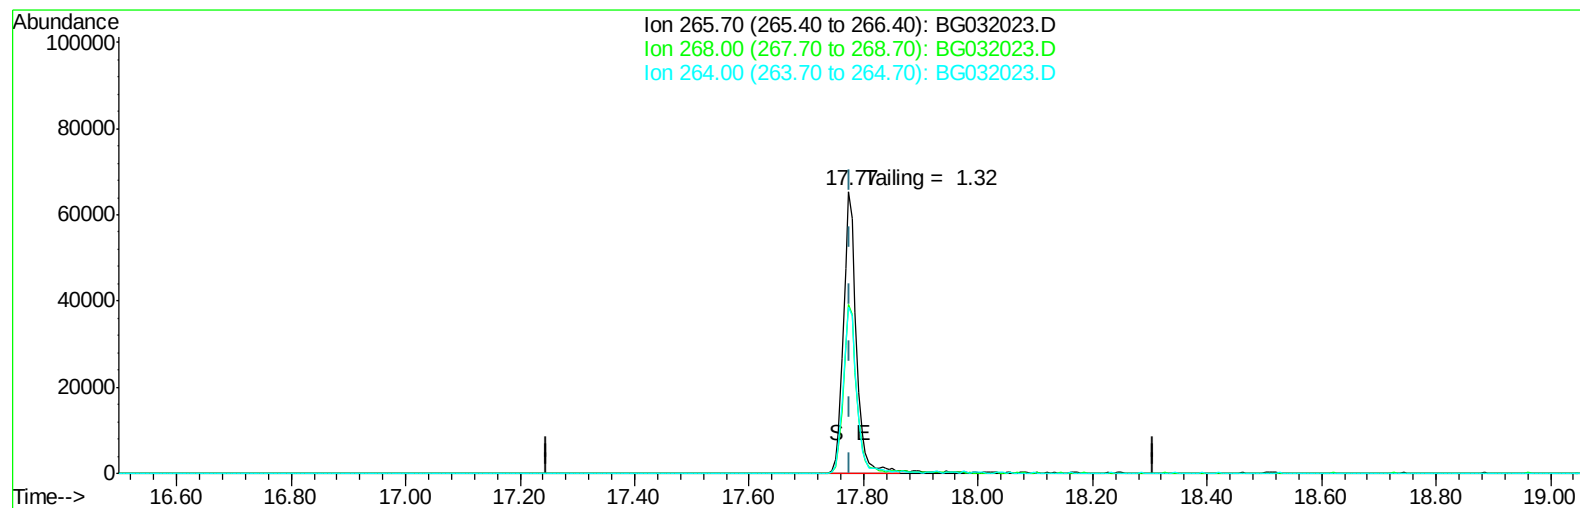

TIC: BG032023.D

(69) Pentachlorophenol (C)



17.774min (-0.002) 21762.70ng

response 101820

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.18
264.00	62.00	58.98
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA G\DATA\BG011218\
Data File : BG032023.D
Acq On : 13 Jan 2018 4:11
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 13 05:52:54 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 12 17:27:17 2018
Response via : Initial Calibration

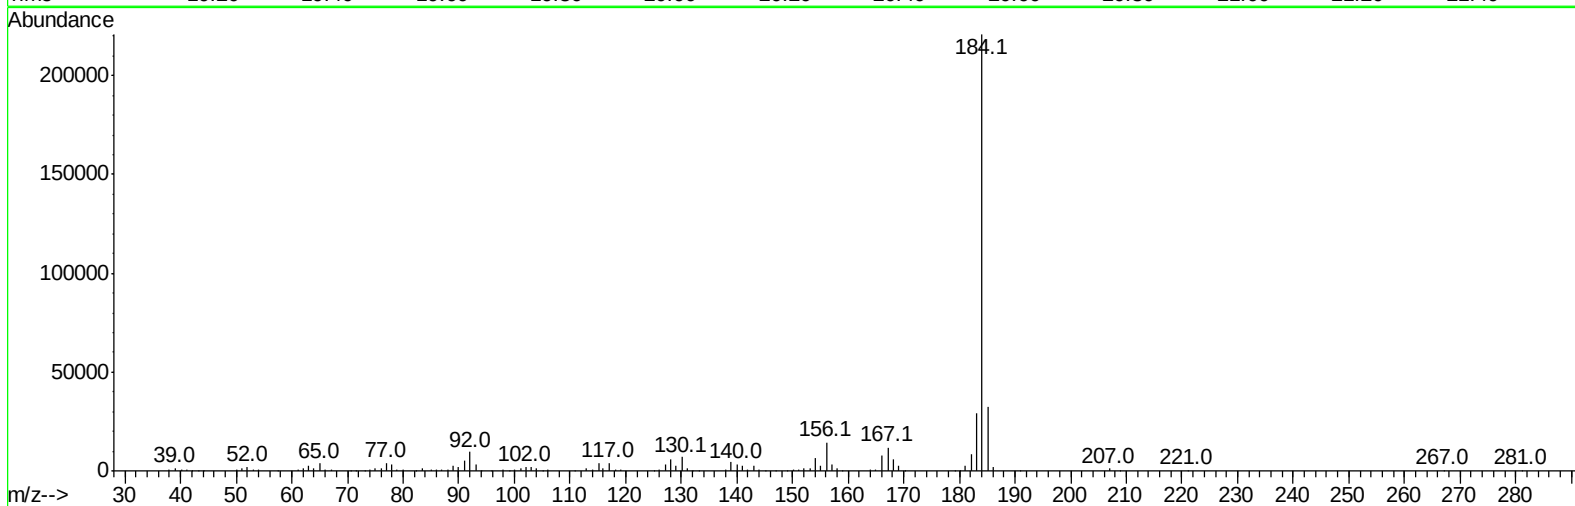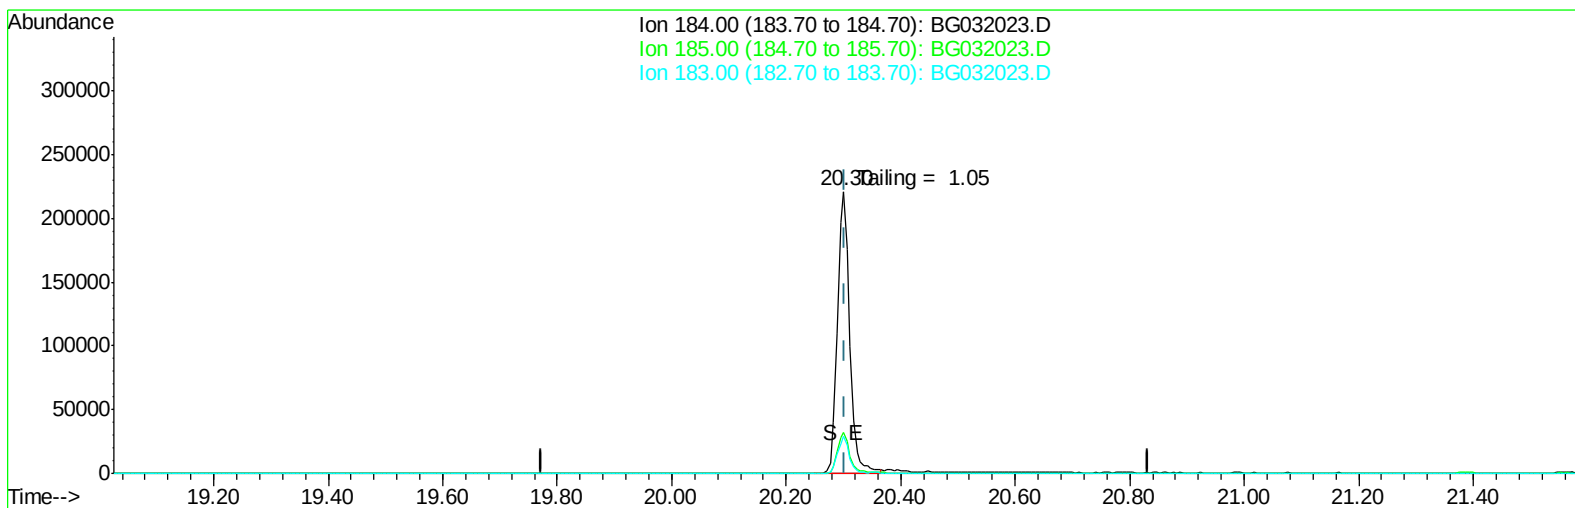

TIC: BG032023.D

(76) Benzidine

20.300min (-0.002) 52693.37ng

response 341274

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.63
183.00	13.30	13.19
0.00	0.00	0.00