


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_G\Data\BG011218\
 Data File : BG031995.D
 Acq On : 12 Jan 2018 10:34
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG011218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 15 10:05:15 2018

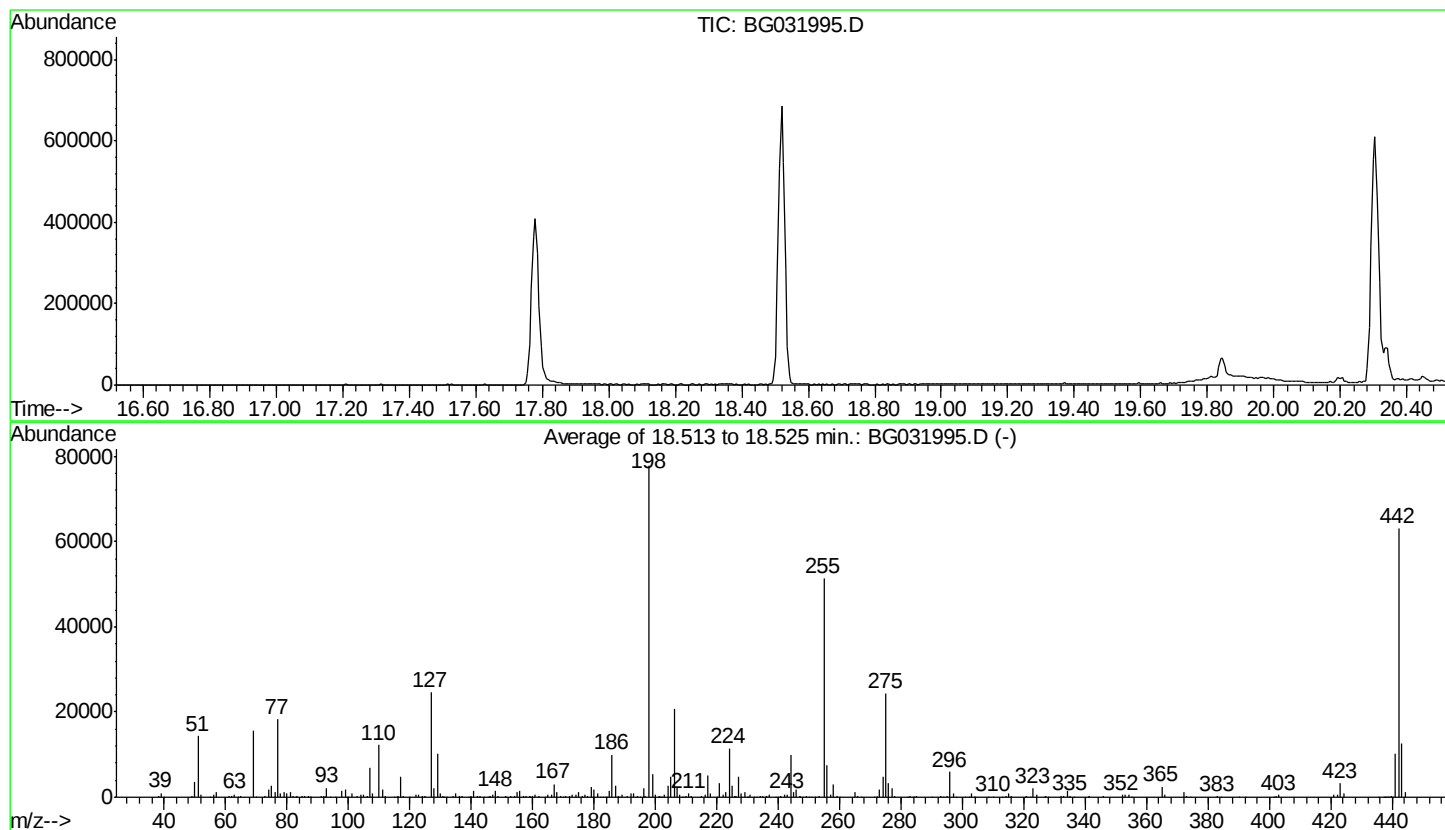

AutoFind: Scans 2591, 2592, 2593; Background Corrected with Scan 2584

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	18.4	14354	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	20.2	15755	PASS
70	69	0.00	2	0.5	75	PASS
127	198	10	80	31.5	24512	PASS
197	198	0.00	2	0.3	213	PASS
198	198	100	100	100.0	77848	PASS
199	198	5	9	7.0	5463	PASS
275	198	10	60	31.2	24312	PASS
365	198	1	100	3.1	2428	PASS
441	442	0.01	24	16.3	10309	PASS
442	198	50	100	81.0	63090	PASS
443	442	15	24	20.2	12755	PASS