


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_G\Data\BG011218\
 Data File : BG032004.D
 Acq On : 12 Jan 2018 16:14
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG011218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 15 10:05:15 2018

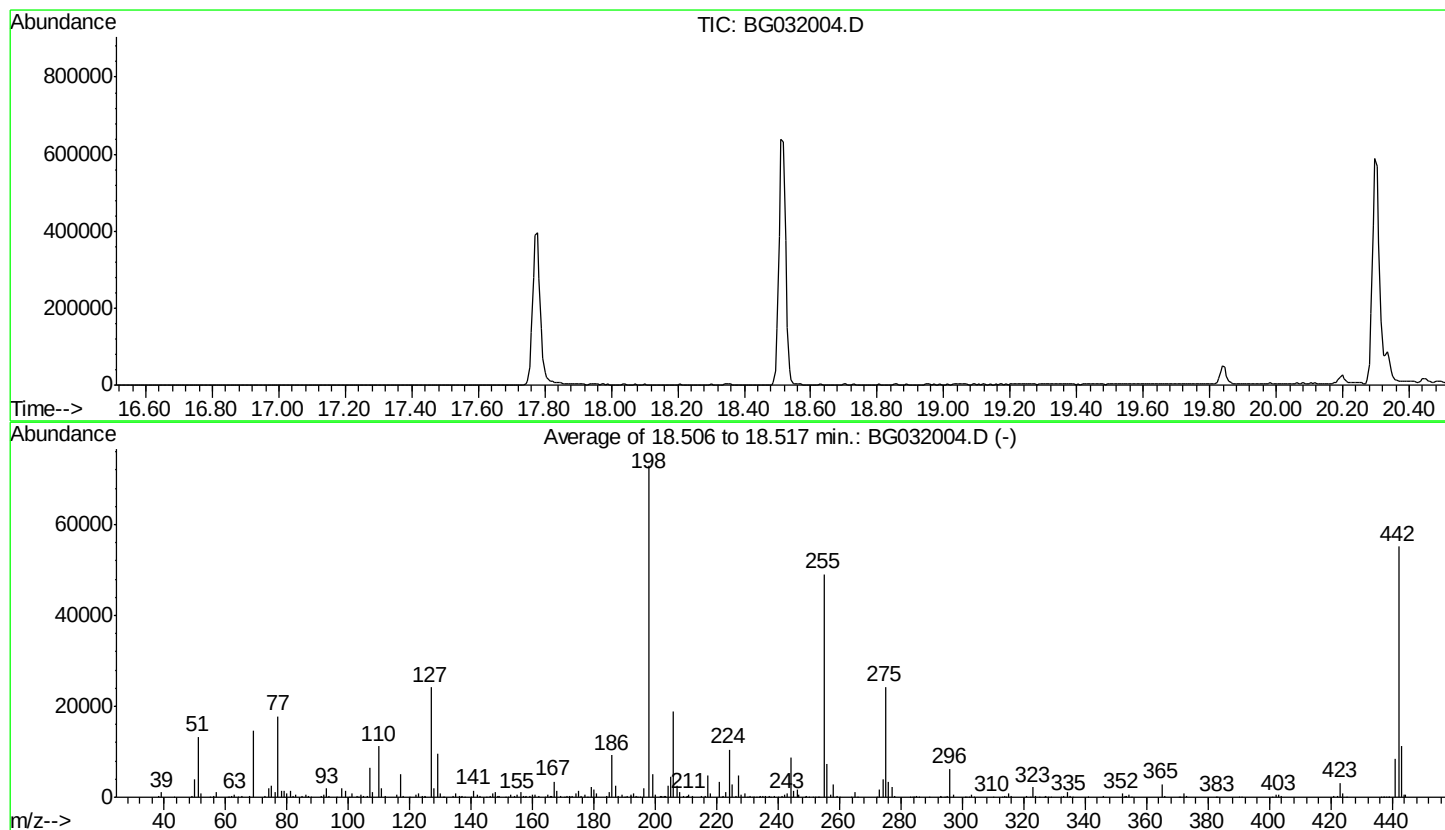

AutoFind: Scans 2590, 2591, 2592; Background Corrected with Scan 2583

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	18.3	13324	PASS
68	69	0.00	2	1.4	212	PASS
69	198	0.00	100	20.1	14662	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	33.0	24098	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	72981	PASS
199	198	5	9	6.9	5040	PASS
275	198	10	60	33.3	24277	PASS
365	198	1	100	3.9	2832	PASS
441	442	0.01	24	15.2	8401	PASS
442	198	50	100	75.5	55093	PASS
443	442	15	24	20.3	11199	PASS