




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011222\
 Data File : BG051948.D
 Acq On : 12 Jan 2022 16:35
 Operator : CG/JU
 Sample : N1100-10
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLP1

Manual IntegrationsAPPROVED

Quant Time: Jan 12 23:54:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 06 14:43:02 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/13/2022
 Supervised By :mohammad ahmed 01/18/2022

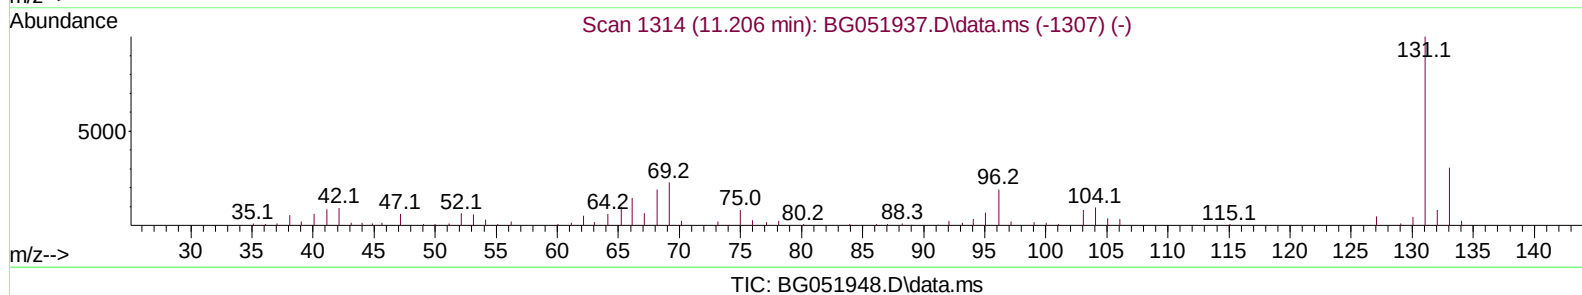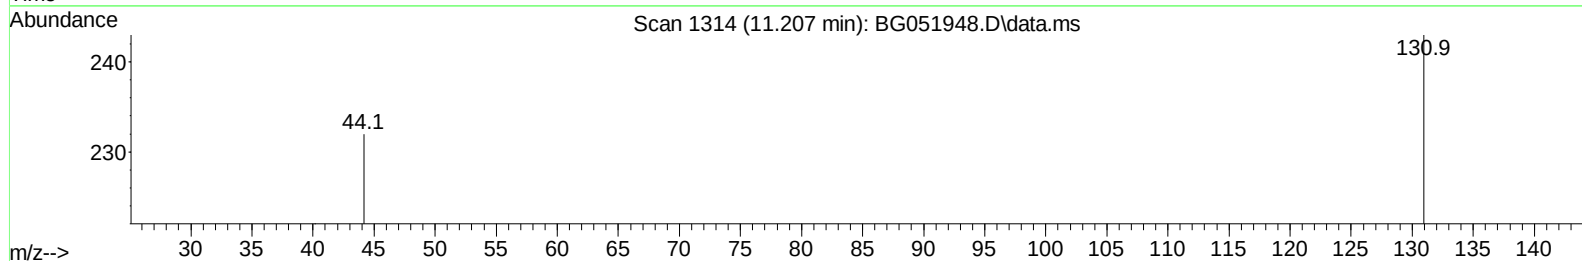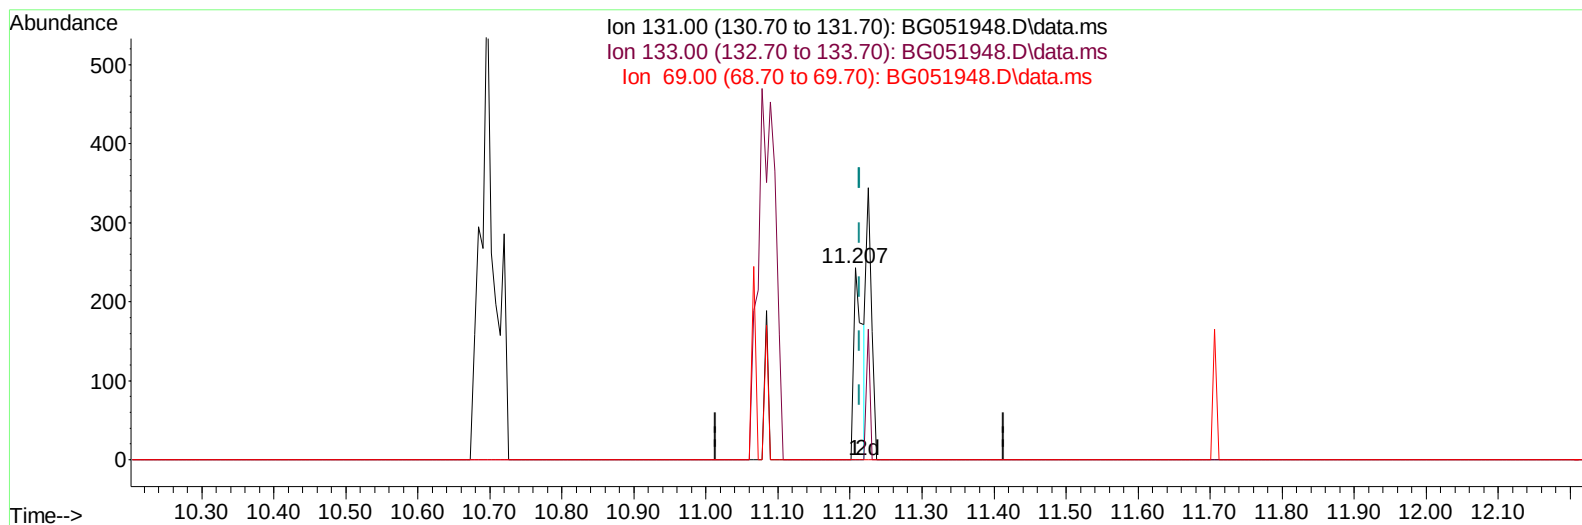

(31) 4-Chloroaniline-d4 (S)

11.207min (-0.006) 0.09 ng/ul

response 207

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	33.20	0.00#
69.00	21.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011222\
 Data File : BG051948.D
 Acq On : 12 Jan 2022 16:35
 Operator : CG/JU
 Sample : N1100-10
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLP1

Manual IntegrationsAPPROVED

Quant Time: Jan 12 23:54:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 06 14:43:02 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/13/2022
 Supervised By :mohammad ahmed 01/18/2022

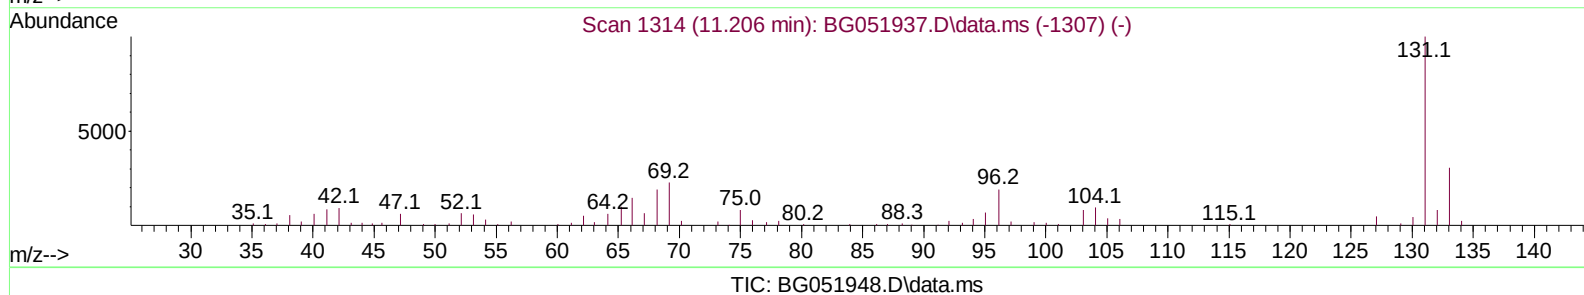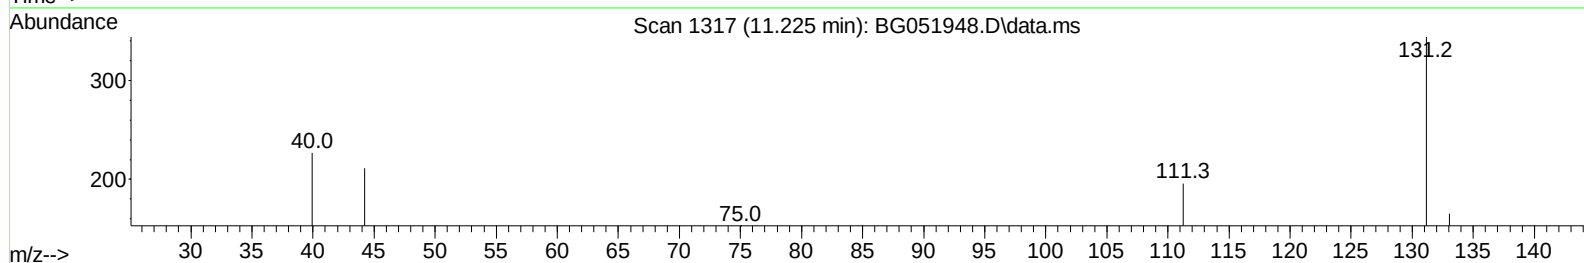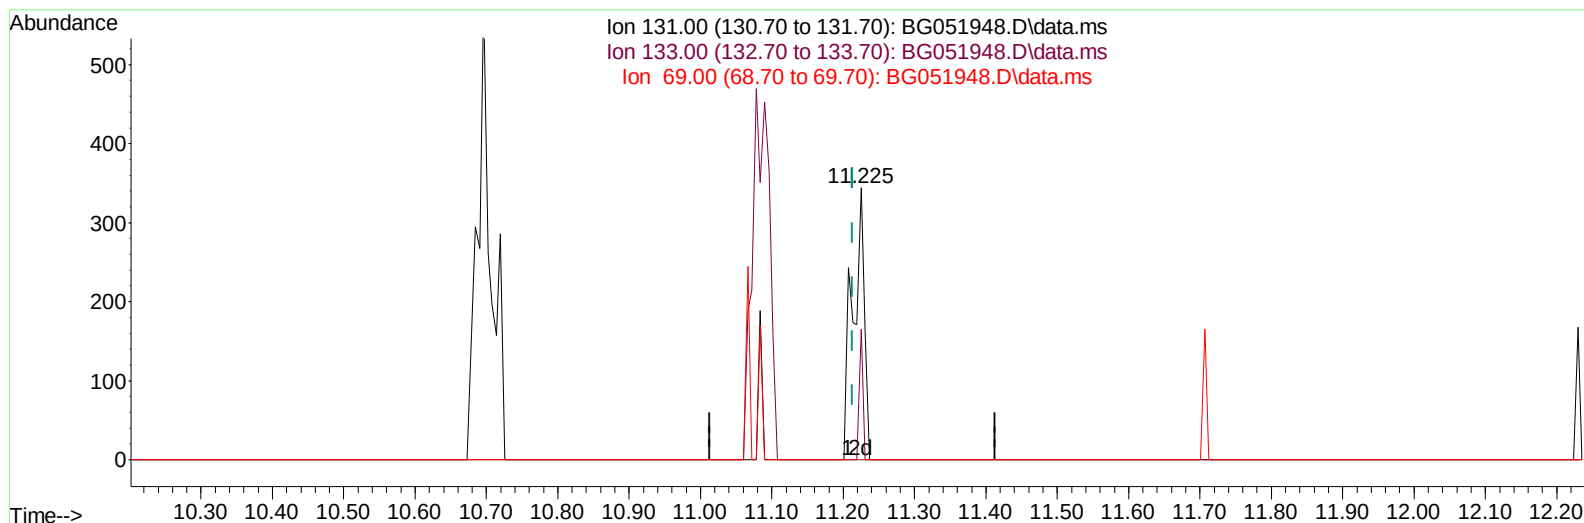

(31) 4-Chloroaniline-d4 (S)

11.225min (+ 0.011) 0.17 ng/ul m

response 385

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	33.20	47.97#
69.00	21.30	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011222\
 Data File : BG051948.D
 Acq On : 12 Jan 2022 16:35
 Operator : CG/JU
 Sample : N1100-10
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLP1

Manual IntegrationsAPPROVED

Quant Time: Jan 12 23:54:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 06 14:43:02 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/13/2022
 Supervised By :mohammad ahmed 01/18/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.247	152	22849	20.000	ng/ul	0.00
20) Naphthalene-d8	11.084	136	94131	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.891	164	70080	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.634	188	186833	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.957	240	190814	20.000	ng/ul	# 0.00
88) Perylene-d12	25.441	264	184813	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.571	96	1743	2.726	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.383	99	41517	18.565	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.548	67	30123	21.219	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.771	132	28020	18.924	ng/ul	0.00
15) 4-Methylphenol-d8	8.946	113	33318	19.166	ng/ul	0.00
21) Nitrobenzene-d5	9.416	128	18726	25.176	ng/ul	0.00
24) 2-Nitrophenol-d4	10.144	143	6143	7.468	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.696	165	26026	16.186	ng/ul	0.00
31) 4-Chloroaniline-d4	11.225	131	385m	0.172	ng/ul	0.01
46) Dimethylphthalate-d6	14.274	166	64760	11.180	ng/ul	0.00
49) Acenaphthylene-d8	14.585	160	163022	23.298	ng/ul	0.00
54) 4-Nitrophenol-d4	15.073	143	2624	2.709	ng/ul	0.00
60) Fluorene-d10	15.877	176	121979	24.152	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0	0.000	ng/ul	
73) Anthracene-d10	17.734	188	214081	24.155	ng/ul	0.00
81) Pyrene-d10	20.013	212	276731	25.199	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.194	264	229027	23.540	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011222\
Data File : BG051948.D
Acq On : 12 Jan 2022 16:35
Operator : CG/JU
Sample : N1100-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLP1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/13/2022
Supervised By :mohammad ahmed 01/18/2022

Quant Time: Jan 12 23:54:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 06 14:43:02 2022
Response via : Initial Calibration

