

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011222\
 Data File : BG051938.D
 Acq On : 12 Jan 2022 10:15
 Operator : CG/JU
 Sample : PB141968BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK968

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051938.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.576	9	15	20	rBV3	7473	11839	1.43%	0.152%
2	3.793	48	52	55	rBV2	970	1515	0.18%	0.019%
3	3.923	72	74	78	rBV4	1466	2028	0.24%	0.026%
4	3.999	83	87	101	rVV	87045	148325	17.88%	1.905%
5	4.351	144	147	154	rBV4	1789	3434	0.41%	0.044%
6	4.645	194	197	200	rBV	942	1265	0.15%	0.016%
7	4.692	200	205	210	rVB	1109	1206	0.15%	0.015%
8	7.383	657	663	672	rVB2	102774	178608	21.53%	2.294%
9	7.459	672	676	681	rBV2	764	1427	0.17%	0.018%
10	7.553	685	692	702	rVB	70824	122186	14.73%	1.569%
11	7.770	722	729	737	rBV	91194	160144	19.30%	2.057%
12	8.135	787	791	795	rBV	890	1509	0.18%	0.019%
13	8.246	804	810	819	rVB	89027	147359	17.76%	1.893%
14	8.945	923	929	939	rBV	113757	201121	24.24%	2.583%
15	9.415	1002	1009	1017	rVV	97800	169745	20.46%	2.180%
16	10.150	1125	1134	1142	rVV2	77687	140340	16.92%	1.803%
17	10.696	1220	1227	1235	rVV	115228	204119	24.61%	2.622%
18	10.749	1235	1236	1241	rVB2	1113	1176	0.14%	0.015%
19	11.084	1285	1293	1300	rBV	118990	209628	25.27%	2.692%
20	11.207	1307	1314	1326	rBV	118209	216292	26.07%	2.778%
21	12.670	1556	1563	1566	rVB3	1516	2851	0.34%	0.037%
22	14.279	1830	1837	1843	rBV	252253	361727	43.60%	4.646%
23	14.414	1854	1860	1862	rBV2	776	1277	0.15%	0.016%
24	14.585	1882	1889	1898	rVB	261107	406174	48.96%	5.217%
25	14.890	1933	1941	1948	rBV	199476	314912	37.96%	4.045%
26	15.061	1963	1970	1982	rBV	100710	177217	21.36%	2.276%
27	15.201	1993	1994	1998	rBV3	1184	1412	0.17%	0.018%
28	15.877	2102	2109	2119	rVB2	343974	522597	63.00%	6.712%
29	15.983	2121	2127	2135	rBV	84516	126606	15.26%	1.626%
30	16.124	2145	2151	2154	rVB2	1042	1941	0.23%	0.025%
31	17.005	2299	2301	2306	rVB2	996	1592	0.19%	0.020%
32	17.557	2391	2395	2396	rBV2	968	1185	0.14%	0.015%
33	17.633	2402	2408	2416	rVV	302844	459537	55.39%	5.902%
34	17.733	2419	2425	2434	rVV	422859	645792	77.85%	8.295%
35	18.644	2577	2580	2584	rVB5	835	1275	0.15%	0.016%
36	19.055	2647	2650	2652	rBV2	1221	1735	0.21%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011222\
 Data File : BG051938.D
 Acq On : 12 Jan 2022 10:15
 Operator : CG/JU
 Sample : PB141968BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK968

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	19.178	2668	2671	2674	rVB3	1362	1587	0.19%	0.020%
38	19.243	2681	2682	2685	rVB	2010	1206	0.15%	0.015%
39	19.272	2685	2687	2689	rBV2	1096	1286	0.16%	0.017%
40	19.578	2734	2739	2745	rBV5	6084	10124	1.22%	0.130%

41	19.654	2748	2752	2757	rVB3	4899	7394	0.89%	0.095%
42	19.860	2783	2787	2789	rBV3	1144	1297	0.16%	0.017%
43	20.013	2806	2813	2821	rBV	580320	829583	100.00%	10.655%
44	20.124	2830	2832	2833	rVB2	2059	1443	0.17%	0.019%
45	20.142	2833	2835	2837	rBV2	1828	2316	0.28%	0.030%

46	20.359	2869	2872	2874	rVB4	1816	1648	0.20%	0.021%
47	20.565	2905	2907	2910	rBV4	2098	2415	0.29%	0.031%
48	20.665	2921	2924	2925	rBV2	2428	1735	0.21%	0.022%
49	20.682	2925	2927	2930	rBV4	2582	2036	0.25%	0.026%
50	20.741	2934	2937	2938	rBV3	2510	3094	0.37%	0.040%

51	20.765	2940	2941	2943	rBV2	2841	2455	0.30%	0.032%
52	20.859	2955	2957	2959	rBV3	2227	1573	0.19%	0.020%
53	20.906	2963	2965	2966	rBV2	2153	1530	0.18%	0.020%
54	21.129	3001	3003	3006	rBV4	2288	3298	0.40%	0.042%
55	21.287	3028	3030	3032	rVB3	2199	1379	0.17%	0.018%

56	21.469	3059	3061	3063	rBV2	2581	1968	0.24%	0.025%
57	21.881	3129	3131	3132	rBV2	3758	2825	0.34%	0.036%
58	21.957	3137	3144	3151	rVV	319615	545252	65.73%	7.003%
59	22.110	3168	3170	3171	rVB	3507	1529	0.18%	0.020%
60	22.486	3232	3234	3238	rBV5	3472	4868	0.59%	0.063%

61	23.032	3325	3327	3330	rBV3	3078	2685	0.32%	0.034%
62	23.155	3345	3348	3351	rBV5	3921	5307	0.64%	0.068%
63	23.220	3357	3359	3360	rVB2	3670	1727	0.21%	0.022%
64	23.749	3447	3449	3450	rBV2	3931	2220	0.27%	0.029%
65	23.784	3453	3455	3456	rBV2	3072	1912	0.23%	0.025%

66	24.060	3501	3502	3503	rVB	3552	1252	0.15%	0.016%
67	24.078	3503	3505	3508	rBV4	2235	2123	0.26%	0.027%
68	24.101	3508	3509	3513	rBV3	3043	3402	0.41%	0.044%
69	24.418	3561	3563	3564	rBV	2634	1968	0.24%	0.025%
70	24.436	3564	3566	3567	rBV2	4080	4131	0.50%	0.053%

71	24.683	3605	3608	3610	rBV4	3748	4732	0.57%	0.061%
72	24.888	3641	3643	3647	rBV4	2603	2319	0.28%	0.030%
73	24.924	3647	3649	3654	rBV6	3310	4601	0.55%	0.059%
74	25.200	3685	3696	3709	rVB2	253595	755085	91.02%	9.698%
75	25.341	3718	3720	3721	rVB2	2507	1290	0.16%	0.017%

76	25.441	3726	3737	3754	rVB3	168889	550197	66.32%	7.067%
----	--------	------	------	------	------	--------	--------	--------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011222\
 Data File : BG051938.D
 Acq On : 12 Jan 2022 10:15
 Operator : CG/JU
 Sample : PB141968BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK968

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

77	25.864	3807	3809	3811	rBV3	2705	2609	0.31%	0.034%
78	25.922	3816	3819	3821	rBV4	3112	3344	0.40%	0.043%
79	26.093	3846	3848	3851	rBV4	2375	2025	0.24%	0.026%
80	26.151	3856	3858	3860	rBV3	2494	1749	0.21%	0.022%
81	26.874	3979	3981	3982	rBV2	3029	2192	0.26%	0.028%
82	27.232	4041	4042	4044	rBV2	2928	2641	0.32%	0.034%
83	27.379	4065	4067	4069	rBV3	2681	1349	0.16%	0.017%
84	27.461	4079	4081	4084	rVB3	4452	4005	0.48%	0.051%
85	27.491	4084	4086	4087	rBV2	4252	2397	0.29%	0.031%
86	27.831	4143	4144	4145	rVB	4280	1509	0.18%	0.019%
87	28.560	4266	4268	4271	rVB4	2942	2220	0.27%	0.029%
88	29.006	4343	4344	4346	rBV2	3674	1819	0.22%	0.023%
89	29.165	4369	4371	4374	rBV4	2503	2805	0.34%	0.036%
90	29.324	4396	4398	4400	rBV2	3425	2331	0.28%	0.030%
91	29.512	4428	4430	4431	rBV2	2568	1345	0.16%	0.017%
92	29.588	4440	4443	4445	rBV3	2510	2942	0.35%	0.038%
93	29.899	4494	4496	4498	rBV2	2507	2321	0.28%	0.030%
94	30.034	4517	4519	4520	rBV2	3904	3381	0.41%	0.043%
95	31.004	4682	4684	4685	rBV	2892	2251	0.27%	0.029%
96	31.150	4707	4709	4710	rBV2	3972	2328	0.28%	0.030%
97	31.844	4826	4827	4829	rBV2	2884	2334	0.28%	0.030%
98	32.108	4871	4872	4874	rBV2	2978	2329	0.28%	0.030%
99	32.179	4883	4884	4886	rBV2	3310	1543	0.19%	0.020%
100	32.631	4959	4961	4962	rBV2	2910	2035	0.25%	0.026%




Sum of corrected areas: 7785692

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011222\
Data File : BG051938.D
Acq On : 12 Jan 2022 10:15
Operator : CG/JU
Sample : PB141968BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK968

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

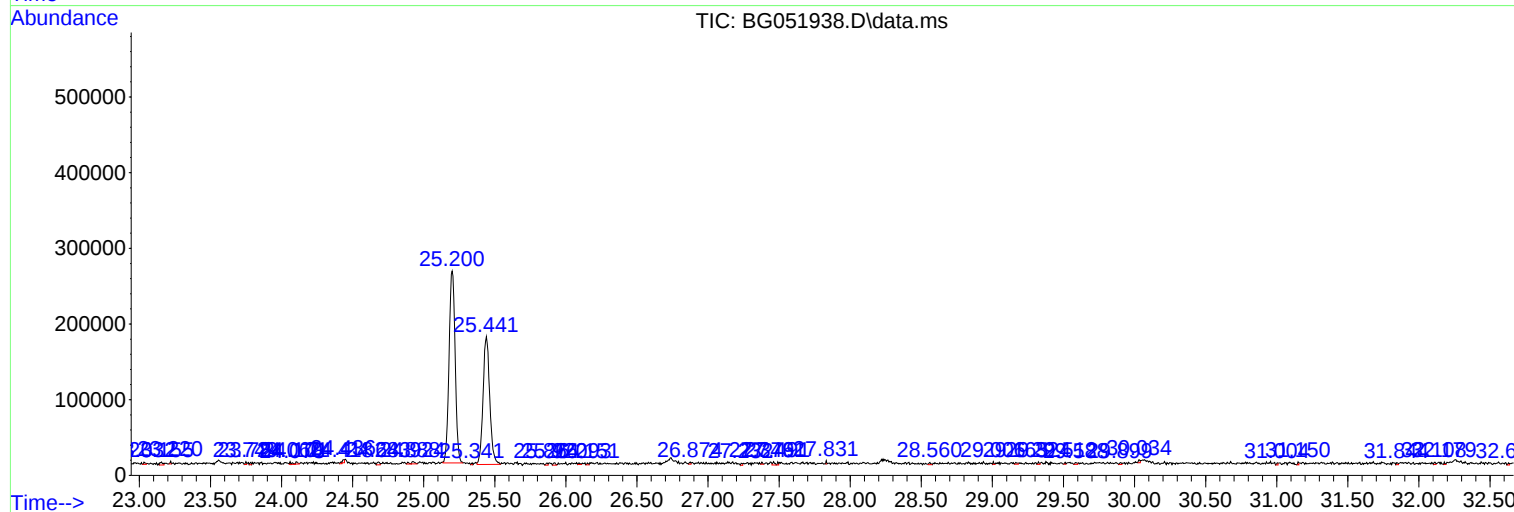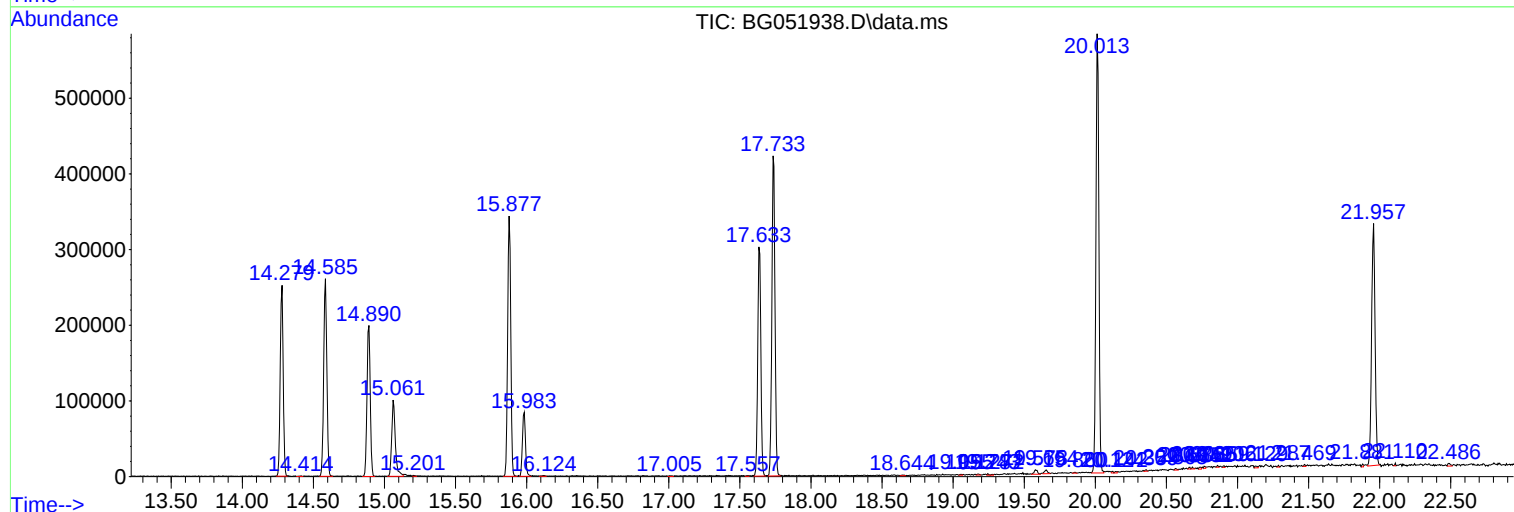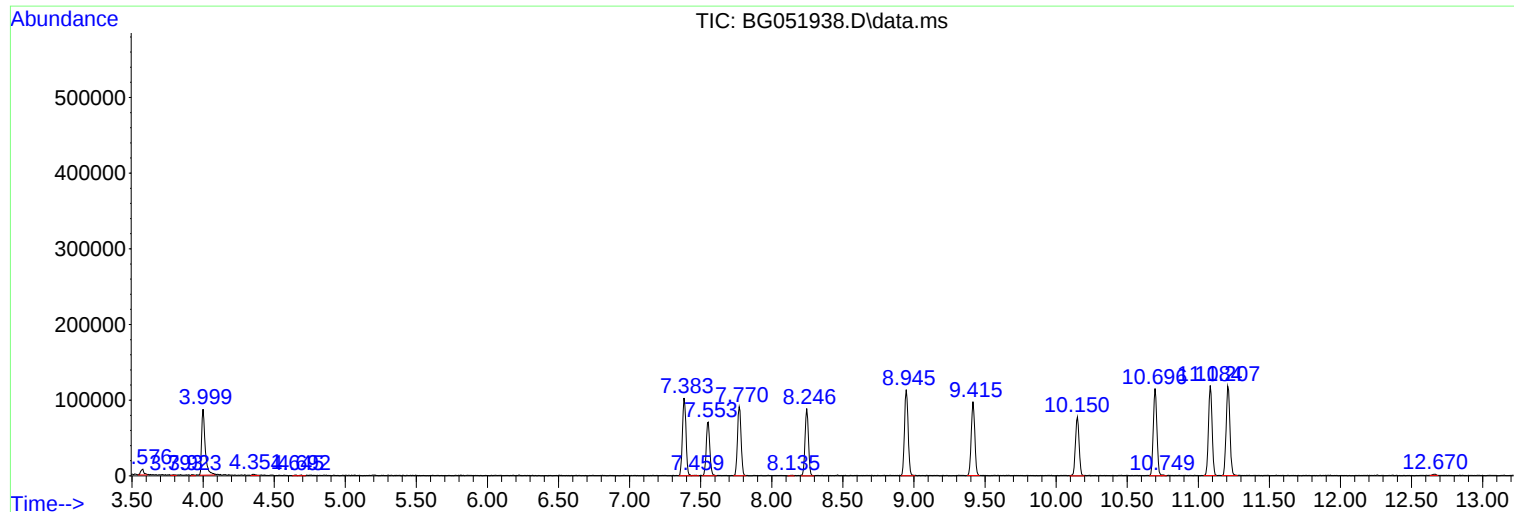

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011222\
Data File : BG051938.D
Acq On : 12 Jan 2022 10:15
Operator : CG/JU
Sample : PB141968BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK968

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011222\
Data File : BG051938.D
Acq On : 12 Jan 2022 10:15
Operator : CG/JU
Sample : PB141968BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK968

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc