

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011222\
 Data File : BG051944.D
 Acq On : 12 Jan 2022 14:04
 Operator : CG/JU
 Sample : N1100-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLN5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051944.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.571	10	14	21	rVB2	6396	10361	1.18%	0.123%
2	3.853	60	62	71	rVB4	1582	3228	0.37%	0.038%
3	4.000	82	87	95	rBV	71060	121994	13.88%	1.449%
4	4.253	127	130	136	rVB4	1907	2867	0.33%	0.034%
5	4.359	144	148	152	rVB2	1617	2545	0.29%	0.030%
6	4.805	219	224	226	rVV2	1231	1249	0.14%	0.015%
7	5.287	303	306	311	rVB	2284	3097	0.35%	0.037%
8	5.528	343	347	351	rBV	742	1266	0.14%	0.015%
9	5.692	370	375	378	rBV	1075	1688	0.19%	0.020%
10	7.214	630	634	636	rBV2	1343	1996	0.23%	0.024%
11	7.255	638	641	647	rVB2	1247	2025	0.23%	0.024%
12	7.384	656	663	672	rBV	111255	195250	22.21%	2.319%
13	7.548	685	691	700	rBV	72675	123829	14.08%	1.471%
14	7.772	722	729	735	rBV	103804	170056	19.34%	2.020%
15	8.242	801	809	816	rBV	81247	138334	15.73%	1.643%
16	8.294	816	818	823	rVB3	1859	2391	0.27%	0.028%
17	8.794	898	903	906	rBV	880	1310	0.15%	0.016%
18	8.946	922	929	938	rBV	133985	230892	26.26%	2.742%
19	9.082	948	952	955	rBV3	1031	1601	0.18%	0.019%
20	9.416	1001	1009	1017	rBV	99646	180165	20.49%	2.140%
21	9.487	1017	1021	1024	rVB3	1530	1748	0.20%	0.021%
22	10.145	1126	1133	1141	rBV	85518	154150	17.53%	1.831%
23	10.697	1218	1227	1236	rBV	128931	228738	26.02%	2.716%
24	10.832	1242	1250	1257	rBV2	60969	103036	11.72%	1.224%
25	11.085	1286	1293	1300	rBV	116646	199634	22.71%	2.371%
26	11.138	1300	1302	1307	rVV2	2287	2501	0.28%	0.030%
27	11.208	1307	1314	1326	rVB	128105	234848	26.71%	2.789%
28	12.665	1556	1562	1565	rVB3	2214	3554	0.40%	0.042%
29	12.730	1568	1573	1582	rVB2	7582	12716	1.45%	0.151%
30	12.953	1606	1611	1615	rVB3	3006	4740	0.54%	0.056%
31	13.493	1698	1703	1706	rVB3	2804	3163	0.36%	0.038%
32	14.087	1800	1804	1808	rVV2	1271	2214	0.25%	0.026%
33	14.204	1821	1824	1828	rVV	996	1336	0.15%	0.016%
34	14.275	1828	1836	1843	rVV	266680	387784	44.10%	4.605%
35	14.586	1882	1889	1899	rVB	284361	451857	51.39%	5.366%
36	14.762	1918	1919	1924	rVB3	2029	1658	0.19%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011222\
 Data File : BG051944.D
 Acq On : 12 Jan 2022 14:04
 Operator : CG/JU
 Sample : N1100-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLN5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	14.891	1934	1941	1948	rVV	192471	313248	35.63%	3.720%
38	15.062	1961	1970	1982	rBV	141113	245250	27.89%	2.912%
39	15.138	1982	1983	1989	rVB4	1862	2132	0.24%	0.025%
40	15.279	2006	2007	2011	rVV3	1816	1799	0.20%	0.021%
41	15.338	2014	2017	2021	rVB	1235	1814	0.21%	0.022%
42	15.673	2069	2074	2077	rBV2	3068	4373	0.50%	0.052%
43	15.714	2079	2081	2087	rVB3	1438	1654	0.19%	0.020%
44	15.878	2102	2109	2116	rBV	378195	573416	65.22%	6.810%
45	15.984	2121	2127	2136	rVB	112294	171629	19.52%	2.038%
46	16.119	2148	2150	2153	rVV	1775	2151	0.24%	0.026%
47	16.272	2172	2176	2180	rBV4	2598	4044	0.46%	0.048%
48	16.313	2180	2183	2188	rBV3	1799	2401	0.27%	0.029%
49	16.548	2220	2223	2226	rBV	1327	1617	0.18%	0.019%
50	16.571	2226	2227	2230	rVV2	2290	2040	0.23%	0.024%
51	16.601	2230	2232	2235	rVB3	2062	1779	0.20%	0.021%
52	16.701	2246	2249	2252	rBV2	1018	1380	0.16%	0.016%
53	16.754	2252	2258	2259	rBV4	1466	1584	0.18%	0.019%
54	17.094	2315	2316	2321	rBV2	803	1478	0.17%	0.018%
55	17.147	2323	2325	2328	rVV2	1329	1768	0.20%	0.021%
56	17.182	2328	2331	2333	rVV2	1204	1545	0.18%	0.018%
57	17.253	2337	2343	2346	rVV4	1395	3077	0.35%	0.037%
58	17.329	2353	2356	2358	rBV3	2127	1504	0.17%	0.018%
59	17.370	2361	2363	2367	rVV3	2453	3041	0.35%	0.036%
60	17.417	2367	2371	2372	rVV3	2221	2497	0.28%	0.030%
61	17.429	2372	2373	2376	rVV2	2740	2227	0.25%	0.026%
62	17.458	2376	2378	2381	rVV3	1679	1469	0.17%	0.017%
63	17.523	2384	2389	2395	rBV6	3287	5520	0.63%	0.066%
64	17.635	2402	2408	2415	rVV	309053	479763	54.57%	5.697%
65	17.735	2419	2425	2432	rVV2	465152	724477	82.40%	8.604%
66	17.811	2435	2438	2443	rVB6	6660	8350	0.95%	0.099%
67	18.005	2469	2471	2473	rVV2	2661	1303	0.15%	0.015%
68	18.034	2473	2476	2481	rVB4	2132	2934	0.33%	0.035%
69	18.111	2487	2489	2493	rVB2	2687	2303	0.26%	0.027%
70	18.146	2493	2495	2497	rBV3	1679	1699	0.19%	0.020%
71	18.281	2514	2518	2522	rVV3	9338	12420	1.41%	0.147%
72	18.457	2546	2548	2551	rVB4	1770	1767	0.20%	0.021%
73	18.504	2551	2556	2561	rBV6	11132	17023	1.94%	0.202%
74	18.686	2583	2587	2589	rBV4	1226	1625	0.18%	0.019%
75	18.721	2591	2593	2594	rBV2	2378	1353	0.15%	0.016%
76	18.768	2600	2601	2602	rBV	2214	1371	0.16%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011222\
 Data File : BG051944.D
 Acq On : 12 Jan 2022 14:04
 Operator : CG/JU
 Sample : N1100-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLN5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

77	18.921	2625	2627	2629	rBV3	1452	1702	0.19%	0.020%
78	18.968	2633	2635	2636	rBV2	1966	1339	0.15%	0.016%
79	19.015	2641	2643	2646	rBV4	1835	1730	0.20%	0.021%
80	19.209	2674	2676	2677	rBV2	1956	1557	0.18%	0.018%
81	19.338	2697	2698	2701	rBV2	2576	1503	0.17%	0.018%
82	19.515	2726	2728	2730	rBV3	2235	2473	0.28%	0.029%
83	19.579	2736	2739	2744	rVB6	8773	12122	1.38%	0.144%
84	19.650	2749	2751	2757	rVB4	7328	10049	1.14%	0.119%
85	20.014	2807	2813	2819	rVB	614914	879233	100.00%	10.441%
86	20.272	2855	2857	2859	rBV3	5442	5372	0.61%	0.064%
87	21.565	3073	3077	3079	rBV5	11452	16515	1.88%	0.196%
88	21.958	3137	3144	3152	rVB	289153	498605	56.71%	5.921%
89	22.687	3266	3268	3272	rBV5	5638	5726	0.65%	0.068%
90	23.409	3389	3391	3392	rBV2	5904	3707	0.42%	0.044%
91	24.702	3609	3611	3612	rBV2	5666	3939	0.45%	0.047%
92	25.207	3686	3697	3710	rVB2	256163	794125	90.32%	9.431%
93	25.448	3727	3738	3751	rVB2	170888	546664	62.18%	6.492%
94	27.609	4105	4106	4109	rBV3	5816	6266	0.71%	0.074%
95	28.244	4212	4214	4216	rBV3	5629	4929	0.56%	0.059%
96	28.773	4302	4304	4306	rBV3	4545	4324	0.49%	0.051%
97	28.914	4326	4328	4329	rBV2	5234	3760	0.43%	0.045%
98	29.765	4471	4473	4474	rBV2	5146	3354	0.38%	0.040%
99	30.594	4612	4614	4616	rBV3	5174	2995	0.34%	0.036%
100	32.180	4882	4884	4886	rBV3	5340	6012	0.68%	0.071%




Sum of corrected areas: 8420647

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011222\
Data File : BG051944.D
Acq On : 12 Jan 2022 14:04
Operator : CG/JU
Sample : N1100-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLN5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

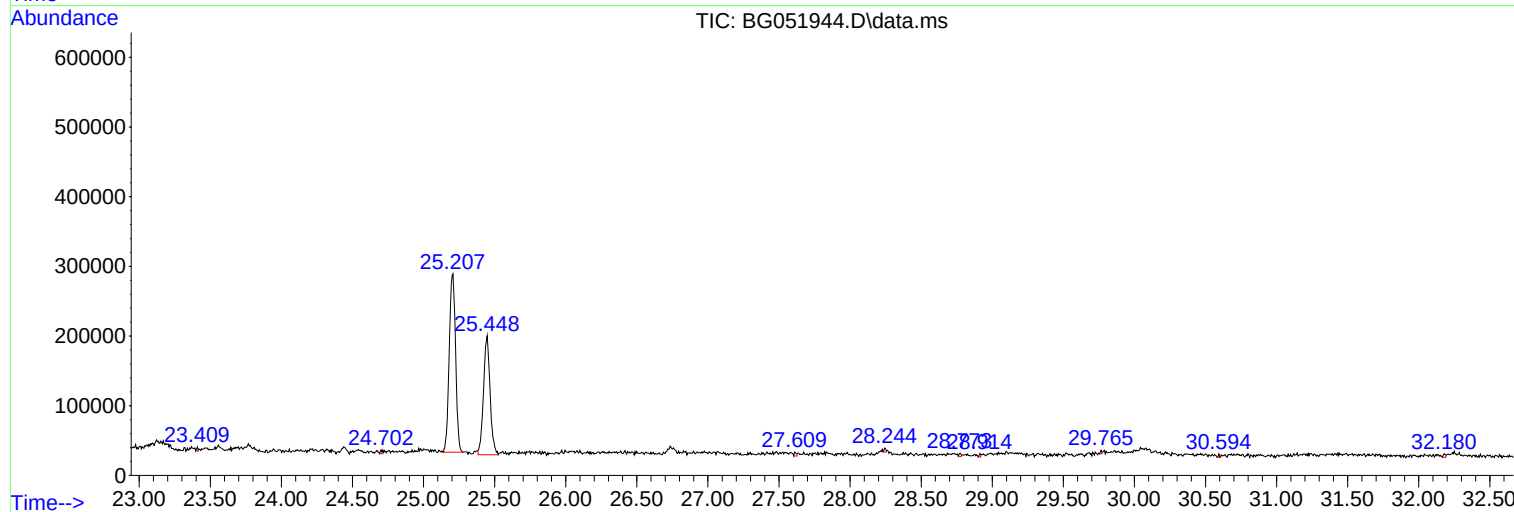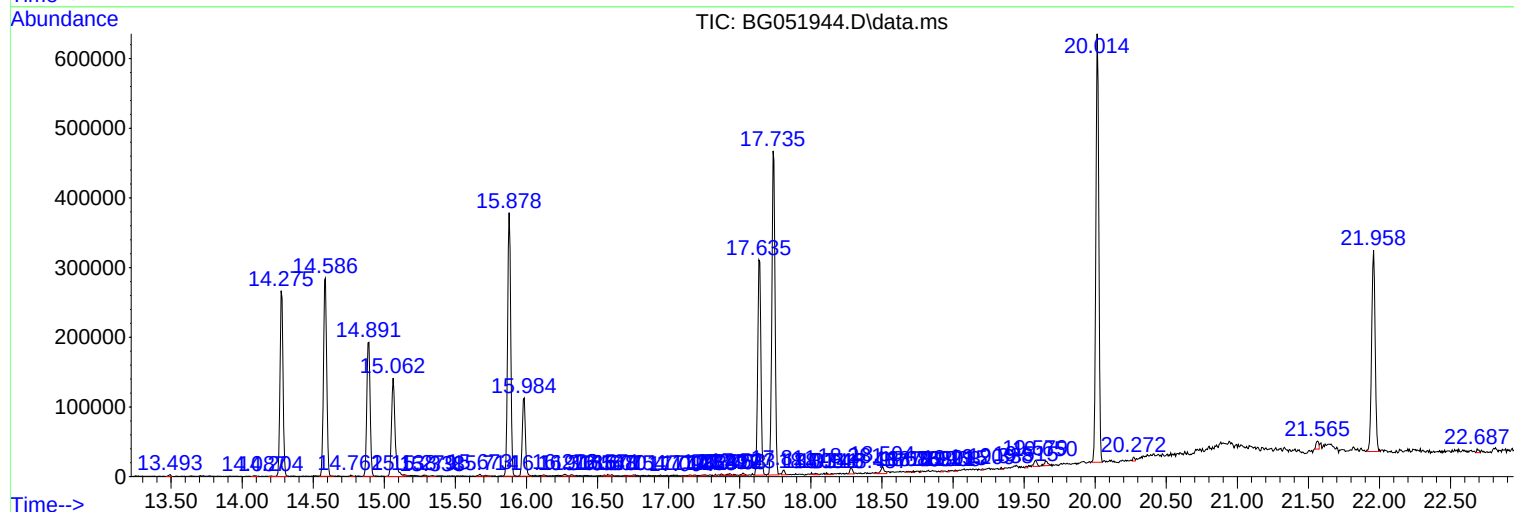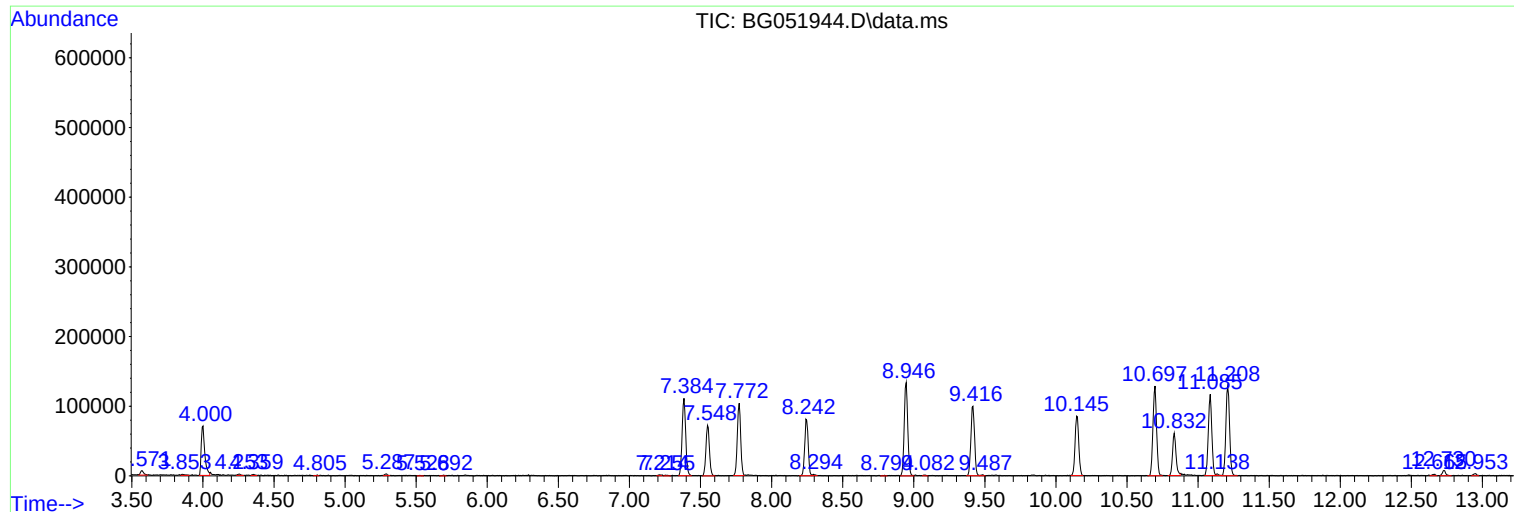

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011222\
Data File : BG051944.D
Acq On : 12 Jan 2022 14:04
Operator : CG/JU
Sample : N1100-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLN5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.832	10.32 ng/ul	103036	Naphthalene-d8	11.085

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
2			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
3			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	86
4			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	83
5			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	83

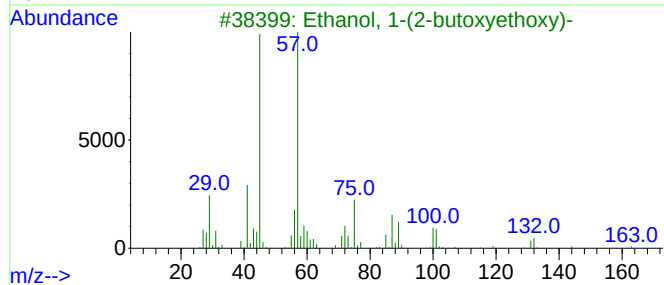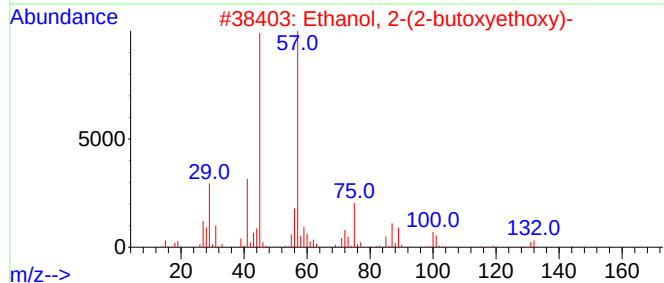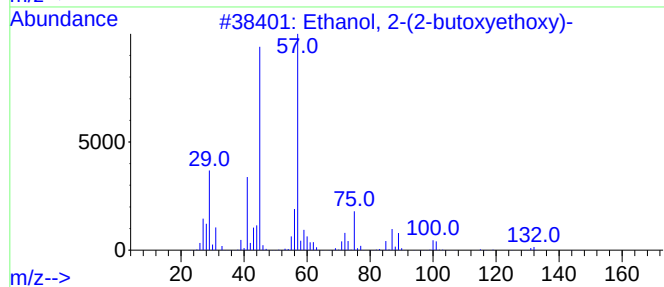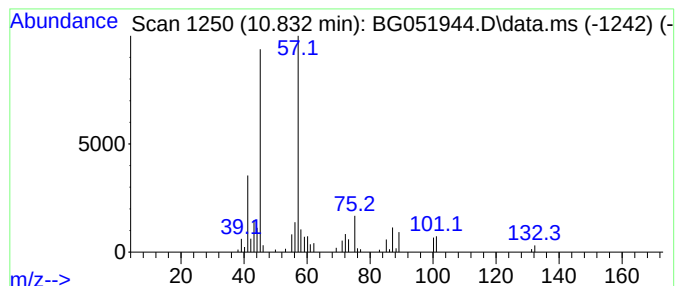

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011222\
Data File : BG051944.D
Acq On : 12 Jan 2022 14:04
Operator : CG/JU
Sample : N1100-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLN5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	10.832	10.3	ng/ul	103036	2	11.085	199634	20.0