

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011222\
 Data File : BG051947.D
 Acq On : 12 Jan 2022 15:58
 Operator : CG/JU
 Sample : N1100-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLP0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051947.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.570	10	14	18	rVV2	5788	7987	0.95%	0.106%
2	4.252	126	130	133	rVB3	2068	3161	0.38%	0.042%
3	4.281	133	135	139	rBV2	1060	1765	0.21%	0.023%
4	4.351	141	147	150	rBV2	1945	3369	0.40%	0.045%
5	5.285	303	306	308	rBV2	2007	2533	0.30%	0.033%
6	7.383	654	663	672	rVV	106596	194016	23.19%	2.563%
7	7.553	685	692	700	rBV	70372	120543	14.41%	1.593%
8	7.770	722	729	739	rBV	93258	159886	19.11%	2.112%
9	8.246	803	810	817	rBV	87263	141687	16.93%	1.872%
10	8.945	922	929	938	rVB	113880	196786	23.52%	2.600%
11	9.415	1001	1009	1017	rVB	98174	173557	20.74%	2.293%
12	9.844	1078	1082	1086	rVB2	1299	2096	0.25%	0.028%
13	10.149	1127	1134	1141	rVB	74432	132487	15.83%	1.750%
14	10.696	1219	1227	1234	rBV	115516	203492	24.32%	2.688%
15	10.831	1244	1250	1259	rBV3	16590	29443	3.52%	0.389%
16	11.083	1284	1293	1303	rBV	119522	204761	24.47%	2.705%
17	11.207	1303	1314	1323	rVB3	59024	111397	13.31%	1.472%
18	12.652	1555	1560	1564	rVB3	1908	3152	0.38%	0.042%
19	13.492	1698	1703	1708	rVB3	2055	2900	0.35%	0.038%
20	14.279	1830	1837	1842	rBV	224844	329728	39.41%	4.356%
21	14.585	1882	1889	1897	rBV	273518	417643	49.91%	5.518%
22	14.890	1933	1941	1948	rBV	202539	307123	36.70%	4.058%
23	15.060	1960	1970	1983	rBV2	80702	152387	18.21%	2.013%
24	15.665	2067	2073	2077	rBV3	2187	3913	0.47%	0.052%
25	15.718	2079	2082	2085	rVV2	1006	1580	0.19%	0.021%
26	15.877	2101	2109	2119	rBV	355779	534106	63.83%	7.056%
27	15.977	2121	2126	2133	rBV2	66042	101447	12.12%	1.340%
28	16.271	2172	2176	2179	rVV3	3237	3428	0.41%	0.045%
29	16.412	2195	2200	2203	rBV	1107	1831	0.22%	0.024%
30	17.146	2321	2325	2328	rBV2	1405	2229	0.27%	0.029%
31	17.316	2350	2354	2356	rBV2	1911	1922	0.23%	0.025%
32	17.522	2386	2389	2394	rBV5	2565	3717	0.44%	0.049%
33	17.639	2401	2409	2415	rVV	282227	439422	52.52%	5.805%
34	17.733	2418	2425	2434	rVV2	417076	650329	77.72%	8.592%
35	18.109	2486	2489	2491	rBV	1539	1677	0.20%	0.022%
36	18.285	2514	2519	2523	rVV2	10055	13122	1.57%	0.173%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011222\
 Data File : BG051947.D
 Acq On : 12 Jan 2022 15:58
 Operator : CG/JU
 Sample : N1100-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLP0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	18.503	2551	2556	2560	rBV5	2021	3171	0.38%	0.042%
38	18.632	2576	2578	2581	rVV4	1592	1968	0.24%	0.026%
39	18.797	2602	2606	2610	rBV3	2705	3722	0.44%	0.049%
40	19.037	2644	2647	2651	rBV5	1876	3366	0.40%	0.044%
41	19.108	2655	2659	2662	rVB3	1726	2265	0.27%	0.030%
42	19.355	2698	2701	2704	rVB5	1819	2245	0.27%	0.030%
43	19.437	2709	2715	2719	rVB5	8685	12792	1.53%	0.169%
44	19.578	2735	2739	2746	rVB8	7899	13452	1.61%	0.178%
45	19.648	2746	2751	2755	rBV2	7040	11574	1.38%	0.153%
46	19.789	2773	2775	2777	rBV3	2571	1620	0.19%	0.021%
47	19.813	2777	2779	2780	rBV	1787	1667	0.20%	0.022%
48	19.907	2794	2795	2798	rBV3	2959	2649	0.32%	0.035%
49	20.013	2805	2813	2822	rVV	563836	836748	100.00%	11.055%
50	20.130	2831	2833	2835	rVB2	2382	1761	0.21%	0.023%
51	20.154	2835	2837	2838	rVB2	3122	1730	0.21%	0.023%
52	20.171	2838	2840	2841	rBV2	4084	2872	0.34%	0.038%
53	20.347	2868	2870	2872	rBV3	3178	3107	0.37%	0.041%
54	20.430	2882	2884	2886	rBV3	2502	2445	0.29%	0.032%
55	20.512	2896	2898	2900	rBV2	3877	2894	0.35%	0.038%
56	20.576	2907	2909	2911	rBV3	3266	2746	0.33%	0.036%
57	20.612	2914	2915	2917	rBV2	2408	2258	0.27%	0.030%
58	20.858	2954	2957	2958	rBV2	4081	2831	0.34%	0.037%
59	20.876	2958	2960	2962	rBV3	2547	2696	0.32%	0.036%
60	21.246	3021	3023	3024	rVB	3784	2077	0.25%	0.027%
61	21.352	3039	3041	3042	rBV2	3700	1982	0.24%	0.026%
62	21.464	3059	3060	3064	rBV3	3846	2612	0.31%	0.035%
63	21.563	3072	3077	3085	rBV4	28929	69932	8.36%	0.924%
64	21.957	3137	3144	3152	rVB	283497	493227	58.95%	6.516%
65	22.262	3194	3196	3197	rBV2	4867	3509	0.42%	0.046%
66	22.891	3302	3303	3305	rBV2	4147	2479	0.30%	0.033%
67	23.514	3406	3409	3410	rBV3	4376	4453	0.53%	0.059%
68	23.625	3426	3428	3432	rVB5	3885	4113	0.49%	0.054%
69	23.661	3432	3434	3435	rBV2	4329	3336	0.40%	0.044%
70	24.178	3520	3522	3524	rBV2	3736	3084	0.37%	0.041%
71	24.442	3561	3567	3572	rVB8	10407	20773	2.48%	0.274%
72	24.524	3579	3581	3583	rVB3	3727	2483	0.30%	0.033%
73	24.548	3583	3585	3587	rBV3	2921	2063	0.25%	0.027%
74	24.947	3652	3653	3655	rVB2	4397	1964	0.23%	0.026%
75	25.200	3685	3696	3707	rVB2	248757	741102	88.57%	9.791%
76	25.440	3727	3737	3752	rVB3	160124	519678	62.11%	6.866%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011222\
 Data File : BG051947.D
 Acq On : 12 Jan 2022 15:58
 Operator : CG/JU
 Sample : N1100-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLP0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

77	25.652	3771	3773	3776	rVB4	3229	1675	0.20%	0.022%
78	25.881	3810	3812	3814	rBV3	3886	4518	0.54%	0.060%
79	25.934	3819	3821	3824	rBV4	3361	4130	0.49%	0.055%
80	26.034	3836	3838	3840	rBV3	3282	2770	0.33%	0.037%
81	26.721	3949	3955	3956	rBV5	9811	14057	1.68%	0.186%
82	26.745	3956	3959	3964	rVB7	12305	21473	2.57%	0.284%
83	26.980	3998	3999	4001	rBV2	4213	2719	0.32%	0.036%
84	27.156	4027	4029	4031	rBV3	3151	2242	0.27%	0.030%
85	27.314	4054	4056	4057	rBV2	2874	2037	0.24%	0.027%
86	27.361	4062	4064	4065	rBV2	3167	2601	0.31%	0.034%
87	27.908	4156	4157	4159	rBV2	3915	2513	0.30%	0.033%
88	28.190	4203	4205	4206	rBV2	4737	4201	0.50%	0.056%
89	28.219	4208	4210	4212	rVV2	5287	5815	0.69%	0.077%
90	28.936	4331	4332	4335	rBV3	3995	2649	0.32%	0.035%
91	29.147	4366	4368	4370	rBV3	4298	3091	0.37%	0.041%
92	30.023	4513	4517	4518	rBV4	5507	7916	0.95%	0.105%
93	30.434	4584	4587	4590	rBV5	3189	4156	0.50%	0.055%
94	30.510	4598	4600	4602	rBV2	3111	1926	0.23%	0.025%
95	30.563	4605	4609	4610	rBV3	3416	3810	0.46%	0.050%
96	31.045	4689	4691	4693	rBV3	4711	3450	0.41%	0.046%
97	31.180	4712	4714	4715	rBV2	3025	2252	0.27%	0.030%
98	31.485	4764	4766	4767	rVB2	3449	1891	0.23%	0.025%
99	31.620	4787	4789	4790	rBV2	2632	1676	0.20%	0.022%
100	31.761	4811	4813	4816	rVB4	3261	3526	0.42%	0.047%




Sum of corrected areas: 7569162

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011222\
Data File : BG051947.D
Acq On : 12 Jan 2022 15:58
Operator : CG/JU
Sample : N1100-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLP0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

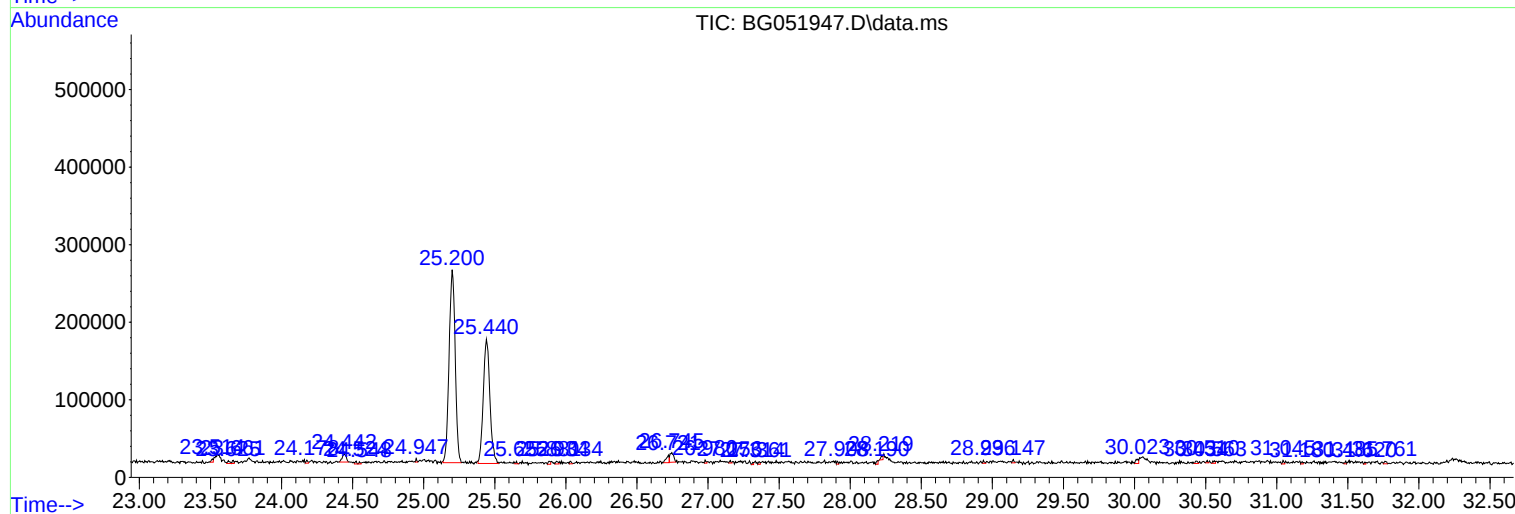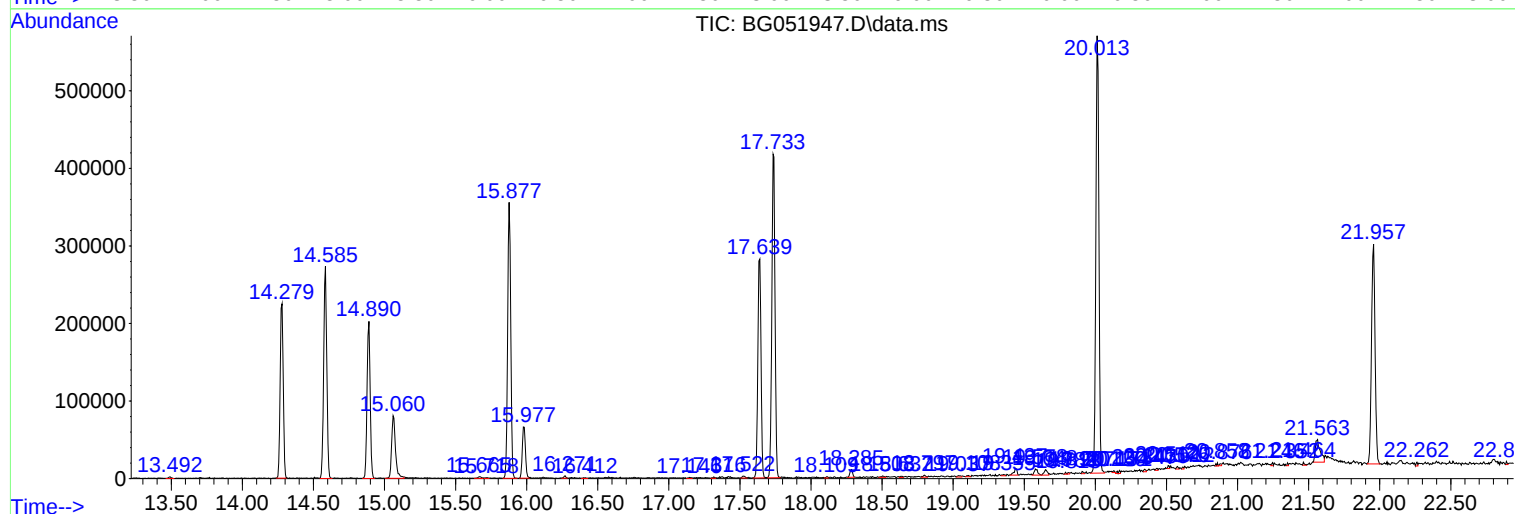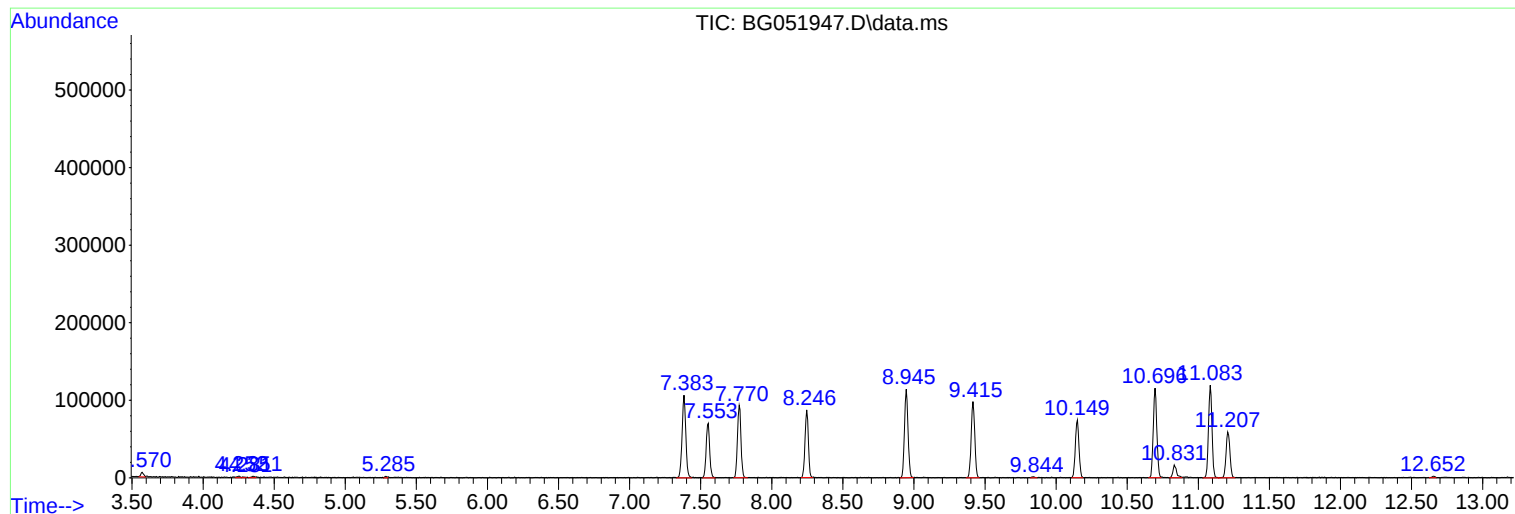

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011222\
Data File : BG051947.D
Acq On : 12 Jan 2022 15:58
Operator : CG/JU
Sample : N1100-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLP0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(2-butoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.831	2.88 ng/ul	29443	Naphthalene-d8	11.083

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	64
2			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	59
3			Ethanol, 2-[2-(2-methylpropoxy)e...	162	C8H18O3	018912-80-6	50
4			Ethanol, 2-[2-(2-butoxyethoxy)et...	206	C10H22O4	000143-22-6	45
5			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	45

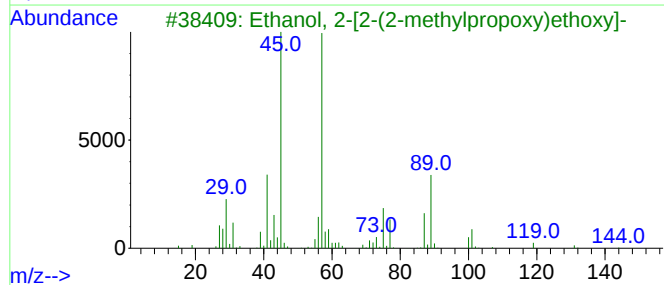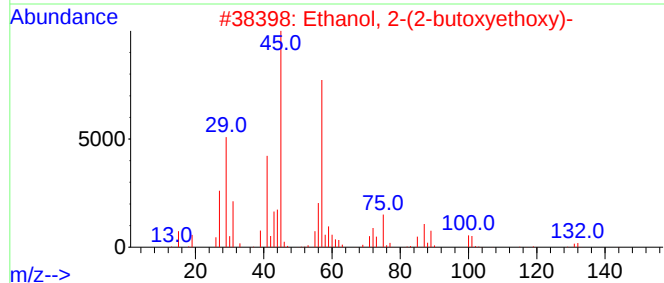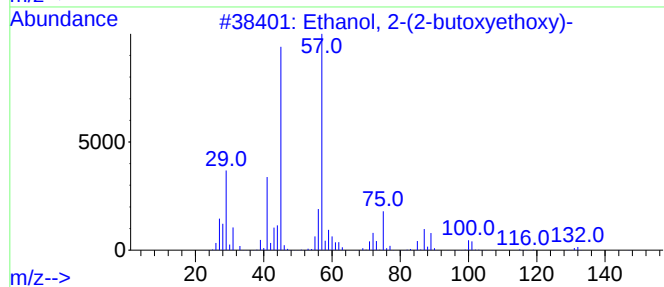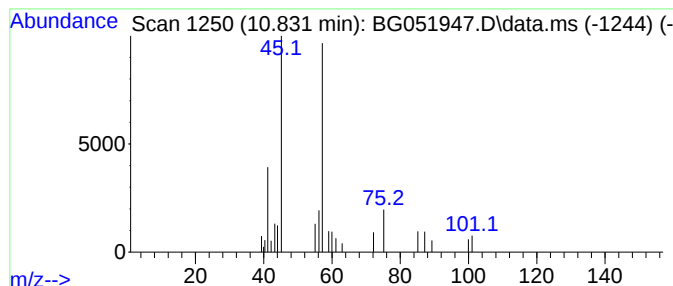

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011222\
Data File : BG051947.D
Acq On : 12 Jan 2022 15:58
Operator : CG/JU
Sample : N1100-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLP0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Trichloroacetic acid, hexad... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.563	2.84 ng/ul	69932	Chrysene-d12	21.957

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Trichloroacetic acid, hexadecyl ...	386	C18H33Cl3O2	074339-54-1	81
2			Pentadecafluorooctanoic acid, oc...	666	C26H37F15O2	1000406-04-8	81
3			Trichloroacetic acid, pentadecyl...	372	C17H31Cl3O2	074339-53-0	81
4			1-Octadecanol	270	C18H38O	000112-92-5	76
5			Dichloroacetic acid, heptadecyl ...	366	C19H36Cl2O2	1000282-98-2	76

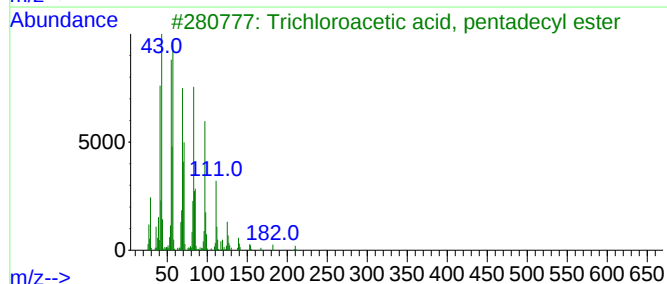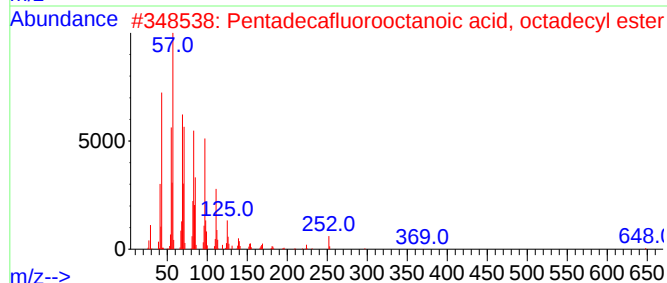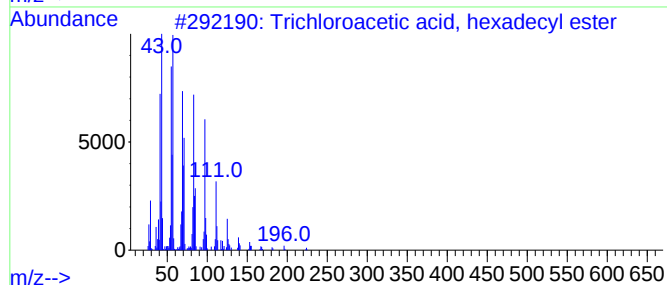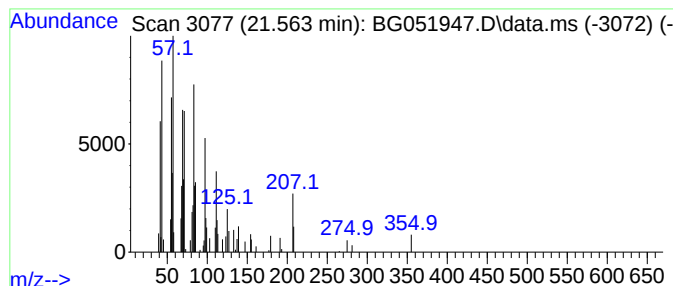

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011222\
Data File : BG051947.D
Acq On : 12 Jan 2022 15:58
Operator : CG/JU
Sample : N1100-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLP0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(2-b...	10.831	2.9	ng/ul	29443	2	11.083	204761	20.0
Trichloroacetic...	21.563	2.8	ng/ul	69932	5	21.957	493227	20.0