

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011222\
 Data File : BG051951.D
 Acq On : 12 Jan 2022 18:29
 Operator : CG/JU
 Sample : PB141967BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK967

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051951.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.573	9	14	24	rVB	5702	10076	1.45%	0.152%
2	3.714	31	38	42	rBV4	967	2403	0.35%	0.036%
3	3.996	82	86	98	rBV	67287	109270	15.77%	1.647%
4	4.231	125	126	129	rBV	1016	1026	0.15%	0.015%
5	4.296	136	137	142	rVB2	1140	1009	0.15%	0.015%
6	4.349	142	146	150	rBV4	1352	2773	0.40%	0.042%
7	7.198	627	631	633	rBV	751	1045	0.15%	0.016%
8	7.380	656	662	672	rVB	79529	139544	20.14%	2.103%
9	7.550	684	691	697	rVB	55301	94153	13.59%	1.419%
10	7.767	721	728	736	rVB	74119	125089	18.05%	1.885%
11	8.032	768	773	775	rVB	818	1044	0.15%	0.016%
12	8.243	802	809	818	rVB	84463	140772	20.31%	2.121%
13	8.696	880	886	888	rBV	1109	1273	0.18%	0.019%
14	8.942	921	928	935	rBV	90009	157807	22.77%	2.378%
15	9.412	1000	1008	1018	rVB	74292	131804	19.02%	1.986%
16	9.782	1065	1071	1072	rBB	690	959	0.14%	0.014%
17	10.147	1126	1133	1140	rBV	63974	111058	16.03%	1.674%
18	10.246	1146	1150	1153	rVB	855	1295	0.19%	0.020%
19	10.293	1153	1158	1160	rBV	657	1102	0.16%	0.017%
20	10.364	1162	1170	1171	rBV2	787	1356	0.20%	0.020%
21	10.693	1220	1226	1234	rBV2	88857	160342	23.14%	2.416%
22	11.081	1284	1292	1302	rVB	111601	200728	28.97%	3.025%
23	11.210	1302	1314	1322	rBV	92010	173603	25.05%	2.616%
24	12.649	1557	1559	1563	rBV2	1051	1490	0.22%	0.022%
25	12.720	1567	1571	1575	rBV2	650	1252	0.18%	0.019%
26	14.276	1829	1836	1842	rBV	208763	295242	42.60%	4.449%
27	14.582	1882	1888	1895	rBV	211013	324345	46.80%	4.888%
28	14.887	1934	1940	1948	rVB	198213	316890	45.73%	4.776%
29	15.064	1964	1970	1980	rBV2	84655	151532	21.87%	2.284%
30	15.334	2014	2016	2021	rBV2	634	1136	0.16%	0.017%
31	15.745	2084	2086	2090	rVB2	969	1000	0.14%	0.015%
32	15.880	2102	2109	2119	rVB	282244	430614	62.14%	6.489%
33	15.980	2121	2126	2134	rBV2	76512	114042	16.46%	1.719%
34	16.121	2146	2150	2154	rBV3	1279	2237	0.32%	0.034%
35	16.373	2190	2193	2195	rBV2	1288	1436	0.21%	0.022%
36	17.425	2369	2372	2376	rVB3	1505	1913	0.28%	0.029%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011222\
 Data File : BG051951.D
 Acq On : 12 Jan 2022 18:29
 Operator : CG/JU
 Sample : PB141967BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK967

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	17.636	2402	2408	2415	rBV	330802	485595	70.07%	7.318%
38	17.736	2418	2425	2433	rBV	375656	550407	79.42%	8.295%
39	18.042	2475	2477	2483	rVB2	977	1437	0.21%	0.022%
40	18.089	2483	2485	2489	rBV	1012	1458	0.21%	0.022%
41	18.277	2515	2517	2520	rVB2	962	971	0.14%	0.015%
42	18.712	2589	2591	2596	rVB3	1291	1167	0.17%	0.018%
43	18.758	2596	2599	2600	rBV	1150	1179	0.17%	0.018%
44	19.011	2638	2642	2645	rBV3	1348	2003	0.29%	0.030%
45	19.211	2673	2676	2677	rBV	1147	1123	0.16%	0.017%
46	19.246	2681	2682	2685	rBV3	1346	1019	0.15%	0.015%
47	19.581	2735	2739	2744	rVB5	4817	9192	1.33%	0.139%
48	19.651	2746	2751	2756	rBV3	5714	8805	1.27%	0.133%
49	19.945	2800	2801	2803	rBV2	2375	1172	0.17%	0.018%
50	20.016	2807	2813	2821	rVB	484283	692990	100.00%	10.443%
51	20.104	2826	2828	2830	rBV2	2255	1436	0.21%	0.022%
52	21.073	2991	2993	2996	rBV3	3797	4031	0.58%	0.061%
53	21.954	3136	3143	3151	rVB	309768	529128	76.35%	7.974%
54	22.794	3284	3286	3292	rBV7	6550	9382	1.35%	0.141%
55	25.197	3686	3695	3704	rVB2	197434	576291	83.16%	8.685%
56	25.444	3727	3737	3753	rVB	174214	544283	78.54%	8.202%




Sum of corrected areas: 6635729

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011222\
Data File : BG051951.D
Acq On : 12 Jan 2022 18:29
Operator : CG/JU
Sample : PB141967BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK967

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

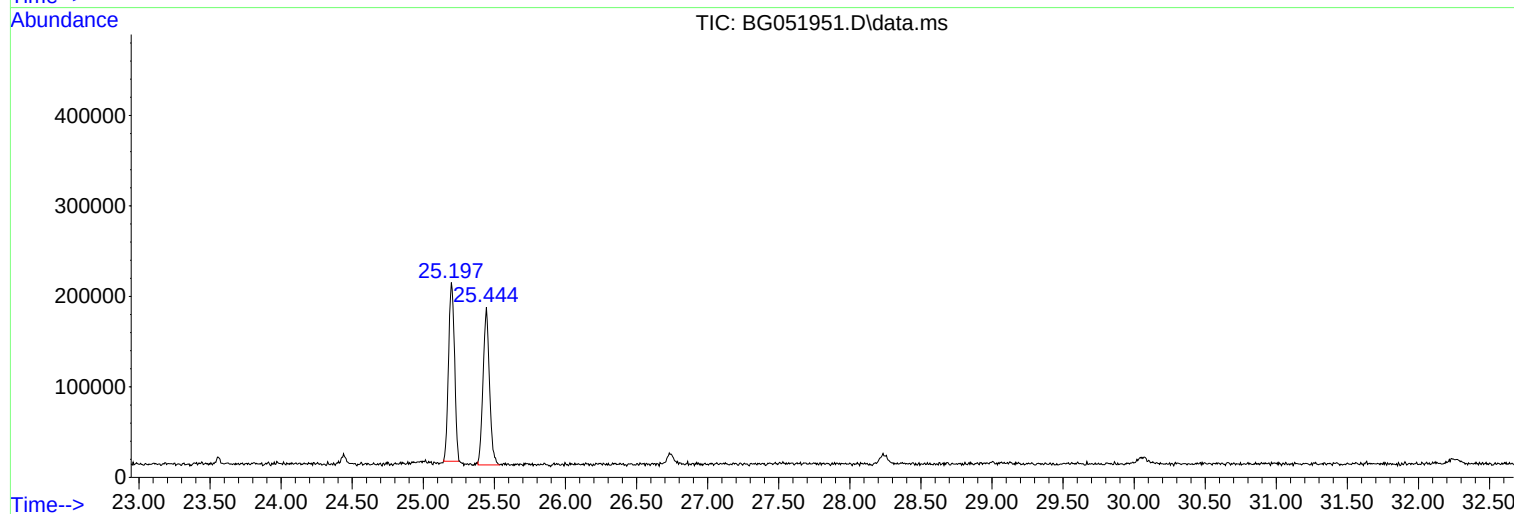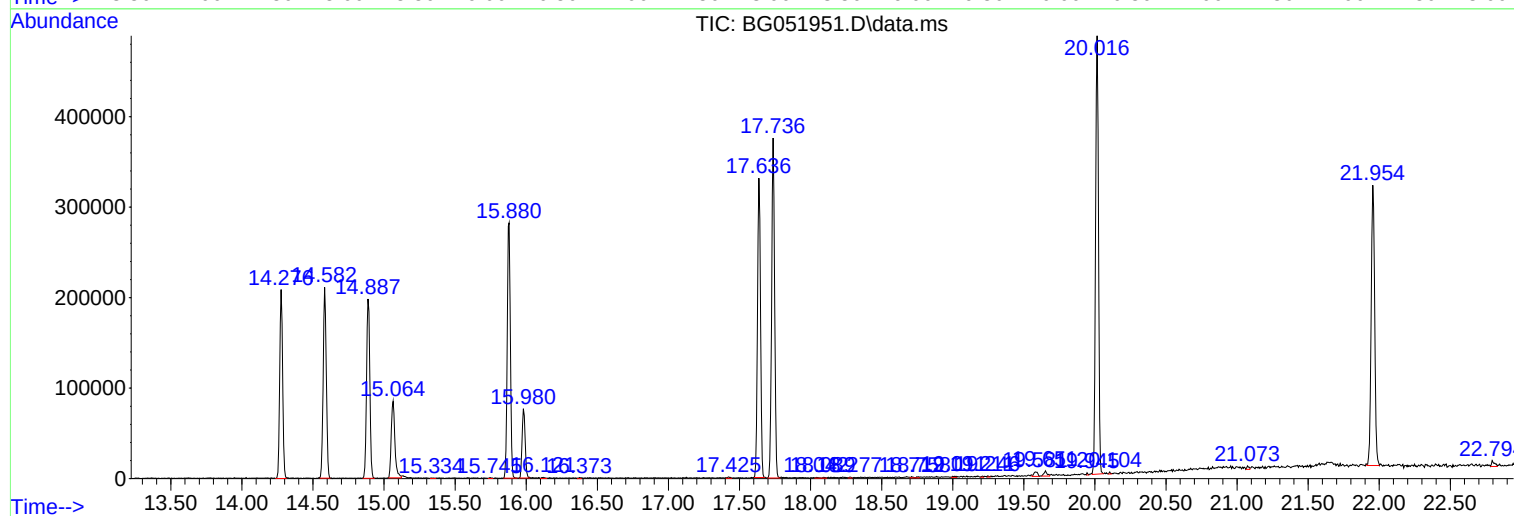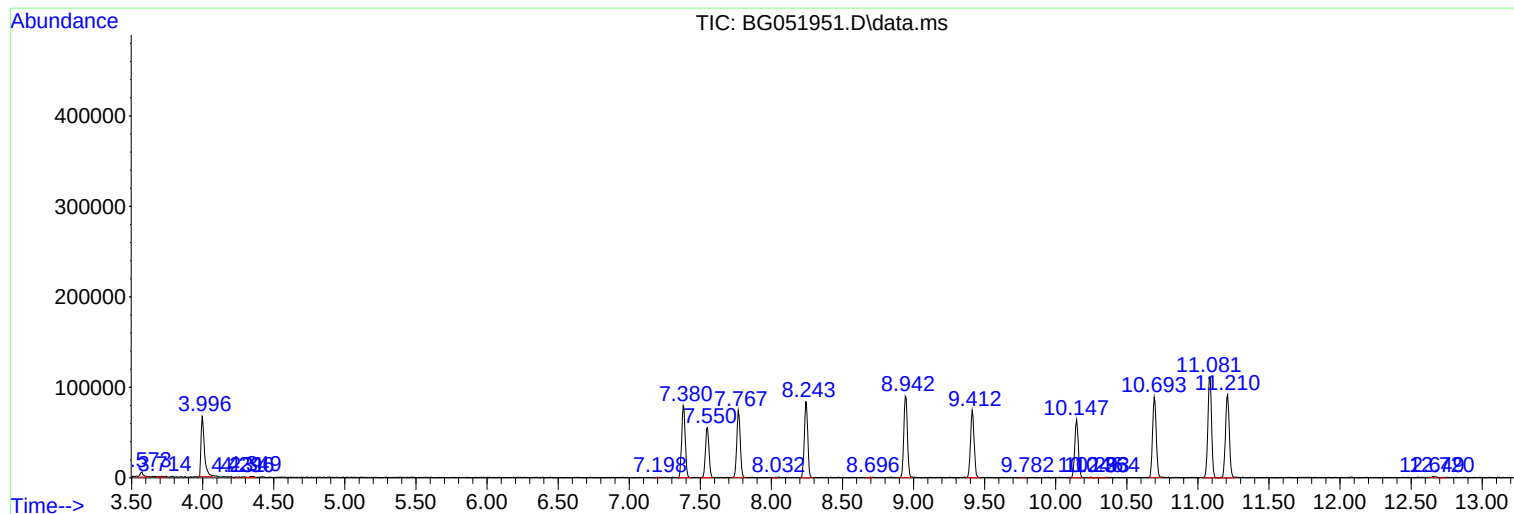

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011222\
Data File : BG051951.D
Acq On : 12 Jan 2022 18:29
Operator : CG/JU
Sample : PB141967BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK967

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011222\
Data File : BG051951.D
Acq On : 12 Jan 2022 18:29
Operator : CG/JU
Sample : PB141967BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK967

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
