
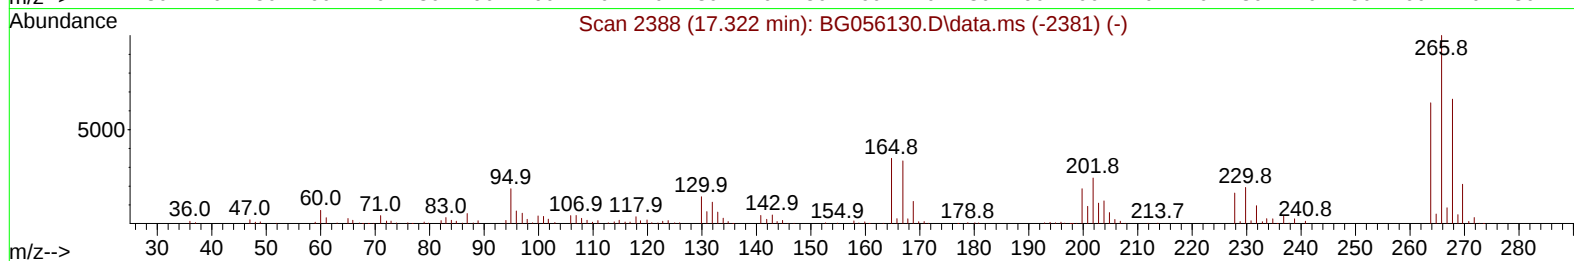
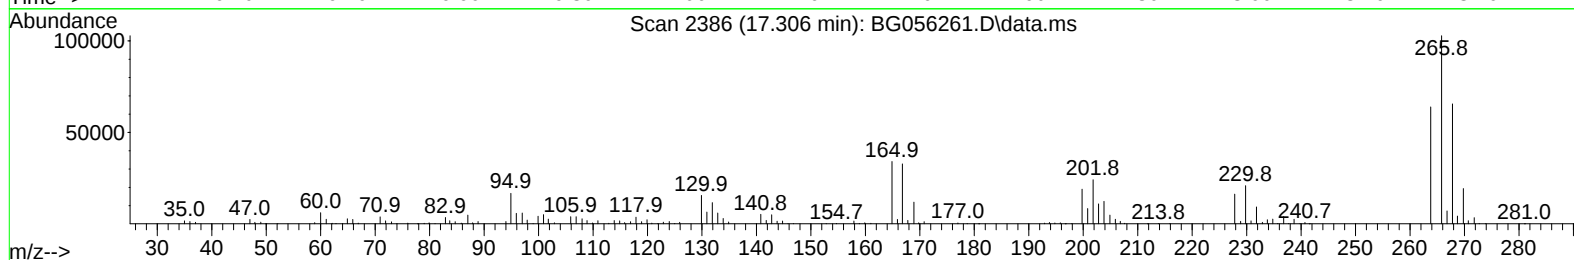


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011223\
Data File : BG056261.D
Acq On : 12 Jan 2023 9:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 13 06:22:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 12 03:38:40 2023
Response via : Initial Calibration

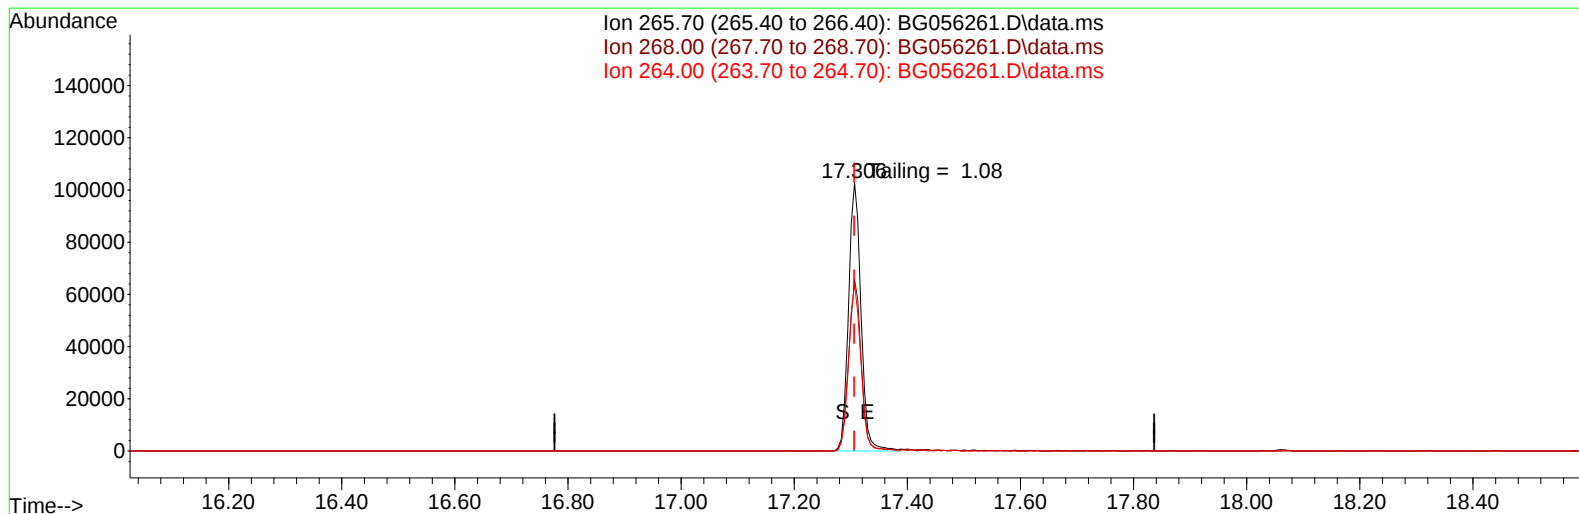

TIC: BG056261.D\data.ms

(70) Pentachlorophenol (C)




17.306min (+ 0.000) 24128.12 ng

response 157883

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	68.02
264.00	64.30	62.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011223\
Data File : BG056261.D
Acq On : 12 Jan 2023 9:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 13 06:22:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 12 03:38:40 2023
Response via : Initial Calibration

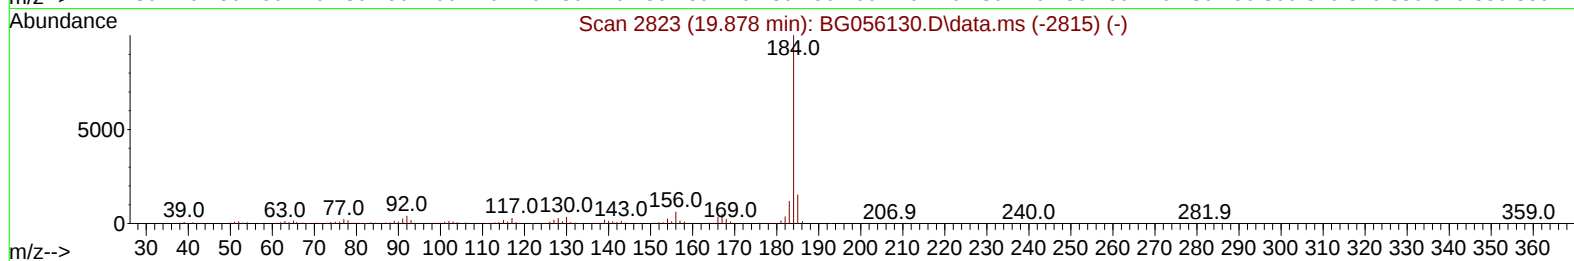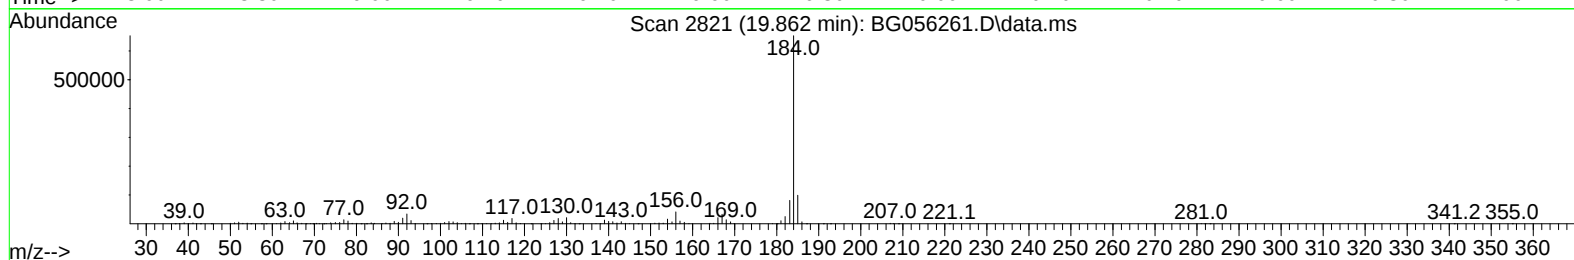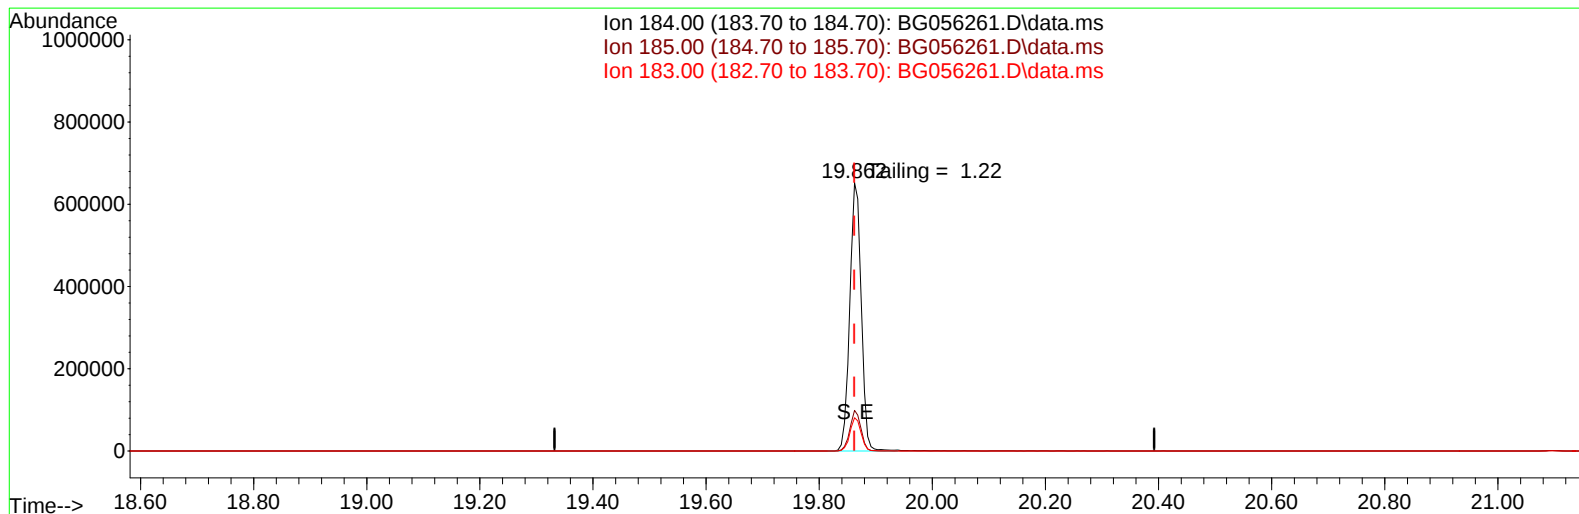

TIC: BG056261.D\data.ms

(77) Benzidine

19.862min (+ 0.000) 432164.38 ng

response 923839

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	15.17
183.00	11.70	12.43
0.00	0.00	0.00