


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011223\
 Data File : BG056261.D
 Acq On : 12 Jan 2023 9:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 12 03:38:40 2023

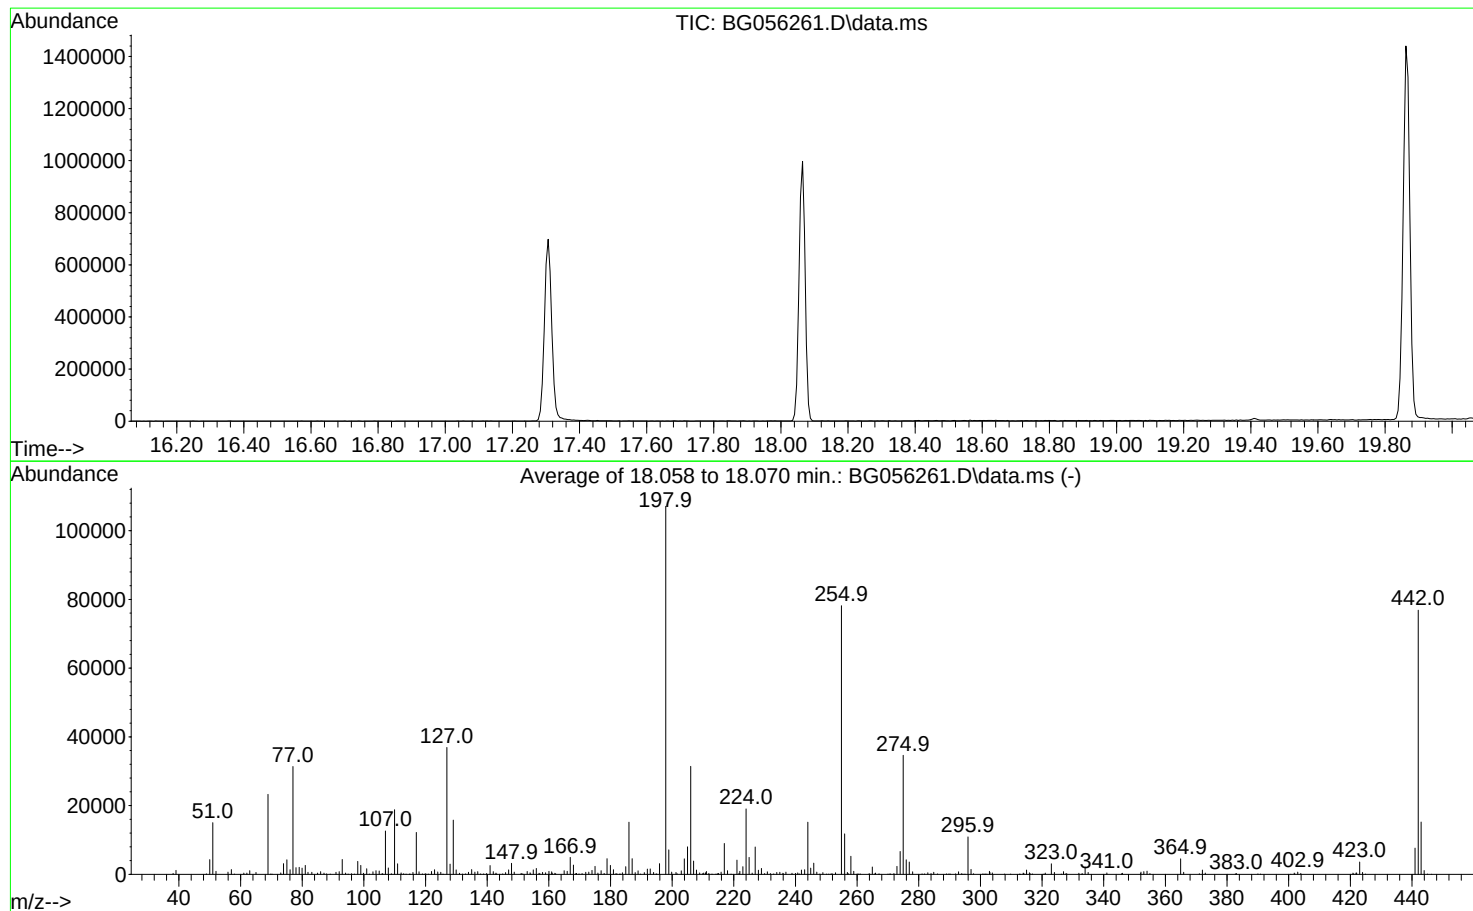




AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	14.0	15008	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	21.7	23267	PASS
70	69	0.00	2	0.4	84	PASS
127	198	10	80	34.5	36899	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	107061	PASS
199	198	5	9	6.6	7113	PASS
275	198	10	60	32.4	34637	PASS
365	198	1	100	4.2	4512	PASS
441	198	0.01	100	7.1	7610	PASS
442	442	50	100	100.0	76875	PASS
443	442	15	24	19.8	15224	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011223\
Data File : BG056261.D
Acq On : 12 Jan 2023 9:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 13 06:22:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 12 03:38:40 2023
Response via : Initial Calibration

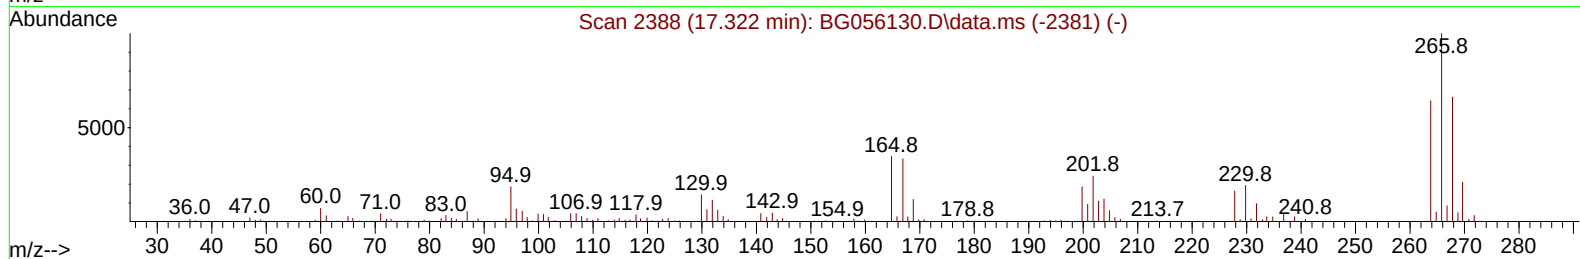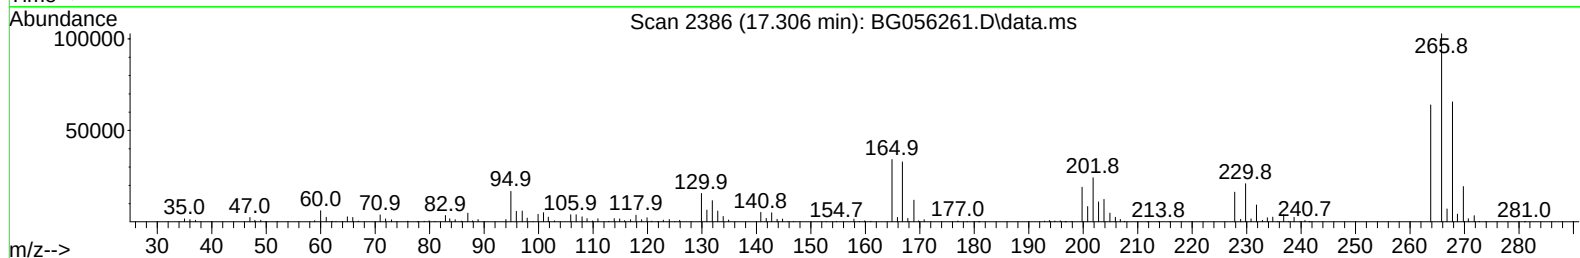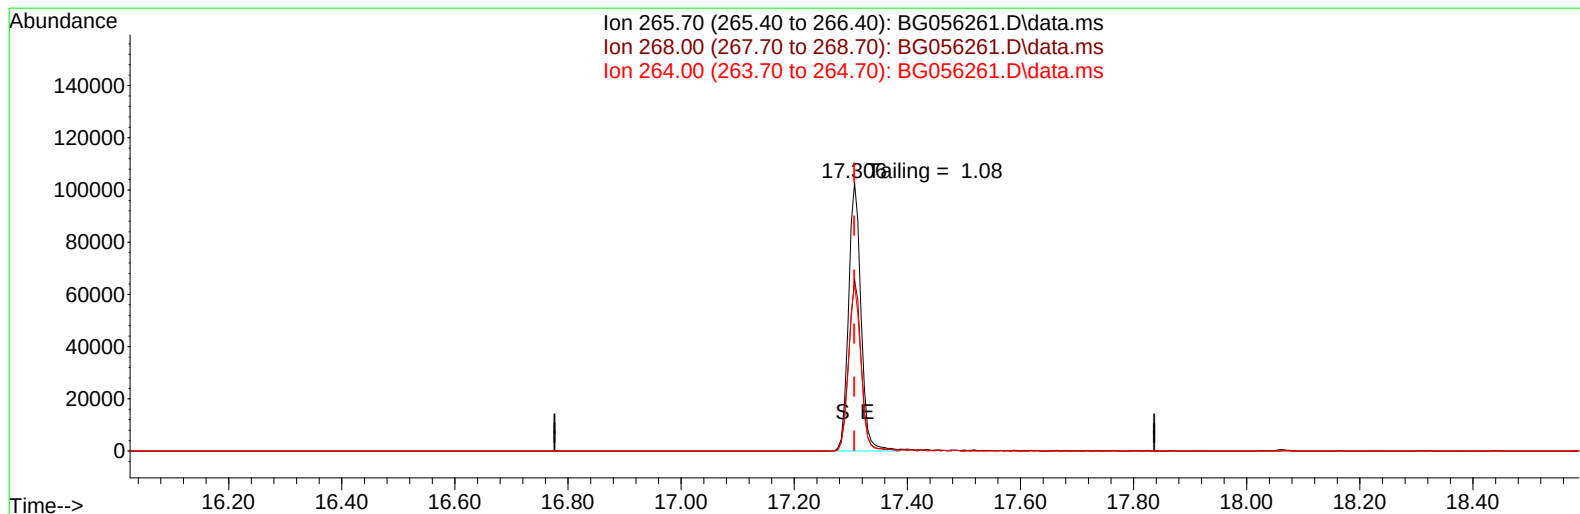

TIC: BG056261.D\data.ms

(70) Pentachlorophenol (C)

17.306min (+ 0.000) 24128.12 ng




response 157883

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	68.02
264.00	64.30	62.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011223\
Data File : BG056261.D
Acq On : 12 Jan 2023 9:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 13 06:22:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 12 03:38:40 2023
Response via : Initial Calibration

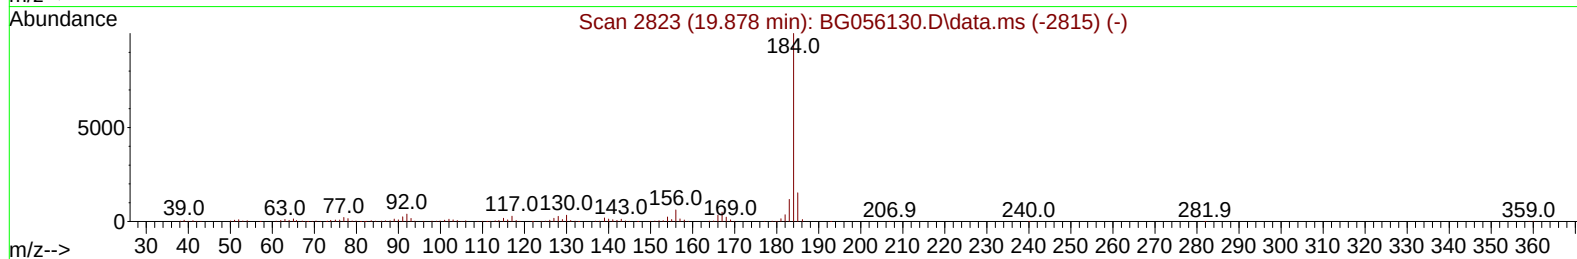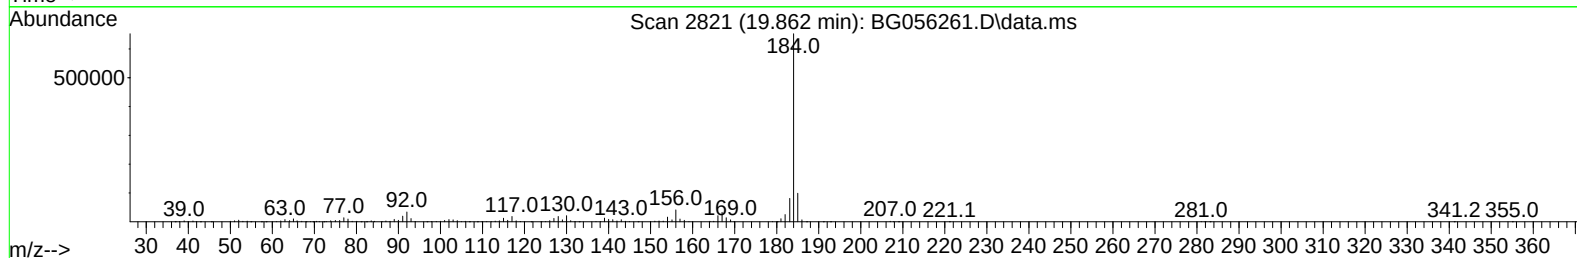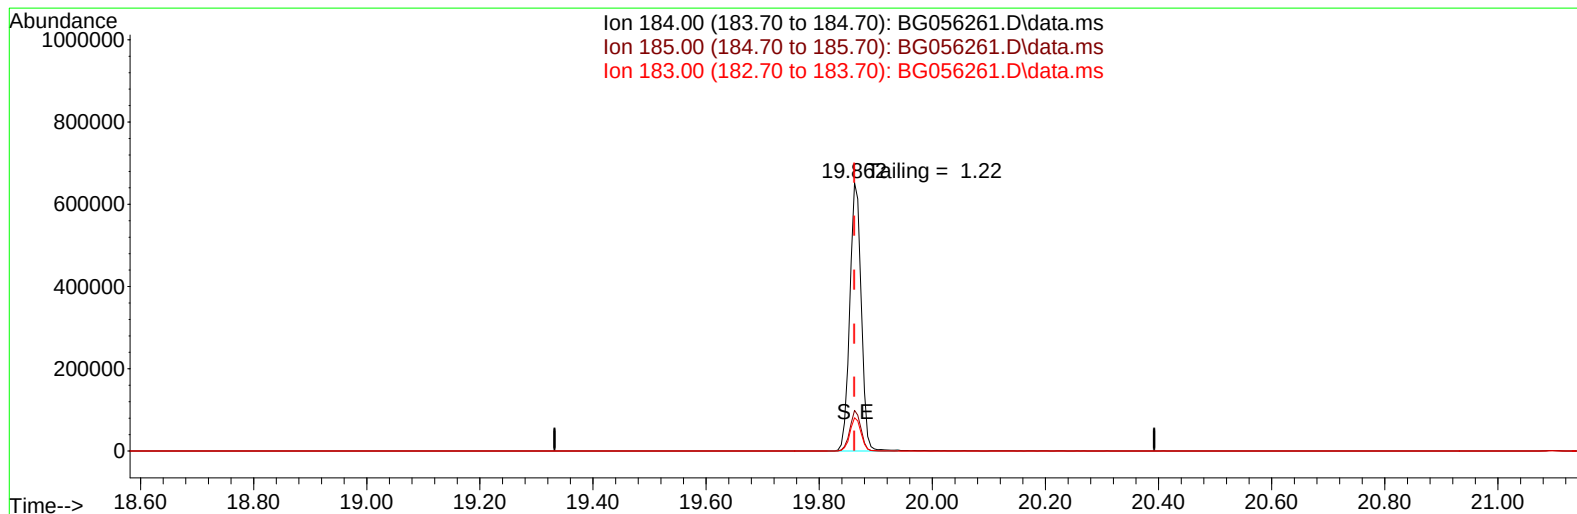

TIC: BG056261.D\data.ms

(77) Benzidine

19.862min (+ 0.000) 432164.38 ng

response 923839

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	15.17
183.00	11.70	12.43
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/12/2023	BNA_G	BG056261.D
Compound Name	Response	Retention Time
DDT	448385	21.096
DDD	15014	20.644
DDE	630	20.138
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15644	464029	3.37

Instrument :
BNA_G
ClientSampleId :
DFTPP