
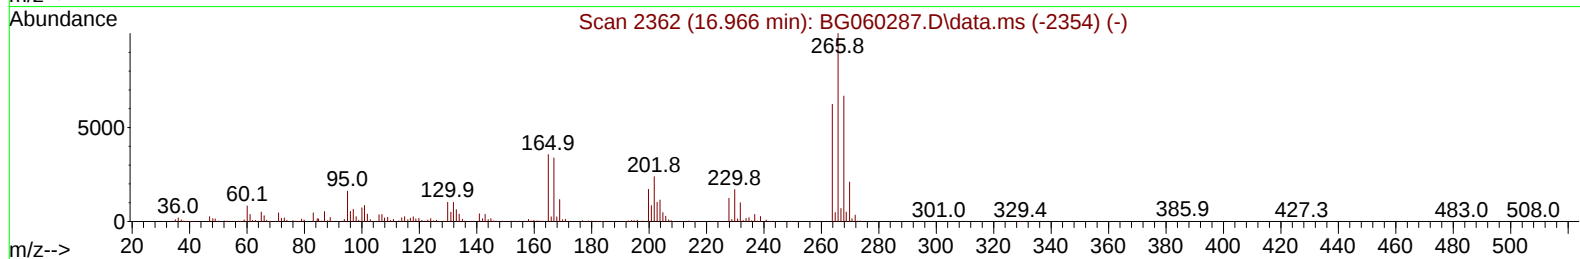
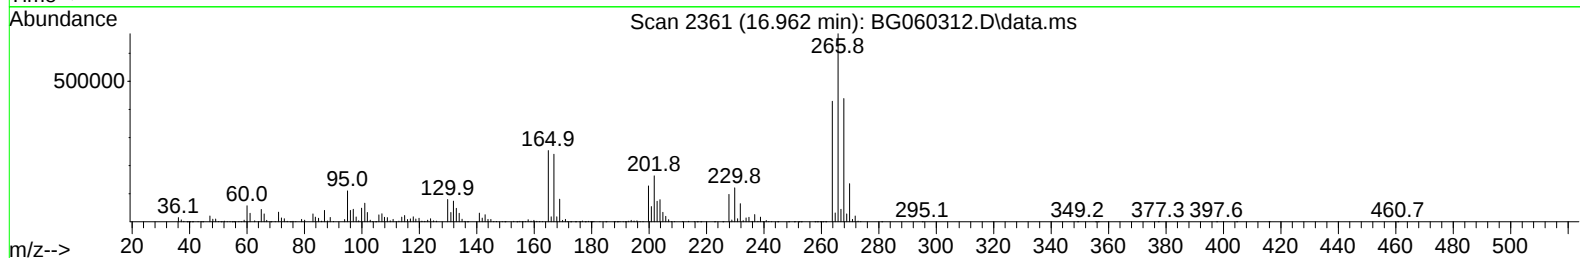


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG011224\  
Data File : BG060312.D  
Acq On : 12 Jan 2024 12:20  
Operator : MA/JU  
Sample : DFTPP  
Misc : 8270 SURROGATES  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 12 13:51:24 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG010824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jan 09 04:07:12 2024  
Response via : Initial Calibration

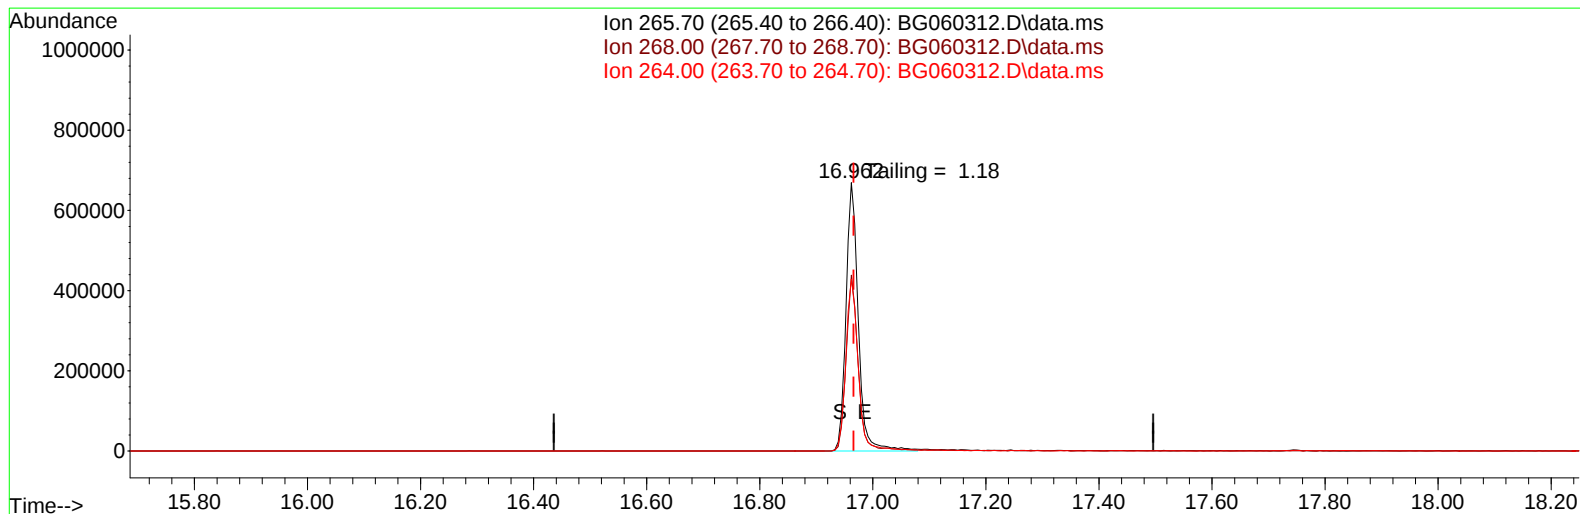

TIC: BG060312.D\data.ms

**(70) Pentachlorophenol (C)**




16.962min (-0.004) 168112.82 ng

response 1018320

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 71.80  | 65.53  |
| 264.00 | 62.30  | 64.07  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG011224\  
Data File : BG060312.D  
Acq On : 12 Jan 2024 12:20  
Operator : MA/JU  
Sample : DFTPP  
Misc : 8270 SURROGATES  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 12 13:51:24 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG010824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jan 09 04:07:12 2024  
Response via : Initial Calibration

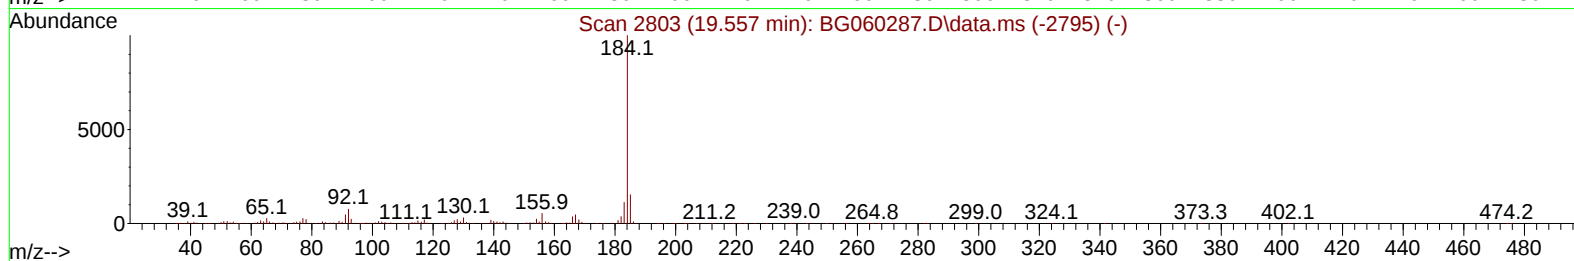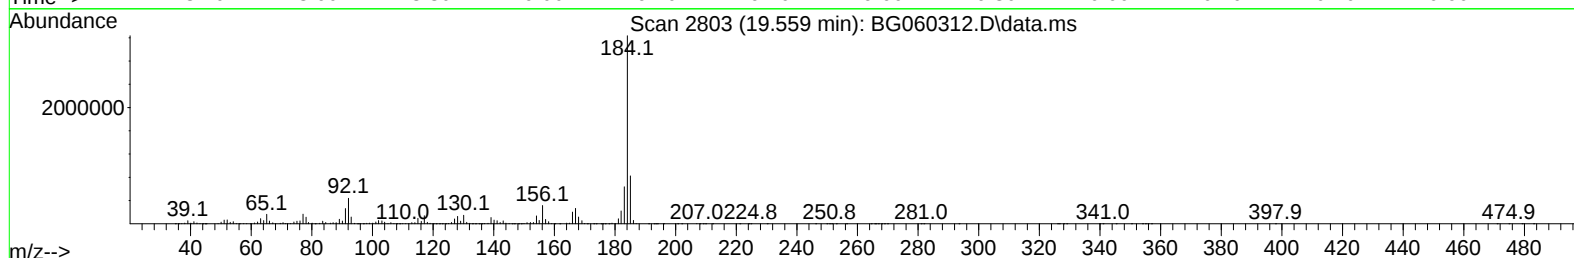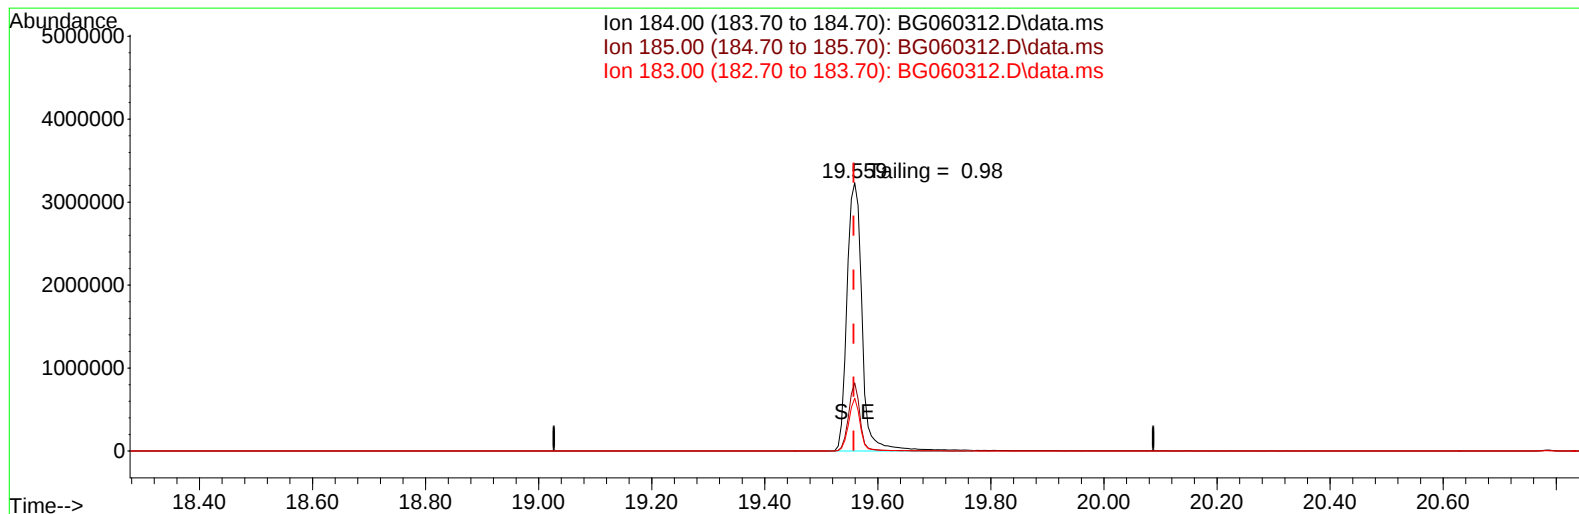

TIC: BG060312.D\data.ms

(77) Benzidine

19.559min (+ 0.002) 205009.62 ng

response 6030548

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.30  | 25.43# |
| 183.00 | 11.20  | 19.70# |
| 0.00   | 0.00   | 0.00   |