


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011224\
Data File : BG060312.D
Acq On : 12 Jan 2024 12:20
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jan 09 04:07:12 2024

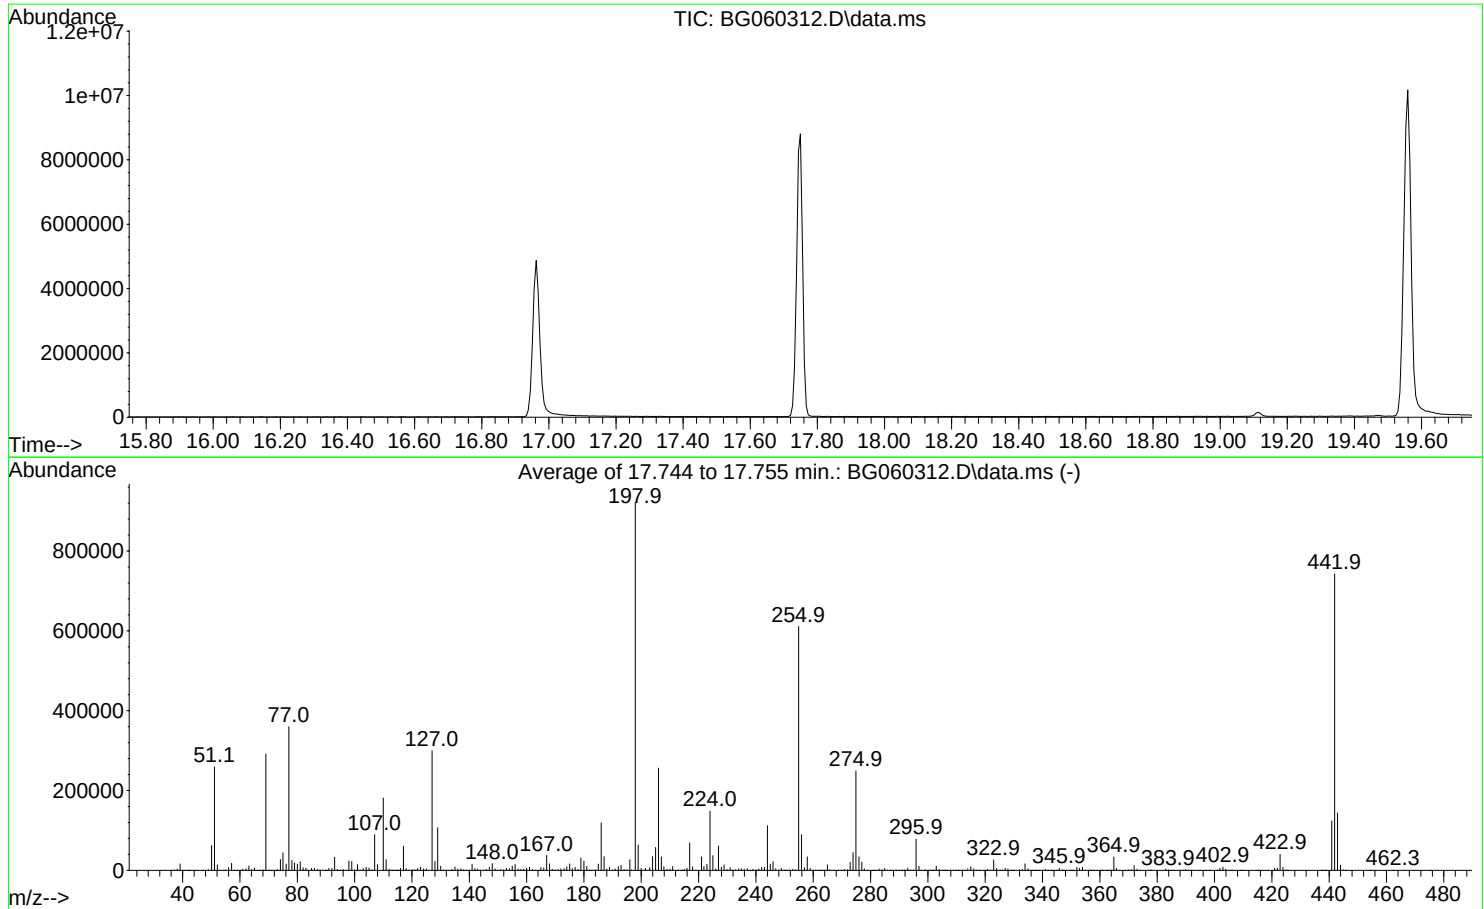




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.2	259435	PASS
68	69	0.00	2	0.4	1267	PASS
69	198	0.00	100	31.6	291553	PASS
70	69	0.00	2	0.4	1202	PASS
127	198	10	80	32.5	299712	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	921493	PASS
199	198	5	9	6.9	63448	PASS
275	198	10	60	27.1	249451	PASS
365	198	1	100	3.6	33413	PASS
441	198	0.01	100	13.4	123717	PASS
442	442	50	100	100.0	742549	PASS
443	442	15	24	19.4	144112	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011224\
 Data File : BG060312.D
 Acq On : 12 Jan 2024 12:20
 Operator : MA/JU
 Sample : DFTPP
 Misc : 8270 SURROGATES
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jan 12 13:51:24 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 09 04:07:12 2024
 Response via : Initial Calibration

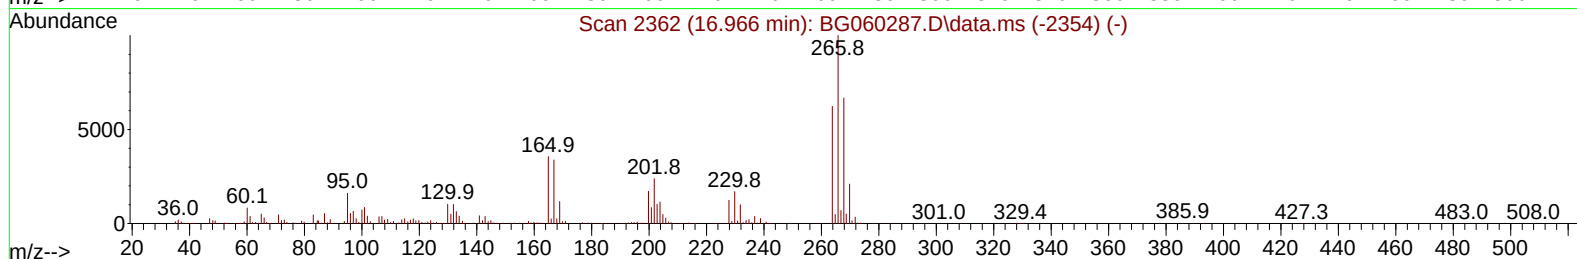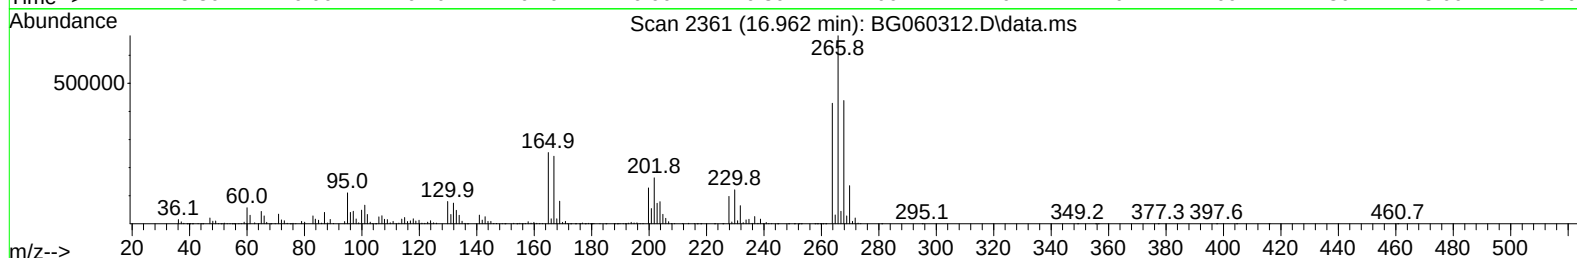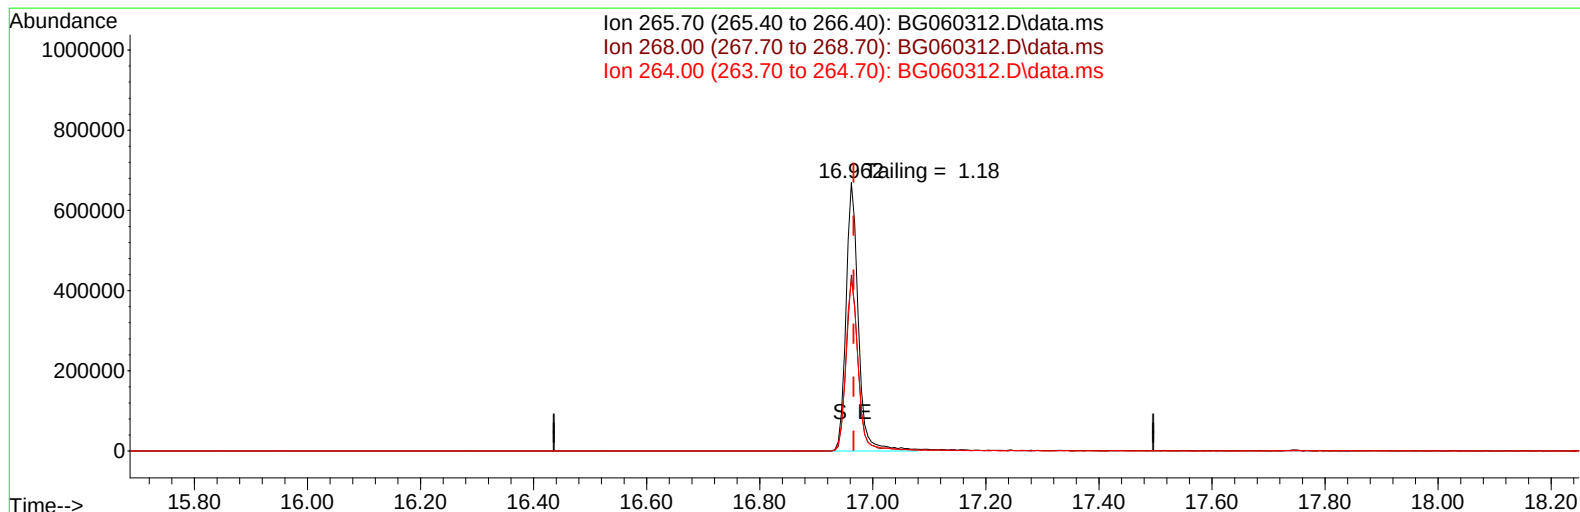

TIC: BG060312.D\data.ms

(70) Pentachlorophenol (C)

16.962min (-0.004) 168112.82 ng




response 1018320

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	71.80	65.53
264.00	62.30	64.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011224\
Data File : BG060312.D
Acq On : 12 Jan 2024 12:20
Operator : MA/JU
Sample : DFTPP
Misc : 8270 SURROGATES
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 12 13:51:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

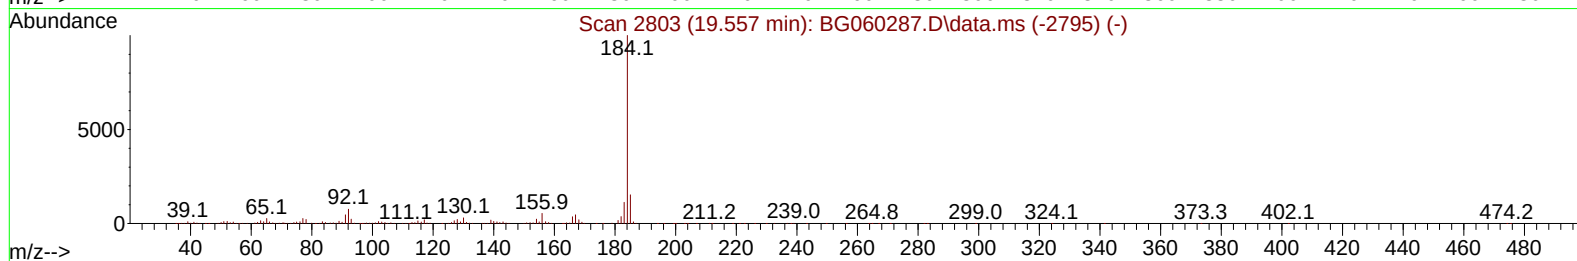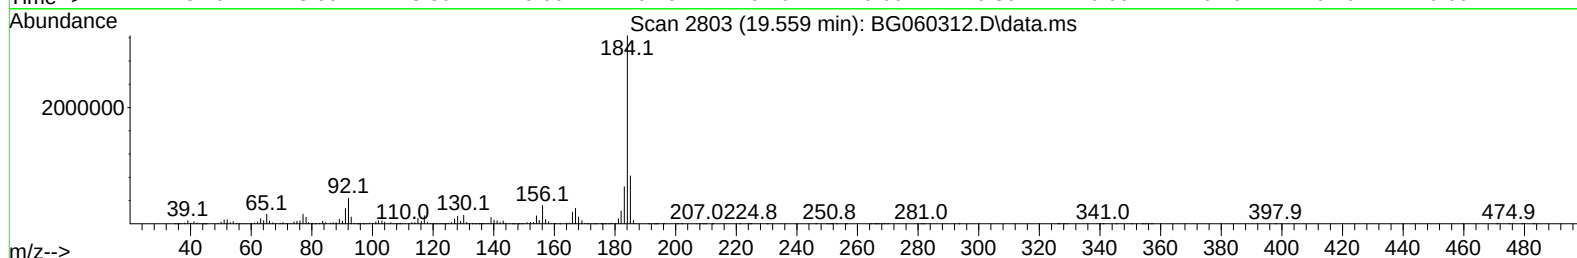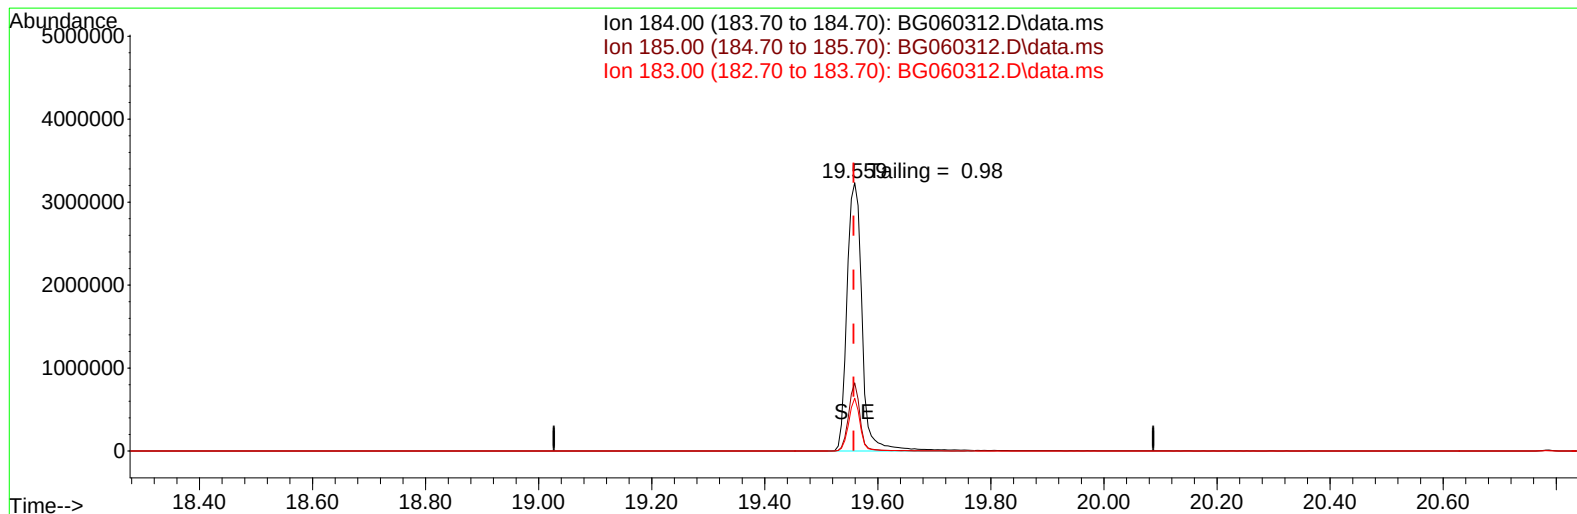

TIC: BG060312.D\data.ms

(77) Benzidine

19.559min (+ 0.002) 205009.62 ng

response 6030548

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	25.43#
183.00	11.20	19.70#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/12/2024	BNA_G	<u>BG060312.D</u>
Compound Name	Response	Retention Time
DDT	3164848	20.787
DDD	112807	20.341
DDE	1410	19.841
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
114217	3279065	3.48

Instrument :
BNA_G
ClientSampleId :
DFTPP