

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG011316\
 Data File : BG020708.D
 Acq On : 13 Jan 2016 19:44
 Operator : SJ/IZ
 Sample : H1096-13
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BC9A6

Quant Time: Jan 14 09:47:48 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG011216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 13 07:56:00 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.04	152	16204	20.00	ng/ul	0.00
18) Naphthalene-d8	10.86	136	70299	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.68	164	51444	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.43	188	138554	20.00	ng/ul	0.00
78) Chrysene-d12	21.70	240	166232	20.00	ng/ul	0.00
86) Perylene-d12	24.95	264	158191	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.40	96	1731	5.22	ng/uL	0.00
5) Phenol-d5	7.20	99	38587	27.79	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.36	67	24426	29.25	ng/ul	0.00
9) 2-Chlorophenol-d4	7.57	132	31666	29.07	ng/ul	0.00
13) 4-Methylphenol-d8	8.75	113	34411	29.38	ng/ul	0.00
19) Nitrobenzene-d5	9.21	128	17236	31.08	ng/ul	0.00
22) 2-Nitrophenol-d4	9.94	143	20589	31.95	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.48	165	36165	29.48	ng/ul	0.00
29) 4-Chloroaniline-d4	11.00	131	49285	40.58	ng/ul	0.00
44) Dimethylphthalate-d6	14.08	166	147319	32.82	ng/ul	0.00
47) Acenaphthylene-d8	14.38	160	164792	32.69	ng/ul	0.00
52) 4-Nitrophenol-d4	14.89	143	21488	35.64	ng/ul	0.00
58) Fluorene-d10	15.67	176	136339	34.07	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.80	200	25697	34.10	ng/ul	0.00
71) Anthracene-d10	17.53	188	245000	36.08	ng/ul	0.00
79) Pyrene-d10	19.81	212	311397	39.38	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.73	264	332897	39.48	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.12	163	53843	11.16	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG011316\
Data File : BG020708.D
Acq On : 13 Jan 2016 19:44
Operator : SJ/IZ
Sample : H1096-13
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BC9A6

Quant Time: Jan 14 09:47:48 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG011216.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 13 07:56:00 2016
Response via : Initial Calibration

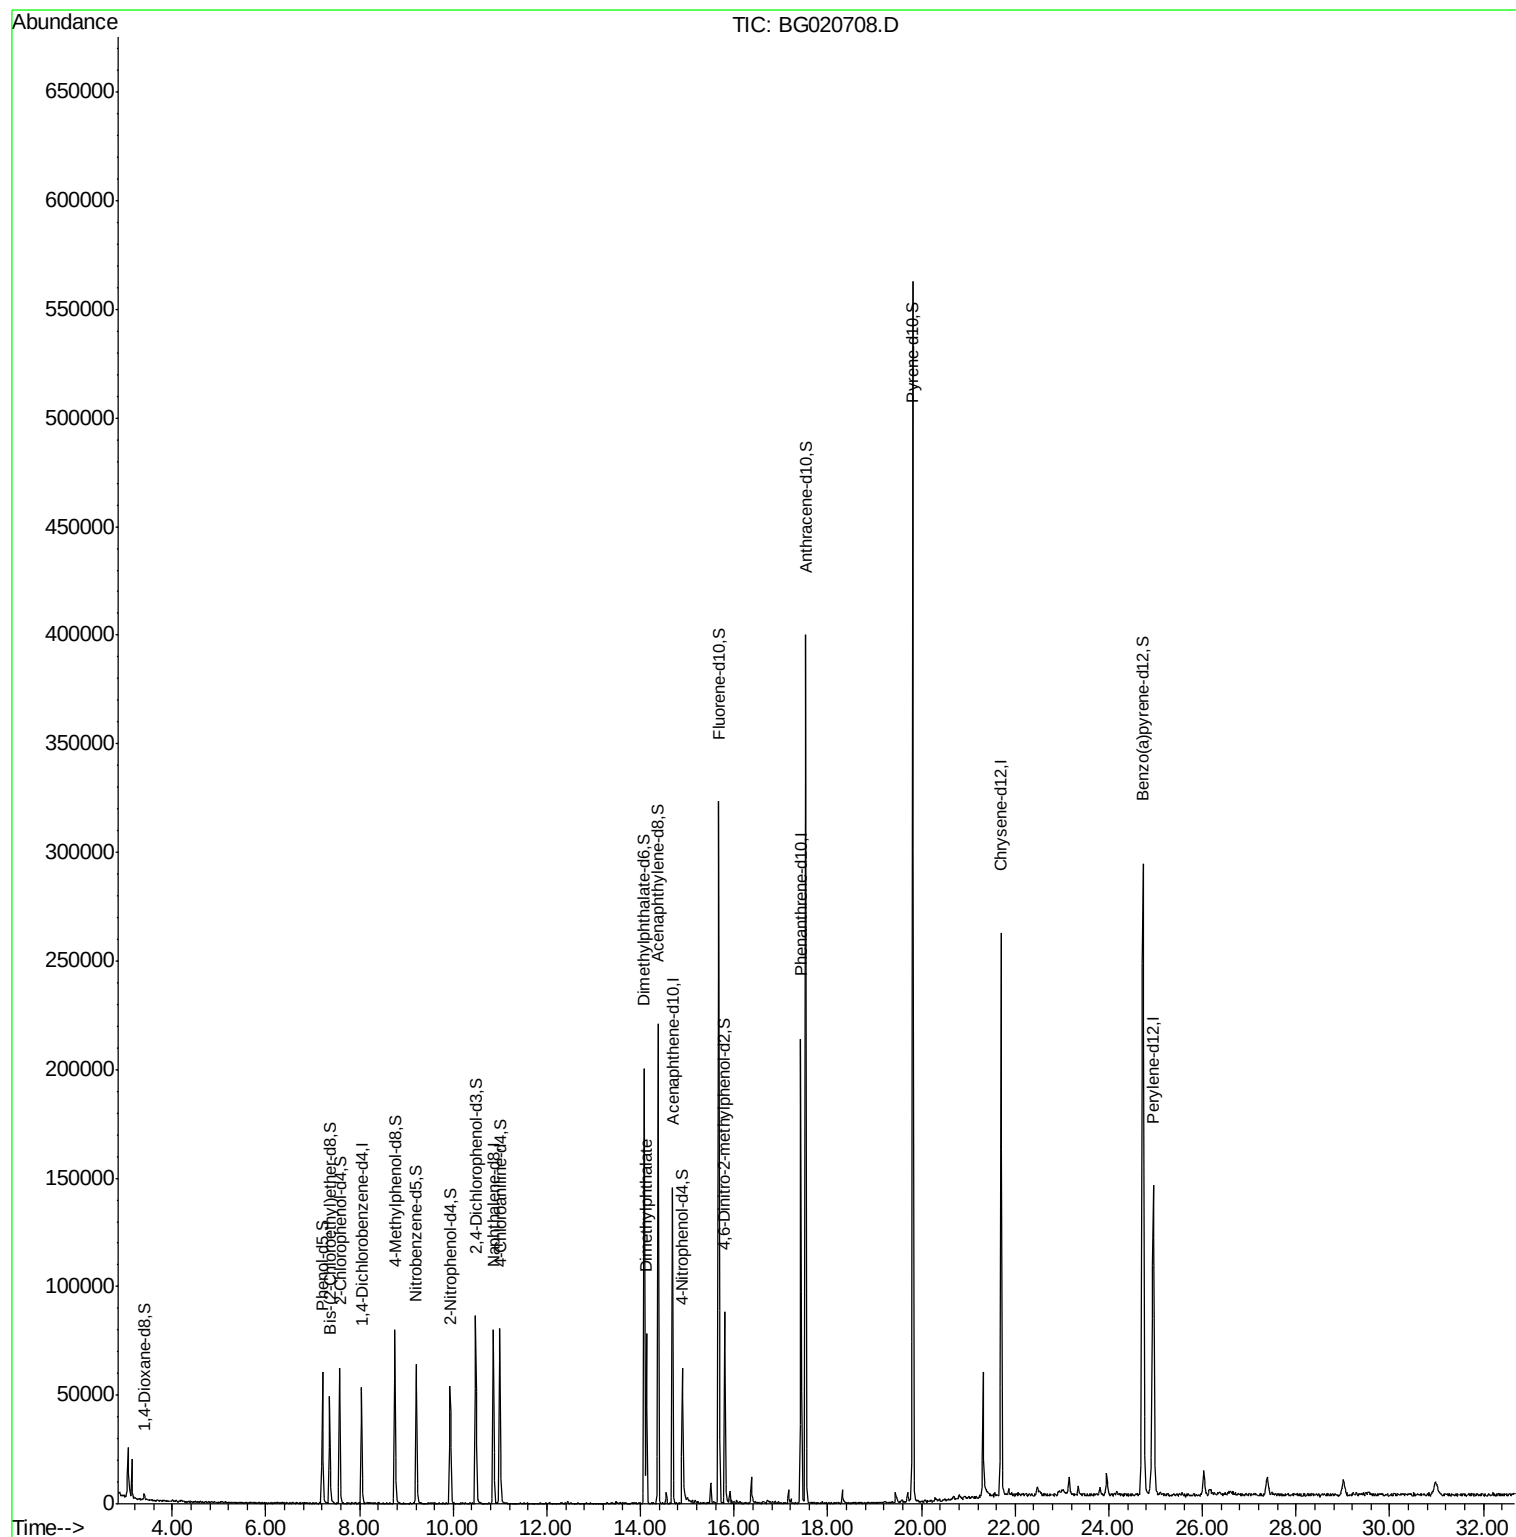

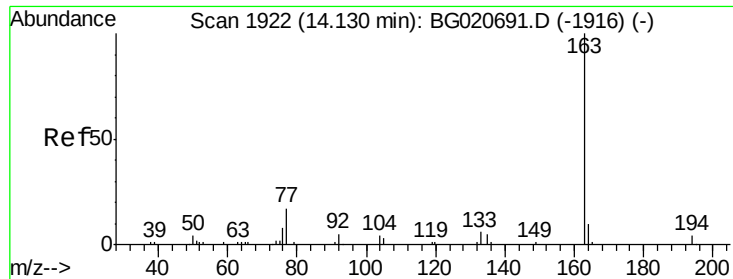

#45

Dimethylphthalate

Concen: 11.16 ng/ul

RT: 14.12 min Scan# 1921

Delta R.T. -0.01 min

Lab File: BG020708.D

Acq: 13 Jan 2016 19:44

Instrument :

BNA_G

ClientSampleId :

BC9A6

Tgt Ion:163 Resp: 53843

Ion Ratio Lower Upper

163 100

194 4.2 4.0 6.0

164 9.7 8.4 12.6

