

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG011316\
 Data File : BG020715.D
 Acq On : 14 Jan 2016 00:17
 Operator : SJ/IZ
 Sample : H1096-20
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BC9C6

Quant Time: Jan 14 10:23:46 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG011216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 13 07:56:00 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.04	152	17654	20.00	ng/ul	0.00
18) Naphthalene-d8	10.86	136	78929	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.68	164	56355	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.43	188	146739	20.00	ng/ul	0.00
78) Chrysene-d12	21.70	240	173615	20.00	ng/ul	0.00
86) Perylene-d12	24.95	264	162914	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.40	96	2022	5.60	ng/uL	0.00
5) Phenol-d5	7.20	99	42482	28.08	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.36	67	27225	29.92	ng/ul	0.00
9) 2-Chlorophenol-d4	7.57	132	35833	30.20	ng/ul	0.00
13) 4-Methylphenol-d8	8.75	113	37819	29.64	ng/ul	0.00
19) Nitrobenzene-d5	9.21	128	18843	30.26	ng/ul	0.00
22) 2-Nitrophenol-d4	9.94	143	22436	31.01	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.48	165	40286	29.25	ng/ul	0.00
29) 4-Chloroaniline-d4	10.99	131	54519	39.99	ng/ul	0.00
44) Dimethylphthalate-d6	14.08	166	156183	31.76	ng/ul	0.00
47) Acenaphthylene-d8	14.38	160	180576	32.70	ng/ul	0.00
52) 4-Nitrophenol-d4	14.89	143	19474	29.49	ng/ul	0.00
58) Fluorene-d10	15.67	176	146198	33.35	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.80	200	23935	29.99	ng/ul	0.00
71) Anthracene-d10	17.53	188	243332	33.83	ng/ul	0.00
79) Pyrene-d10	19.81	212	295542	35.78	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.73	264	310972	35.81	ng/ul	0.00


Target Compounds						Qvalue
45) Dimethylphthalate	14.12	163	52907	10.01	ng/ul#	96




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG011316\
Data File : BG020715.D
Acq On : 14 Jan 2016 00:17
Operator : SJ/IZ
Sample : H1096-20
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BC9C6

Quant Time: Jan 14 10:23:46 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG011216.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 13 07:56:00 2016
Response via : Initial Calibration

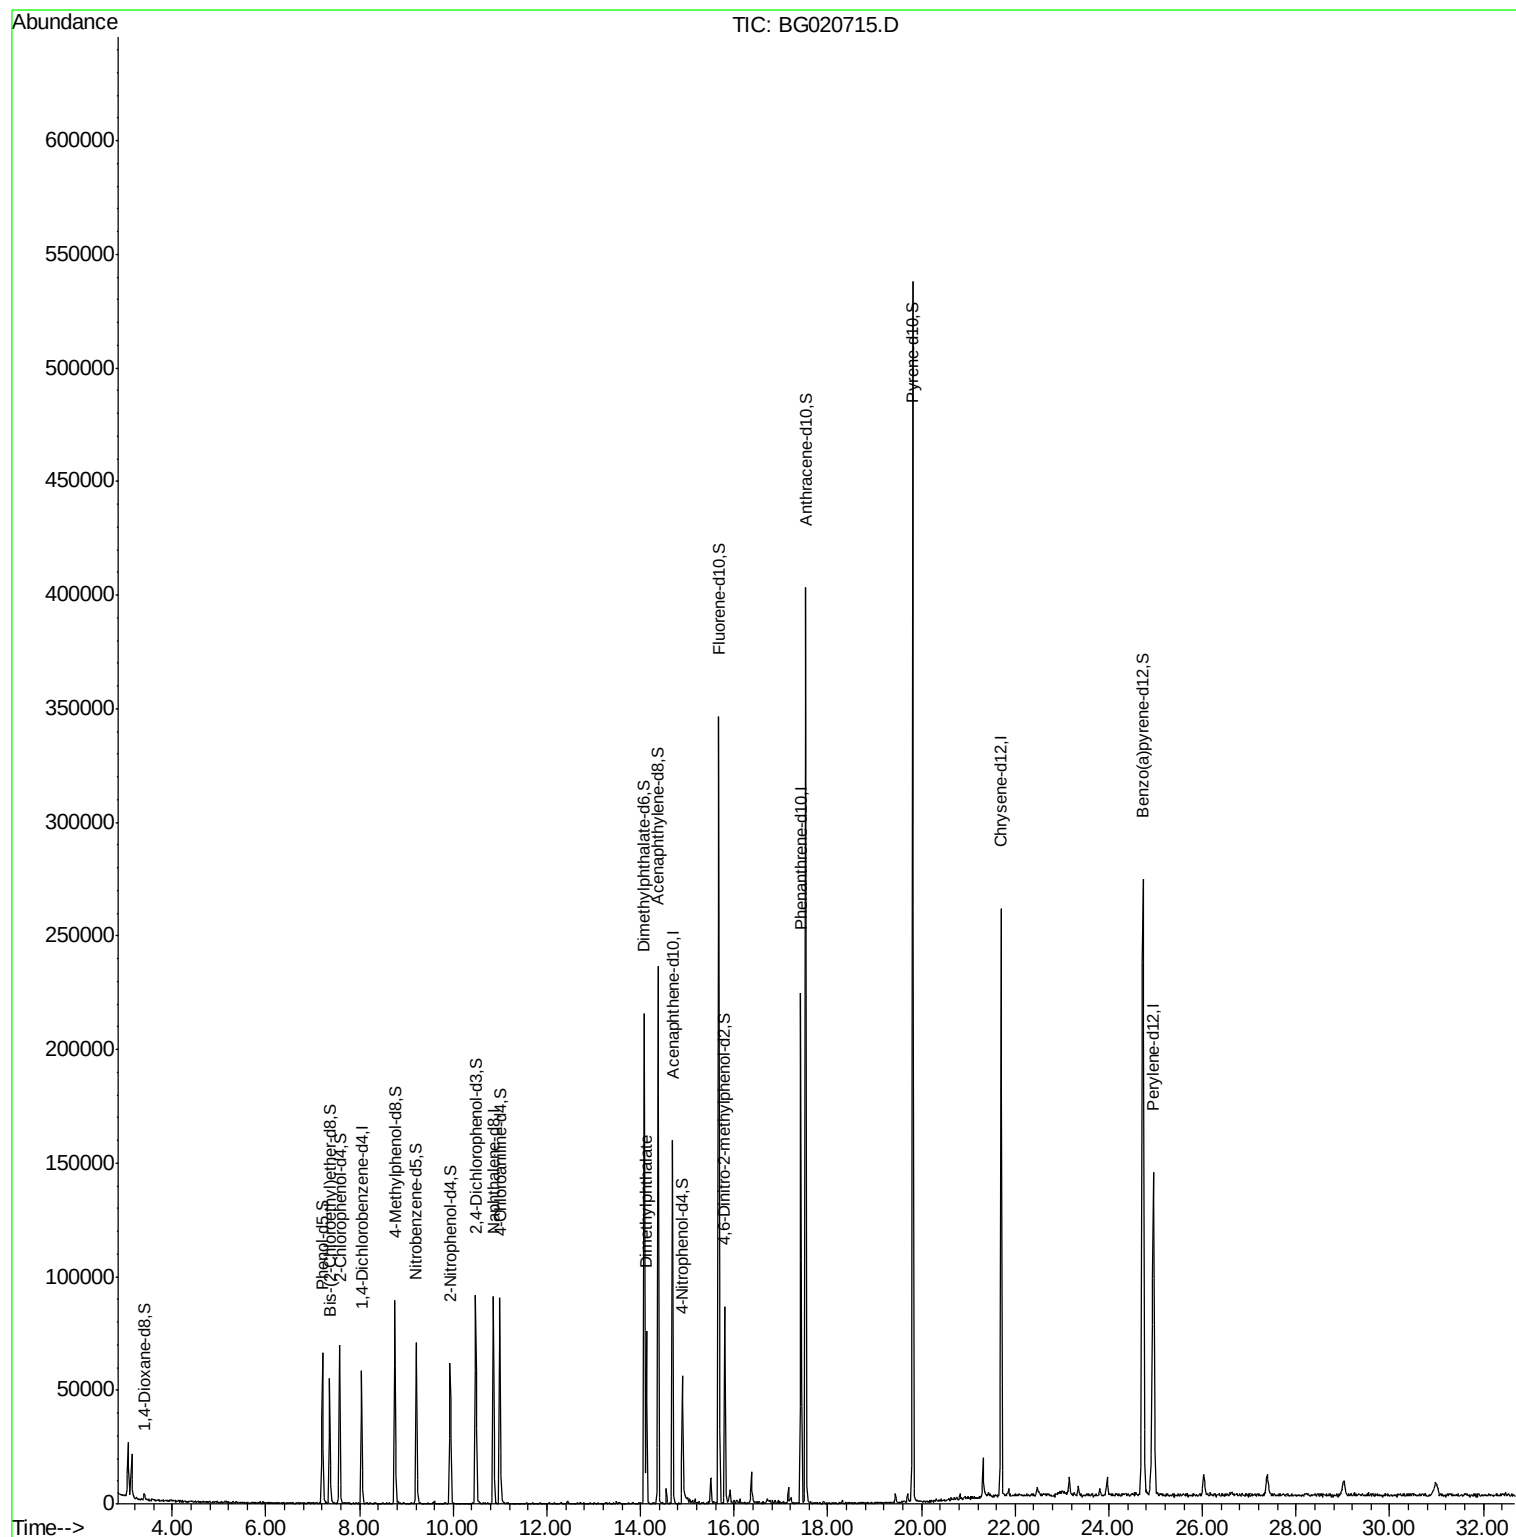

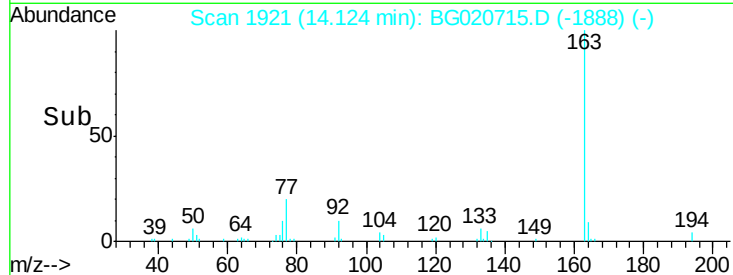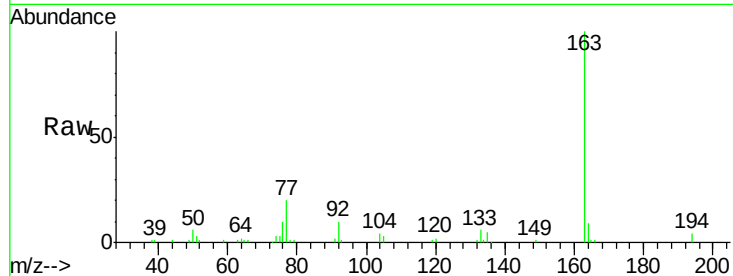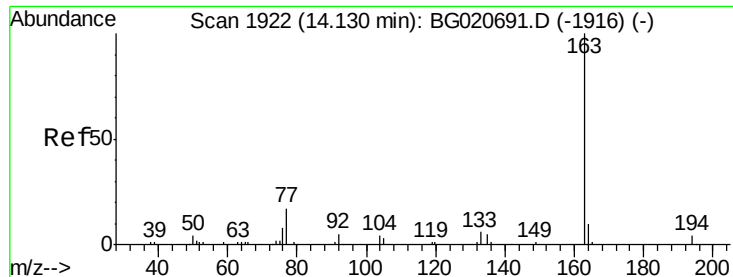

#45
 Dimethylphthalate
 Concen: 10.01 ng/ul
 RT: 14.12 min Scan# 1921
 Delta R.T. -0.01 min
 Lab File: BG020715.D
 Acq: 14 Jan 2016 00:17

Instrument :
 BNA_G
 ClientSampleId :
 BC9C6

Tgt Ion:	163	Resp:	52907
Ion	Ratio	Lower	Upper
163	100		
194	3.8	4.0	6.0#
164	9.1	8.4	12.6

