
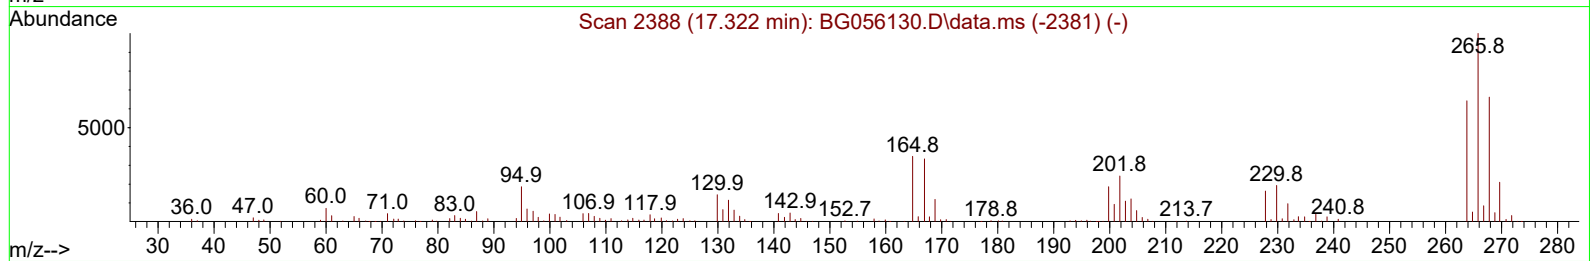
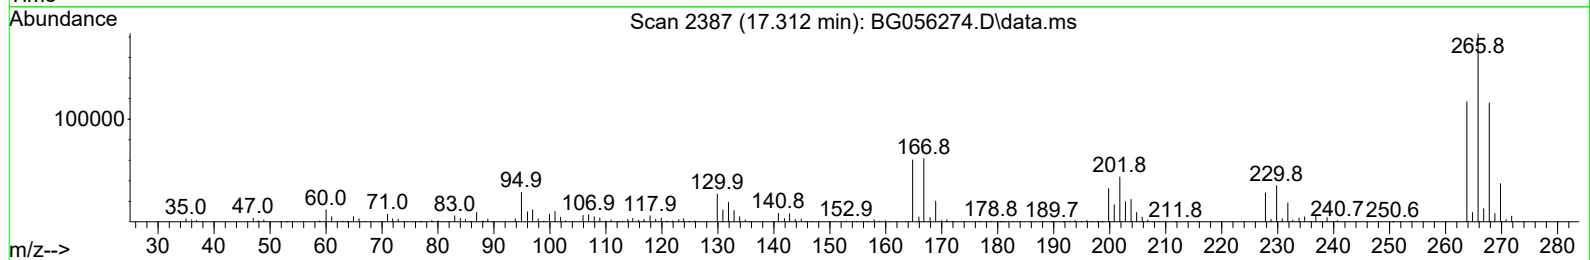


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011323\
Data File : BG056274.D
Acq On : 13 Jan 2023 12:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 16 03:27:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 12 03:38:40 2023
Response via : Initial Calibration

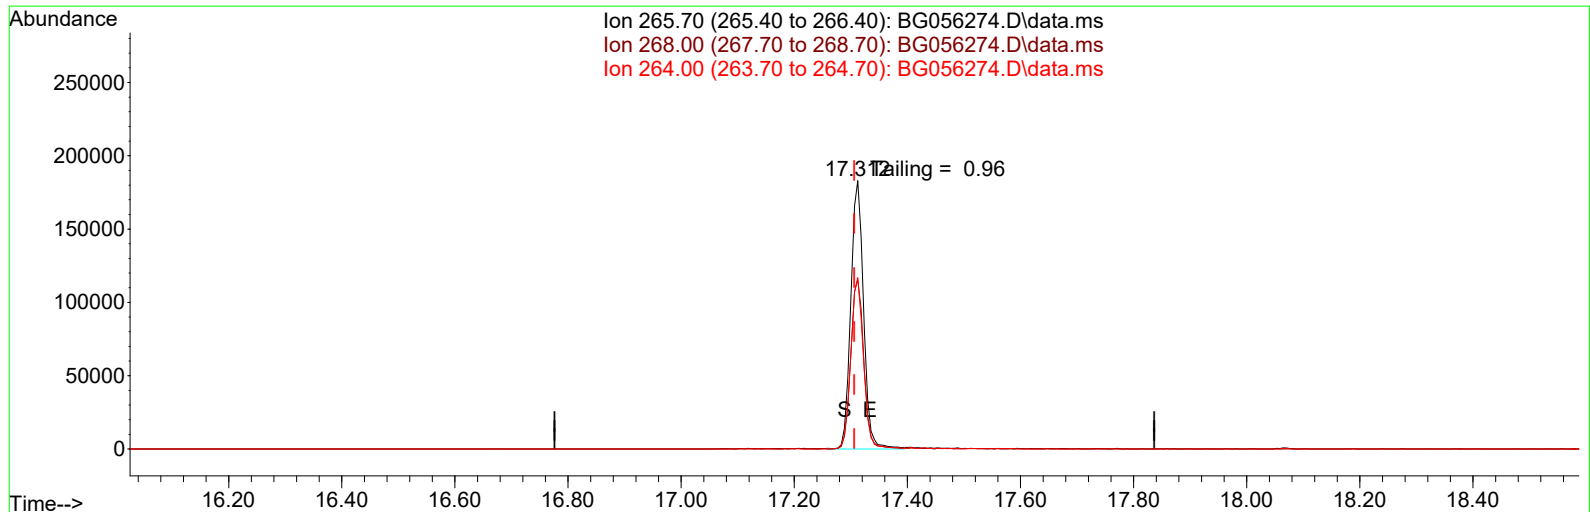

TIC: BG056274.D\data.ms

(70) Pentachlorophenol (C)




17.312min (+ 0.006) 238485.60 ng

response 285119

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	63.16
264.00	64.30	63.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011323\
 Data File : BG056274.D
 Acq On : 13 Jan 2023 12:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 16 03:27:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 12 03:38:40 2023
 Response via : Initial Calibration

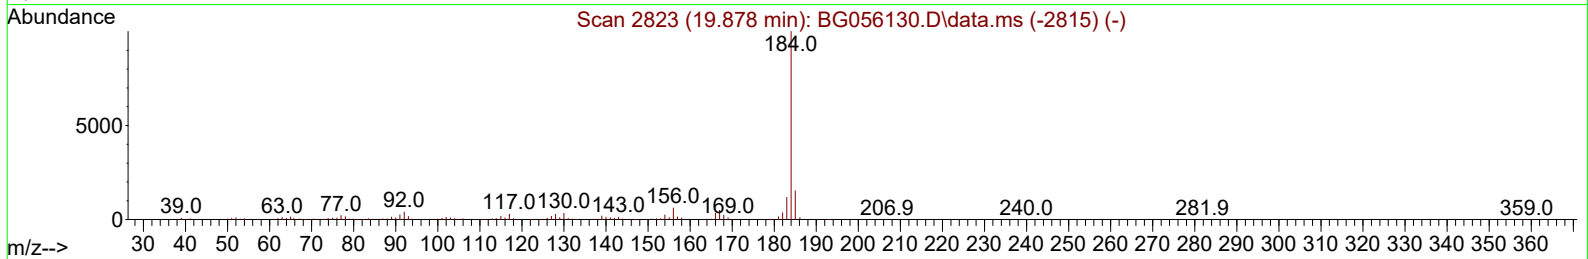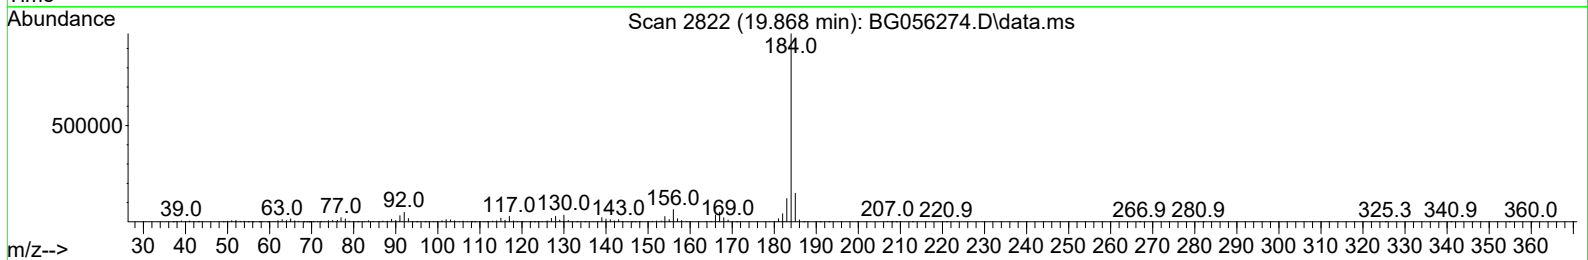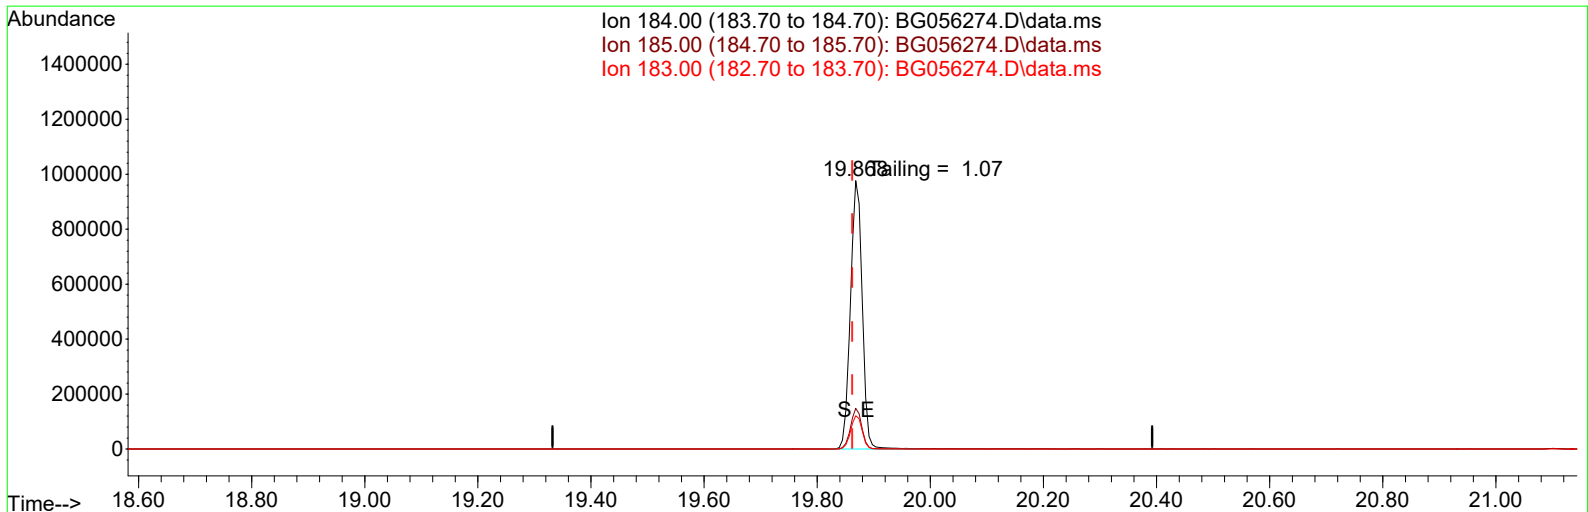

TIC: BG056274.D\data.ms

(77) Benzidine**19.868min (+ 0.006) 12482.88 ng****response 1418663**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	15.16
183.00	11.70	12.39
0.00	0.00	0.00