


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011323\
Data File : BG056274.D
Acq On : 13 Jan 2023 12:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jan 12 03:38:40 2023

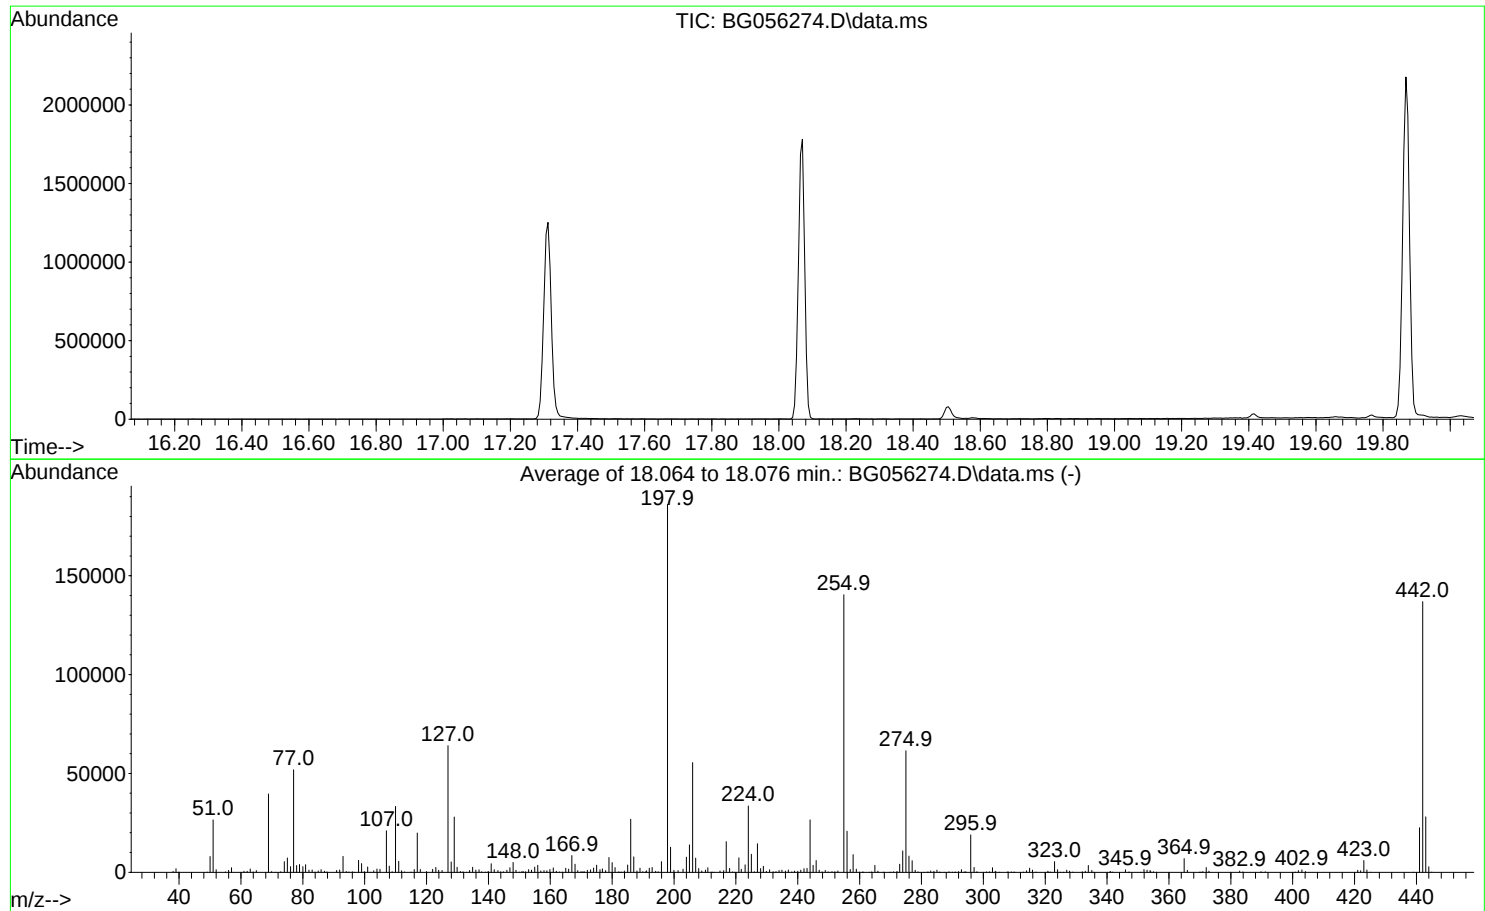




AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	14.3	26538	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	21.3	39587	PASS
70	69	0.00	2	1.0	400	PASS
127	198	10	80	34.4	64035	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	186077	PASS
199	198	5	9	6.8	12643	PASS
275	198	10	60	33.0	61456	PASS
365	198	1	100	3.7	6919	PASS
441	198	0.01	100	12.1	22549	PASS
442	442	50	100	100.0	136885	PASS
443	442	15	24	20.5	28061	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011323\
Data File : BG056274.D
Acq On : 13 Jan 2023 12:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 16 03:27:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 12 03:38:40 2023
Response via : Initial Calibration

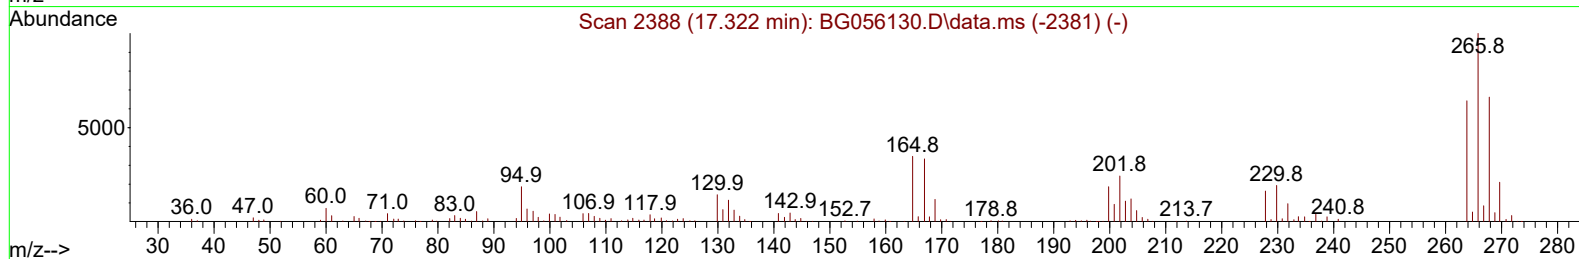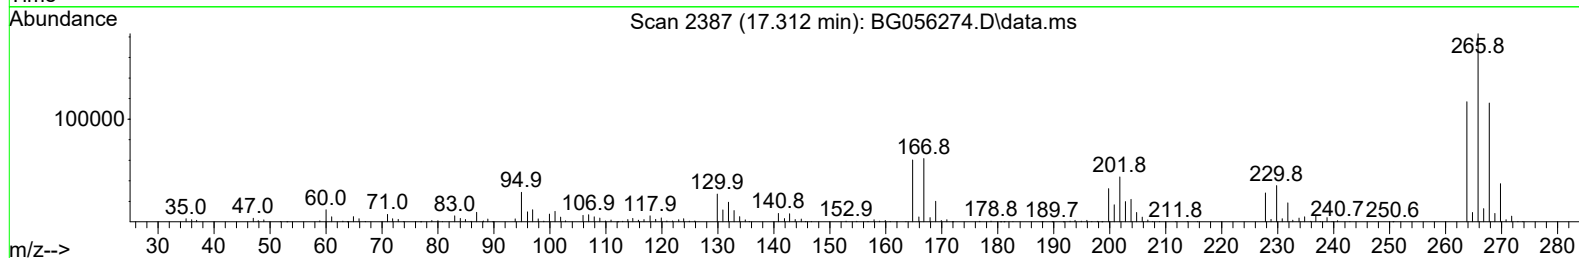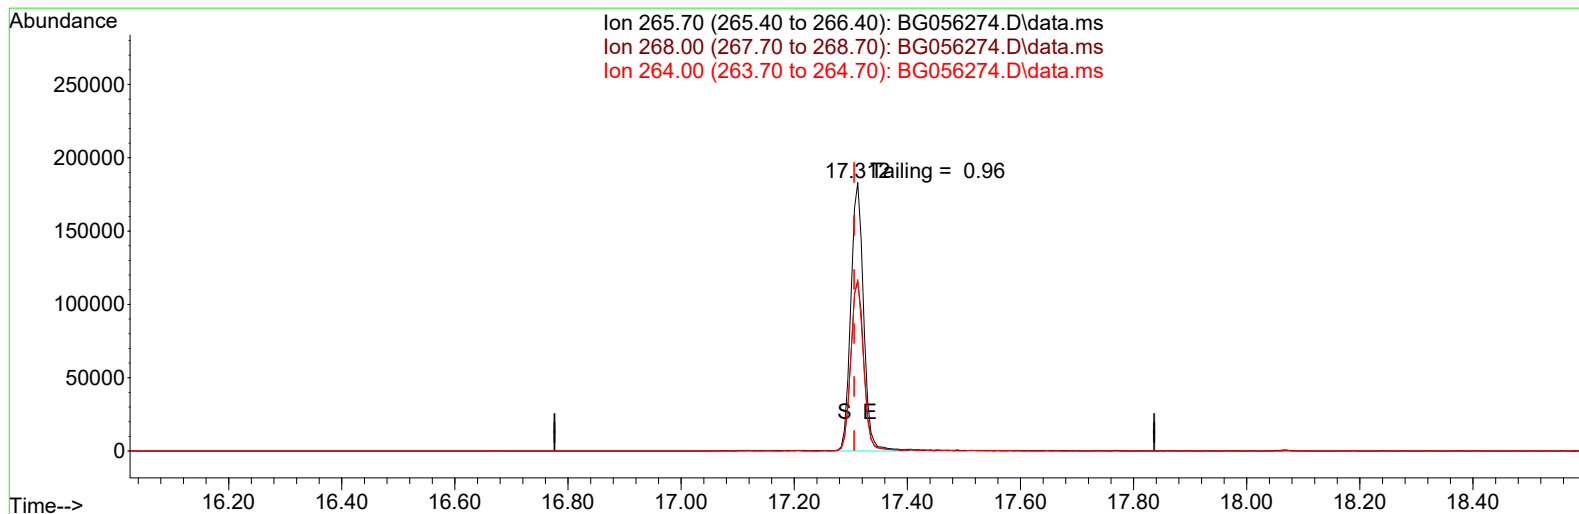

TIC: BG056274.D\data.ms

(70) Pentachlorophenol (C)

17.312min (+ 0.006) 238485.60 ng




response 285119

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	63.16
264.00	64.30	63.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011323\
 Data File : BG056274.D
 Acq On : 13 Jan 2023 12:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jan 16 03:27:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 12 03:38:40 2023
 Response via : Initial Calibration

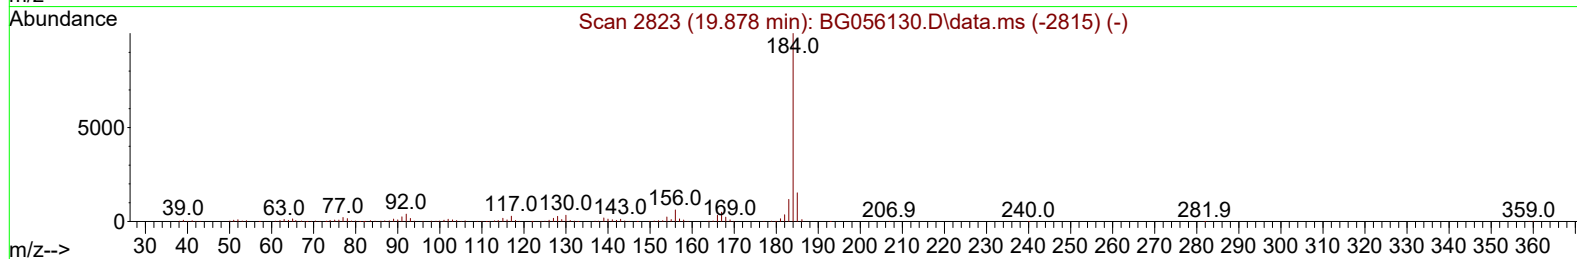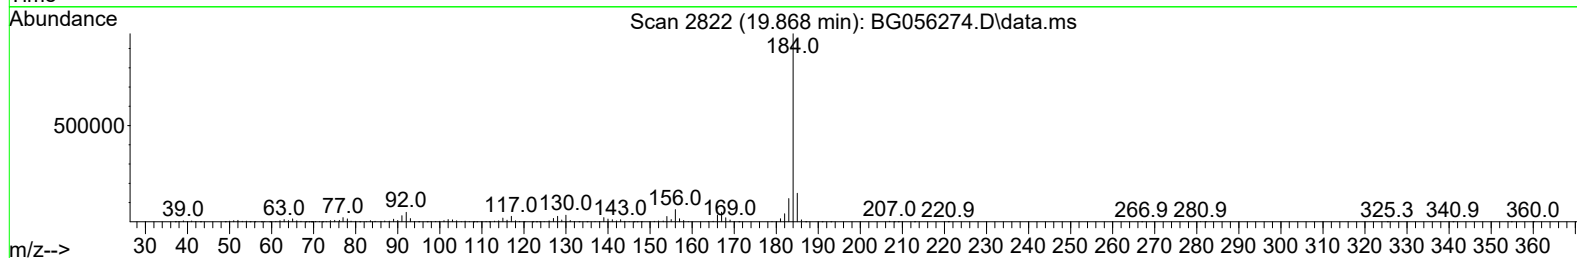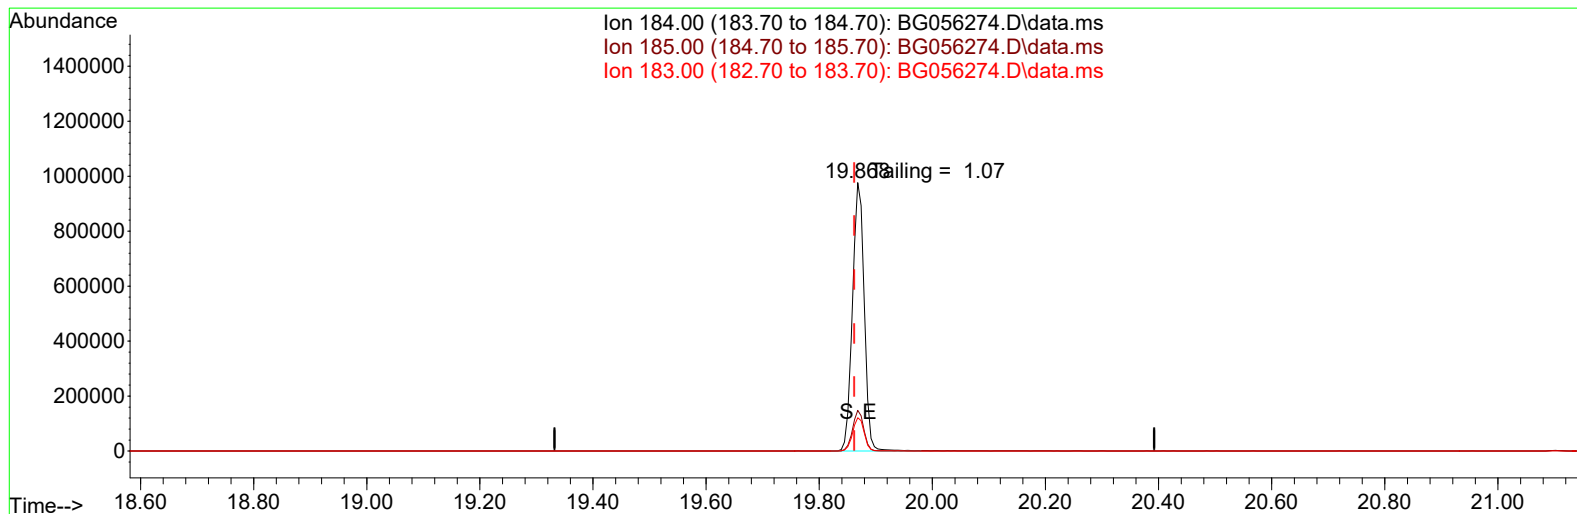

TIC: BG056274.D\data.ms

(77) Benzidine

19.868min (+ 0.006) 12482.88 ng

response 1418663

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	15.16
183.00	11.70	12.39
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/13/2023	BNA_G	BG056274.D
Compound Name	Response	Retention Time
DDT	718712	21.102
DDD	33833	20.65
DDE	1771	20.144
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
35604	754316	4.72

Instrument :
BNA_G
ClientSampleId :
DFTPP