

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG011416\
 Data File : BG020734.D
 Acq On : 14 Jan 2016 21:50
 Operator : SJ/IZ
 Sample : H1101-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BC9B2

Manual Integrations
 APPROVED

mohammad
 1/15/2016 2:43:58 PM

Quant Time: Jan 15 00:11:31 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG011216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 14 23:48:02 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.04	152	17857	20.00	ng/ul	0.00
18) Naphthalene-d8	10.86	136	75253	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.68	164	53963	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.43	188	137528	20.00	ng/ul	0.00
78) Chrysene-d12	21.70	240	166777	20.00	ng/ul	0.00
86) Perylene-d12	24.95	264	149925	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.41	96	2000	5.47	ng/uL	0.00
5) Phenol-d5	7.20	99	48370	31.61	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.36	67	30477	33.12	ng/ul	0.00
9) 2-Chlorophenol-d4	7.57	132	39991	33.32	ng/ul	0.00
13) 4-Methylphenol-d8	8.75	113	42201	32.70	ng/ul	0.00
19) Nitrobenzene-d5	9.21	128	20904	35.21	ng/ul	0.00
22) 2-Nitrophenol-d4	9.94	143	24968	36.19	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.48	165	43719	33.29	ng/ul	0.00
29) 4-Chloroaniline-d4	11.00	131	59194	45.54	ng/ul	0.00
44) Dimethylphthalate-d6	14.08	166	161537	34.30	ng/ul	0.00
47) Acenaphthylene-d8	14.38	160	190815	36.08	ng/ul	0.00
52) 4-Nitrophenol-d4	14.89	143	20946m	33.12	ng/ul	0.00
58) Fluorene-d10	15.67	176	152674	36.37	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.80	200	23725	31.72	ng/ul	0.00
71) Anthracene-d10	17.53	188	251626	37.33	ng/ul	0.00
79) Pyrene-d10	19.81	212	296390	37.36	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.73	264	317929	39.78	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.13	163	81181	16.04	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG011416\
Data File : BG020734.D
Acq On : 14 Jan 2016 21:50
Operator : SJ/IZ
Sample : H1101-04
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
BC9B2

Manual Integrations
APPROVED

mohammad
1/15/2016 2:43:58 PM

Quant Time: Jan 15 00:11:31 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG011216.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 14 23:48:02 2016
Response via : Initial Calibration

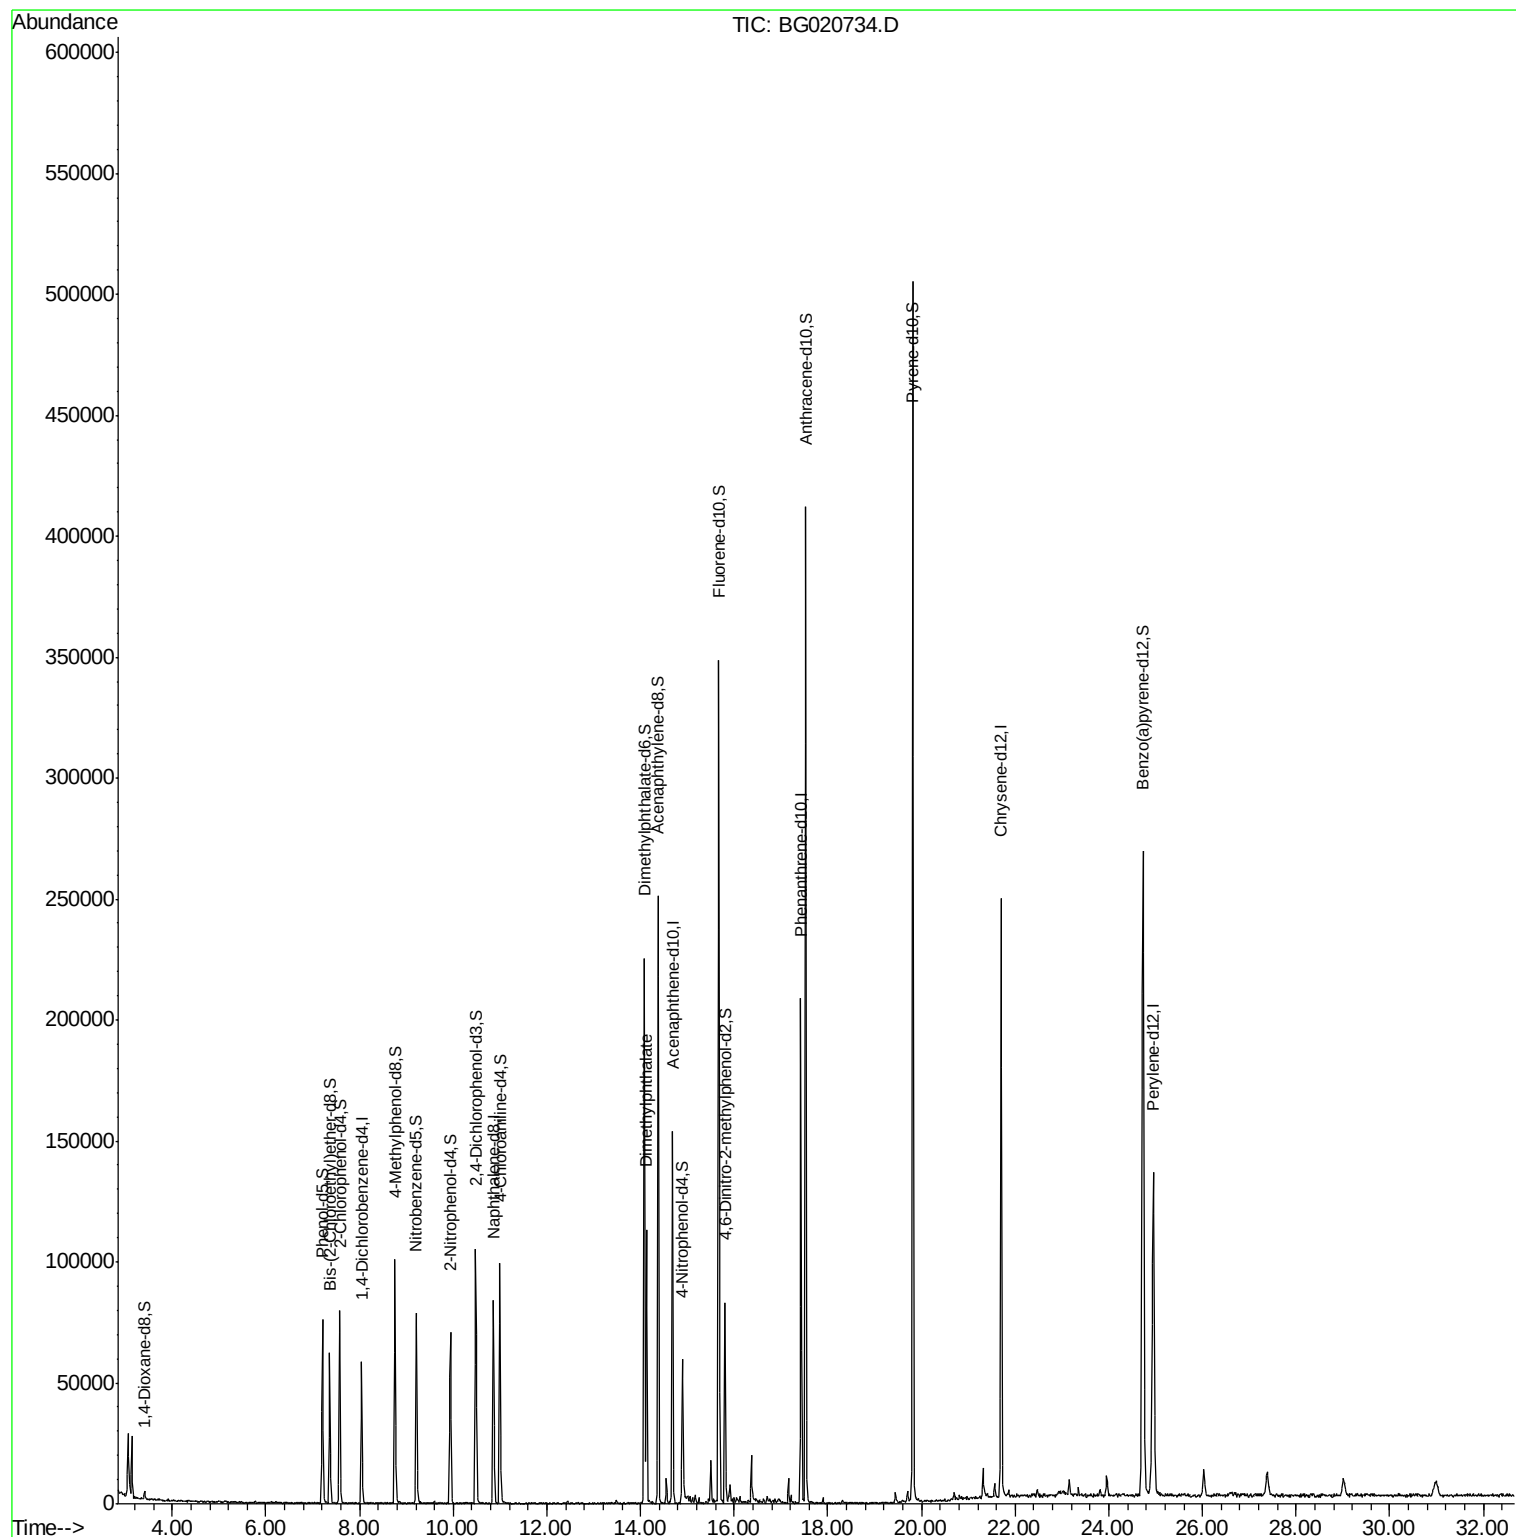

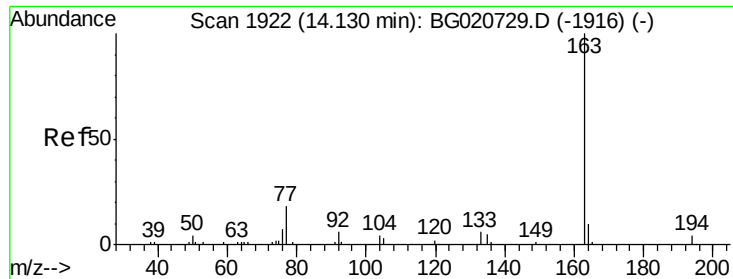


#45
 Dimethylphthalate
 Concen: 16.04 ng/ul
 RT: 14.13 min Scan# 1922
 Delta R.T. -0.00 min
 Lab File: BG020734.D
 Acq: 14 Jan 2016 21:50

Instrument :
 BNA_G
 ClientSampleId :
 BC9B2

Tgt Ion	Ratio	Resp	Lower	Upper
163	100	81181		
194	4.3		4.0	6.0
164	9.6		8.4	12.6

Manual Integrations
 APPROVED

mohammad
 1/15/2016 2:43:58 PM

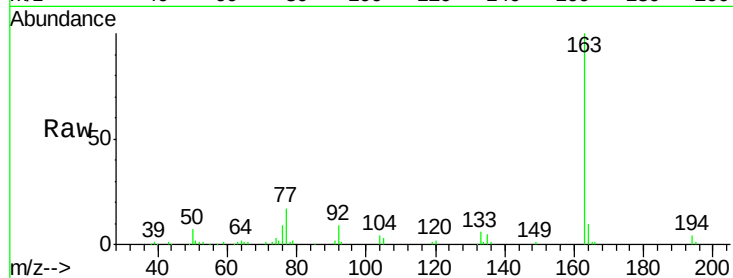

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

