

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG011416\
 Data File : BG020737.D
 Acq On : 14 Jan 2016 23:48
 Operator : SJ/IZ
 Sample : H1101-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BC9F1

Manual Integrations
 APPROVED

mohammad
 1/15/2016 2:43:33 PM

Quant Time: Jan 15 01:25:15 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG011216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 14 23:48:02 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.04	152	19535	20.00	ng/ul	0.00
18) Naphthalene-d8	10.86	136	85479	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.68	164	61706	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.43	188	154609	20.00	ng/ul	0.00
78) Chrysene-d12	21.70	240	180976	20.00	ng/ul	0.00
86) Perylene-d12	24.95	264	169605	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.40	96	1223	3.06	ng/uL	0.00
5) Phenol-d5	7.21	99	27392	16.36	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.36	67	17597	17.48	ng/ul	0.00
9) 2-Chlorophenol-d4	7.58	132	22322	17.00	ng/ul	0.00
13) 4-Methylphenol-d8	8.75	113	12457	8.82	ng/ul	0.00
19) Nitrobenzene-d5	9.21	128	12753	18.91	ng/ul	0.00
22) 2-Nitrophenol-d4	9.94	143	14512	18.52	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.48	165	24461	16.40	ng/ul	0.00
29) 4-Chloroaniline-d4	11.00	131	27410	18.56	ng/ul	0.00
44) Dimethylphthalate-d6	14.08	166	97521	18.11	ng/ul	0.00
47) Acenaphthylene-d8	14.37	160	111288	18.40	ng/ul	0.00
52) 4-Nitrophenol-d4	14.90	143	10928m	15.11	ng/ul	0.00
58) Fluorene-d10	15.67	176	89958	18.74	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.80	200	13087	15.56	ng/ul	0.00
71) Anthracene-d10	17.53	188	149636	19.75	ng/ul	0.00
79) Pyrene-d10	19.81	212	177977	20.67	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.73	264	179441	19.85	ng/ul	0.00

Target Compounds

						Qvalue
45) Dimethylphthalate	14.13	163	56853	9.83	ng/ul	99
70) Phenanthrene	17.47	178	21309	2.32	ng/ul	99
77) Fluoranthene	19.48	202	40792	3.65	ng/ul	99
80) Pyrene	19.84	202	46197	4.03	ng/ul	99
83) Benzo(a)anthracene	21.68	228	22659	2.01	ng/ul	97
85) Chrysene	21.75	228	23620	2.21	ng/ul	97
88) Benzo(b)fluoranthene	23.91	252	22099	2.02	ng/ul#	98
91) Benzo(a)pyrene	24.80	252	19696	1.87	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG011416\
Data File : BG020737.D
Acq On : 14 Jan 2016 23:48
Operator : SJ/IZ
Sample : H1101-10
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
BC9F1

Manual Integrations
APPROVED

mohammad
1/15/2016 2:43:33 PM

Quant Time: Jan 15 01:25:15 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG011216.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 14 23:48:02 2016
Response via : Initial Calibration

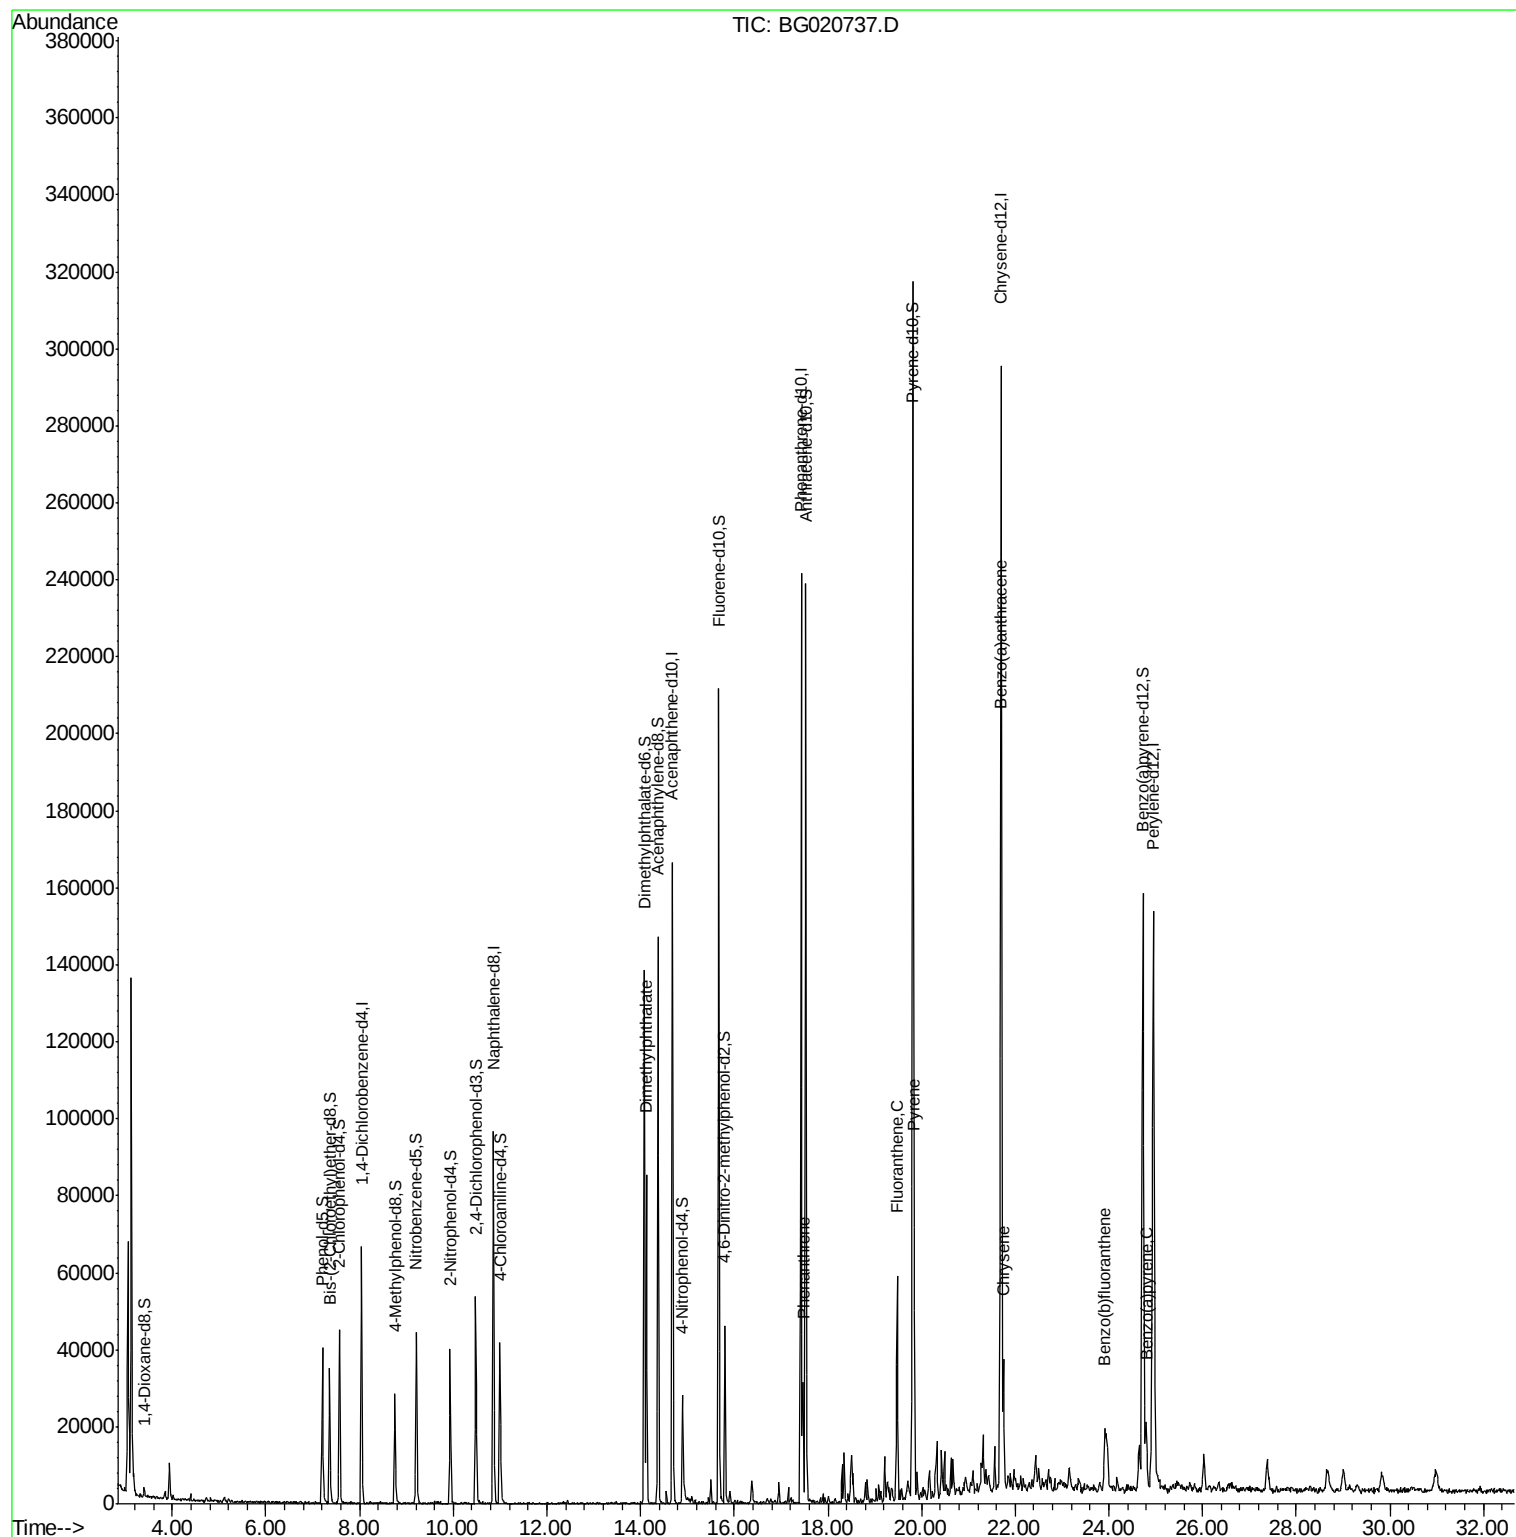

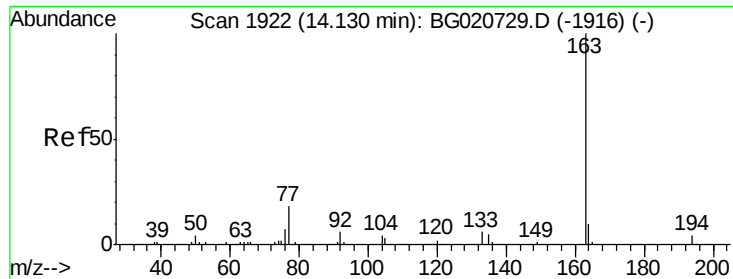

#45

Dimethylphthalate

Concen: 9.83 ng/ul

RT: 14.13 min Scan# 1921

Delta R.T. -0.00 min

Lab File: BG020737.D


Acq: 14 Jan 2016 23:48

Instrument :

BNA_G

ClientSampled :




BC9F1

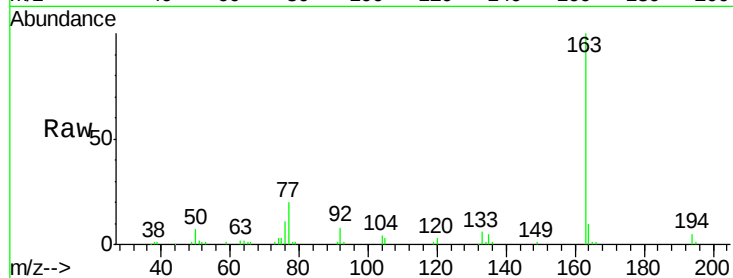

Tgt Ion:	163	Resp:	56853
Ion Ratio	Lower	Upper	
163	100		
194	4.6	4.0	6.0
164	10.2	8.4	12.6

Manual Integrations
APPROVED

mohammad
1/15/2016 2:43:33 PM

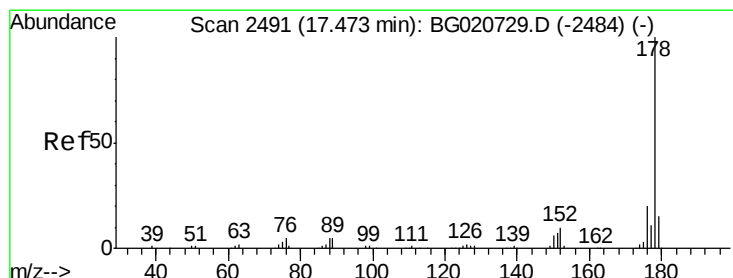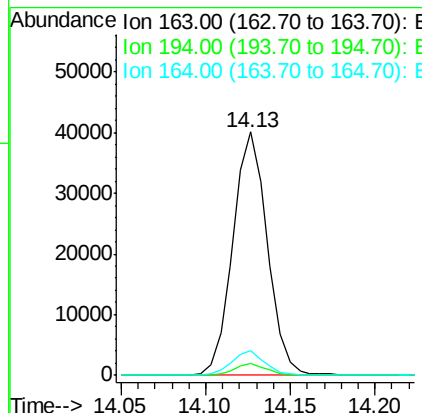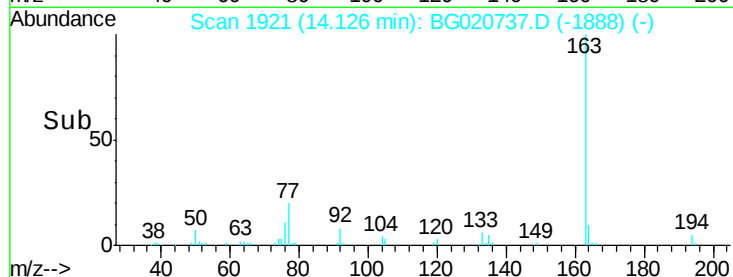

#70

Phenanthrene

Concen: 2.32 ng/ul




RT: 17.47 min Scan# 2490


Delta R.T. -0.00 min

Lab File: BG020737.D

Acq: 14 Jan 2016 23:48

Tgt Ion:	178	Resp:	21309
Ion Ratio	Lower	Upper	
178	100		
179	15.3	12.3	18.5
176	18.3	15.4	23.0

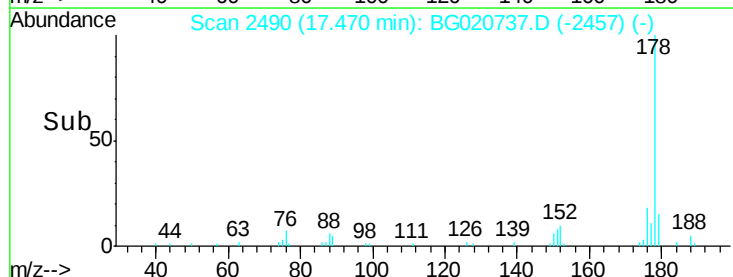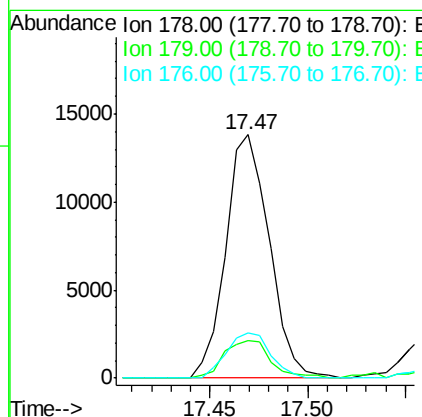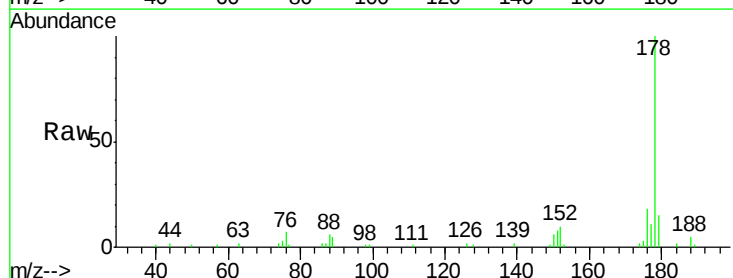

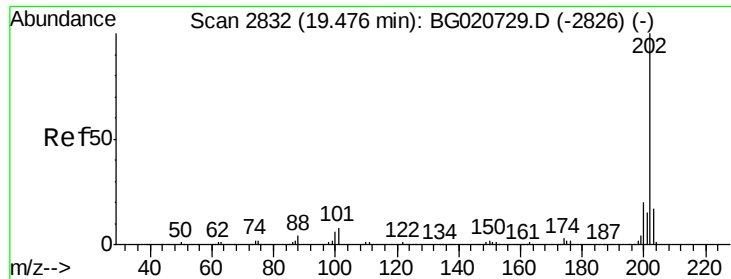





#77
Fluoranthene
Concen: 3.65 ng/ul
RT: 19.48 min Scan# 2832
Delta R.T. 0.00 min
Lab File: BG020737.D
Acq: 14 Jan 2016 23:48

Instrument :
BNA_G
ClientSampleId :
BC9F1

Tgt Ion	Ratio	Resp	Lower	Upper
202	100	40792		
101	7.3	6.1	9.1	
100	5.8	4.6	7.0	




Manual Integrations
APPROVED


mohammad
1/15/2016 2:43:33 PM

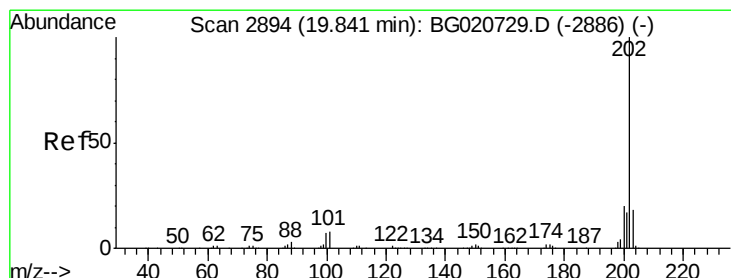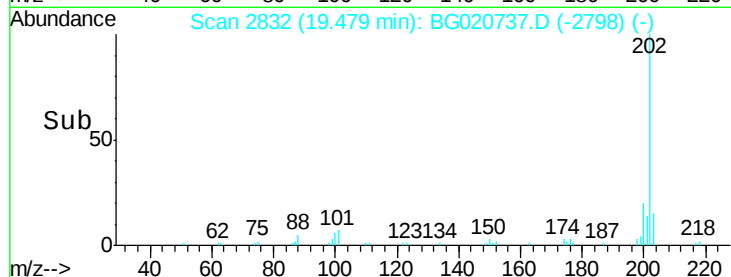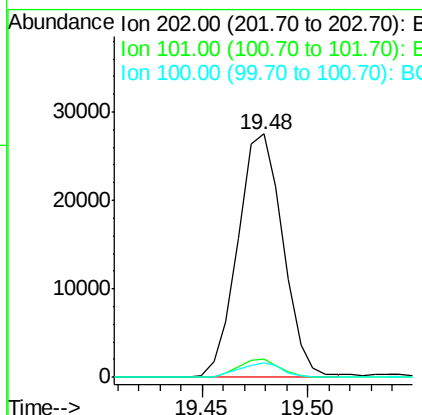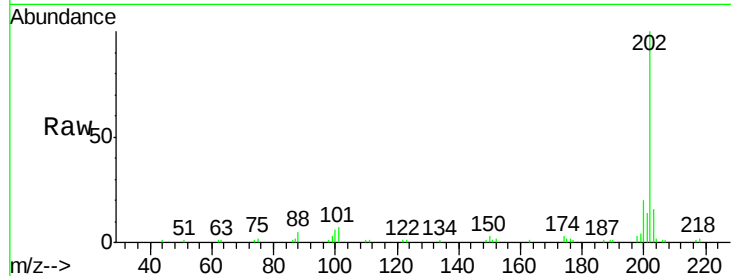

#80
Pyrene
Concen: 4.03 ng/ul
RT: 19.84 min Scan# 2893
Delta R.T. -0.00 min
Lab File: BG020737.D
Acq: 14 Jan 2016 23:48

Tgt Ion	Ratio	Resp	Lower	Upper
202	100	46197		
101	8.3	6.9	10.3	
100	7.6	5.6	8.4	

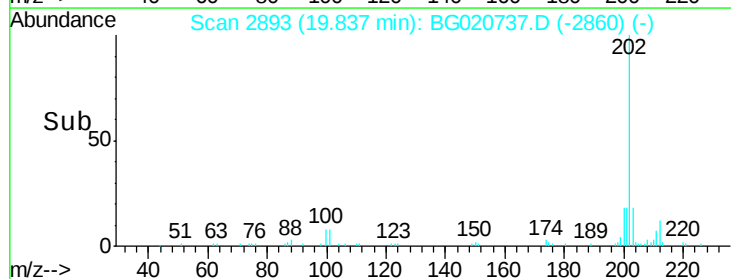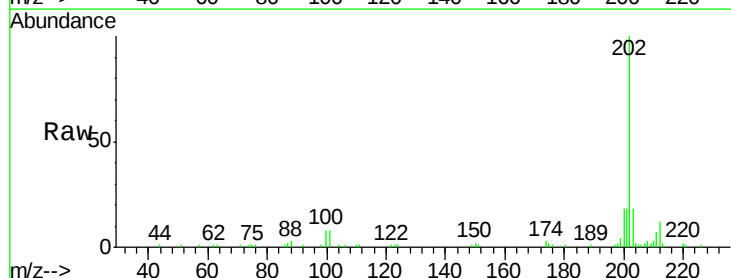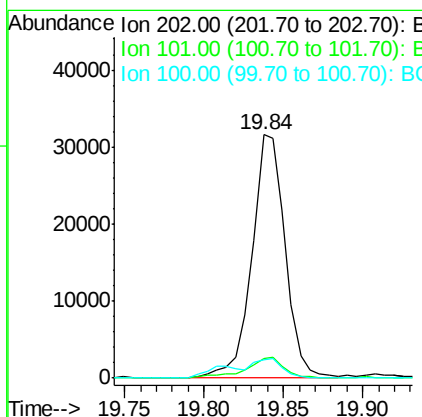

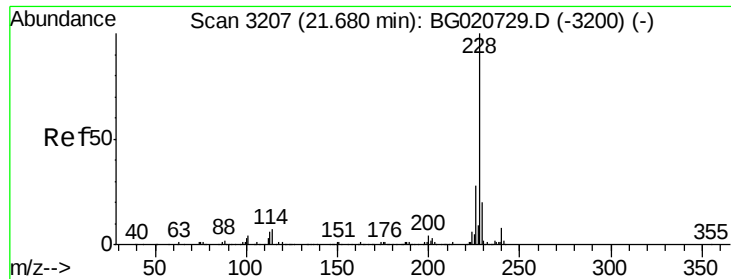





#83
Benzo(a)anthracene
Concen: 2.01 ng/ul
RT: 21.68 min Scan# 3207
Delta R.T. 0.00 min
Lab File: BG020737.D
Acq: 14 Jan 2016 23:48

Instrument :
BNA_G
ClientSampleId :
BC9F1

Tgt Ion	Ratio	Resp	Lower	Upper
228	100	22659		
229	20.1	16.0	24.0	
226	24.9	21.8	32.8	




Manual Integrations
APPROVED


mohammad
1/15/2016 2:43:33 PM

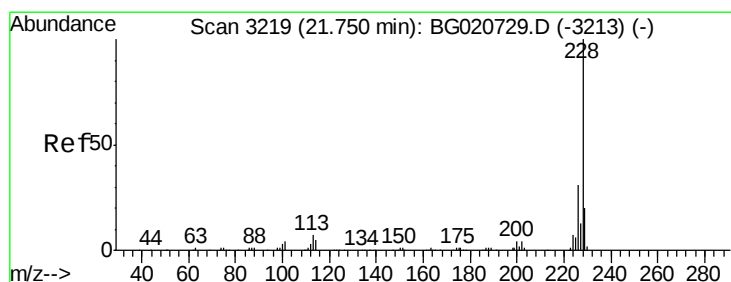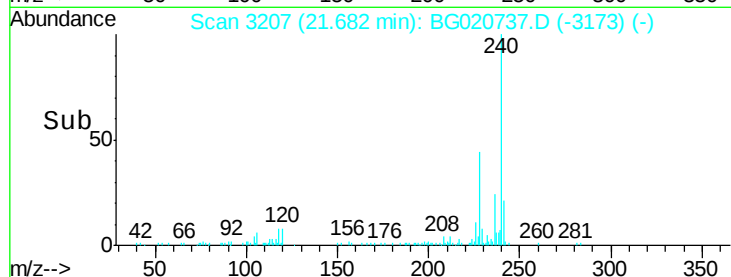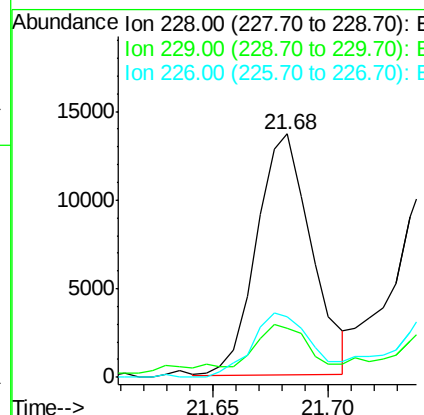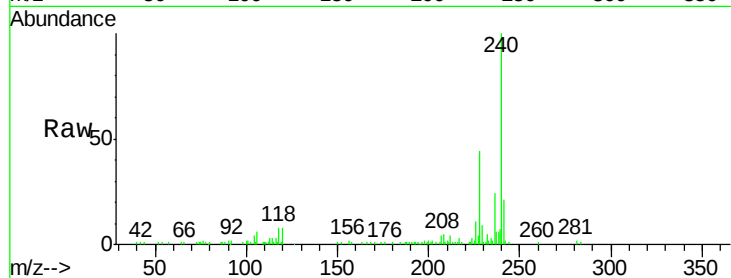

#85
Chrysene
Concen: 2.21 ng/ul
RT: 21.75 min Scan# 3218
Delta R.T. -0.00 min
Lab File: BG020737.D
Acq: 14 Jan 2016 23:48

Tgt Ion	Ratio	Resp	Lower	Upper
228	100	23620		
226	31.2	24.1	36.1	
229	21.6	16.0	24.0	

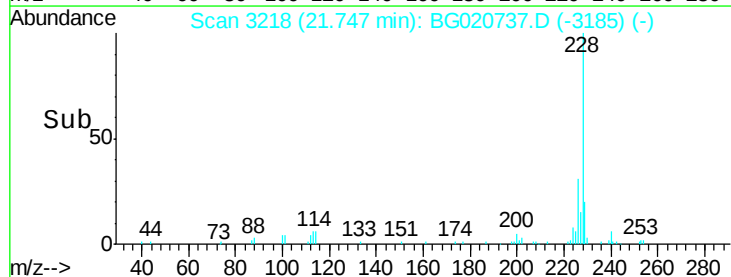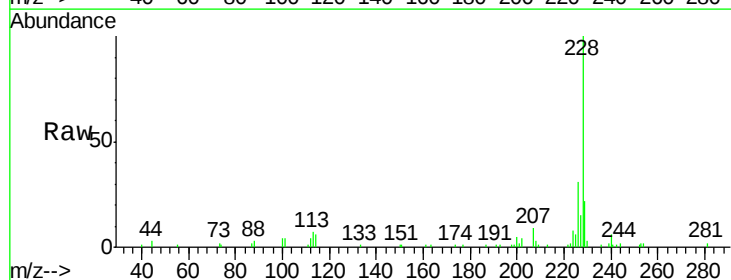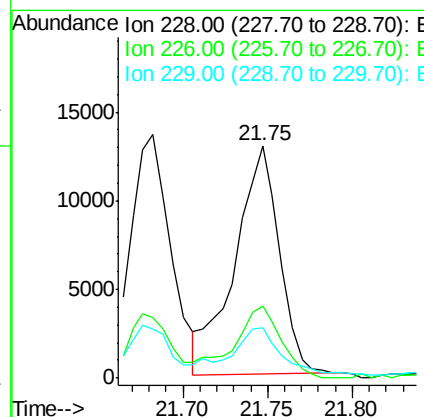

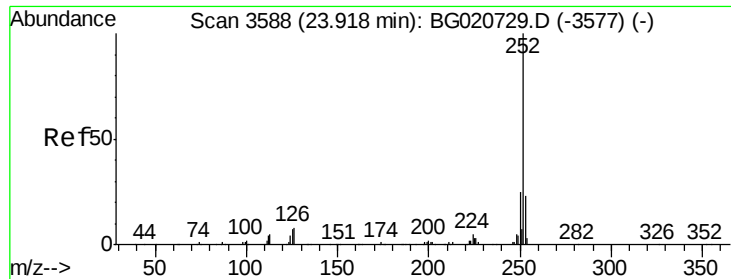





#88
Benzo(b)fluoranthene
Concen: 2.02 ng/ul
RT: 23.91 min Scan# 3587
Delta R.T. -0.00 min
Lab File: BG020737.D
Acq: 14 Jan 2016 23:48

Instrument :
BNA_G
ClientSampleId :
BC9F1

Tgt Ion	Ratio	Resp	Lower	Upper
252	100	22099		
253	22.1		17.4	26.0
125	7.4		4.9	7.3#

Manual Integrations
APPROVED

mohammad
1/15/2016 2:43:33 PM

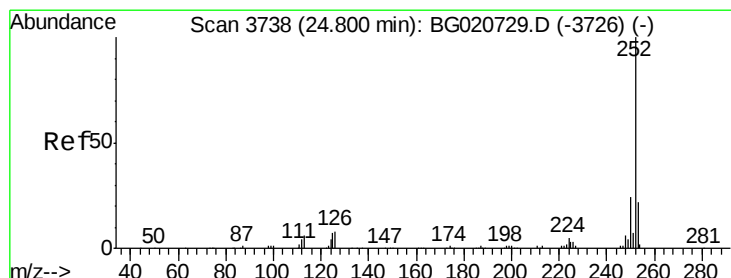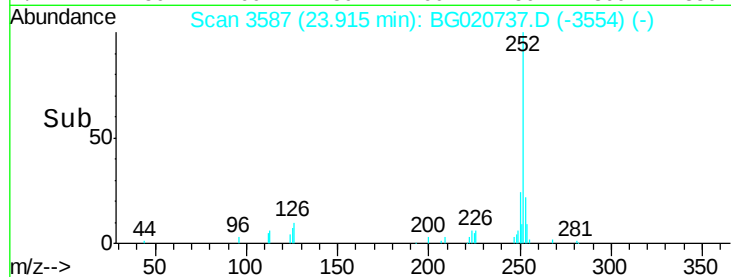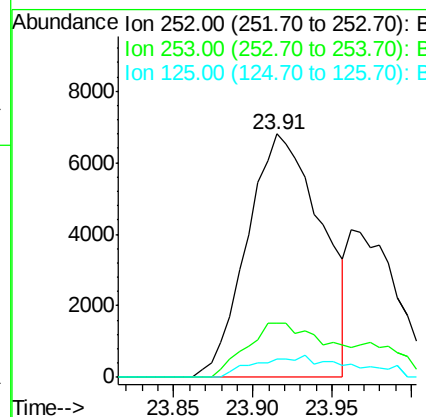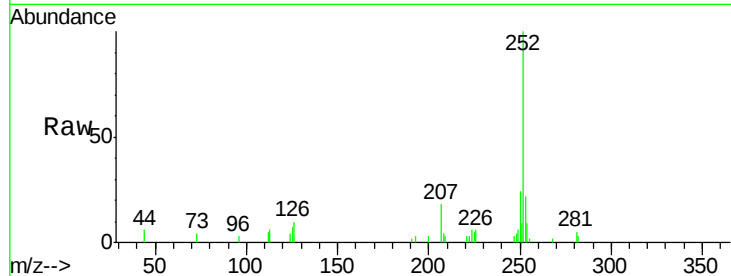

#91
Benzo(a)pyrene
Concen: 1.87 ng/ul
RT: 24.80 min Scan# 3737
Delta R.T. -0.00 min
Lab File: BG020737.D
Acq: 14 Jan 2016 23:48

Tgt Ion	Ratio	Resp	Lower	Upper
252	100	19696		
253	22.3		17.2	25.8
125	7.8		5.8	8.6

