

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG011420\
 Data File : BG044045.D
 Acq On : 14 Jan 2020 20:44
 Operator : JU
 Sample : L1108-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 INWOOD-BH-01-B

Manual Integrations
 APPROVED

mohammad
 1/16/2020 1:42:04 PM

Quant Time: Jan 14 23:58:33 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG123019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 31 13:32:23 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.95	152	131788	20.00	ng	-0.02
21) Naphthalene-d8	10.75	136	541838	20.00	ng	-0.02
39) Acenaphthene-d10	14.58	164	333215	20.00	ng	-0.02
64) Phenanthrene-d10	17.32	188	663730	20.00	ng	-0.01
76) Chrysene-d12	21.59	240	561869	20.00	ng	0.00
87) Perylene-d12	24.82	264	641646	20.00	ng	0.09
System Monitoring Compounds						
5) 2-Fluorophenol	5.53	112	789836	110.04	ng	0.00
7) Phenol-d6	7.12	99	1094433	109.08	ng	0.00
23) Nitrobenzene-d5	9.10	82	651285	64.30	ng	-0.02
42) 2,4,6-Tribromophenol	16.07	330	368093	105.56	ng	-0.02
45) 2-Fluorobiphenyl	13.21	172	1303790	70.89	ng	-0.02
79) Terphenyl-d14	19.94	244	1592836	63.57	ng	-0.02
Target Compounds						
10) Phenol	7.15	94	22598	2.186	ng	88
50) Dimethylphthalate	14.03	163	122569	5.181	ng	98
71) Phenanthrene	17.37	178	470241	14.771	ng	94
72) Anthracene	17.45	178	88834	2.823	ng	93
75) Fluoranthene	19.37	202	837753	23.010	ng	96
78) Pyrene	19.74	202	742232	20.238	ng	94
81) Benzo(a)anthracene	21.57	228	465953	13.374	ng	93
83) Chrysene	21.63	228	409828	12.380	ng	94
86) Indeno(1,2,3-cd)pyrene	28.52	276	282567m	6.281	ng	
88) Benzo(b)fluoranthene	23.78	252	514593m	13.566	ng	
89) Benzo(k)fluoranthene	23.81	252	238724m	6.618	ng	
90) Benzo(a)pyrene	24.66	252	410253	11.459	ng	99
92) Benzo(a,h,i)perylene	29.73	276	270487m	7.573	ng	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG011420\
Data File : BG044045.D
Acq On : 14 Jan 2020 20:44
Operator : JU
Sample : L1108-02
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
INWOOD-BH-01-B

Manual Integrations
APPROVED

mohammad
1/16/2020 1:42:04 PM

Quant Time: Jan 14 23:58:33 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 13:32:23 2019
Response via : Initial Calibration

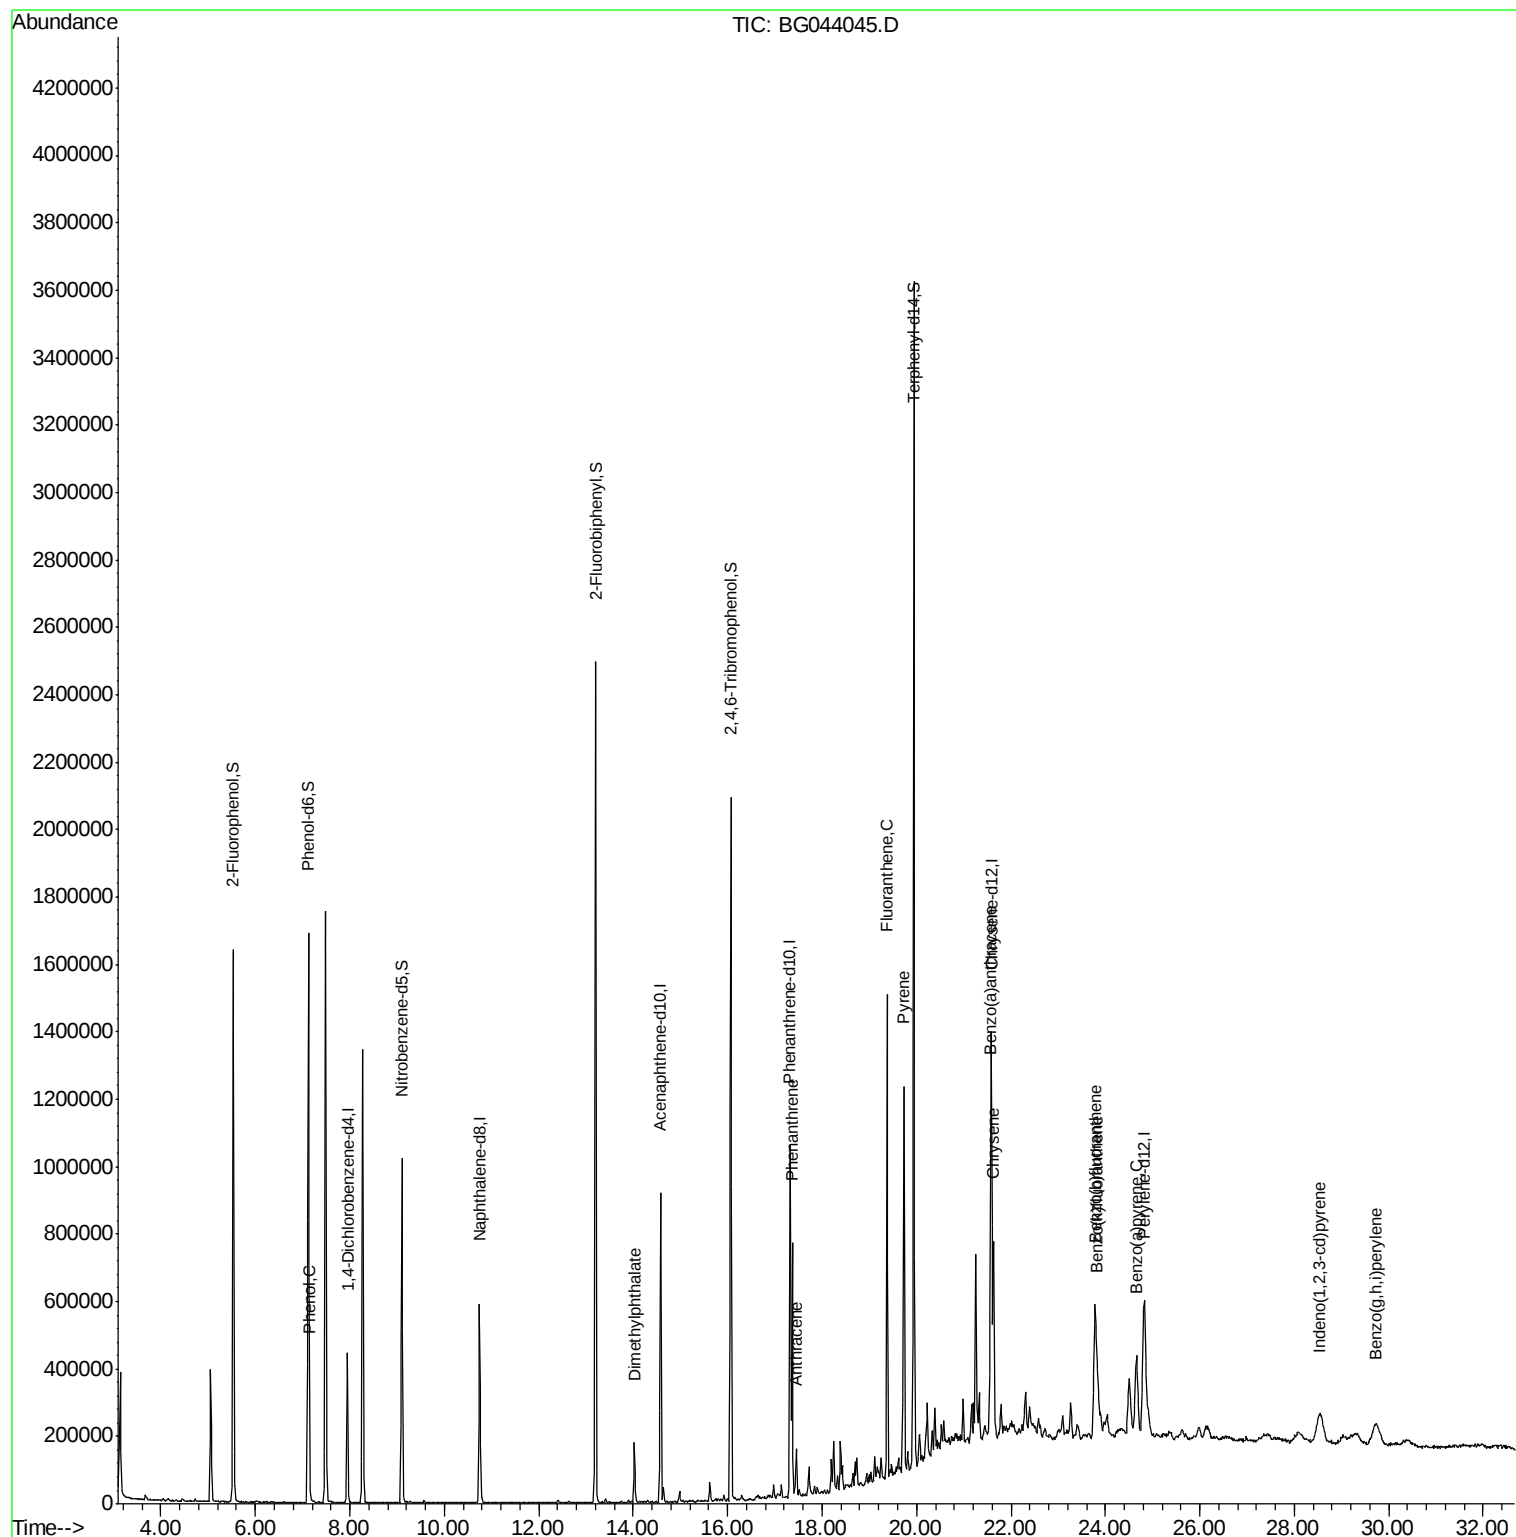



#1





1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.95 min Scan# 827
Delta R.T. -0.02 min
Lab File: BG044045.D
Acq: 14 Jan 2020 20:44

Instrument :
BNA_G
ClientSampleId :
INWOOD-BH-01-B

Tot Ion	Ratio	Lower	Upper
152	100		
150	163.1	127.0	190.4
115	61.0	47.8	71.8

Manual Integrations
APPROVED




mohammad
1/16/2020 1:42:04 PM

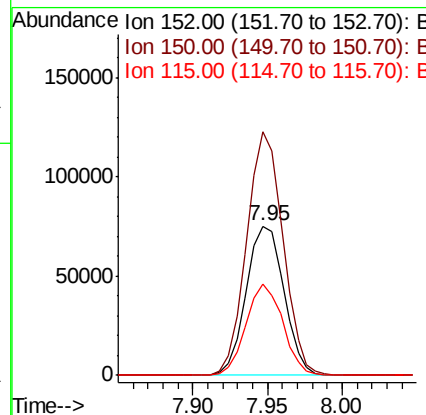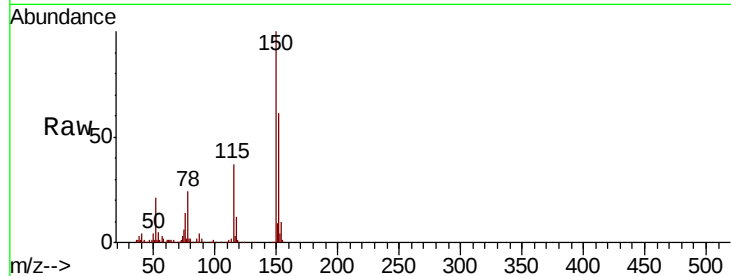


#5

2-Fluorophenol
Concen: 110.043 ng
RT: 5.53 min Scan# 416
Delta R.T. -0.01 min
Lab File: BG044045.D
Acq: 14 Jan 2020 20:44

Tgt Ion	Ratio	Lower	Upper
112	100		
64	58.0	47.8	71.6
63	31.0	24.3	36.5

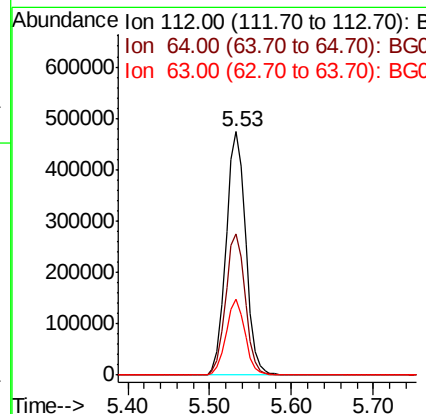



#7

Phenol-d6

Concen: 109.085 ng

RT: 7.12 min Scan# 686

Delta R.T. -0.01 min

Lab File: BG044045.D

Acq: 14 Jan 2020 20:44

Instrument :

BNA_G

ClientSampleId :

INWOOD-BH-01-B

Tot Ion: 99 Resp: 1094433

Ion Ratio Lower Upper

99 100

42 18.5 14.9 22.3





71 32.2 26.4 39.6

Manual Integrations

APPROVED

mohammad

1/16/2020 1:42:04 PM

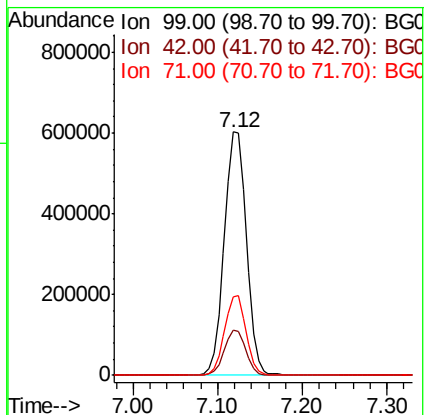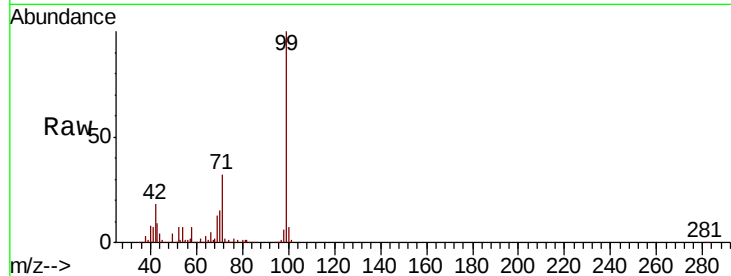

#10

Phenol

Concen: 2.186 ng

RT: 7.15 min Scan# 691

Delta R.T. -0.01 min

Lab File: BG044045.D

Acq: 14 Jan 2020 20:44




Tgt Ion: 94 Resp: 22598

Ion Ratio Lower Upper

94 100

65 29.6 8.1 48.1

66 46.8 15.6 55.6

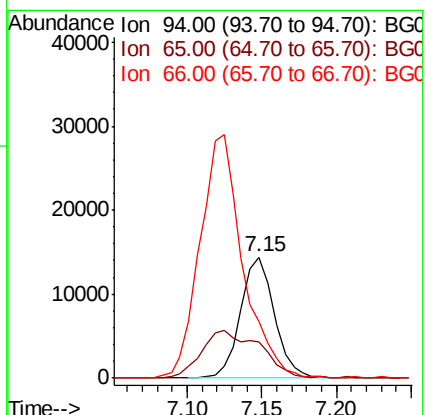







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.75 min Scan# 1304
Delta R.T. -0.02 min
Lab File: BG044045.D
Acq: 14 Jan 2020 20:44

Instrument :
BNA_G
ClientSampleId :
INWOOD-BH-01-B

Tot Ion	Ratio	Lower	Upper
136	100		
137	11.7	8.8	13.2
54	7.8	7.0	10.4
68	6.1	4.9	7.3




Manual Integrations
APPROVED


mohammad
1/16/2020 1:42:04 PM

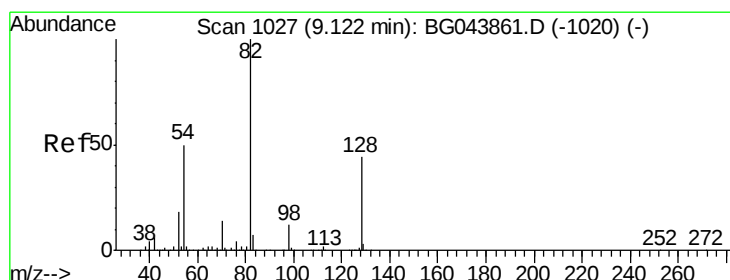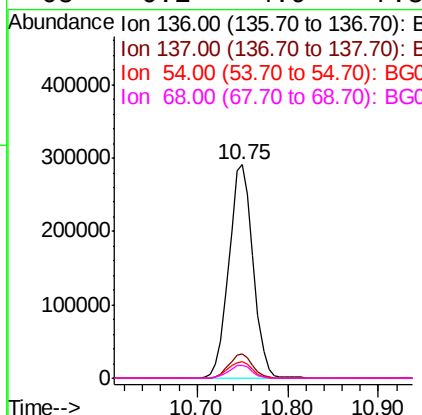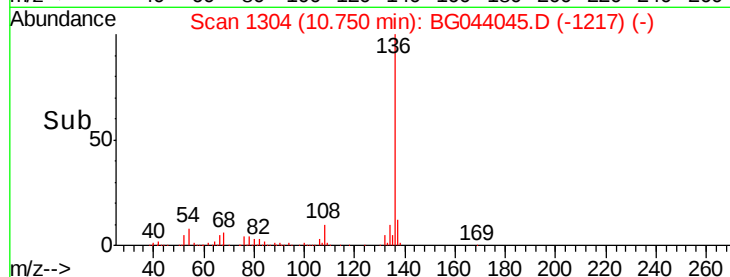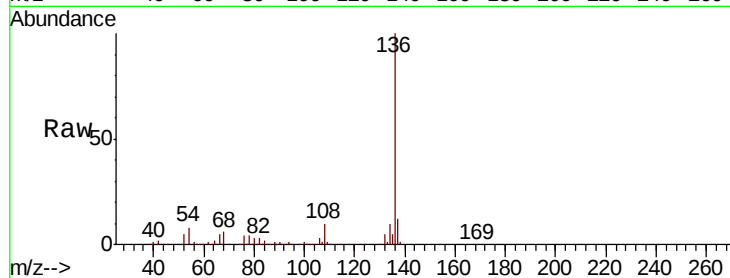

#23
Nitrobenzene-d5
Concen: 64.302 ng
RT: 9.10 min Scan# 1024
Delta R.T. -0.02 min
Lab File: BG044045.D
Acq: 14 Jan 2020 20:44

Tgt Ion	Ratio	Lower	Upper
82	100		
128	46.8	35.1	52.7
54	48.8	40.1	60.1

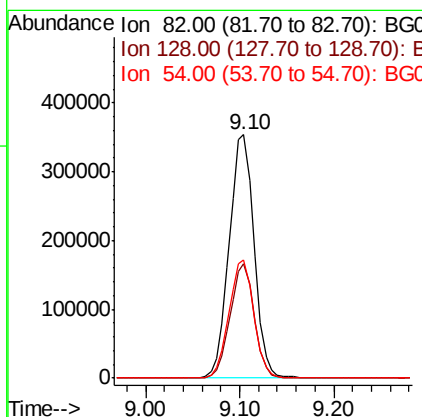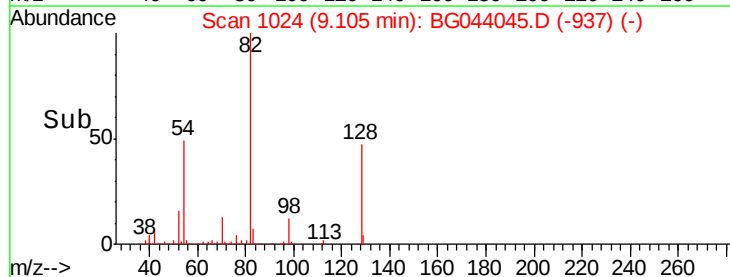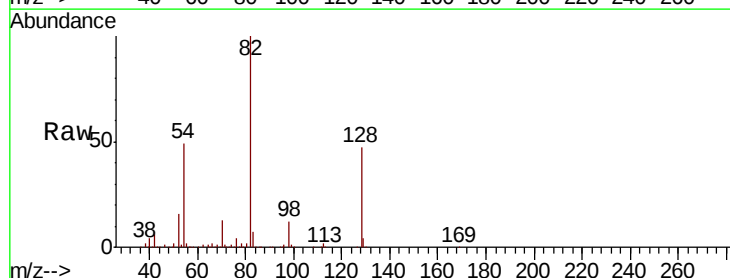

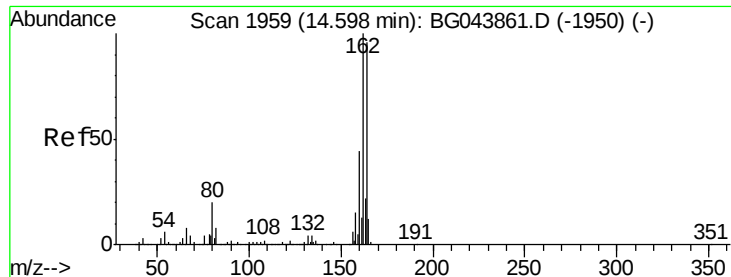

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.58 min Scan# 1956

Delta R.T. -0.02 min

Lab File: BG044045.D

Acq: 14 Jan 2020 20:44

Instrument :

BNA_G


ClientSampleId :

INWOOD-BH-01-B




Tot Ion:	164	Resp:	333215
Ion Ratio	Lower	Upper	
164	100		
162	103.6	83.0	124.4
160	45.7	36.1	54.1

Manual Integrations
APPROVED

mohammad
1/16/2020 1:42:04 PM

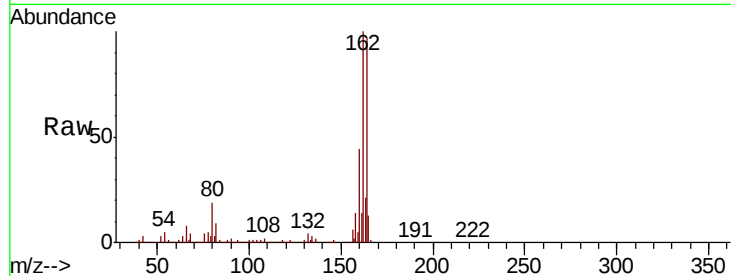

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

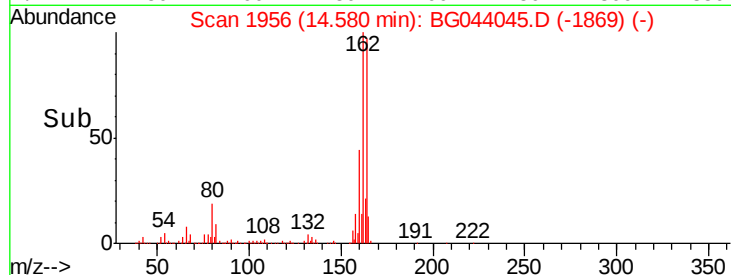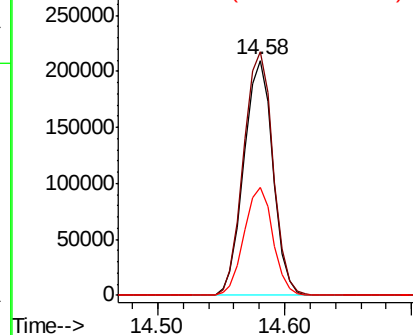

#42

2,4,6-Tribromophenol

Concen: 105.561 ng


RT: 16.07 min Scan# 2209

Delta R.T. -0.02 min



Lab File: BG044045.D


Acq: 14 Jan 2020 20:44

Tgt Ion:	330	Resp:	368093
Ion Ratio	Lower	Upper	
330	100		
332	96.3	77.2	115.8
141	39.8	33.1	49.7



Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

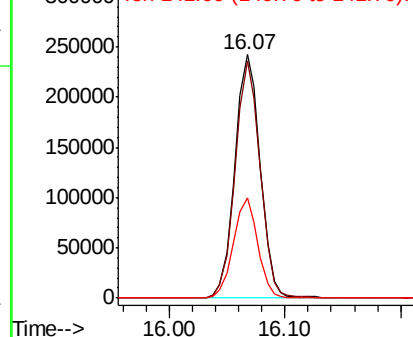







#45
2-Fluorobiphenyl
Concen: 70.890 ng
RT: 13.21 min Scan# 1722
Delta R.T. -0.02 min
Lab File: BG044045.D
Acq: 14 Jan 2020 20:44

Instrument :
BNA_G
ClientSampleId :
INWOOD-BH-01-B

Tot Ion:172 Resp: 1303790
Ion Ratio Lower Upper
172 100
171 40.5 35.8 53.8
170 27.7 24.2 36.4




Manual Integrations
APPROVED


mohammad
1/16/2020 1:42:04 PM

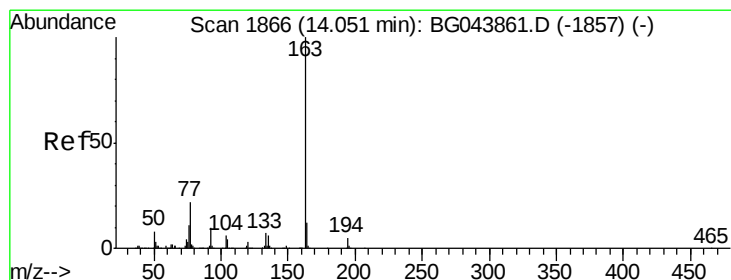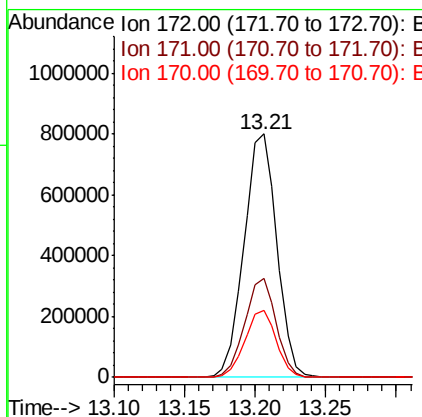

#50
Dimethylphthalate
Concen: 5.181 ng
RT: 14.03 min Scan# 1862
Delta R.T. -0.02 min
Lab File: BG044045.D
Acq: 14 Jan 2020 20:44

Tgt Ion:163 Resp: 122569
Ion Ratio Lower Upper
163 100
194 3.8 3.7 5.5
164 10.7 9.3 13.9

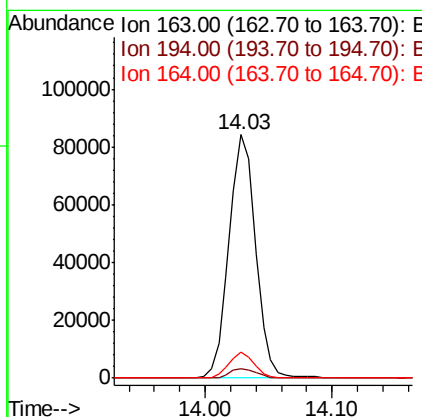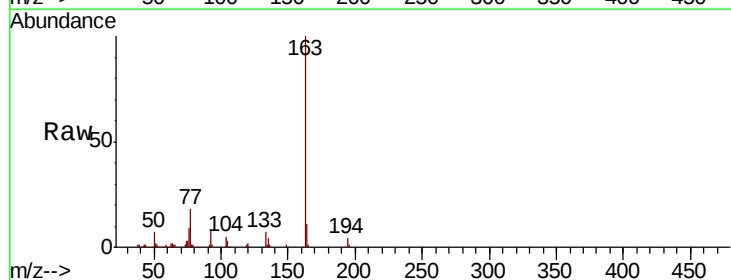

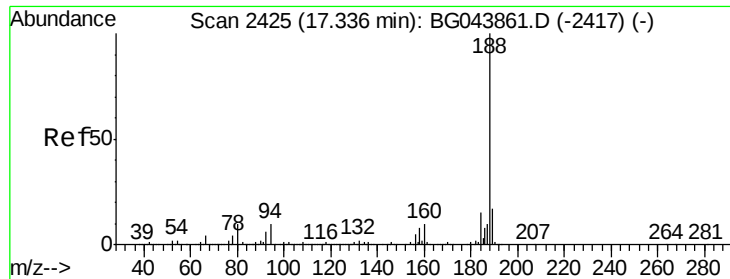





#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.32 min Scan# 2423
Delta R.T. -0.01 min
Lab File: BG044045.D
Acq: 14 Jan 2020 20:44

Instrument :
BNA_G
ClientSampleId :
INWOOD-BH-01-B

Tot Ion	Ratio	Resp	Lower	Upper
188	100	663730		
94	9.2		7.9	11.9
80	9.8		8.2	12.4




Manual Integrations
APPROVED


mohammad
1/16/2020 1:42:04 PM

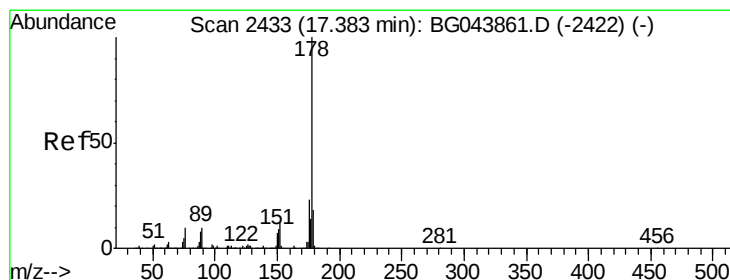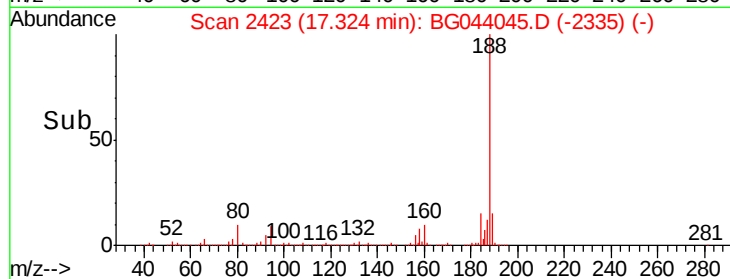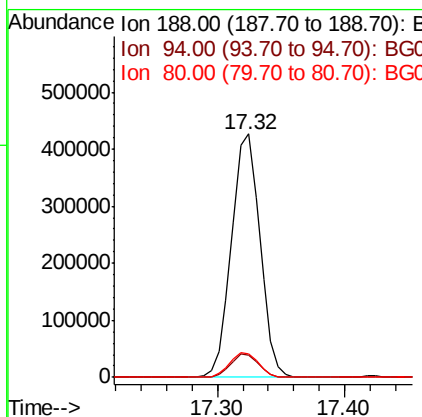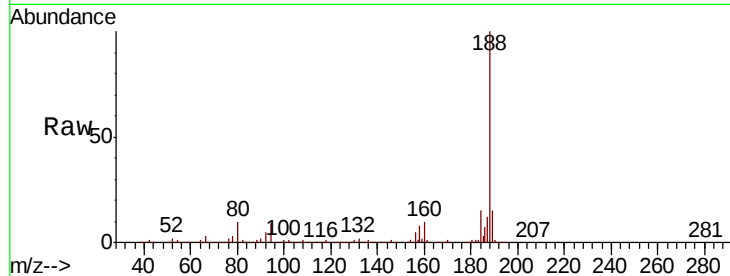

#71
Phenanthrene
Concen: 14.771 ng
RT: 17.37 min Scan# 2430
Delta R.T. -0.02 min
Lab File: BG044045.D
Acq: 14 Jan 2020 20:44

Tgt Ion	Ratio	Resp	Lower	Upper
178	100	470241		
176	20.5		18.6	28.0
179	15.7		14.4	21.6

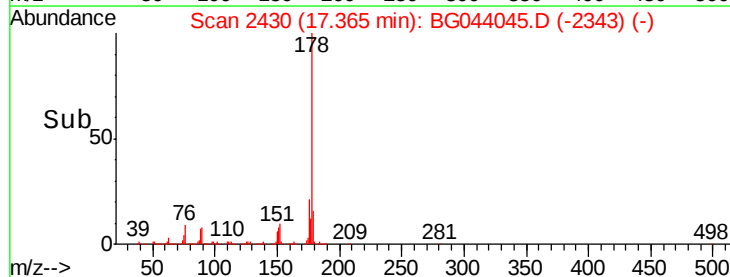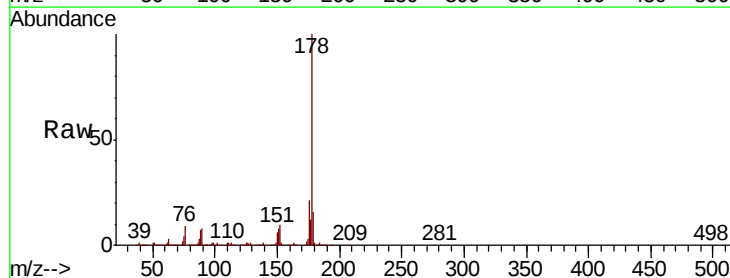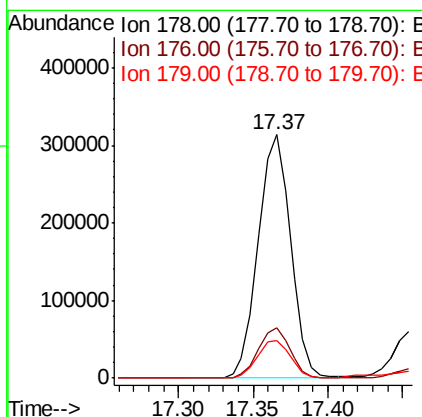

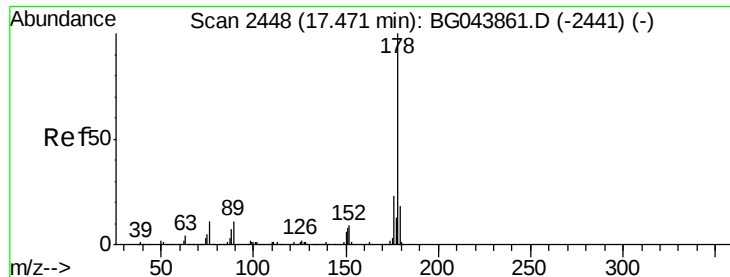

#72

Anthracene

Concen: 2.823 ng

RT: 17.45 min Scan# 2445

Delta R.T. -0.02 min

Lab File: BG044045.D

Acq: 14 Jan 2020 20:44

Instrument :

BNA_G


ClientSampleId :

INWOOD-BH-01-B




Tot Ion:	178	Resp:	88834
Ion Ratio	Lower	Upper	
178	100		
176	20.1	18.3	27.5
179	14.7	14.6	22.0

Manual Integrations
APPROVED

mohammad
1/16/2020 1:42:04 PM

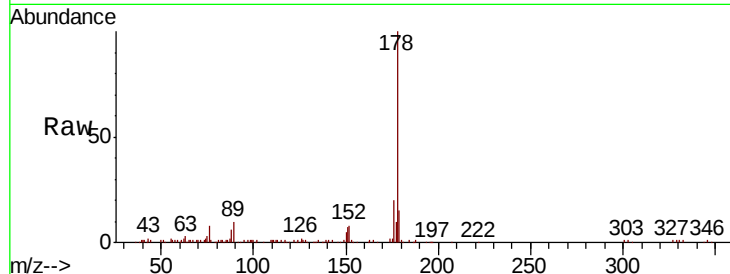

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E

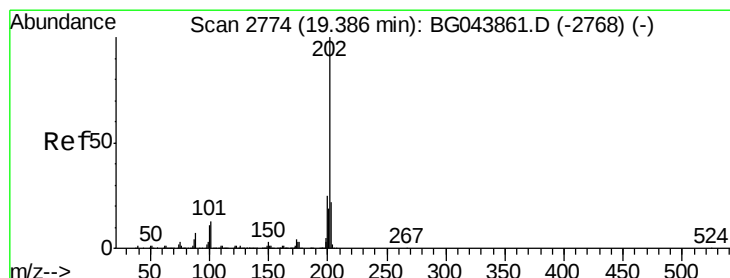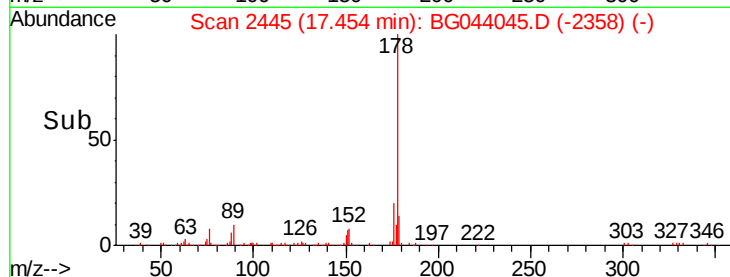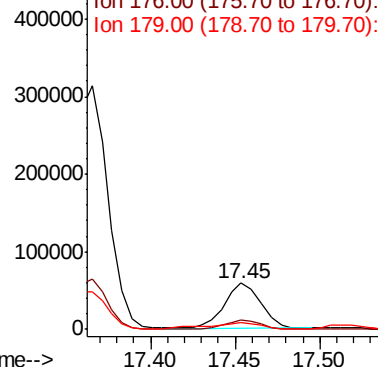

#75

Fluoranthene

Concen: 23.010 ng

RT: 19.37 min Scan# 2772




Delta R.T. -0.01 min


Lab File: BG044045.D

Acq: 14 Jan 2020 20:44

Tgt Ion:	202	Resp:	837753
Ion Ratio	Lower	Upper	
202	100		
101	12.0	0.0	33.3
203	19.5	1.6	41.6

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 203.00 (202.70 to 203.70): E

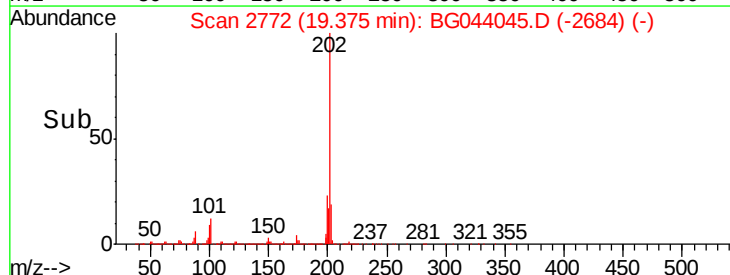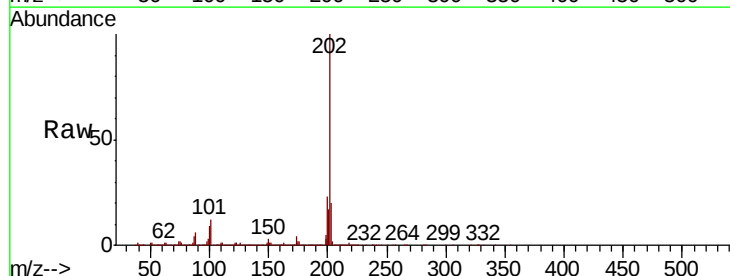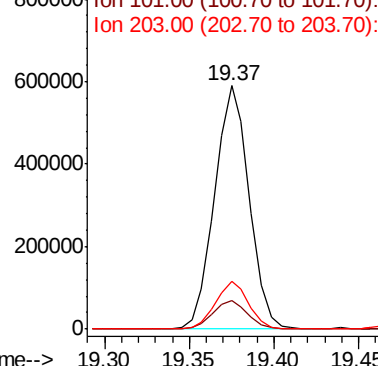







#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.59 min Scan# 3149
Delta R.T. 0.00 min
Lab File: BG044045.D
Acq: 14 Jan 2020 20:44

Instrument :
BNA_G
ClientSampleId :
INWOOD-BH-01-B

Tot Ion	Ratio	Lower	Upper
240	100		
120	11.7	9.6	14.4
236	28.8	22.2	33.2




Manual Integrations
APPROVED


mohammad
1/16/2020 1:42:04 PM

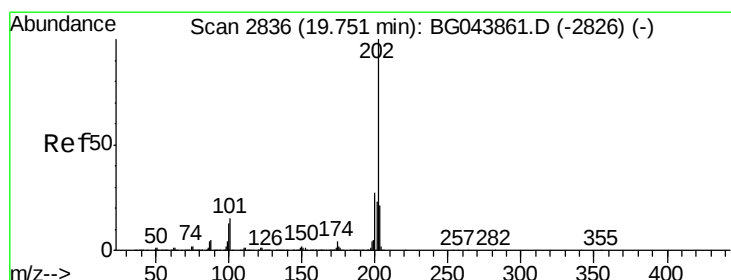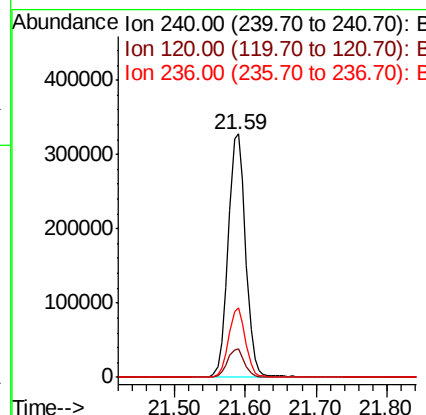

#78
Pyrene
Concen: 20.238 ng
RT: 19.74 min Scan# 2834
Delta R.T. -0.01 min
Lab File: BG044045.D
Acq: 14 Jan 2020 20:44

Tgt Ion	Ratio	Lower	Upper
202	100		
200	23.3	21.7	32.5
203	19.4	17.0	25.6

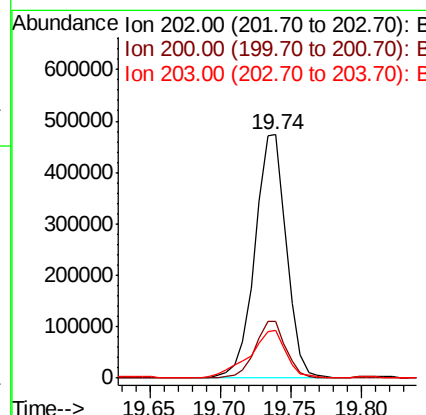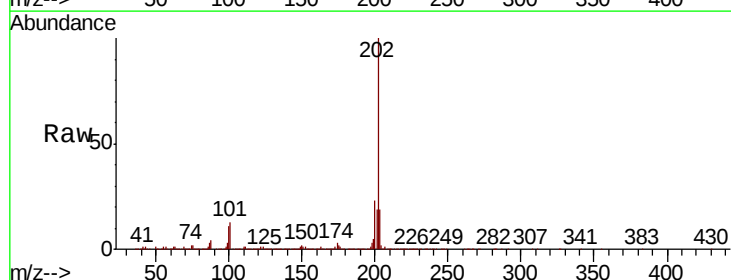




#79
 Terphenyl-d14
 Concen: 63.574 ng
 RT: 19.94 min Scan# 2868
 Delta R.T. -0.02 min
 Lab File: BG044045.D
 Acq: 14 Jan 2020 20:44

Instrument :
 BNA_G
 ClientSampleId :
 INWOOD-BH-01-B




Tot Ion	Ratio	Lower	Upper
244	100		
212	9.5	8.6	13.0
122	13.5	11.9	17.9

Manual Integrations
 APPROVED

mohammad
 1/16/2020 1:42:04 PM

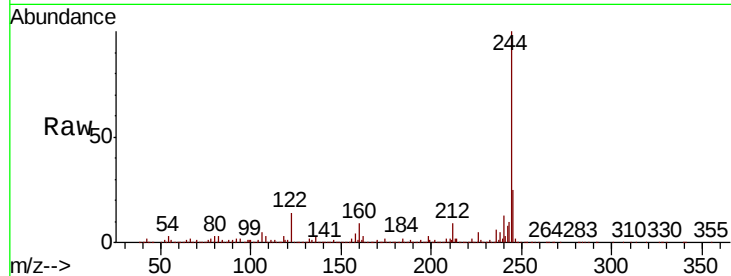




Abundance Ion 244.00 (243.70 to 244.70): E
 1500000 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

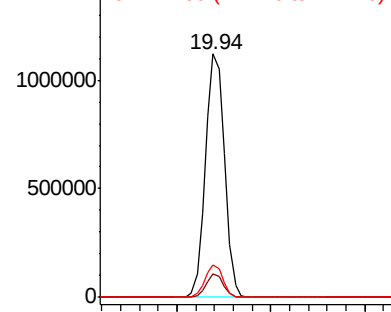


#81
 Benzo(a)anthracene
 Concen: 13.374 ng
 RT: 21.57 min Scan# 3145
 Delta R.T. -0.01 min
 Lab File: BG044045.D
 Acq: 14 Jan 2020 20:44

Tgt Ion	Ratio	Lower	Upper
228	100		
226	28.3	26.2	39.4
229	21.2	18.9	28.3

Abundance Ion 228.00 (227.70 to 228.70): E
 Ion 226.00 (225.70 to 226.70): E
 Ion 229.00 (228.70 to 229.70): E

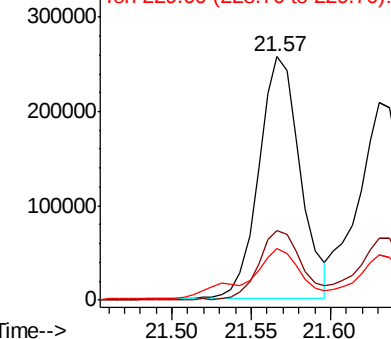







#83
Chrysene
Concen: 12.380 ng
RT: 21.63 min Scan# 3156
Delta R.T. -0.01 min
Lab File: BG044045.D
Acq: 14 Jan 2020 20:44

Instrument :
BNA_G
ClientSampleId :
INWOOD-BH-01-B

Tot Ion	Ion	Ratio	Resp	Lower	Upper
228	100		409828		
226	31.3		28.8	43.2	
229	22.9		19.0	28.6	




Manual Integrations
APPROVED


mohammad
1/16/2020 1:42:04 PM

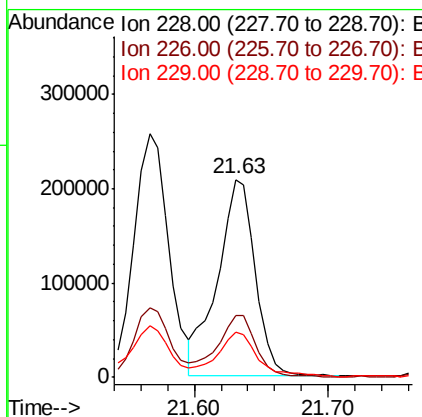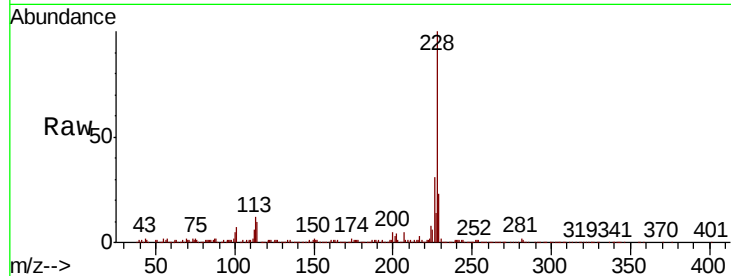

#86
Indeno(1,2,3-cd)pyrene
Concen: 6.281 ng m
RT: 28.52 min Scan# 4329
Delta R.T. 0.25 min
Lab File: BG044045.D
Acq: 14 Jan 2020 20:44

Tgt Ion	Ion	Ratio	Resp	Lower	Upper
276	100		282567		
138	0.6		21.0	31.4#	
277	0.0		21.1	31.7#	

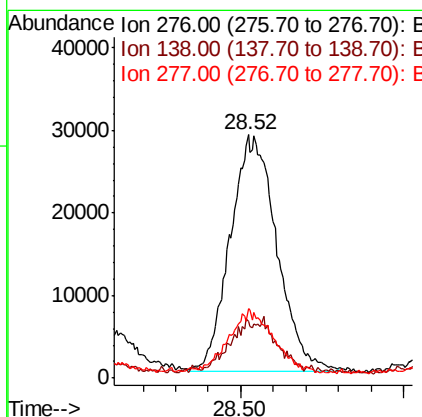




#87
Pervlene-d12
Concen: 20.000 ng
RT: 24.82 min Scan# 3698
Delta R.T. 0.09 min
Lab File: BG044045.D
Acq: 14 Jan 2020 20:44

Instrument :
BNA_G
ClientSampleId :
INWOOD-BH-01-B

Tot Ion	Ratio	Lower	Upper
264	100		
260	25.6	20.4	30.6
265	22.2	17.4	26.2

Manual Integrations
APPROVED

mohammad
1/16/2020 1:42:04 PM



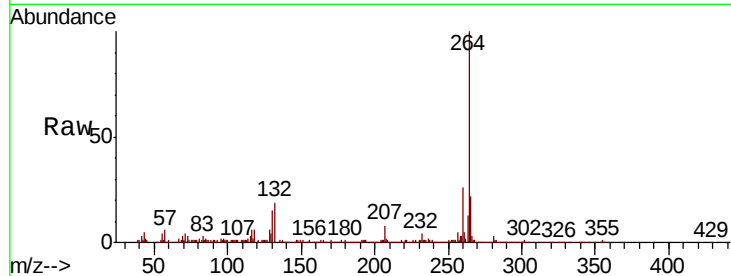


Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

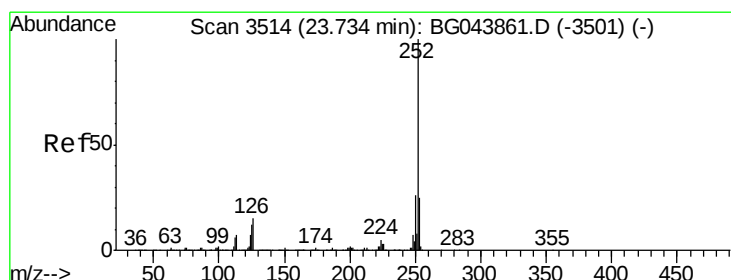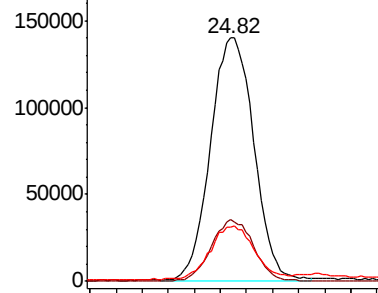

#88
Benzo(b)fluoranthene
Concen: 13.566 ng m
RT: 23.78 min Scan# 3522
Delta R.T. 0.05 min
Lab File: BG044045.D
Acq: 14 Jan 2020 20:44




Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.7	19.7	29.5
125	12.1	9.4	14.2


Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

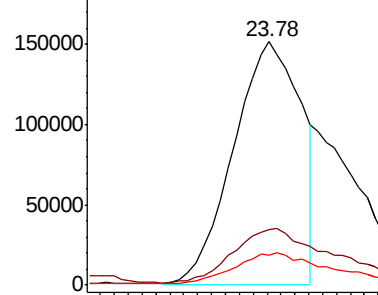







#89
Benzo(k)fluoranthene
Concen: 6.618 ng m
RT: 23.81 min Scan# 3527
Delta R.T. 0.01 min
Lab File: BG044045.D
Acq: 14 Jan 2020 20:44

Instrument :
BNA_G
ClientSampleId :
INWOOD-BH-01-B

Tot Ion	Ratio	Lower	Upper
252	100		
253	24.5	19.4	29.2
125	13.7	9.9	14.9




Manual Integrations
APPROVED


mohammad
1/16/2020 1:42:04 PM

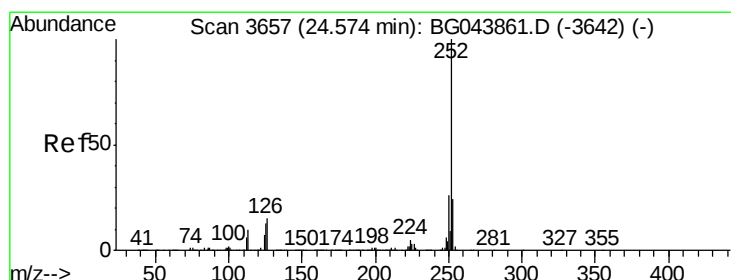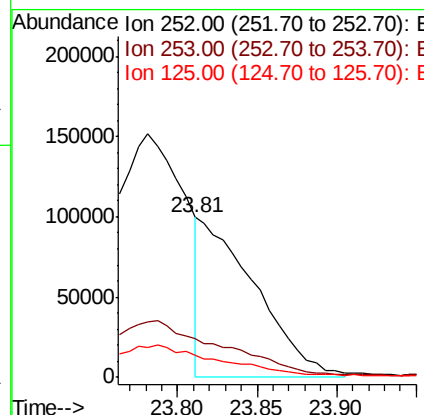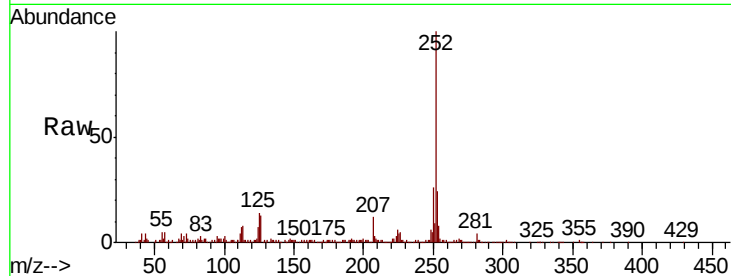

#90
Benzo(a)pyrene
Concen: 11.459 ng
RT: 24.66 min Scan# 3671
Delta R.T. 0.08 min
Lab File: BG044045.D
Acq: 14 Jan 2020 20:44

Tgt Ion	Ratio	Lower	Upper
252	100		
253	24.8	19.3	28.9
125	13.1	10.4	15.6

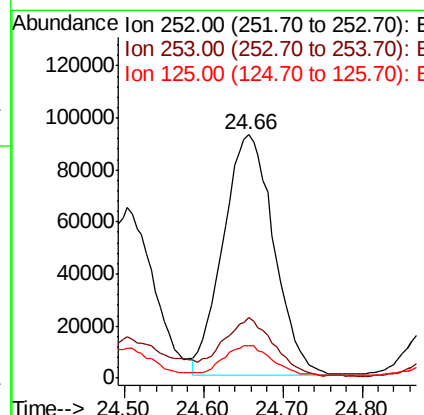




#92
 Benzo(a,h,i)perylene
 Concen: 7.573 ng m
 RT: 29.73 min Scan# 4535
 Delta R.T. 0.36 min
 Lab File: BG044045.D
 Acq: 14 Jan 2020 20:44

Instrument :
 BNA_G
 ClientSampleId :
 INWOOD-BH-01-B

Tot Ion	Ratio	Lower	Upper
276	100		
277	26.0	20.2	30.4
138	24.2	19.0	28.6

Manual Integrations
 APPROVED

mohammad
 1/16/2020 1:42:04 PM

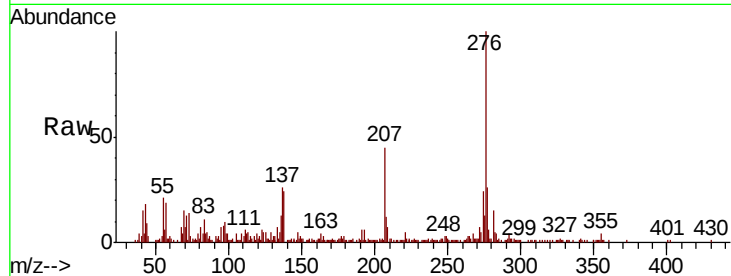

Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

