


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG011420\
 Data File : BG044032.D
 Acq On : 14 Jan 2020 11:08
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 31 13:32:23 2019

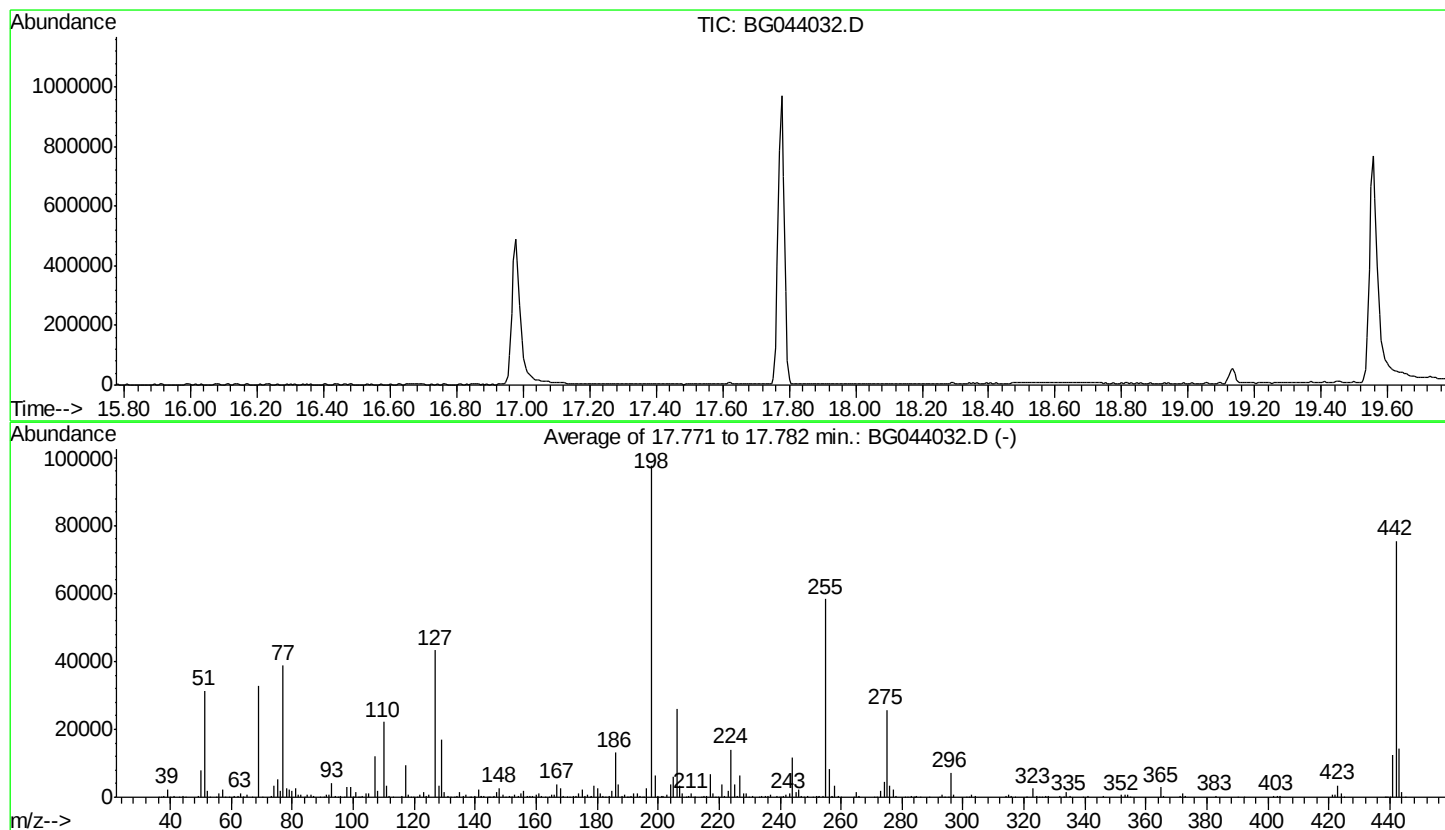

AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2492

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.2	31493	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.7	32968	PASS
70	69	0.00	2	0.6	203	PASS
127	198	10	80	44.2	43208	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	97685	PASS
199	198	5	9	6.6	6419	PASS
275	198	10	60	26.4	25789	PASS
365	198	1	100	3.1	3005	PASS
441	198	0.01	100	12.8	12545	PASS
442	198	50	100	77.4	75576	PASS
443	442	15	24	19.2	14483	PASS