

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011422\
 Data File : BG051973.D
 Acq On : 14 Jan 2022 12:57
 Operator : CG/JU
 Sample : N1100-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLP1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051973.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.573	10	14	19	rBV3	6290	9460	1.14%	0.124%
2	3.849	59	61	69	rVB	3801	5493	0.66%	0.072%
3	3.996	82	86	100	rBV	56403	95705	11.50%	1.251%
4	4.343	143	145	153	rVB3	1446	2411	0.29%	0.032%
5	4.560	181	182	188	rBV2	738	1234	0.15%	0.016%
6	5.289	302	306	309	rBV3	1611	2097	0.25%	0.027%
7	7.380	656	662	674	rVB	100264	183281	22.03%	2.395%
8	7.550	685	691	700	rVB	70117	114627	13.78%	1.498%
9	7.774	721	729	735	rBV	86341	151559	18.22%	1.981%
10	7.821	735	737	744	rVB	2005	3115	0.37%	0.041%
11	8.244	803	809	815	rBV2	77532	130289	15.66%	1.703%
12	8.943	921	928	936	rBV2	113491	196299	23.59%	2.565%
13	9.413	1001	1008	1017	rVB	90873	161778	19.44%	2.114%
14	9.835	1077	1080	1084	rVB2	3666	5106	0.61%	0.067%
15	10.147	1126	1133	1142	rVB2	77511	139927	16.82%	1.829%
16	10.693	1218	1226	1236	rBV	112716	202492	24.34%	2.646%
17	10.840	1247	1251	1254	rBV2	1732	2224	0.27%	0.029%
18	11.087	1285	1293	1300	rBV	108498	189102	22.73%	2.471%
19	11.210	1307	1314	1325	rVB	114529	206473	24.82%	2.698%
20	12.479	1525	1530	1535	rBV2	1857	2769	0.33%	0.036%
21	12.655	1556	1560	1564	rBV3	2140	2811	0.34%	0.037%
22	13.278	1661	1666	1670	rBV4	1365	1784	0.21%	0.023%
23	13.425	1689	1691	1696	rBV	873	1222	0.15%	0.016%
24	13.701	1734	1738	1742	rBV3	4412	5800	0.70%	0.076%
25	13.771	1745	1750	1753	rBV2	909	1463	0.18%	0.019%
26	14.277	1830	1836	1844	rVB	244093	352964	42.42%	4.613%
27	14.512	1873	1876	1882	rBV2	1493	2173	0.26%	0.028%
28	14.582	1882	1888	1896	rBV	259494	404607	48.63%	5.288%
29	14.770	1915	1920	1923	rVB2	3129	3562	0.43%	0.047%
30	14.887	1934	1940	1947	rVB	183674	296346	35.62%	3.873%
31	15.064	1962	1970	1983	rBV	115383	202612	24.35%	2.648%
32	15.169	1986	1988	1992	rVB2	971	1195	0.14%	0.016%
33	15.287	2003	2008	2010	rVB	1226	1544	0.19%	0.020%
34	15.522	2044	2048	2051	rBV3	999	1437	0.17%	0.019%
35	15.669	2069	2073	2077	rBV4	1062	1654	0.20%	0.022%
36	15.710	2077	2080	2085	rVB3	3009	4500	0.54%	0.059%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011422\
 Data File : BG051973.D
 Acq On : 14 Jan 2022 12:57
 Operator : CG/JU
 Sample : N1100-10
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLP1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	15.880	2102	2109	2116	rVB	348641	532358	63.99%	6.957%
38	15.980	2121	2126	2135	rVB	110811	165254	19.86%	2.160%
39	16.121	2147	2150	2152	rBV	1937	1666	0.20%	0.022%
40	16.262	2170	2174	2177	rBV2	1610	2455	0.30%	0.032%
41	16.656	2239	2241	2245	rVB3	1522	1143	0.14%	0.015%
42	16.756	2255	2258	2263	rVB2	2788	3580	0.43%	0.047%
43	16.990	2296	2298	2300	rVB3	1383	1107	0.13%	0.014%
44	17.090	2312	2315	2318	rBV2	1324	2013	0.24%	0.026%
45	17.149	2321	2325	2329	rVB2	1106	1859	0.22%	0.024%
46	17.308	2351	2352	2357	rBV	983	1531	0.18%	0.020%
47	17.366	2359	2362	2367	rVB4	2916	4149	0.50%	0.054%
48	17.425	2367	2372	2375	rBV2	1902	3245	0.39%	0.042%
49	17.531	2386	2390	2393	rBV4	1116	1213	0.15%	0.016%
50	17.637	2402	2408	2414	rBV	305573	461200	55.43%	6.027%
51	17.737	2418	2425	2433	rVV2	427709	665525	79.99%	8.697%
52	17.807	2435	2437	2441	rVB2	2673	3581	0.43%	0.047%
53	17.913	2452	2455	2456	rBV2	1559	1565	0.19%	0.020%
54	17.983	2464	2467	2468	rBV	1304	1126	0.14%	0.015%
55	18.118	2488	2490	2491	rVB2	2627	1184	0.14%	0.015%
56	18.283	2516	2518	2523	rBV2	3841	4793	0.58%	0.063%
57	18.406	2534	2539	2540	rBV5	1185	1935	0.23%	0.025%
58	18.500	2552	2555	2559	rBV4	3775	5270	0.63%	0.069%
59	18.571	2565	2567	2572	rVB4	1362	1571	0.19%	0.021%
60	18.782	2601	2603	2605	rVB2	1870	1231	0.15%	0.016%
61	18.800	2605	2606	2609	rBV2	1512	1804	0.22%	0.024%
62	19.017	2639	2643	2646	rBV2	1973	3279	0.39%	0.043%
63	19.088	2654	2655	2659	rVB3	1481	1190	0.14%	0.016%
64	19.252	2680	2683	2685	rBV3	1461	1635	0.20%	0.021%
65	19.364	2700	2702	2704	rBV2	1325	1327	0.16%	0.017%
66	19.434	2712	2714	2716	rBV3	2073	1824	0.22%	0.024%
67	19.581	2735	2739	2742	rBV5	5260	7071	0.85%	0.092%
68	19.610	2742	2744	2746	rVB3	2575	1615	0.19%	0.021%
69	19.657	2747	2752	2755	rBV2	5899	7510	0.90%	0.098%
70	19.710	2759	2761	2763	rBV2	1455	1391	0.17%	0.018%
71	19.763	2767	2770	2772	rBV3	2111	2976	0.36%	0.039%
72	19.910	2793	2795	2798	rBV4	2345	1856	0.22%	0.024%
73	19.951	2801	2802	2804	rBV2	2540	2198	0.26%	0.029%
74	20.016	2806	2813	2820	rBV	576527	831983	100.00%	10.873%
75	20.192	2841	2843	2845	rBV3	2064	2130	0.26%	0.028%
76	21.144	3003	3005	3006	rBV	2949	1619	0.19%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011422\
Data File : BG051973.D
Acq On : 14 Jan 2022 12:57
Operator : CG/JU
Sample : N1100-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLP1

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Title : SVOA CALIBRATION

77	21.561	3072	3076	3085	rBV7	18204	50046	6.02%	0.654%
78	21.960	3137	3144	3152	rVB	294430	510185	61.32%	6.667%
79	22.107	3167	3169	3171	rBV3	4744	3194	0.38%	0.042%
80	25.209	3686	3697	3708	rVB2	250899	748685	89.99%	9.784%
81	25.450	3727	3738	3751	rVB2	161660	506862	60.92%	6.624%




Sum of corrected areas: 7652049

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011422\
Data File : BG051973.D
Acq On : 14 Jan 2022 12:57
Operator : CG/JU
Sample : N1100-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLP1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

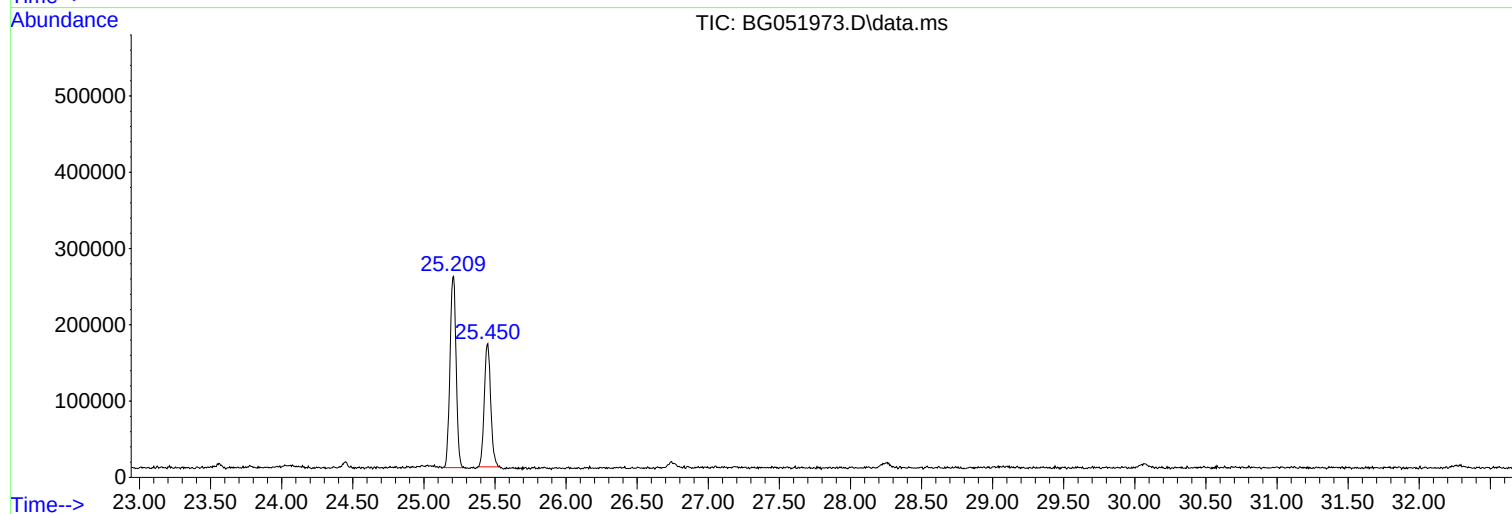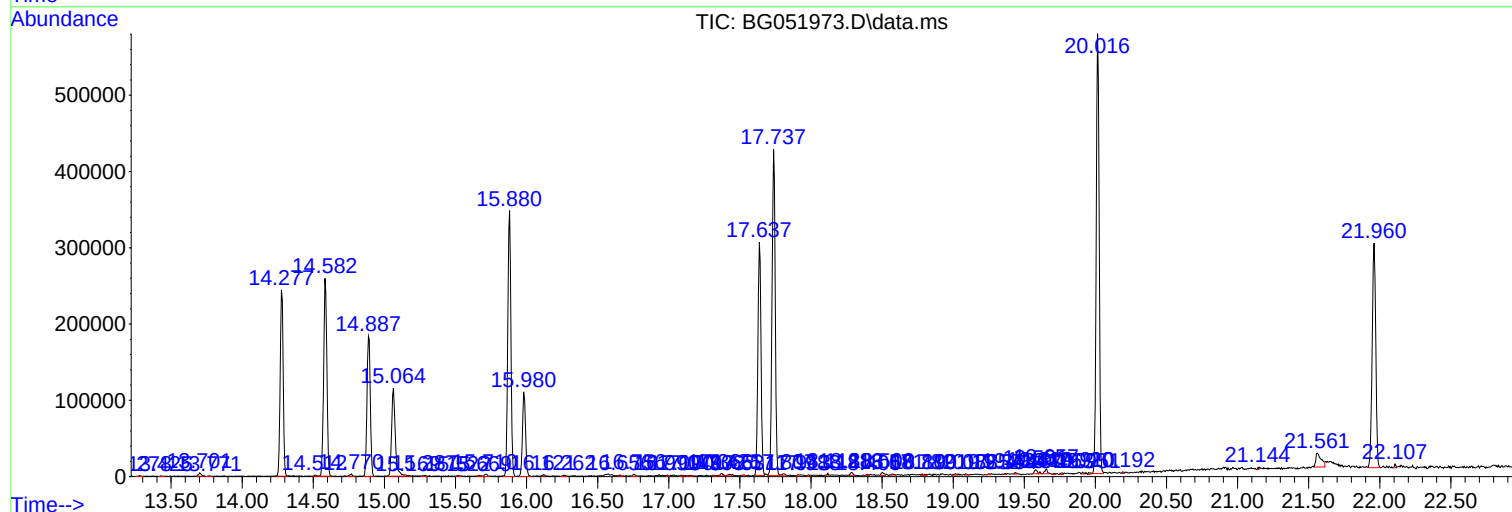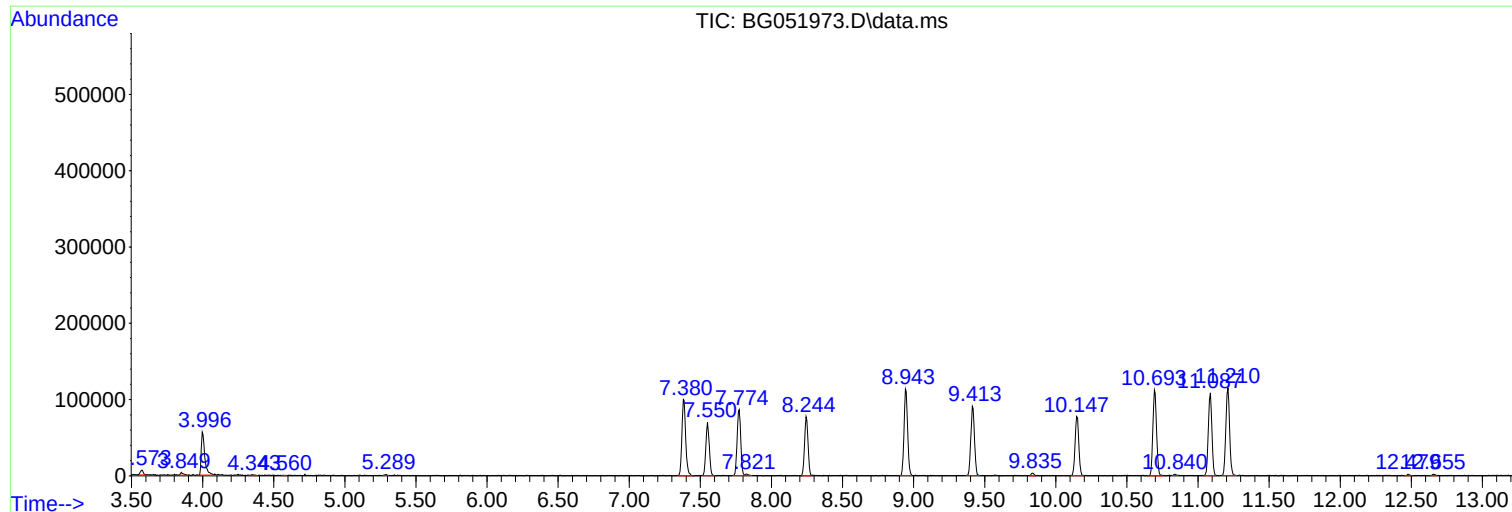

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011422\
Data File : BG051973.D
Acq On : 14 Jan 2022 12:57
Operator : CG/JU
Sample : N1100-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLP1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011422\
Data File : BG051973.D
Acq On : 14 Jan 2022 12:57
Operator : CG/JU
Sample : N1100-10
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLP1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------