

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011422\
 Data File : BG051976.D
 Acq On : 14 Jan 2022 14:50
 Operator : CG/JU
 Sample : N1100-17
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLT1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051976.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.570	10	14	21	rBV	5867	9353	1.07%	0.121%
2	3.852	58	62	64	rBV3	1203	1609	0.18%	0.021%
3	3.905	69	71	75	rVB2	1029	1338	0.15%	0.017%
4	3.999	83	87	98	rBV	43390	69062	7.93%	0.896%
5	4.246	127	129	133	rVB3	4477	4591	0.53%	0.060%
6	4.416	155	158	161	rVB2	1085	1389	0.16%	0.018%
7	4.445	161	163	168	rBV2	1264	1564	0.18%	0.020%
8	5.174	282	287	289	rBV2	736	1179	0.14%	0.015%
9	5.285	302	306	312	rBV3	5380	9000	1.03%	0.117%
10	7.383	656	663	673	rBV	94281	176355	20.24%	2.287%
11	7.553	684	692	700	rVB	62514	107498	12.34%	1.394%
12	7.770	722	729	737	rVB	82563	141203	16.21%	1.831%
13	8.246	802	810	815	rBV	75528	125693	14.43%	1.630%
14	8.293	815	818	824	rVB3	9045	13902	1.60%	0.180%
15	8.945	923	929	937	rVB	106467	179291	20.58%	2.325%
16	9.068	946	950	953	rBV	1134	1795	0.21%	0.023%
17	9.415	1001	1009	1019	rBV	84884	152592	17.52%	1.979%
18	9.838	1076	1081	1087	rVB2	4131	6390	0.73%	0.083%
19	10.149	1128	1134	1144	rVB	70015	126857	14.56%	1.645%
20	10.696	1220	1227	1234	rBV2	104633	181209	20.80%	2.350%
21	11.083	1285	1293	1301	rBV	105902	184253	21.15%	2.390%
22	11.207	1306	1314	1326	rBV2	105128	193181	22.17%	2.506%
23	12.470	1527	1529	1530	rBV	2466	1565	0.18%	0.020%
24	12.658	1557	1561	1563	rBV	1609	1995	0.23%	0.026%
25	13.275	1663	1666	1672	rVB2	937	1351	0.16%	0.018%
26	13.369	1679	1682	1686	rVB2	1038	1200	0.14%	0.016%
27	13.698	1734	1738	1746	rBV4	5422	8426	0.97%	0.109%
28	14.085	1802	1804	1806	rBV3	1059	1252	0.14%	0.016%
29	14.279	1831	1837	1843	rBV	235764	342871	39.36%	4.447%
30	14.514	1872	1877	1878	rBV2	1617	1781	0.20%	0.023%
31	14.585	1882	1889	1897	rVB	249430	385117	44.21%	4.995%
32	14.767	1915	1920	1925	rVB3	2628	4202	0.48%	0.054%
33	14.890	1934	1941	1948	rVB	191520	297835	34.19%	3.863%
34	15.060	1964	1970	1986	rBV	97396	175517	20.15%	2.276%
35	15.289	2002	2009	2012	rVB3	6099	9601	1.10%	0.125%
36	15.513	2045	2047	2051	rVB3	1302	1475	0.17%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011422\
 Data File : BG051976.D
 Acq On : 14 Jan 2022 14:50
 Operator : CG/JU
 Sample : N1100-17
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLT1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	15.677	2070	2075	2078	rBV3	1031	1822	0.21%	0.024%
38	15.712	2078	2081	2086	rVB2	3892	4382	0.50%	0.057%
39	15.877	2102	2109	2117	rBV	352274	519698	59.65%	6.740%
40	15.983	2121	2127	2137	rVB	94951	140576	16.14%	1.823%

41	16.124	2145	2151	2154	rVB3	2093	3910	0.45%	0.051%
42	16.265	2172	2175	2180	rBV3	1523	1861	0.21%	0.024%
43	16.552	2221	2224	2225	rBV	1900	1702	0.20%	0.022%
44	16.576	2225	2228	2230	rVB2	2159	2179	0.25%	0.028%
45	16.735	2252	2255	2256	rBV	1906	1417	0.16%	0.018%

46	16.758	2256	2259	2263	rVB3	2120	3025	0.35%	0.039%
47	16.987	2294	2298	2300	rBV3	1488	1240	0.14%	0.016%
48	17.022	2302	2304	2308	rVB3	1549	1919	0.22%	0.025%
49	17.363	2360	2362	2369	rVB2	4840	6697	0.77%	0.087%
50	17.428	2369	2373	2377	rBV4	2323	4749	0.55%	0.062%

51	17.463	2377	2379	2383	rVB3	1711	1876	0.22%	0.024%
52	17.504	2383	2386	2388	rBV2	1167	1243	0.14%	0.016%
53	17.639	2402	2409	2416	rBV	309573	459808	52.78%	5.964%
54	17.692	2416	2418	2419	rVV	2842	2529	0.29%	0.033%
55	17.739	2419	2426	2434	rVV	442787	686426	78.79%	8.903%

56	17.810	2434	2438	2442	rVV4	11438	14149	1.62%	0.184%
57	17.851	2443	2445	2449	rVB4	1624	1524	0.17%	0.020%
58	18.027	2472	2475	2480	rVB3	2078	3557	0.41%	0.046%
59	18.068	2480	2482	2485	rBV2	1518	2049	0.24%	0.027%
60	18.115	2485	2490	2492	rBV5	2082	3338	0.38%	0.043%

61	18.280	2516	2518	2522	rBV4	4053	5429	0.62%	0.070%
62	18.515	2552	2558	2562	rBV5	3753	7473	0.86%	0.097%
63	18.544	2562	2563	2565	rBV2	1958	1470	0.17%	0.019%
64	18.614	2572	2575	2576	rBV2	1383	1232	0.14%	0.016%
65	18.902	2622	2624	2626	rBV3	1785	1758	0.20%	0.023%

66	18.984	2636	2638	2640	rBV2	1556	1528	0.18%	0.020%
67	19.067	2648	2652	2654	rBV4	1735	2559	0.29%	0.033%
68	19.090	2654	2656	2662	rVB4	1747	2588	0.30%	0.034%
69	19.208	2674	2676	2677	rVB2	1667	1169	0.13%	0.015%
70	19.349	2697	2700	2704	rBV5	2311	4494	0.52%	0.058%

71	19.443	2711	2716	2721	rVB5	3903	6631	0.76%	0.086%
72	19.496	2721	2725	2726	rBV3	1729	1952	0.22%	0.025%
73	19.548	2732	2734	2737	rBV	5106	5586	0.64%	0.072%
74	19.578	2737	2739	2743	rVB3	6239	7694	0.88%	0.100%
75	19.654	2749	2752	2759	rVB	7231	10417	1.20%	0.135%

76	19.866	2787	2788	2790	rBV2	1692	1399	0.16%	0.018%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011422\
 Data File : BG051976.D
 Acq On : 14 Jan 2022 14:50
 Operator : CG/JU
 Sample : N1100-17
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLT1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

77	20.018	2807	2814	2820	rBV	602761	871199	100.00%	11.299%
78	20.083	2823	2825	2826	rBV2	1914	1434	0.16%	0.019%
79	20.189	2841	2843	2846	rBV4	2669	1753	0.20%	0.023%
80	20.494	2893	2895	2898	rBV2	2921	2841	0.33%	0.037%
81	20.518	2898	2899	2900	rBV	3813	2132	0.24%	0.028%
82	21.557	3072	3076	3080	rBV6	22337	41567	4.77%	0.539%
83	21.957	3137	3144	3152	rVB	311743	531690	61.03%	6.896%
84	22.503	3234	3237	3243	rVB6	14580	22866	2.62%	0.297%
85	23.772	3448	3453	3462	rVB3	19560	41144	4.72%	0.534%
86	25.205	3687	3697	3710	rVB	278104	790823	90.77%	10.257%
87	25.446	3728	3738	3752	rVB	167045	535982	61.52%	6.952%
88	26.046	3838	3840	3842	rBV3	4398	4267	0.49%	0.055%
89	30.986	4679	4681	4684	rBV3	3868	3849	0.44%	0.050%




Sum of corrected areas: 7710094

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011422\
Data File : BG051976.D
Acq On : 14 Jan 2022 14:50
Operator : CG/JU
Sample : N1100-17
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLT1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

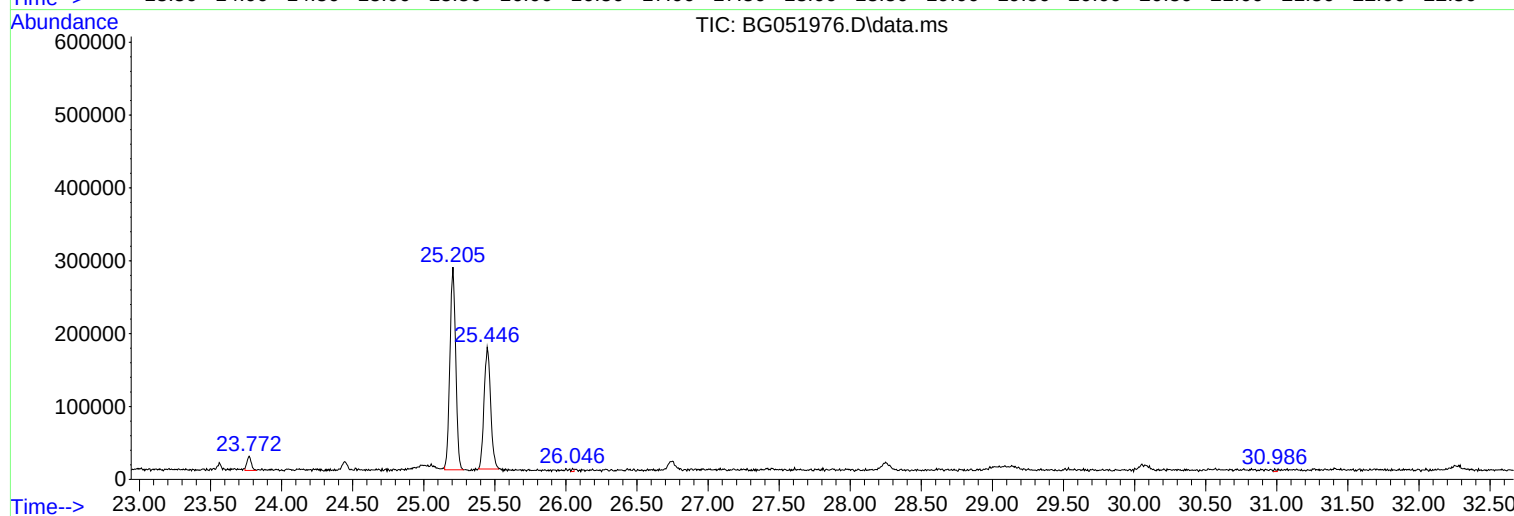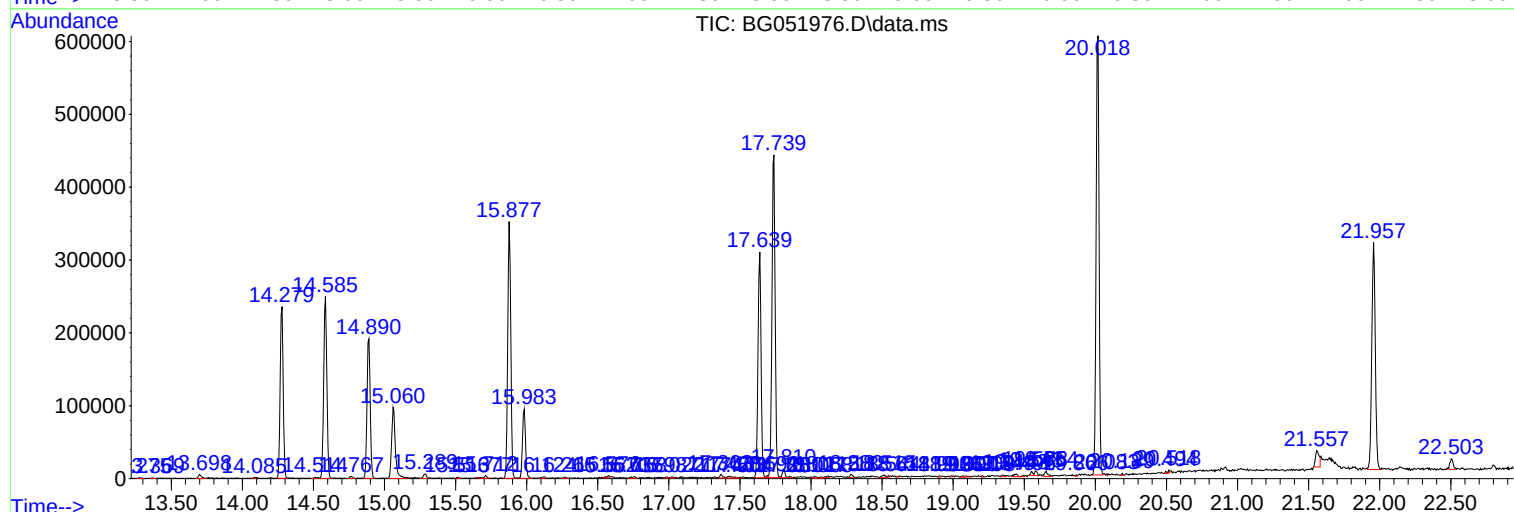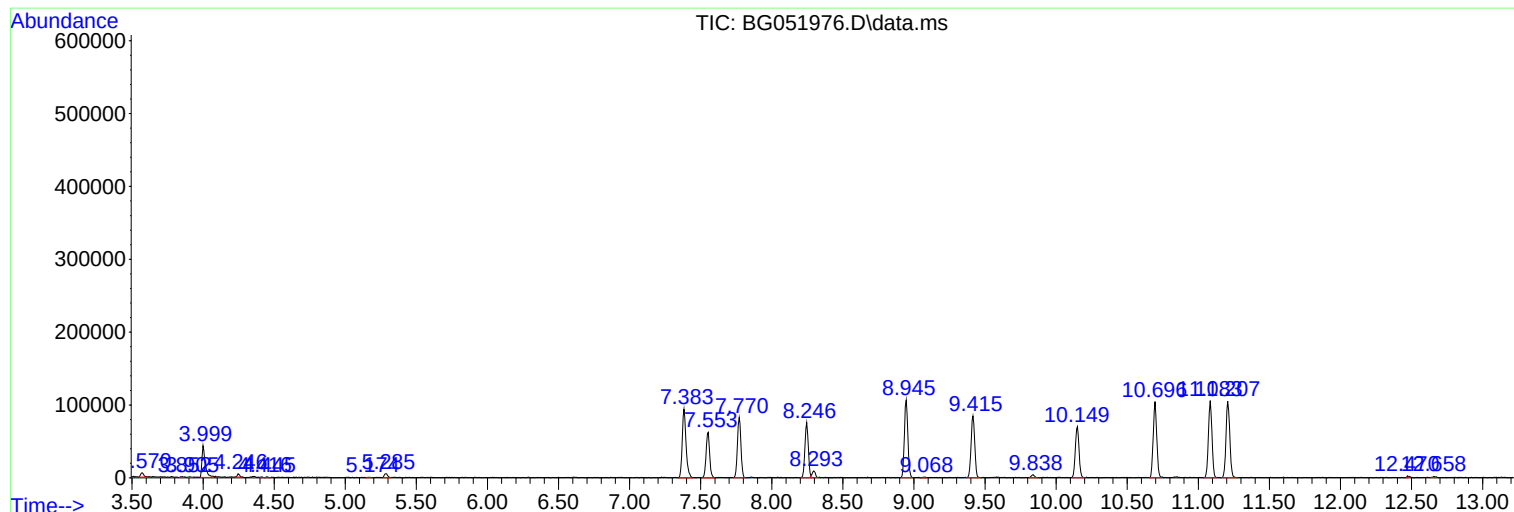

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011422\
Data File : BG051976.D
Acq On : 14 Jan 2022 14:50
Operator : CG/JU
Sample : N1100-17
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLT1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011422\
Data File : BG051976.D
Acq On : 14 Jan 2022 14:50
Operator : CG/JU
Sample : N1100-17
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLT1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc