

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011422\
 Data File : BG051977.D
 Acq On : 14 Jan 2022 15:28
 Operator : CG/JU
 Sample : N1100-19
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLT3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051977.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.570	10	14	22	rVB3	8064	13240	1.57%	0.165%
2	3.904	69	71	74	rBV4	1598	1984	0.24%	0.025%
3	3.998	83	87	95	rBV	63813	104547	12.44%	1.303%
4	4.110	105	106	110	rVB4	1728	1735	0.21%	0.022%
5	4.357	143	148	151	rBV3	2476	3604	0.43%	0.045%
6	4.897	238	240	243	rVB3	1056	1145	0.14%	0.014%
7	5.285	301	306	307	rBV3	1564	1869	0.22%	0.023%
8	5.408	323	327	330	rVB3	1299	1940	0.23%	0.024%
9	5.490	340	341	344	rBV	1466	1557	0.19%	0.019%
10	5.996	423	427	430	rBV3	1177	1107	0.13%	0.014%
11	6.483	507	510	512	rBV	1137	1314	0.16%	0.016%
12	6.765	553	558	560	rVB	1021	1082	0.13%	0.013%
13	7.382	656	663	676	rVB2	99567	175690	20.90%	2.190%
14	7.552	685	692	699	rVB	64950	111486	13.26%	1.389%
15	7.770	722	729	737	rVB	90072	149154	17.74%	1.859%
16	8.246	803	810	816	rBV	87750	146885	17.47%	1.831%
17	8.298	816	819	824	rVB4	8937	11598	1.38%	0.145%
18	8.422	836	840	844	rBV	719	1337	0.16%	0.017%
19	8.945	922	929	939	rVB2	109705	192473	22.89%	2.399%
20	9.415	1002	1009	1016	rBV	93034	162805	19.37%	2.029%
21	9.837	1077	1081	1086	rVB2	3976	6219	0.74%	0.078%
22	10.149	1124	1134	1143	rVB2	76757	140396	16.70%	1.750%
23	10.695	1219	1227	1235	rBV	114016	198167	23.57%	2.470%
24	10.836	1246	1251	1253	rBV4	2442	3469	0.41%	0.043%
25	11.083	1285	1293	1302	rVB	121804	215172	25.59%	2.682%
26	11.206	1307	1314	1326	rVV	111536	207399	24.67%	2.585%
27	12.481	1526	1531	1535	rVB2	1619	2211	0.26%	0.028%
28	13.274	1664	1666	1670	rVB2	1204	1401	0.17%	0.017%
29	13.697	1734	1738	1744	rBV4	4686	6999	0.83%	0.087%
30	14.091	1800	1805	1810	rVB	21935	30480	3.63%	0.380%
31	14.279	1831	1837	1843	rVB	250785	353538	42.05%	4.406%
32	14.508	1874	1876	1878	rBV	1670	1096	0.13%	0.014%
33	14.584	1882	1889	1895	rVV	266662	404320	48.09%	5.039%
34	14.766	1916	1920	1924	rBV3	2596	3813	0.45%	0.048%
35	14.889	1933	1941	1951	rBV	217742	344782	41.01%	4.297%
36	15.066	1964	1971	1986	rBV	111489	200228	23.82%	2.495%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011422\
 Data File : BG051977.D
 Acq On : 14 Jan 2022 15:28
 Operator : CG/JU
 Sample : N1100-19
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLT3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	15.213	1994	1996	1999	rBV3	1329	1738	0.21%	0.022%
38	15.512	2043	2047	2052	rVB2	1708	2249	0.27%	0.028%
39	15.712	2077	2081	2085	rVB3	2460	3138	0.37%	0.039%
40	15.876	2103	2109	2116	rVB	360091	535297	63.67%	6.671%

41	15.982	2121	2127	2136	rVV	98395	148780	17.70%	1.854%
42	16.117	2147	2150	2155	rVB2	2330	2538	0.30%	0.032%
43	16.270	2172	2176	2181	rVB3	2461	2884	0.34%	0.036%
44	16.505	2214	2216	2220	rVB3	1194	1435	0.17%	0.018%
45	16.540	2220	2222	2224	rBV2	1644	1156	0.14%	0.014%

46	16.581	2226	2229	2231	rVB3	2161	2235	0.27%	0.028%
47	16.763	2255	2260	2265	rVB4	1683	3152	0.37%	0.039%
48	16.928	2285	2288	2289	rBV3	1512	1473	0.18%	0.018%
49	17.087	2312	2315	2320	rBV	1499	2283	0.27%	0.028%
50	17.151	2324	2326	2331	rBV	930	1385	0.16%	0.017%

51	17.310	2348	2353	2357	rVB2	1262	2257	0.27%	0.028%
52	17.368	2360	2363	2368	rVB4	2422	3560	0.42%	0.044%
53	17.427	2369	2373	2376	rVB3	1588	2022	0.24%	0.025%
54	17.639	2402	2409	2416	rBV	349033	534564	63.58%	6.662%
55	17.739	2418	2426	2432	rVV	443466	677665	80.61%	8.445%

56	17.809	2435	2438	2441	rBV3	6355	7274	0.87%	0.091%
57	17.927	2456	2458	2462	rVB2	1126	1169	0.14%	0.015%
58	18.162	2496	2498	2500	rVB2	1319	1212	0.14%	0.015%
59	18.279	2516	2518	2524	rVB3	4466	5492	0.65%	0.068%
60	18.350	2527	2530	2534	rBV2	972	1437	0.17%	0.018%

61	18.391	2534	2537	2538	rBV2	1446	1158	0.14%	0.014%
62	18.508	2552	2557	2560	rBV3	3839	4392	0.52%	0.055%
63	18.690	2586	2588	2589	rBV2	1481	1089	0.13%	0.014%
64	18.749	2596	2598	2602	rVB3	2094	2412	0.29%	0.030%
65	18.802	2602	2607	2610	rBV3	1580	3338	0.40%	0.042%

66	18.890	2620	2622	2626	rVB3	1748	1844	0.22%	0.023%
67	19.090	2654	2656	2658	rVB2	1589	1179	0.14%	0.015%
68	19.131	2658	2663	2665	rBV3	1630	2044	0.24%	0.025%
69	19.254	2682	2684	2686	rVB2	1734	1179	0.14%	0.015%
70	19.272	2686	2687	2689	rBV	2132	1733	0.21%	0.022%

71	19.442	2712	2716	2719	rVB2	3158	3944	0.47%	0.049%
72	19.472	2719	2721	2723	rBV2	1589	1081	0.13%	0.013%
73	19.513	2726	2728	2730	rBV3	1899	1672	0.20%	0.021%
74	19.554	2730	2735	2737	rBV2	8115	11375	1.35%	0.142%
75	19.577	2737	2739	2743	rVB4	5286	6862	0.82%	0.086%

76	19.648	2748	2751	2759	rVV2	5608	9312	1.11%	0.116%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011422\
 Data File : BG051977.D
 Acq On : 14 Jan 2022 15:28
 Operator : CG/JU
 Sample : N1100-19
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLT3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

77	19.724	2762	2764	2769	rBV4	1107	1649	0.20%	0.021%
78	19.859	2785	2787	2789	rBV2	2203	1716	0.20%	0.021%
79	20.018	2807	2814	2822	rVB	560294	840710	100.00%	10.477%
80	20.429	2883	2884	2886	rVB2	2941	1379	0.16%	0.017%
81	20.464	2886	2890	2891	rBV3	2151	2523	0.30%	0.031%
82	21.563	3074	3077	3081	rBV5	7692	12333	1.47%	0.154%
83	21.956	3138	3144	3154	rVB	334516	582091	69.24%	7.254%
84	25.199	3687	3696	3710	rVB2	252786	763280	90.79%	9.512%
85	25.446	3727	3738	3754	rVB3	188254	611115	72.69%	7.616%




Sum of corrected areas: 8024047

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011422\
Data File : BG051977.D
Acq On : 14 Jan 2022 15:28
Operator : CG/JU
Sample : N1100-19
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLT3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

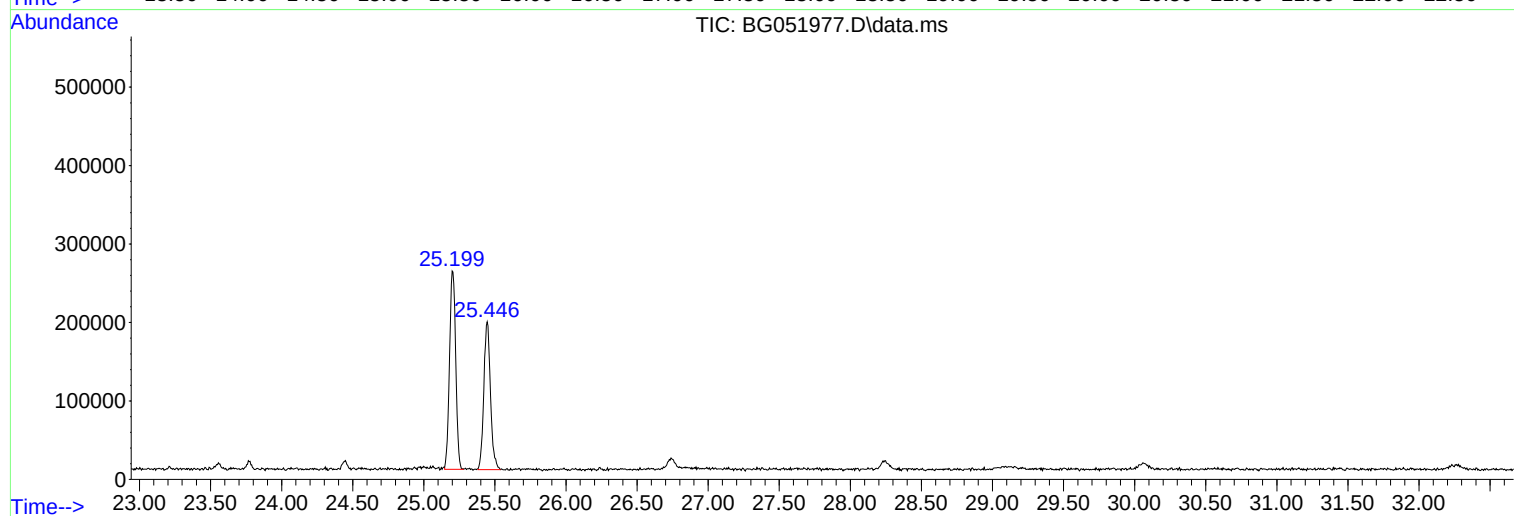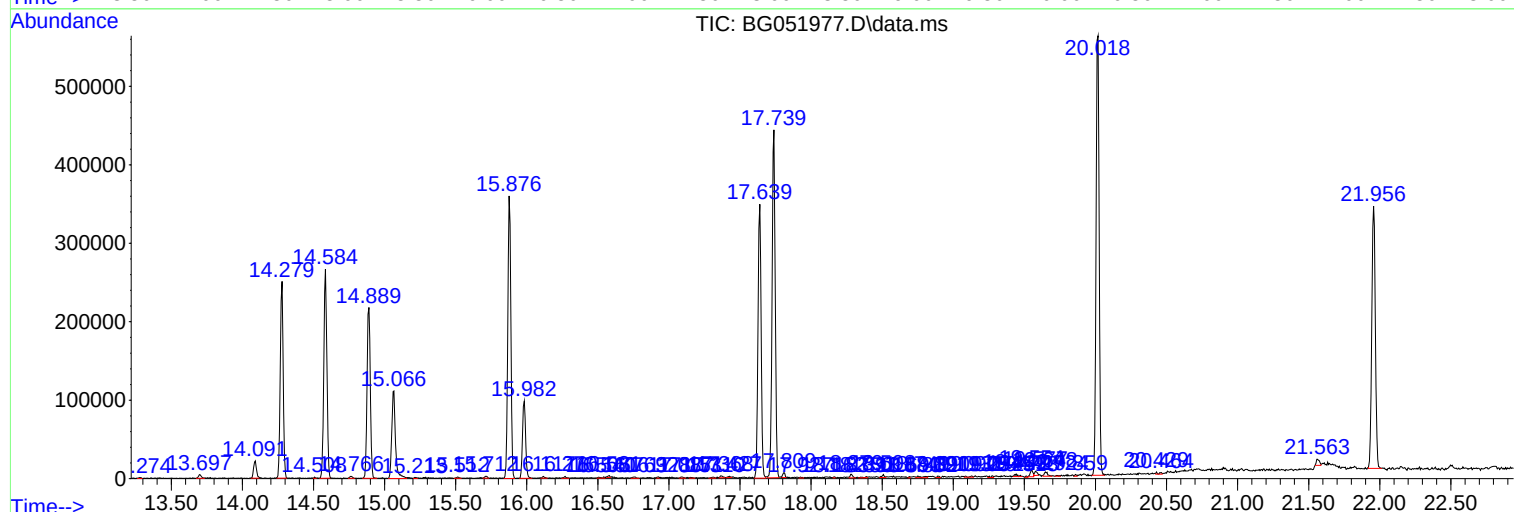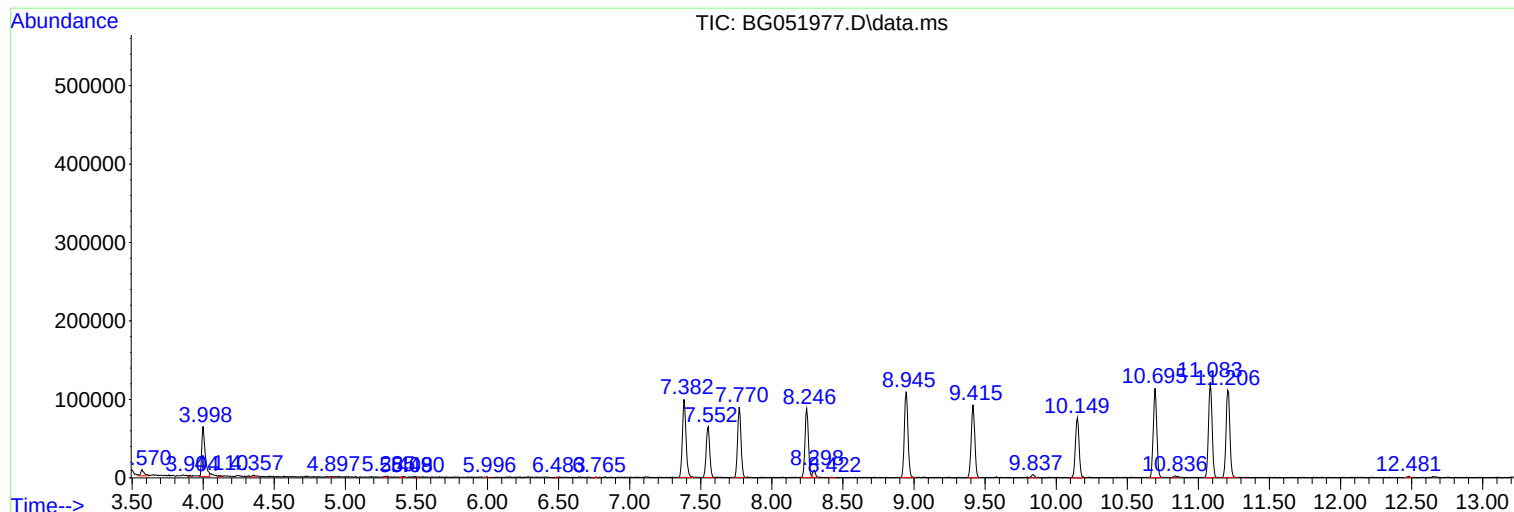

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011422\
Data File : BG051977.D
Acq On : 14 Jan 2022 15:28
Operator : CG/JU
Sample : N1100-19
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLT3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011422\
Data File : BG051977.D
Acq On : 14 Jan 2022 15:28
Operator : CG/JU
Sample : N1100-19
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLT3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc