

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011422\
 Data File : BG051978.D
 Acq On : 14 Jan 2022 16:06
 Operator : CG/JU
 Sample : N1100-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLS5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051978.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.573	10	14	17	rVB2	5668	7926	1.06%	0.102%
2	3.931	72	75	80	rVB3	1036	2099	0.28%	0.027%
3	4.002	83	87	97	rBV2	17608	31846	4.26%	0.408%
4	4.114	103	106	109	rVB4	2351	3226	0.43%	0.041%
5	4.249	125	129	133	rVB3	4496	6751	0.90%	0.087%
6	4.349	142	146	153	rVB4	2090	3494	0.47%	0.045%
7	4.448	160	163	165	rVV3	1596	1915	0.26%	0.025%
8	5.224	293	295	300	rVB4	1231	1453	0.19%	0.019%
9	5.288	300	306	313	rBV2	6187	10820	1.45%	0.139%
10	5.594	354	358	361	rBV3	1623	1588	0.21%	0.020%
11	6.093	440	443	447	rBV2	1178	1806	0.24%	0.023%
12	6.234	465	467	472	rVB4	1533	2167	0.29%	0.028%
13	6.487	506	510	512	rBV4	2401	3469	0.46%	0.044%
14	6.504	512	513	521	rVB5	2974	3302	0.44%	0.042%
15	6.610	525	531	536	rBV5	2565	5546	0.74%	0.071%
16	6.710	542	548	549	rBV3	2233	3497	0.47%	0.045%
17	6.734	549	552	555	rVB	1711	2368	0.32%	0.030%
18	6.775	555	559	563	rBV2	5167	5963	0.80%	0.076%
19	6.833	565	569	570	rVV3	2237	2826	0.38%	0.036%
20	6.863	570	574	576	rVV4	2620	4569	0.61%	0.059%
21	6.892	576	579	585	rVV4	4168	6801	0.91%	0.087%
22	6.986	594	595	602	rVV2	1409	1852	0.25%	0.024%
23	7.057	602	607	610	rVB2	1629	2038	0.27%	0.026%
24	7.098	610	614	615	rBV2	1895	1998	0.27%	0.026%
25	7.109	615	616	621	rVV2	2148	2930	0.39%	0.038%
26	7.221	630	635	641	rVB3	4320	7189	0.96%	0.092%
27	7.321	648	652	656	rBV3	1660	2782	0.37%	0.036%
28	7.380	656	662	670	rVV	96631	178241	23.84%	2.285%
29	7.550	684	691	698	rBV	70020	118442	15.84%	1.519%
30	7.621	698	703	708	rVV4	2099	3432	0.46%	0.044%
31	7.673	710	712	714	rVV2	1420	1532	0.20%	0.020%
32	7.726	717	721	722	rVV3	2179	2922	0.39%	0.037%
33	7.767	722	728	736	rVV	88313	158289	21.17%	2.029%
34	7.844	740	741	746	rVV2	1820	2406	0.32%	0.031%
35	8.038	771	774	777	rVB3	1477	1872	0.25%	0.024%
36	8.179	791	798	799	rVV3	2391	4693	0.63%	0.060%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011422\
 Data File : BG051978.D
 Acq On : 14 Jan 2022 16:06
 Operator : CG/JU
 Sample : N1100-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLS5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	8.243	801	809	815	rVV	93220	166150	22.22%	2.130%
38	8.296	815	818	827	rVB5	5243	8735	1.17%	0.112%
39	8.378	827	832	836	rBV2	2609	4272	0.57%	0.055%
40	8.431	836	841	845	rBV4	1871	3247	0.43%	0.042%
41	8.484	845	850	856	rVV4	6259	11011	1.47%	0.141%
42	8.731	887	892	894	rBV3	1489	1978	0.26%	0.025%
43	8.801	897	904	907	rBV4	5204	10711	1.43%	0.137%
44	8.942	921	928	935	rBV	107306	191188	25.57%	2.451%
45	9.095	952	954	958	rVV3	2035	3300	0.44%	0.042%
46	9.142	958	962	964	rVV2	3104	4442	0.59%	0.057%
47	9.160	964	965	970	rVV2	2094	2106	0.28%	0.027%
48	9.412	1001	1008	1016	rVV	90696	166204	22.23%	2.131%
49	9.577	1032	1036	1038	rBV	1444	2358	0.32%	0.030%
50	9.594	1038	1039	1042	rVV2	2002	1624	0.22%	0.021%
51	9.700	1054	1057	1062	rVV2	1048	1804	0.24%	0.023%
52	9.841	1072	1081	1084	rVB2	4608	7409	0.99%	0.095%
53	10.147	1126	1133	1142	rBV2	71873	130835	17.50%	1.677%
54	10.258	1147	1152	1156	rVB2	1242	1703	0.23%	0.022%
55	10.693	1219	1226	1237	rVB	108166	198977	26.61%	2.551%
56	10.834	1246	1250	1251	rBV2	1970	1881	0.25%	0.024%
57	10.957	1264	1271	1273	rBV	772	1486	0.20%	0.019%
58	11.086	1285	1293	1302	rVB	124498	228317	30.54%	2.927%
59	11.210	1307	1314	1321	rBV2	92499	176348	23.59%	2.261%
60	12.085	1461	1463	1467	rVB3	1667	1856	0.25%	0.024%
61	12.479	1526	1530	1534	rVB4	4263	5627	0.75%	0.072%
62	12.614	1549	1553	1556	rBV	1033	1504	0.20%	0.019%
63	12.649	1556	1559	1568	rVB3	1963	3778	0.51%	0.048%
64	13.095	1632	1635	1637	rBV	1499	1463	0.20%	0.019%
65	13.372	1676	1682	1685	rBV3	1703	3085	0.41%	0.040%
66	13.430	1690	1692	1700	rVB3	1597	2578	0.34%	0.033%
67	13.701	1729	1738	1745	rVV5	9875	19625	2.62%	0.252%
68	13.759	1745	1748	1749	rBV2	1711	1516	0.20%	0.019%
69	13.930	1771	1777	1780	rBV6	1993	3752	0.50%	0.048%
70	14.100	1800	1806	1811	rBV8	3677	8739	1.17%	0.112%
71	14.159	1813	1816	1820	rBV7	2303	3933	0.53%	0.050%
72	14.212	1823	1825	1826	rVV2	2510	1710	0.23%	0.022%
73	14.276	1830	1836	1843	rVV	231790	335406	44.86%	4.300%
74	14.323	1843	1844	1847	rVV3	3198	2791	0.37%	0.036%
75	14.353	1847	1849	1852	rBV4	3130	3780	0.51%	0.048%
76	14.423	1858	1861	1863	rBV4	3682	5237	0.70%	0.067%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011422\
 Data File : BG051978.D
 Acq On : 14 Jan 2022 16:06
 Operator : CG/JU
 Sample : N1100-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGLS5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

77	14.535	1878	1880	1882	rBV2	5000	4552	0.61%	0.058%
78	14.582	1882	1888	1894	rVB	280737	425034	56.85%	5.450%
79	14.646	1895	1899	1902	rBV5	9753	16070	2.15%	0.206%
80	14.682	1902	1905	1910	rVB6	13429	17357	2.32%	0.223%
81	14.723	1910	1912	1916	rVB5	6764	8640	1.16%	0.111%
82	14.770	1916	1920	1924	rBV7	9197	17617	2.36%	0.226%
83	14.846	1929	1933	1934	rBV4	15954	18973	2.54%	0.243%
84	14.887	1935	1940	1949	rVB	236946	380408	50.88%	4.877%
85	14.975	1950	1955	1960	rBV7	16473	34830	4.66%	0.447%
86	15.063	1964	1970	1976	rBV2	89352	159128	21.28%	2.040%
87	15.880	2103	2109	2116	rBV	329475	536060	71.70%	6.873%
88	15.980	2122	2126	2132	rBV2	76016	123986	16.58%	1.590%
89	17.636	2404	2408	2415	rVB	282898	444816	59.50%	5.703%
90	17.736	2421	2425	2433	rVB	371316	542458	72.56%	6.955%
91	20.021	2809	2814	2819	rVB	479475	712984	95.37%	9.142%
92	21.825	3117	3121	3131	rVB3	67851	152524	20.40%	1.956%
93	21.960	3138	3144	3150	rVB	297768	504251	67.45%	6.465%
94	25.203	3687	3696	3709	rVB2	248330	747632	100.00%	9.586%
95	25.449	3728	3738	3752	rVB3	171562	589856	78.90%	7.563%
96	25.996	3829	3831	3833	rVB3	5684	3227	0.43%	0.041%
97	28.234	4208	4212	4213	rBV4	11022	14867	1.99%	0.191%
98	28.880	4320	4322	4324	rBV3	4103	3642	0.49%	0.047%
99	32.123	4872	4874	4875	rBV2	3069	1936	0.26%	0.025%
100	32.346	4910	4912	4913	rBV2	3542	2055	0.27%	0.026%




Sum of corrected areas: 7799419

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011422\
Data File : BG051978.D
Acq On : 14 Jan 2022 16:06
Operator : CG/JU
Sample : N1100-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLS5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

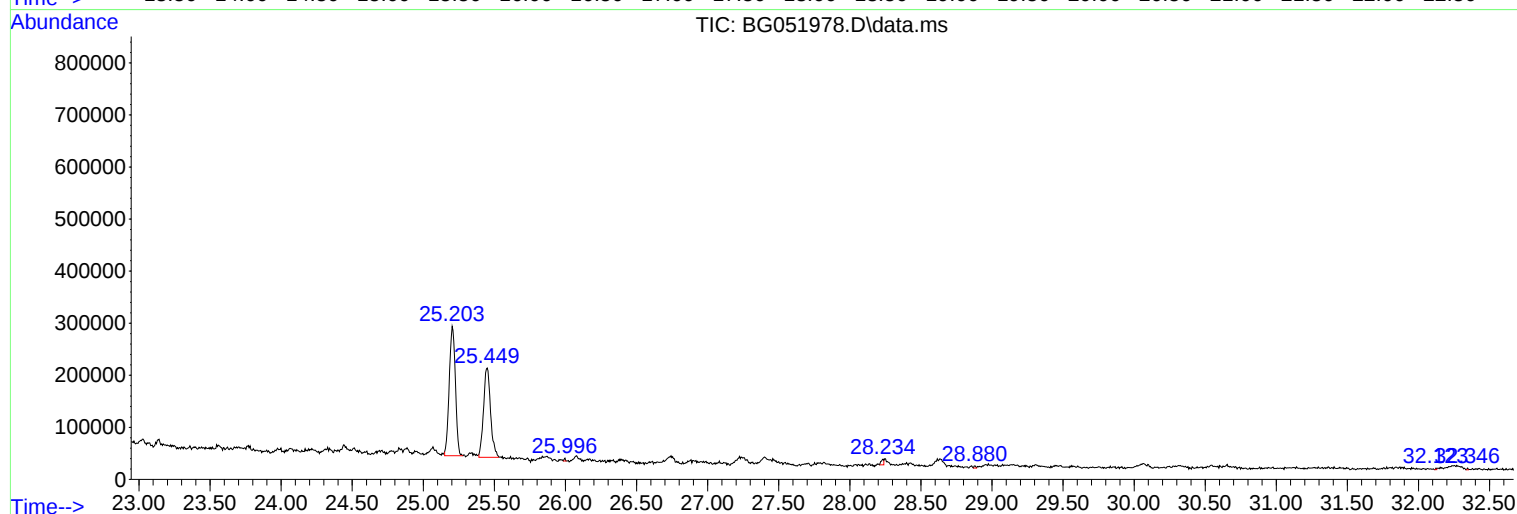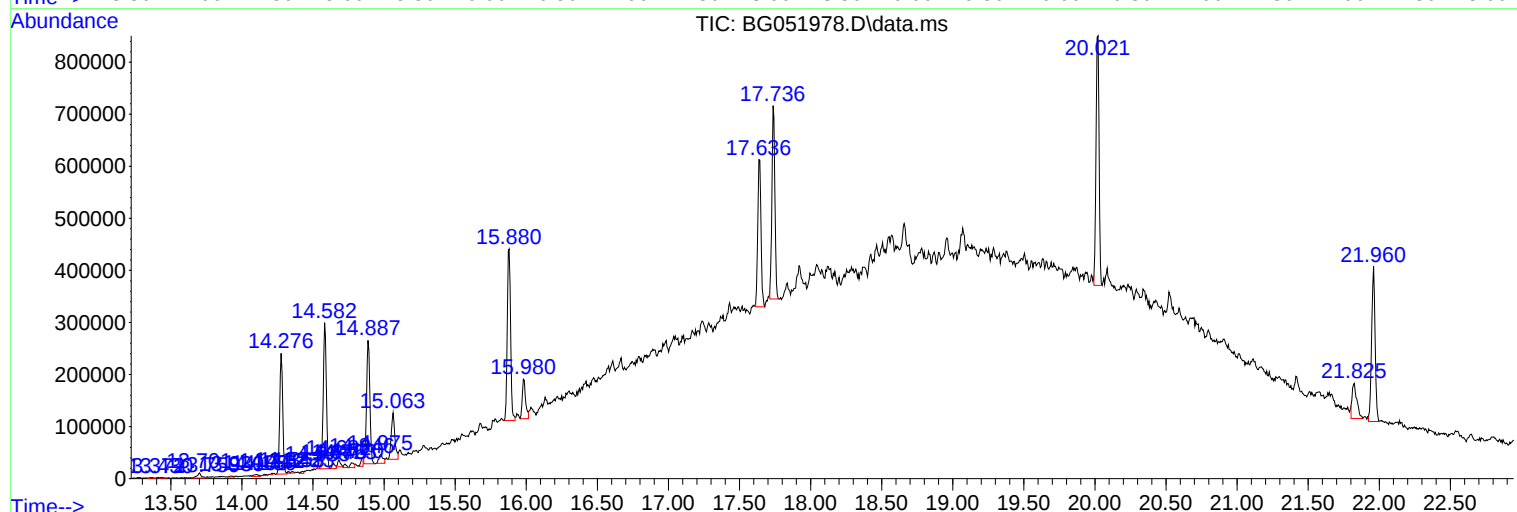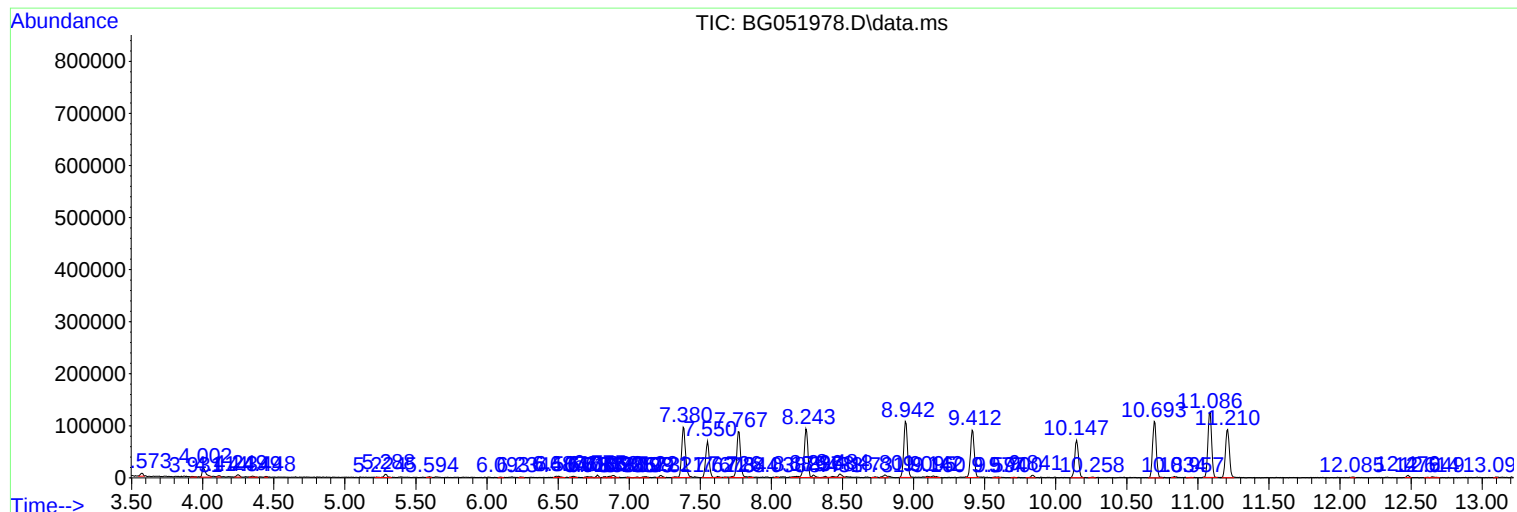

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011422\
Data File : BG051978.D
Acq On : 14 Jan 2022 16:06
Operator : CG/JU
Sample : N1100-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLS5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011422\
Data File : BG051978.D
Acq On : 14 Jan 2022 16:06
Operator : CG/JU
Sample : N1100-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGLS5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc