

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011422\
 Data File : BG051985.D
 Acq On : 14 Jan 2022 21:08
 Operator : CG/JU
 Sample : PB142015BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK015

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051985.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.535	7	8	10	rBV2	1064	848	0.11%	0.011%
2	3.570	10	14	20	rVV4	6327	9573	1.26%	0.124%
3	3.641	24	26	28	rBV	1151	896	0.12%	0.012%
4	3.917	68	73	77	rBV	581	1055	0.14%	0.014%
5	3.999	82	87	102	rBV	68362	119982	15.76%	1.553%
6	4.363	147	149	153	rVB3	1732	1753	0.23%	0.023%
7	4.445	162	163	169	rBV2	1077	1453	0.19%	0.019%
8	4.663	197	200	202	rBV2	795	956	0.13%	0.012%
9	4.692	202	205	208	rVV	955	1043	0.14%	0.014%
10	4.751	213	215	218	rBV2	732	789	0.10%	0.010%
11	4.939	242	247	248	rBV	925	1287	0.17%	0.017%
12	5.097	271	274	278	rBV	539	902	0.12%	0.012%
13	5.203	290	292	296	rBV	931	820	0.11%	0.011%
14	5.979	421	424	427	rBV	659	904	0.12%	0.012%
15	6.020	427	431	436	rVB	787	1268	0.17%	0.016%
16	6.625	530	534	535	rBV	1098	808	0.11%	0.010%
17	7.324	647	653	655	rBV	411	786	0.10%	0.010%
18	7.383	656	663	673	rVV	99490	170189	22.35%	2.203%
19	7.553	685	692	699	rVB	63162	105897	13.91%	1.371%
20	7.770	723	729	737	rVB	88357	151703	19.93%	1.964%
21	7.829	737	739	743	rVB	873	835	0.11%	0.011%
22	8.246	804	810	816	rVB	83496	138796	18.23%	1.797%
23	8.863	910	915	918	rBV	442	779	0.10%	0.010%
24	8.945	923	929	938	rBV	122497	209234	27.48%	2.708%
25	9.415	1001	1009	1016	rBV	91388	161456	21.21%	2.090%
26	10.149	1126	1134	1141	rVB2	83932	146168	19.20%	1.892%
27	10.531	1198	1199	1204	rVB	681	772	0.10%	0.010%
28	10.696	1220	1227	1236	rBV	120892	219361	28.81%	2.839%
29	10.825	1246	1249	1252	rBV	707	912	0.12%	0.012%
30	10.989	1270	1277	1279	rBB	541	940	0.12%	0.012%
31	11.089	1286	1294	1302	rVB	117527	216260	28.40%	2.799%
32	11.207	1306	1314	1322	rBV	123404	225597	29.63%	2.920%
33	12.182	1476	1480	1483	rVB2	580	903	0.12%	0.012%
34	12.382	1509	1514	1515	rBV2	641	1004	0.13%	0.013%
35	12.658	1556	1561	1565	rBV4	1993	3269	0.43%	0.042%
36	13.627	1722	1726	1728	rBV4	467	794	0.10%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011422\
 Data File : BG051985.D
 Acq On : 14 Jan 2022 21:08
 Operator : CG/JU
 Sample : PB142015BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK015

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

37	14.279	1830	1837	1845	rVB	269307	386584	50.78%	5.004%
38	14.585	1880	1889	1899	rBV	283690	452118	59.38%	5.852%
39	14.749	1915	1917	1922	rBV	550	872	0.11%	0.011%
40	14.890	1933	1941	1949	rBV	239584	365920	48.06%	4.737%
41	15.066	1965	1971	1985	rBV	117947	217354	28.55%	2.814%
42	15.425	2028	2032	2036	rVB	774	1307	0.17%	0.017%
43	15.472	2036	2040	2043	rBV	690	1241	0.16%	0.016%
44	15.730	2081	2084	2088	rVV	1262	1088	0.14%	0.014%
45	15.883	2103	2110	2116	rVB	380752	596428	78.34%	7.720%
46	15.983	2121	2127	2136	rBV	103733	149679	19.66%	1.937%
47	16.130	2150	2152	2154	rVB	922	778	0.10%	0.010%
48	16.359	2188	2191	2194	rBV	830	1191	0.16%	0.015%
49	16.511	2214	2217	2219	rVB	1003	880	0.12%	0.011%
50	16.576	2223	2228	2230	rVB	1031	1397	0.18%	0.018%
51	16.658	2240	2242	2246	rVB	972	959	0.13%	0.012%
52	16.823	2268	2270	2273	rBV	740	944	0.12%	0.012%
53	16.923	2285	2287	2289	rVB	946	793	0.10%	0.010%
54	17.034	2305	2306	2311	rBV2	1461	1559	0.20%	0.020%
55	17.117	2315	2320	2322	rVV2	1096	1111	0.15%	0.014%
56	17.152	2322	2326	2327	rBV3	1442	1105	0.15%	0.014%
57	17.205	2332	2335	2336	rBV	1283	888	0.12%	0.011%
58	17.293	2346	2350	2353	rVB3	801	1155	0.15%	0.015%
59	17.369	2361	2363	2365	rVV2	1394	1027	0.13%	0.013%
60	17.416	2369	2371	2372	rVV2	1798	995	0.13%	0.013%
61	17.428	2372	2373	2376	rVV3	1365	1045	0.14%	0.014%
62	17.504	2384	2386	2388	rVB2	1594	1471	0.19%	0.019%
63	17.534	2388	2391	2393	rBV2	1322	1704	0.22%	0.022%
64	17.639	2402	2409	2416	rBV	358104	538235	70.70%	6.967%
65	17.739	2419	2426	2434	rBV	488070	719868	94.55%	9.318%
66	17.857	2443	2446	2447	rBV2	1316	996	0.13%	0.013%
67	17.868	2447	2448	2452	rBV4	1629	1738	0.23%	0.022%
68	17.968	2464	2465	2469	rVB4	1125	1005	0.13%	0.013%
69	18.286	2516	2519	2524	rBV5	1595	2120	0.28%	0.027%
70	18.432	2541	2544	2546	rBV2	653	819	0.11%	0.011%
71	18.532	2558	2561	2563	rBV3	1590	2051	0.27%	0.027%
72	18.609	2572	2574	2575	rBV2	1485	959	0.13%	0.012%
73	18.650	2578	2581	2582	rBV3	1685	1351	0.18%	0.017%
74	18.667	2582	2584	2585	rBV2	1411	1066	0.14%	0.014%
75	18.779	2601	2603	2605	rVB3	1816	1097	0.14%	0.014%
76	18.797	2605	2606	2610	rVB4	2175	2081	0.27%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011422\
 Data File : BG051985.D
 Acq On : 14 Jan 2022 21:08
 Operator : CG/JU
 Sample : PB142015BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK015

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
 Title : SVOA CALIBRATION

77	18.832	2610	2612	2615	rBV3	1781	2162	0.28%	0.028%
78	18.873	2615	2619	2620	rBV4	1469	1992	0.26%	0.026%
79	18.914	2625	2626	2627	rBV	1839	1196	0.16%	0.015%
80	18.979	2635	2637	2638	rBV2	2080	1469	0.19%	0.019%
81	19.020	2643	2644	2646	rVB2	2570	1245	0.16%	0.016%
82	19.049	2646	2649	2650	rBV3	2210	2511	0.33%	0.033%
83	19.137	2661	2664	2667	rBV5	2734	4428	0.58%	0.057%
84	19.184	2671	2672	2673	rBV	2808	1521	0.20%	0.020%
85	19.584	2736	2740	2746	rBV9	9710	15021	1.97%	0.194%
86	20.018	2808	2814	2820	rVB	532363	761345	100.00%	9.855%
87	20.142	2833	2835	2838	rBV4	5062	5736	0.75%	0.074%
88	20.377	2873	2875	2877	rBV3	6221	6131	0.81%	0.079%
89	21.963	3139	3145	3154	rVB	258621	466171	61.23%	6.034%
90	25.217	3689	3699	3707	rVB	205227	599331	78.72%	7.758%
91	25.452	3730	3739	3754	rVB3	149303	490163	64.38%	6.345%




Sum of corrected areas: 7725393

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011422\
Data File : BG051985.D
Acq On : 14 Jan 2022 21:08
Operator : CG/JU
Sample : PB142015BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK015

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

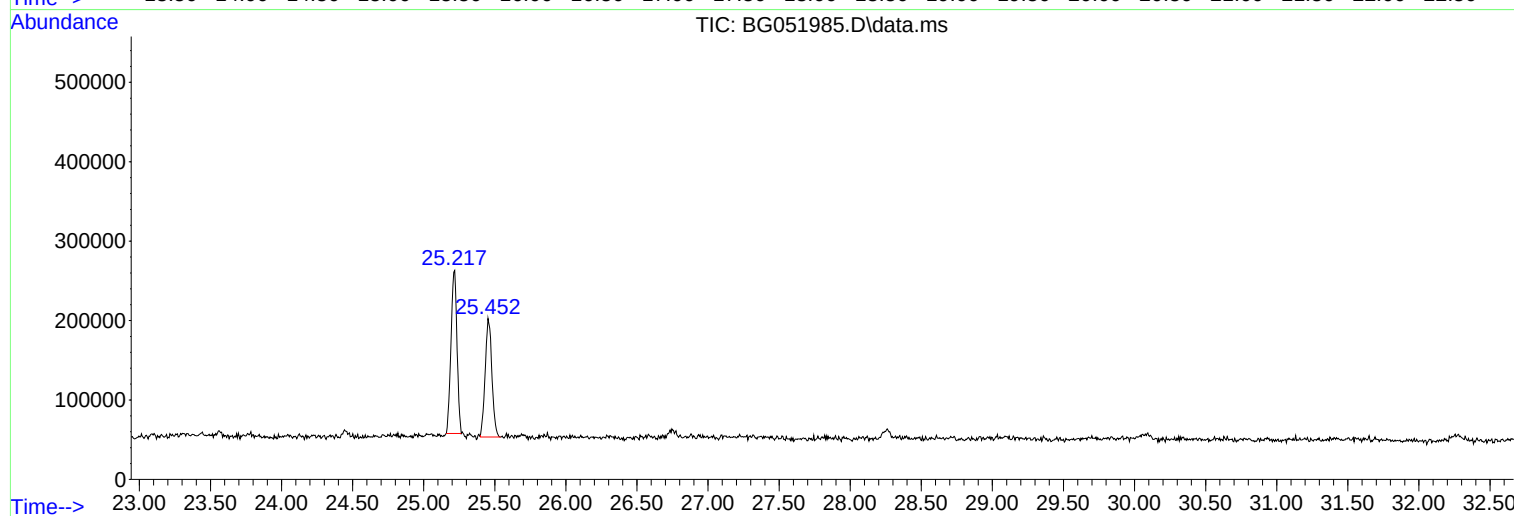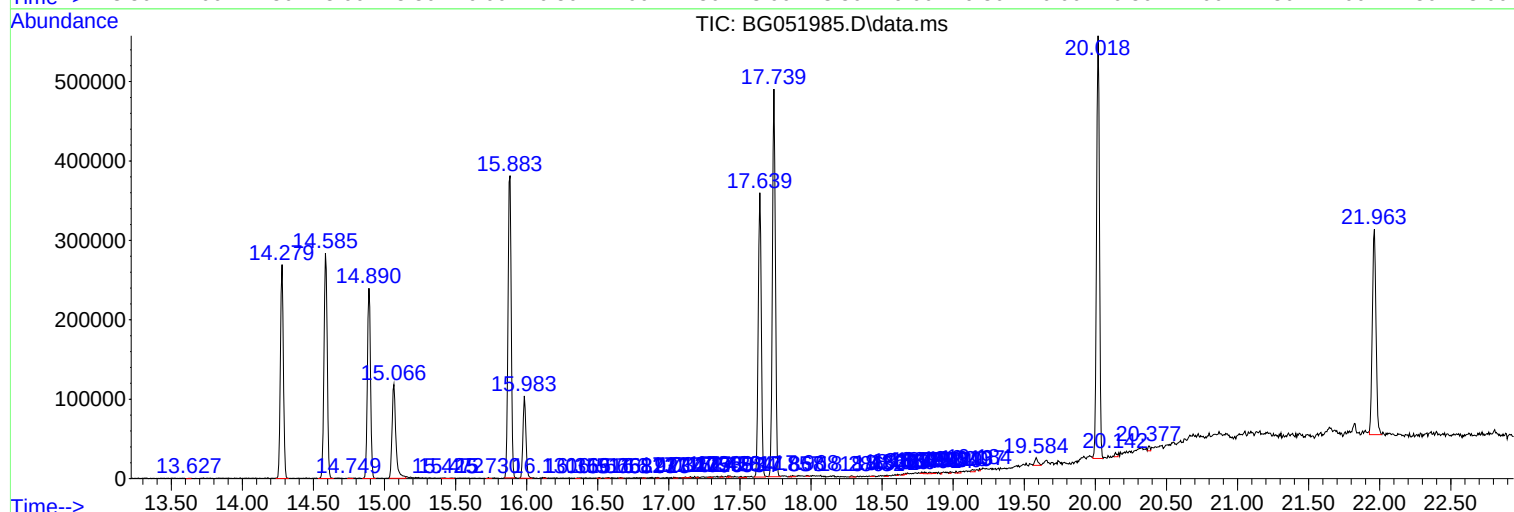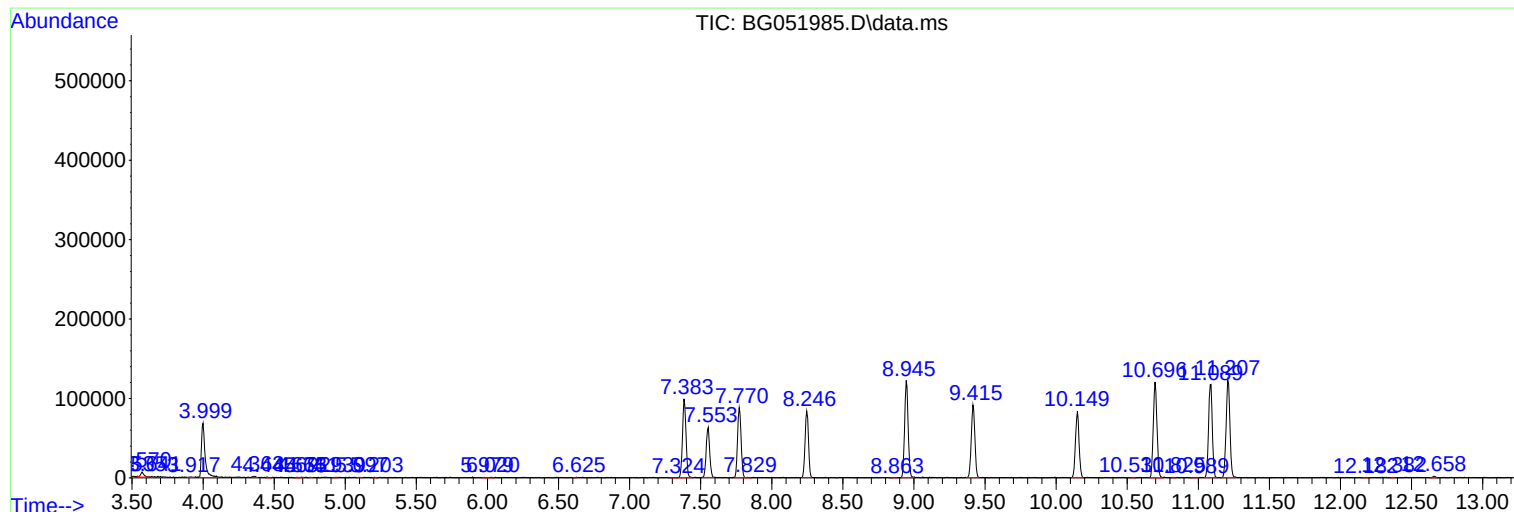

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011422\
Data File : BG051985.D
Acq On : 14 Jan 2022 21:08
Operator : CG/JU
Sample : PB142015BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK015

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011422\
Data File : BG051985.D
Acq On : 14 Jan 2022 21:08
Operator : CG/JU
Sample : PB142015BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK015

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc