

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG011516\
 Data File : BG020757.D
 Acq On : 15 Jan 2016 18:00
 Operator : SJ/IZ
 Sample : H1101-17 5X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BC9F8

Quant Time: Jan 15 22:20:40 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG011216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 15 22:12:27 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.04	152	16351	20.00	ng/ul	0.00
18) Naphthalene-d8	10.86	136	71342	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.68	164	48407	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.43	188	116841	20.00	ng/ul	0.00
78) Chrysene-d12	21.70	240	140106	20.00	ng/ul	0.00
86) Perylene-d12	24.96	264	136017	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	7.21	99	4818	3.44	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.37	67	2810	3.33	ng/ul	0.00
9) 2-Chlorophenol-d4	7.58	132	4428	4.03	ng/ul	0.00
13) 4-Methylphenol-d8	8.76	113	3440	2.91	ng/ul	0.00
19) Nitrobenzene-d5	9.22	128	2087	3.71	ng/ul	0.00
22) 2-Nitrophenol-d4	9.94	143	2584	3.95	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.49	165	4545	3.65	ng/ul	0.00
29) 4-Chloroaniline-d4	11.01	131	1424	1.16	ng/ul	0.02
44) Dimethylphthalate-d6	14.08	166	16931	4.01	ng/ul	0.00
47) Acenaphthylene-d8	14.38	160	20563	4.33	ng/ul	0.00
52) 4-Nitrophenol-d4	14.92	143	553	0.97	ng/ul	0.03
58) Fluorene-d10	15.67	176	16493	4.38	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.81	200	1327	2.09	ng/ul	0.00
71) Anthracene-d10	17.53	188	25113	4.39	ng/ul	0.00
79) Pyrene-d10	19.81	212	29353	4.40	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.74	264	30064	4.15	ng/ul	0.00

Target Compounds


						Qvalue
28) Naphthalene	10.90	128	4493	1.11	ng/ul	97
45) Dimethylphthalate	14.12	163	7532	1.66	ng/ul	97
50) Acenaphthene	14.74	153	4419	1.28	ng/ul	95
59) Fluorene	15.73	166	7221	1.70	ng/ul	92
70) Phenanthrene	17.47	178	155736	22.40	ng/ul	99
72) Anthracene	17.56	178	21450	3.06	ng/ul	99
75) Carbazole	17.83	167	9010	1.57	ng/ul	96
77) Fluoranthene	19.48	202	266157	31.50	ng/ul	99
80) Pyrene	19.85	202	339540	38.22	ng/ul	99
83) Benzo(a)anthracene	21.69	228	169290	19.37	ng/ul	98
85) Chrysene	21.75	228	187075	22.64	ng/ul	96
88) Benzo(b)fluoranthene	23.92	252	156387	17.85	ng/ul#	96
89) Benzo(k)fluoranthene	23.92	252	156387	18.07	ng/ul	96
91) Benzo(a)pyrene	24.80	252	139041	16.49	ng/ul	99
92) Indeno(1,2,3-cd)pyrene	28.68	276	76680	7.71	ng/ul	96
94) Benzo(g,h,i)perylene	29.85	276	44125	5.38	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG011516\
Data File : BG020757.D
Acq On : 15 Jan 2016 18:00
Operator : SJ/IZ
Sample : H1101-17 5X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BC9F8

Quant Time: Jan 15 22:20:40 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG011216.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 15 22:12:27 2016
Response via : Initial Calibration




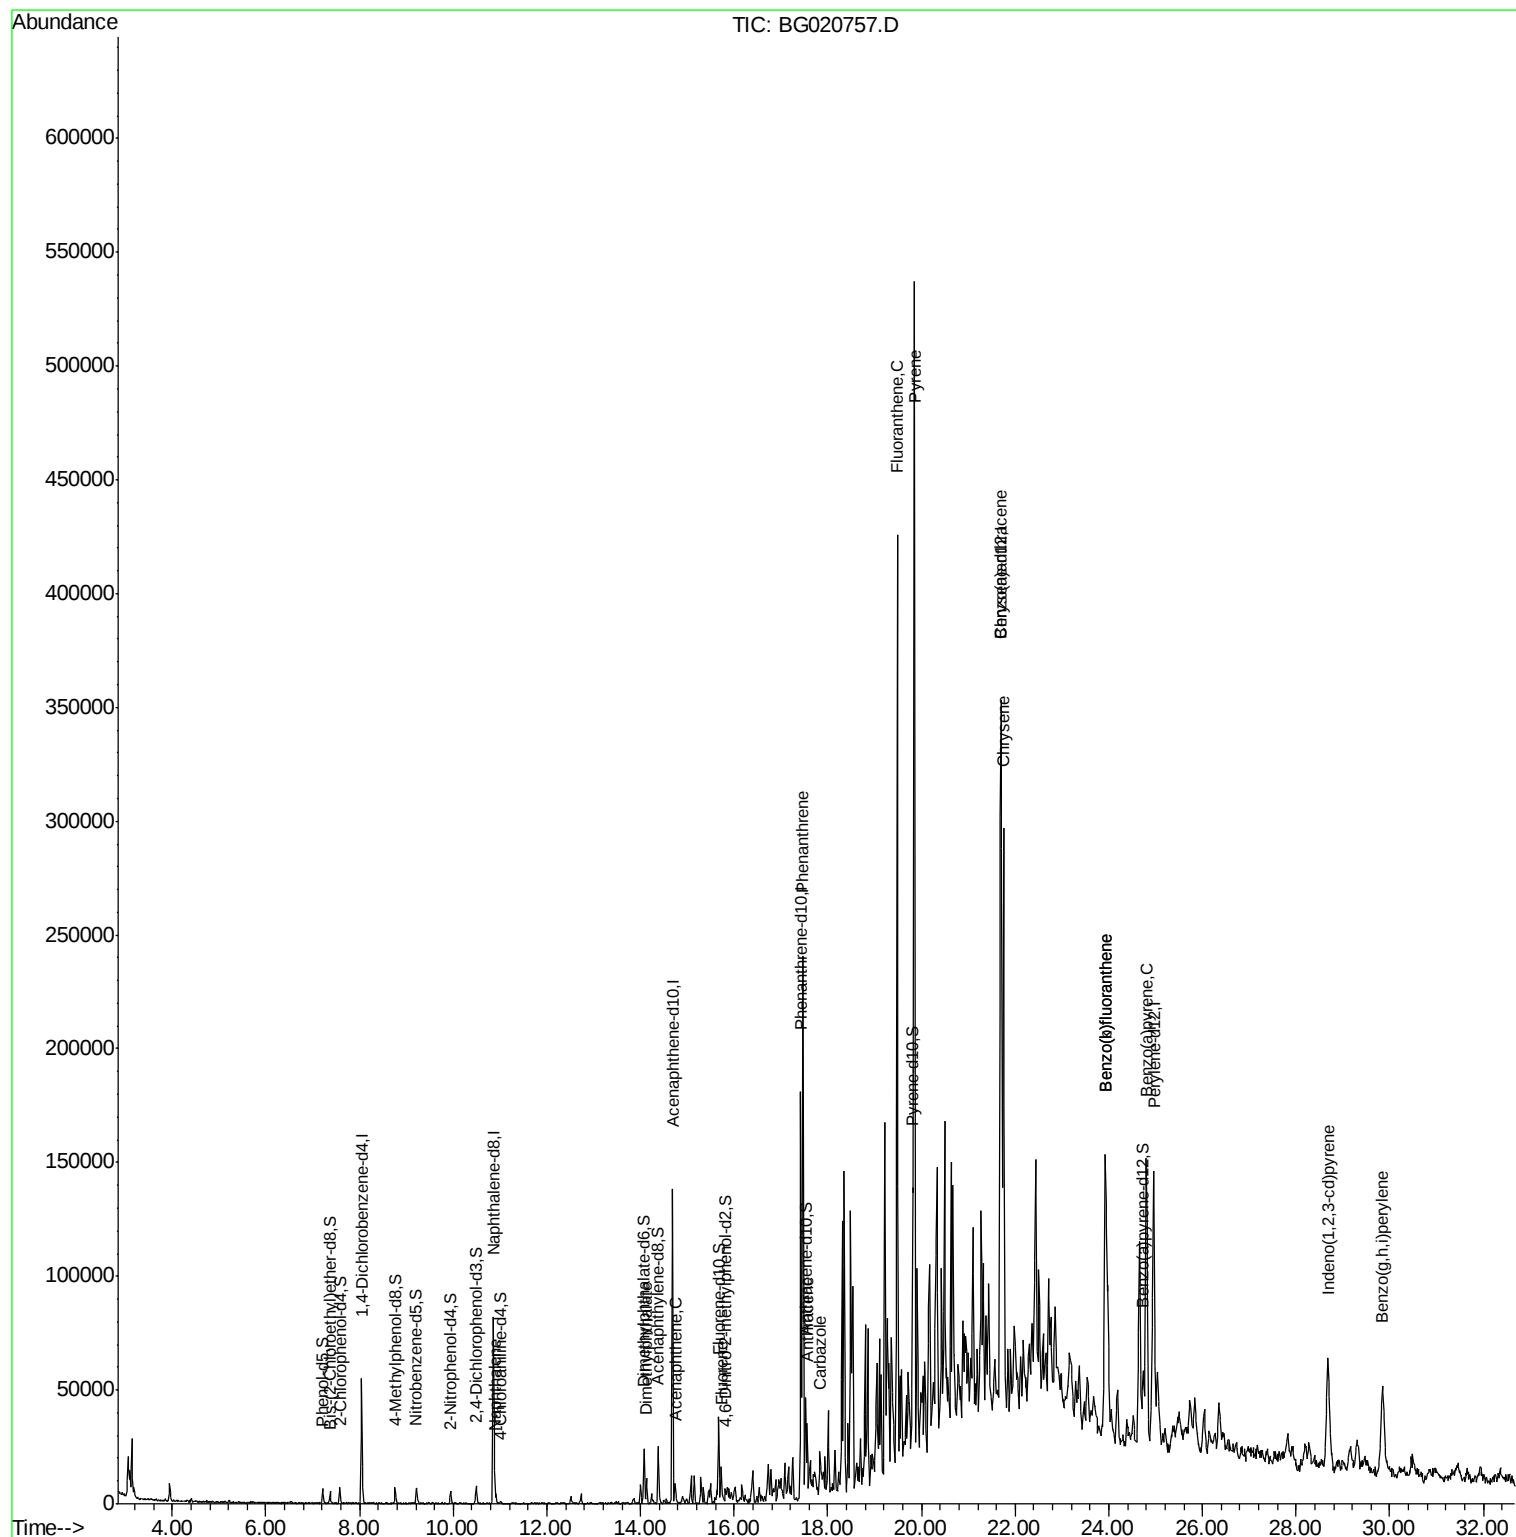


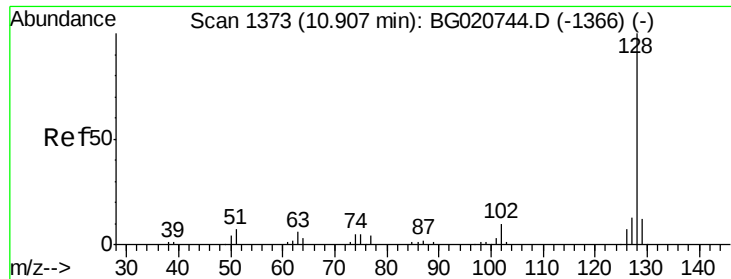

#28
Naphthalene
Concen: 1.11 ng/ul
RT: 10.90 min Scan# 1373
Delta R.T. -0.00 min
Lab File: BG020757.D
Acq: 15 Jan 2016 18:00




Instrument :
BNA_G
ClientSampleId :
BC9F8


Tgt Ion:128 Resp: 4493
Ion Ratio Lower Upper
128 100
129 11.0 8.3 12.5
127 11.9 10.8 16.2

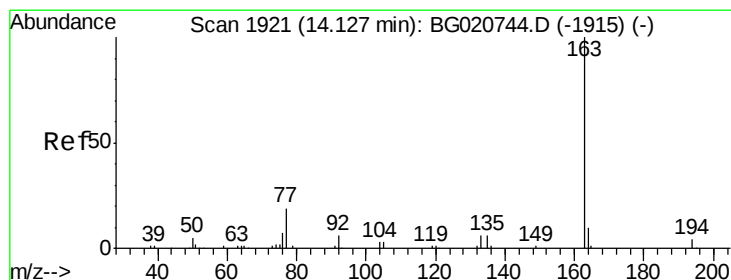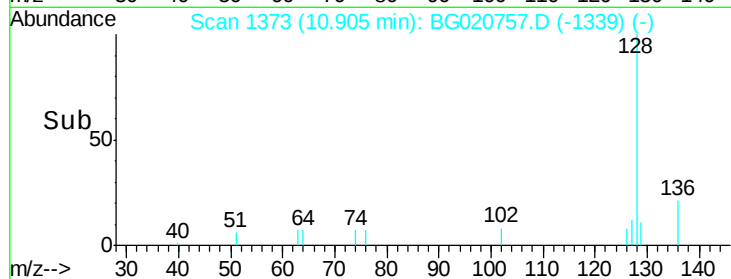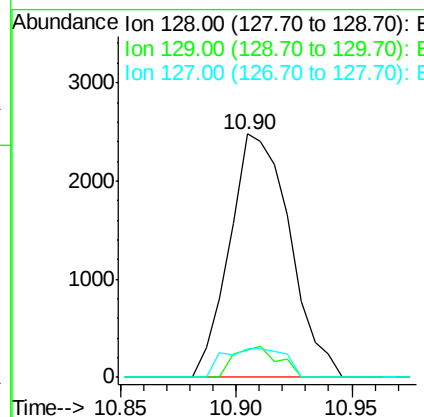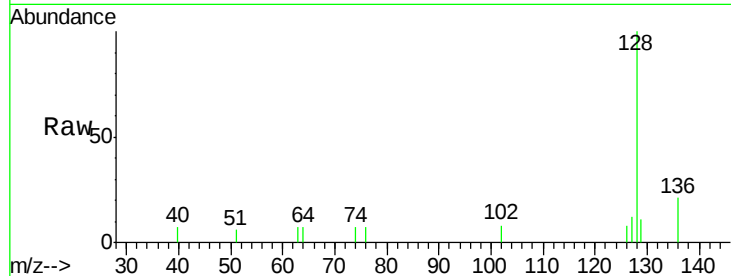

#45
Dimethylphthalate
Concen: 1.66 ng/ul
RT: 14.12 min Scan# 1921
Delta R.T. -0.00 min
Lab File: BG020757.D
Acq: 15 Jan 2016 18:00

Tgt Ion:163 Resp: 7532
Ion Ratio Lower Upper
163 100
194 5.6 4.0 6.0
164 11.7 8.4 12.6

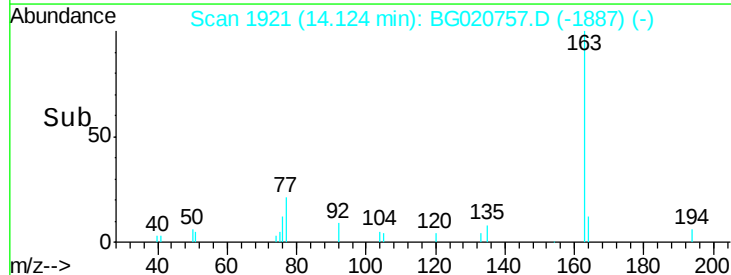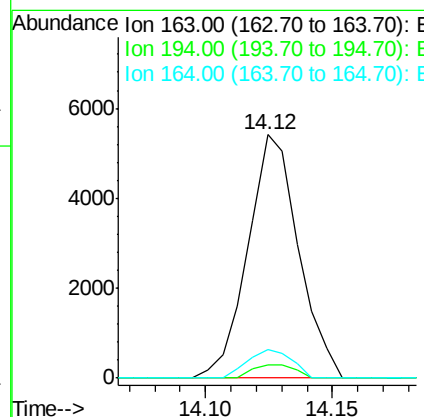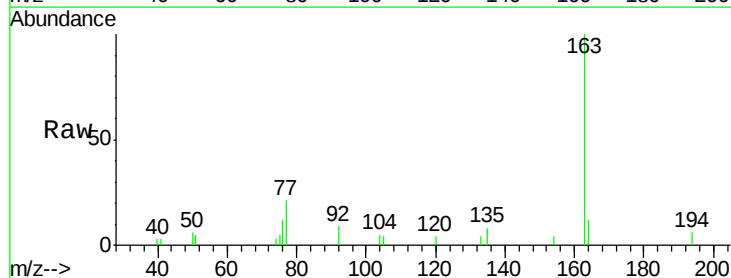

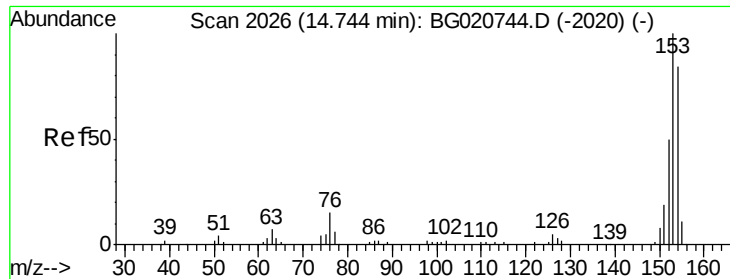

#50

Acenaphthene

Concen: 1.28 ng/ul

RT: 14.74 min Scan# 2026

Delta R.T. -0.00 min

Lab File: BG020757.D

Acq: 15 Jan 2016 18:00

Instrument :

BNA_G

ClientSampleId :

BC9F8


Tgt Ion:153 Resp: 4419

Ion Ratio Lower Upper

153 100

152 48.5 37.9 56.9




154 80.9 69.8 104.6

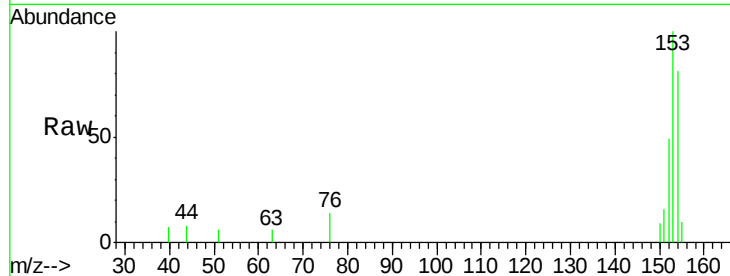

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

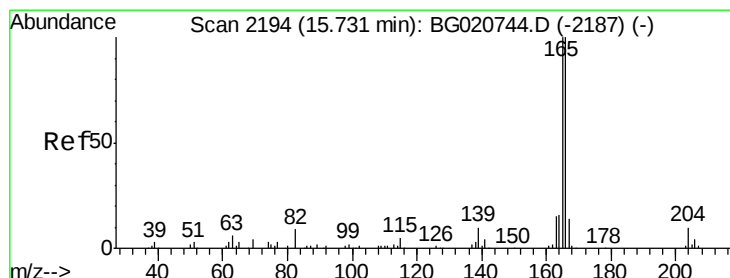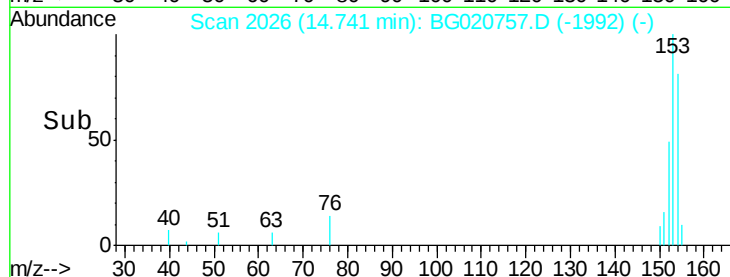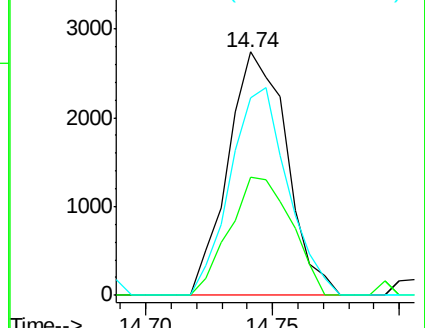

#59

Fluorene

Concen: 1.70 ng/ul

RT: 15.73 min Scan# 2194

Delta R.T. -0.00 min

Lab File: BG020757.D

Acq: 15 Jan 2016 18:00


Tgt Ion:166 Resp: 7221

Ion Ratio Lower Upper

166 100

165 89.3 78.4 117.6



167 15.4 11.1 16.7

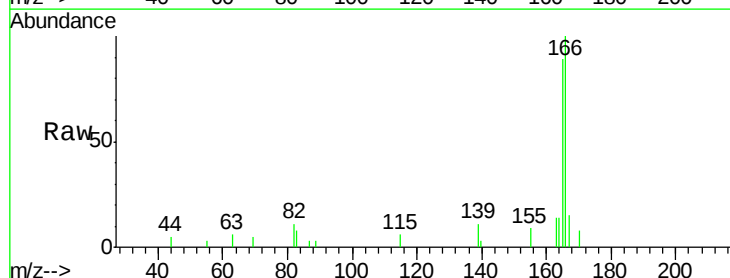


Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

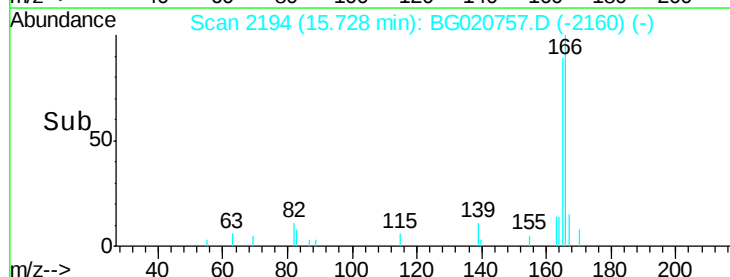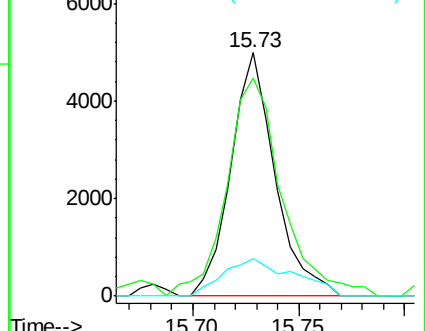

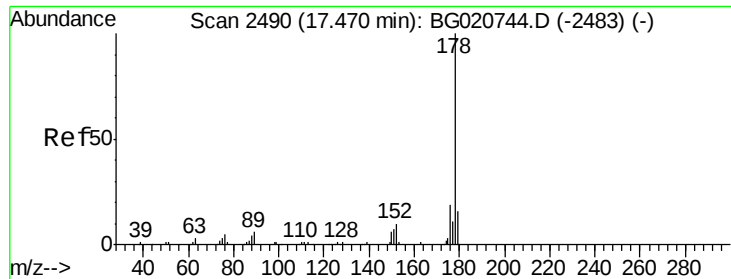

#70

Phenanthrene

Concen: 22.40 ng/ul

RT: 17.47 min Scan# 2490

Delta R.T. -0.00 min

Lab File: BG020757.D

Acq: 15 Jan 2016 18:00

Instrument :

BNA_G

ClientSampleId :

BC9F8


Tgt Ion:178 Resp: 155736

Ion Ratio Lower Upper

178 100

179 15.7 12.3 18.5




176 18.9 15.4 23.0

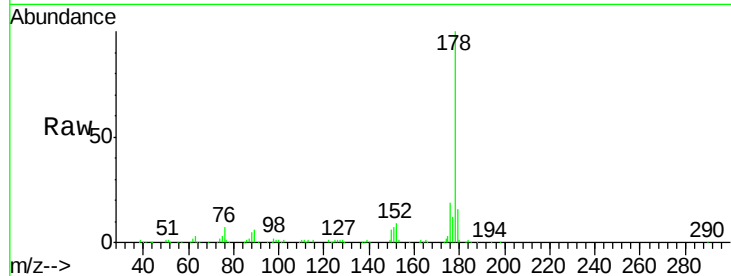

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

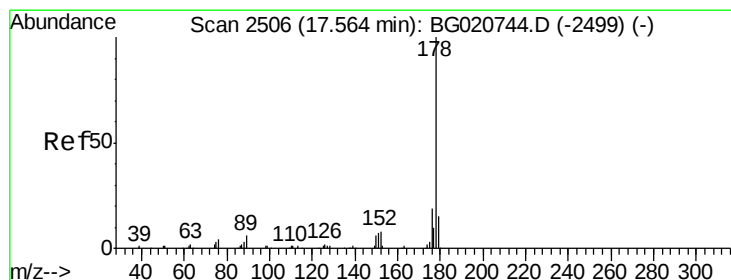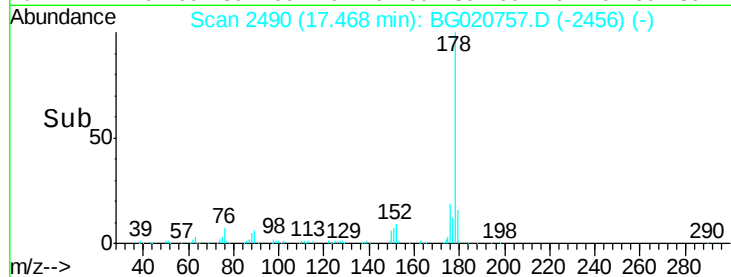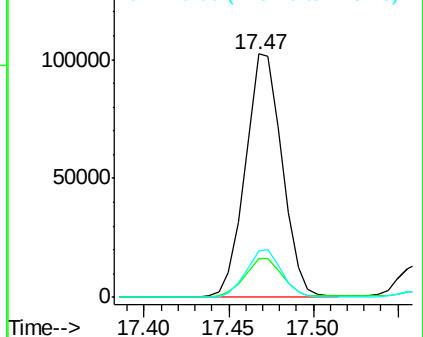

#72

Anthracene

Concen: 3.06 ng/ul

RT: 17.56 min Scan# 2506

Delta R.T. -0.00 min

Lab File: BG020757.D

Acq: 15 Jan 2016 18:00


Tgt Ion:178 Resp: 21450

Ion Ratio Lower Upper

178 100

179 16.5 13.4 20.2



176 18.8 15.4 23.0

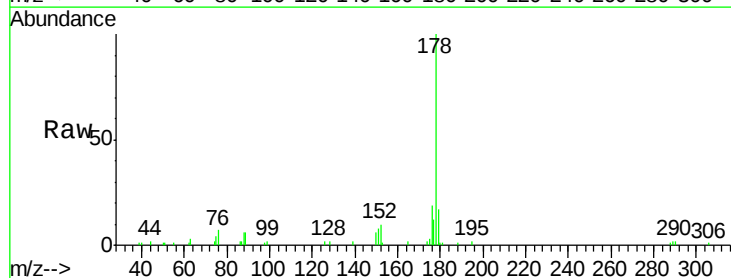


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

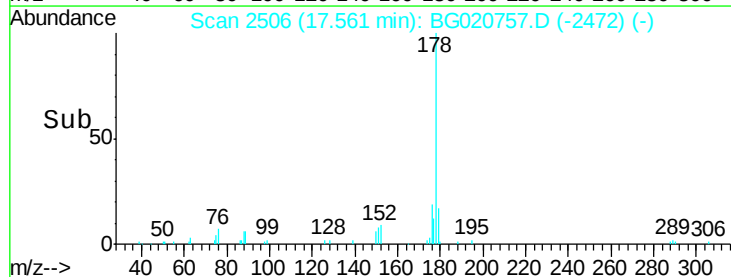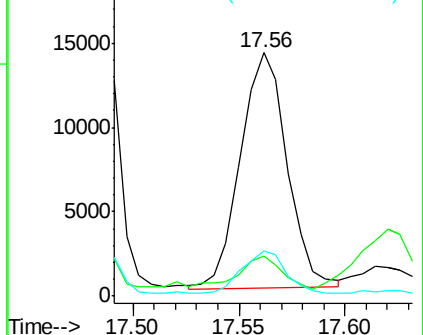

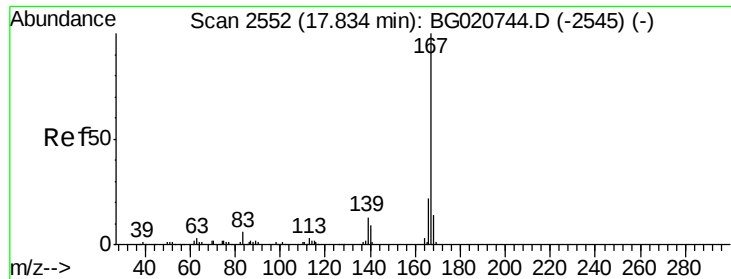

#75

Carbazole

Concen: 1.57 ng/ul

RT: 17.83 min Scan# 2552

Delta R.T. -0.00 min

Lab File: BG020757.D

Acq: 15 Jan 2016 18:00

Instrument :

BNA_G

ClientSampleId :

BC9F8


Tgt Ion:167 Resp: 9010

Ion Ratio Lower Upper

167 100

166 23.7 17.0 25.4




139 11.9 9.1 13.7

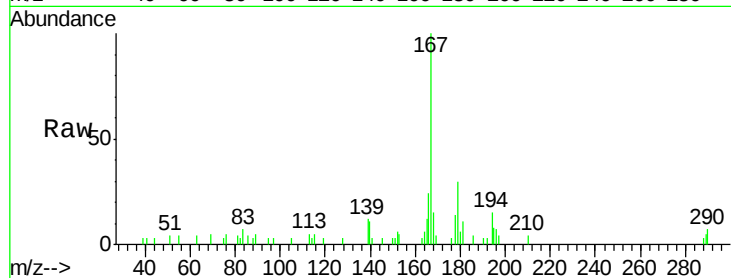

Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E

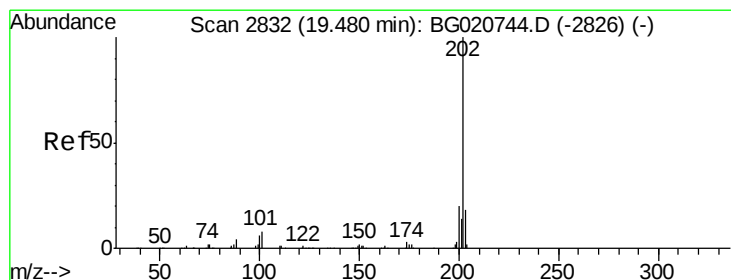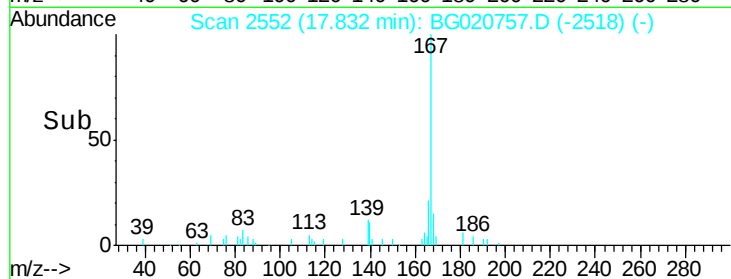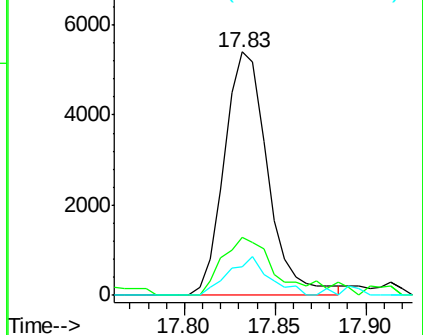

#77

Fluoranthene

Concen: 31.50 ng/ul

RT: 19.48 min Scan# 2833

Delta R.T. 0.00 min

Lab File: BG020757.D

Acq: 15 Jan 2016 18:00


Tgt Ion:202 Resp: 266157

Ion Ratio Lower Upper

202 100

101 7.0 6.1 9.1



100 5.6 4.6 7.0

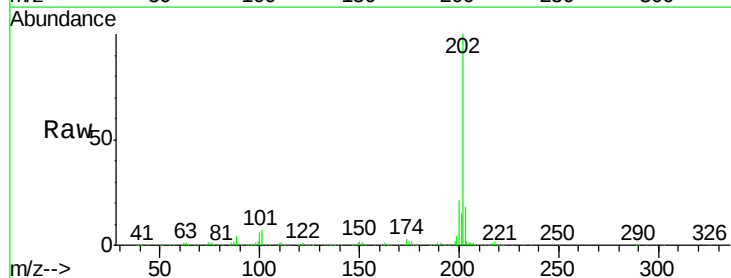


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

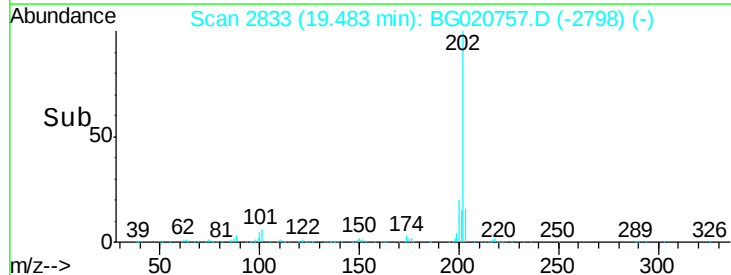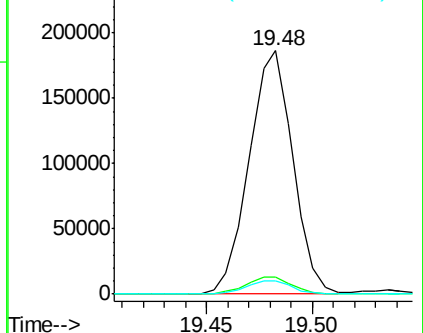


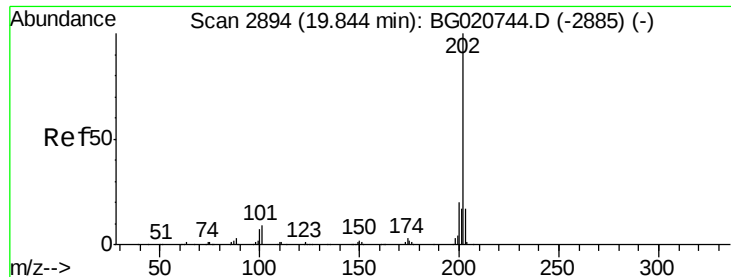




#80
 Pyrene
 Concen: 38.22 ng/ul
 RT: 19.85 min Scan# 2895
 Delta R.T. 0.00 min
 Lab File: BG020757.D
 Acq: 15 Jan 2016 18:00

Instrument :
 BNA_G
 ClientSampleId :
 BC9F8

Tgt Ion:	202	Resp:	339540
Ion	Ratio	Lower	Upper
202	100		
101	7.9	6.9	10.3
100	7.1	5.6	8.4

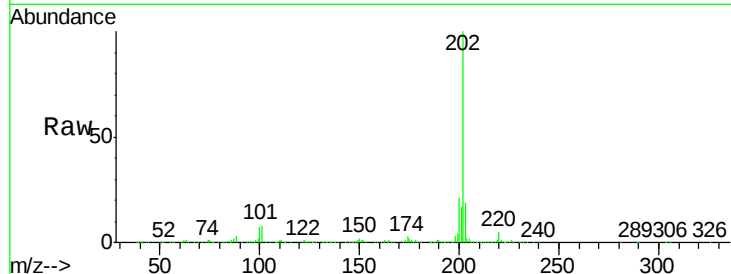


Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): B

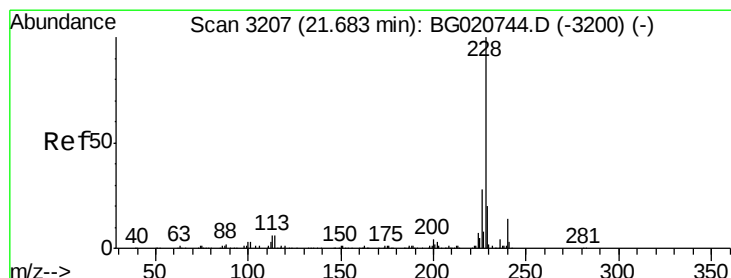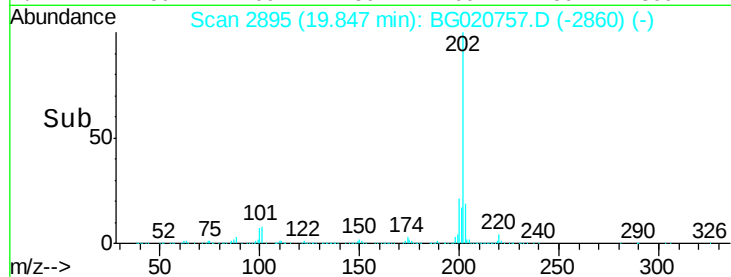
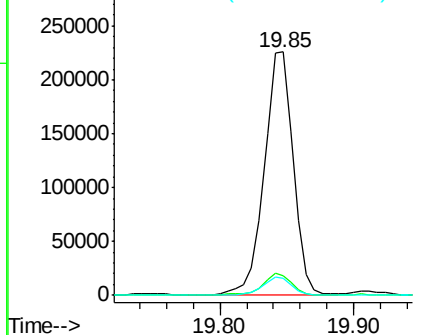



#83
 Benzo(a)anthracene
 Concen: 19.37 ng/ul
 RT: 21.69 min Scan# 3208
 Delta R.T. 0.00 min
 Lab File: BG020757.D
 Acq: 15 Jan 2016 18:00

Tgt Ion:	228	Resp:	169290
Ion	Ratio	Lower	Upper
228	100		
229	21.5	16.0	24.0
226	26.8	21.8	32.8

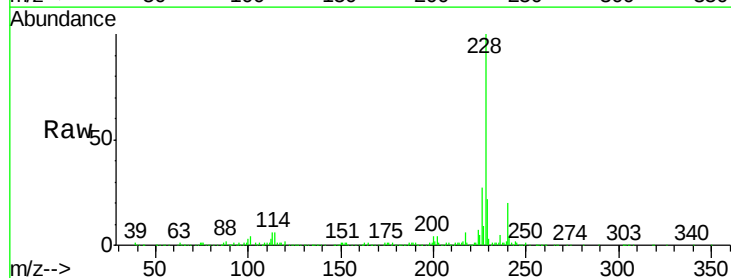

Abundance Ion 228.00 (227.70 to 228.70): E
 Ion 229.00 (228.70 to 229.70): E
 Ion 226.00 (225.70 to 226.70): E

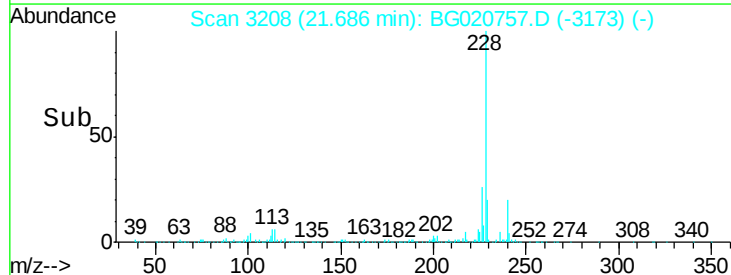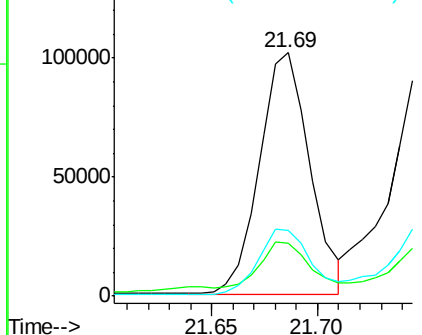

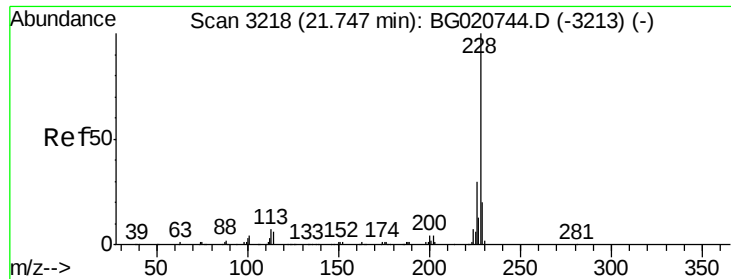

#85

Chrysene

Concen: 22.64 ng/ul

RT: 21.75 min Scan# 3219

Delta R.T. 0.00 min

Lab File: BG020757.D

Acq: 15 Jan 2016 18:00

Instrument :

BNA_G

ClientSampleId :

BC9F8


Tgt Ion:228 Resp: 187075

Ion Ratio Lower Upper

228 100

226 32.2 24.1 36.1




229 22.2 16.0 24.0

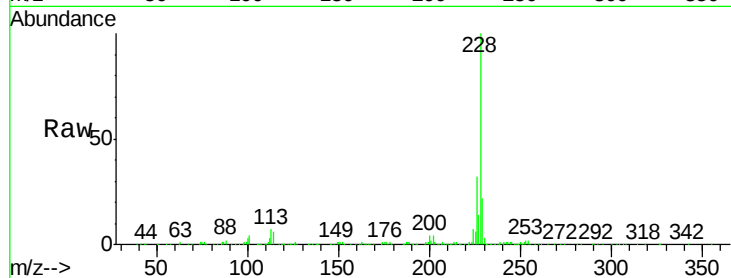

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

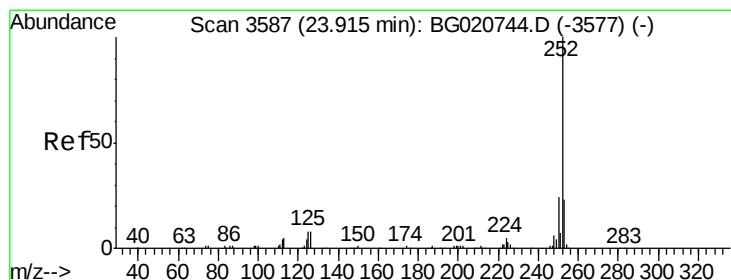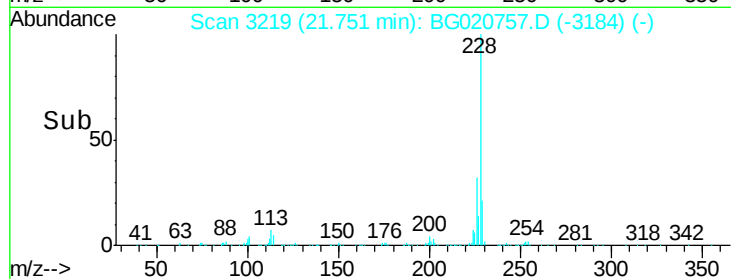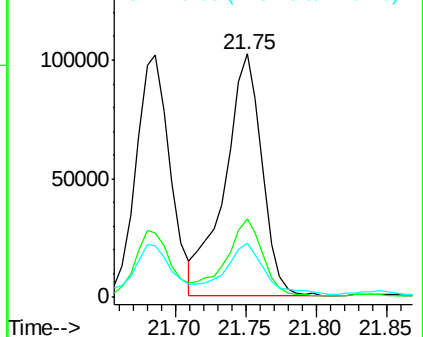

#88

Benzo(b)fluoranthene

Concen: 17.85 ng/ul

RT: 23.92 min Scan# 3589

Delta R.T. 0.01 min

Lab File: BG020757.D

Acq: 15 Jan 2016 18:00


Tgt Ion:252 Resp: 156387

Ion Ratio Lower Upper

252 100

253 23.4 17.4 26.0



125 7.8 4.9 7.3#

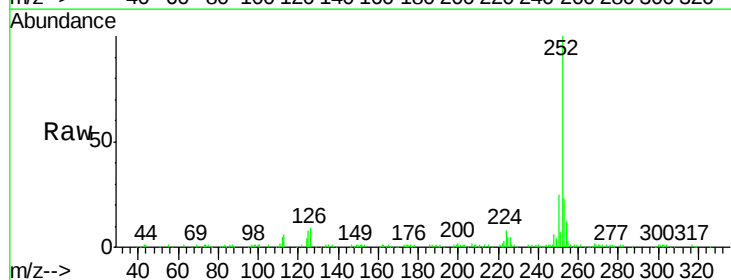


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

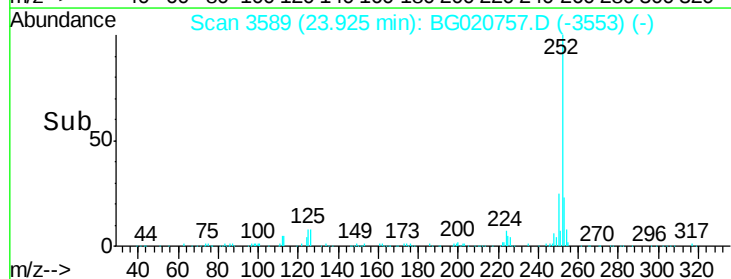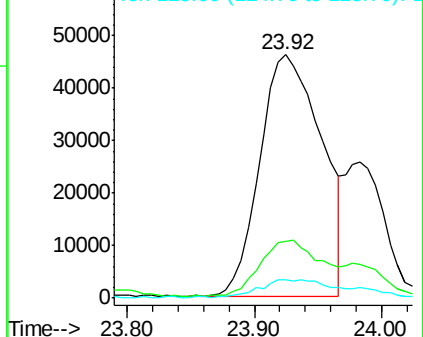

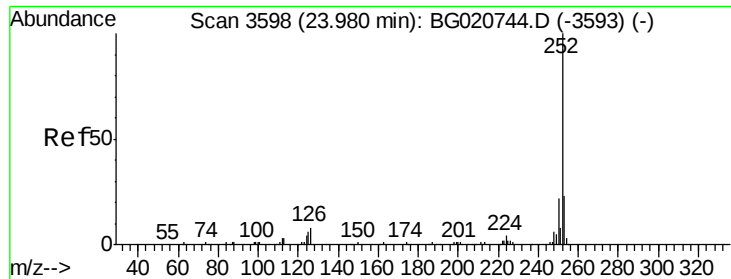

#89

Benzo(k)fluoranthene

Concen: 18.07 ng/u1

RT: 23.92 min Scan# 3589

Delta R.T. -0.06 min

Lab File: BG020757.D

Acq: 15 Jan 2016 18:00





Instrument :

BNA_G

ClientSampleId :

BC9F8

Tgt Ion:	252	Resp:	156387
Ion Ratio	Lower	Upper	
252	100		
253	23.4	17.1	25.7
125	7.8	5.4	8.0

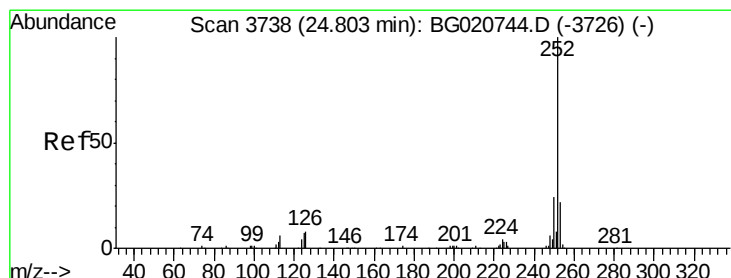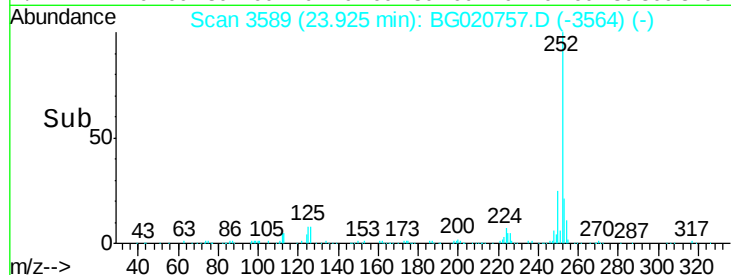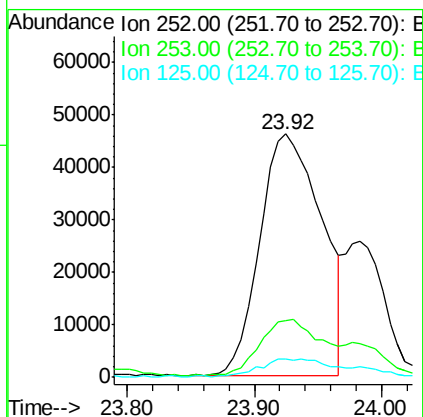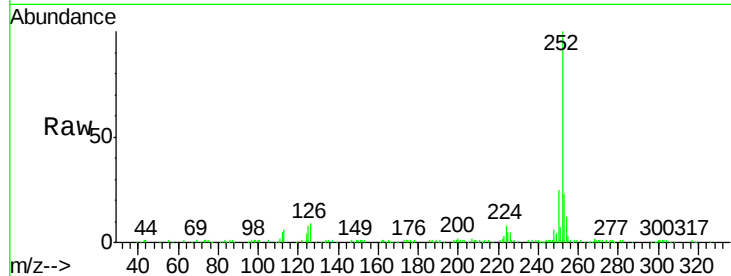

#91

Benzo(a)pyrene

Concen: 16.49 ng/u1




RT: 24.80 min Scan# 3738


Delta R.T. -0.00 min

Lab File: BG020757.D

Acq: 15 Jan 2016 18:00

Tgt Ion:	252	Resp:	139041
Ion Ratio	Lower	Upper	
252	100		
253	21.0	17.2	25.8
125	6.5	5.8	8.6

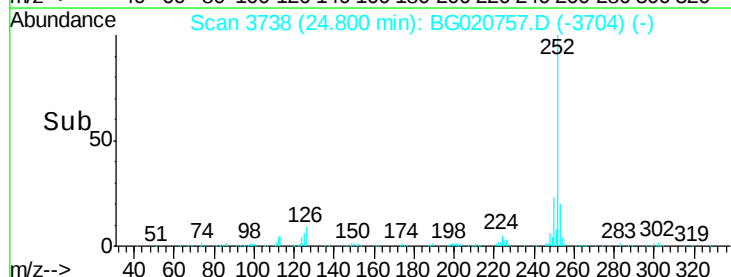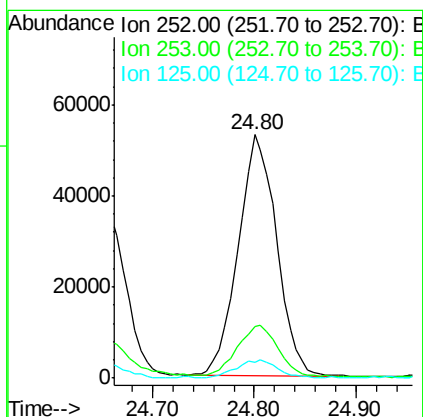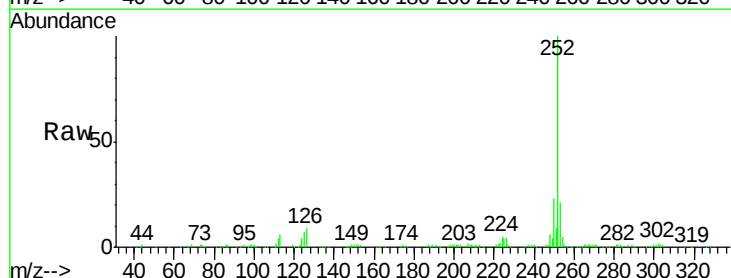

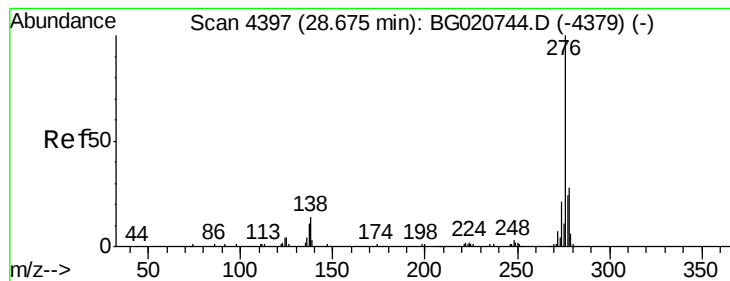

#92

Indeno(1,2,3-cd)pyrene

Concen: 7.71 ng/u1

RT: 28.68 min Scan# 4398

Delta R.T. 0.00 min

Lab File: BG020757.D

Acq: 15 Jan 2016 18:00

Instrument :

BNA_G

ClientSampleId :

BC9F8


Tgt Ion:276 Resp: 76680

Ion Ratio Lower Upper

276 100

138 13.5 10.9 16.3




277 26.3 18.9 28.3

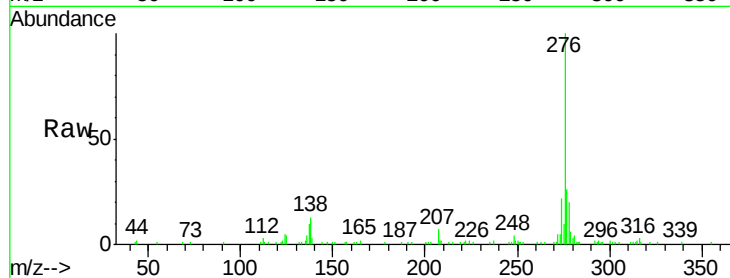

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

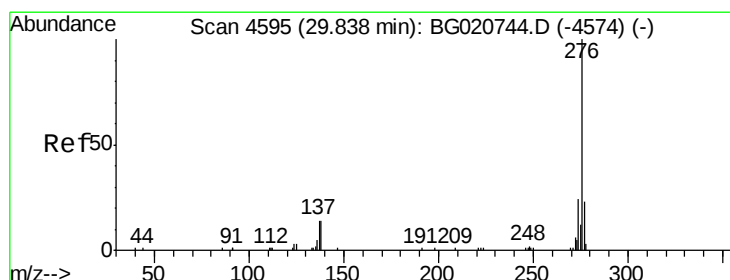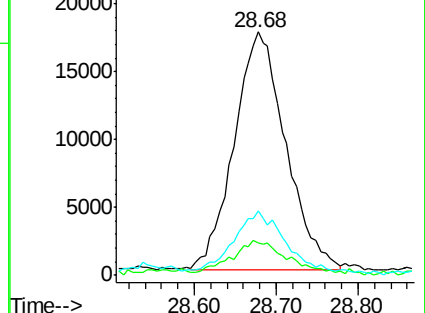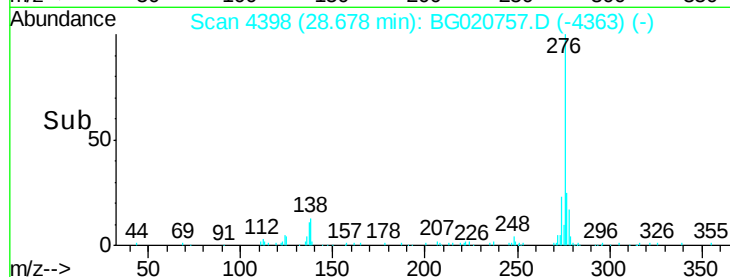

#94

Benzo(g,h,i)perylene

Concen: 5.38 ng/u1

RT: 29.85 min Scan# 4597

Delta R.T. 0.01 min

Lab File: BG020757.D

Acq: 15 Jan 2016 18:00


Tgt Ion:276 Resp: 44125

Ion Ratio Lower Upper

276 100

138 15.1 11.2 16.8

277 23.5 19.0 28.6

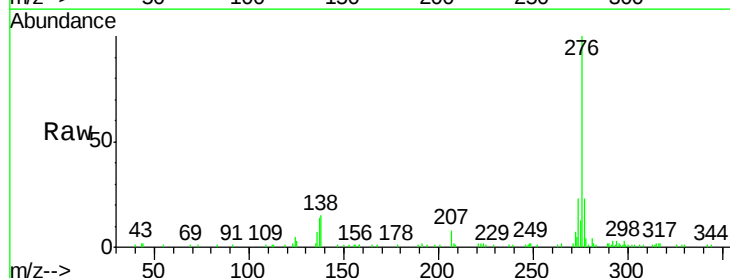

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

