

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG011516\
 Data File : BG020755.D
 Acq On : 15 Jan 2016 16:41
 Operator : SJ/IZ
 Sample : H1101-17 10X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BC9F8

Manual Integrations
 APPROVED

Sohil
 1/16/2016 3:03:22 AM

Quant Time: Jan 16 00:11:17 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG011216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 15 22:12:27 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.04	152	16901	20.00	ng/ul	0.00
18) Naphthalene-d8	10.86	136	72818	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.68	164	49559	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.43	188	123504	20.00	ng/ul	0.00
78) Chrysene-d12	21.70	240	145245	20.00	ng/ul	0.00
86) Perylene-d12	24.95	264	137640	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	7.21	99	1960	1.35	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.37	67	1388m	1.59	ng/ul	0.01
9) 2-Chlorophenol-d4	7.57	132	1962	1.73	ng/ul	0.00
13) 4-Methylphenol-d8	8.76	113	1421m	1.16	ng/ul	0.00
19) Nitrobenzene-d5	9.23	128	813	1.42	ng/ul	0.01
22) 2-Nitrophenol-d4	9.95	143	1139	1.71	ng/ul	0.01
26) 2,4-Dichlorophenol-d3	10.49	165	1906	1.50	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	
44) Dimethylphthalate-d6	14.08	166	8668	2.00	ng/ul	0.00
47) Acenaphthylene-d8	14.38	160	10183	2.10	ng/ul	0.00
52) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
58) Fluorene-d10	15.67	176	8269	2.14	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	0.00	200	0d	0.00	ng/ul	
71) Anthracene-d10	17.53	188	13136	2.17	ng/ul	0.00
79) Pyrene-d10	19.81	212	14963	2.17	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.72	264	16335	2.23	ng/ul	0.00

Target Compounds

					Qvalue
70) Phenanthrene	17.47	178	80597	10.97 ng/ul	99
72) Anthracene	17.56	178	11044	1.49 ng/ul	98
77) Fluoranthene	19.48	202	140697	15.75 ng/ul	99
80) Pyrene	19.84	202	178325	19.36 ng/ul	99
83) Benzo(a)anthracene	21.68	228	88597	9.78 ng/ul	98
85) Chrysene	21.75	228	93183	10.88 ng/ul	96
88) Benzo(b)fluoranthene	23.92	252	79440	8.96 ng/ul	98
89) Benzo(k)fluoranthene	23.98	252	31258m	3.57 ng/ul	
91) Benzo(a)pyrene	24.80	252	71972m	8.44 ng/ul	
92) Indeno(1,2,3-cd)pyrene	28.68	276	39761	3.95 ng/ul	99
94) Benzo(g,h,i)perylene	29.84	276	43249m	5.21 ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG011516\
Data File : BG020755.D
Acq On : 15 Jan 2016 16:41
Operator : SJ/IZ
Sample : H1101-17 10X
Misc :
ALS Vial : 25 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
BC9F8

Manual Integrations
APPROVED

Sohil
1/16/2016 3:03:22 AM

Quant Time: Jan 16 00:11:17 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG011216.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 15 22:12:27 2016
Response via : Initial Calibration

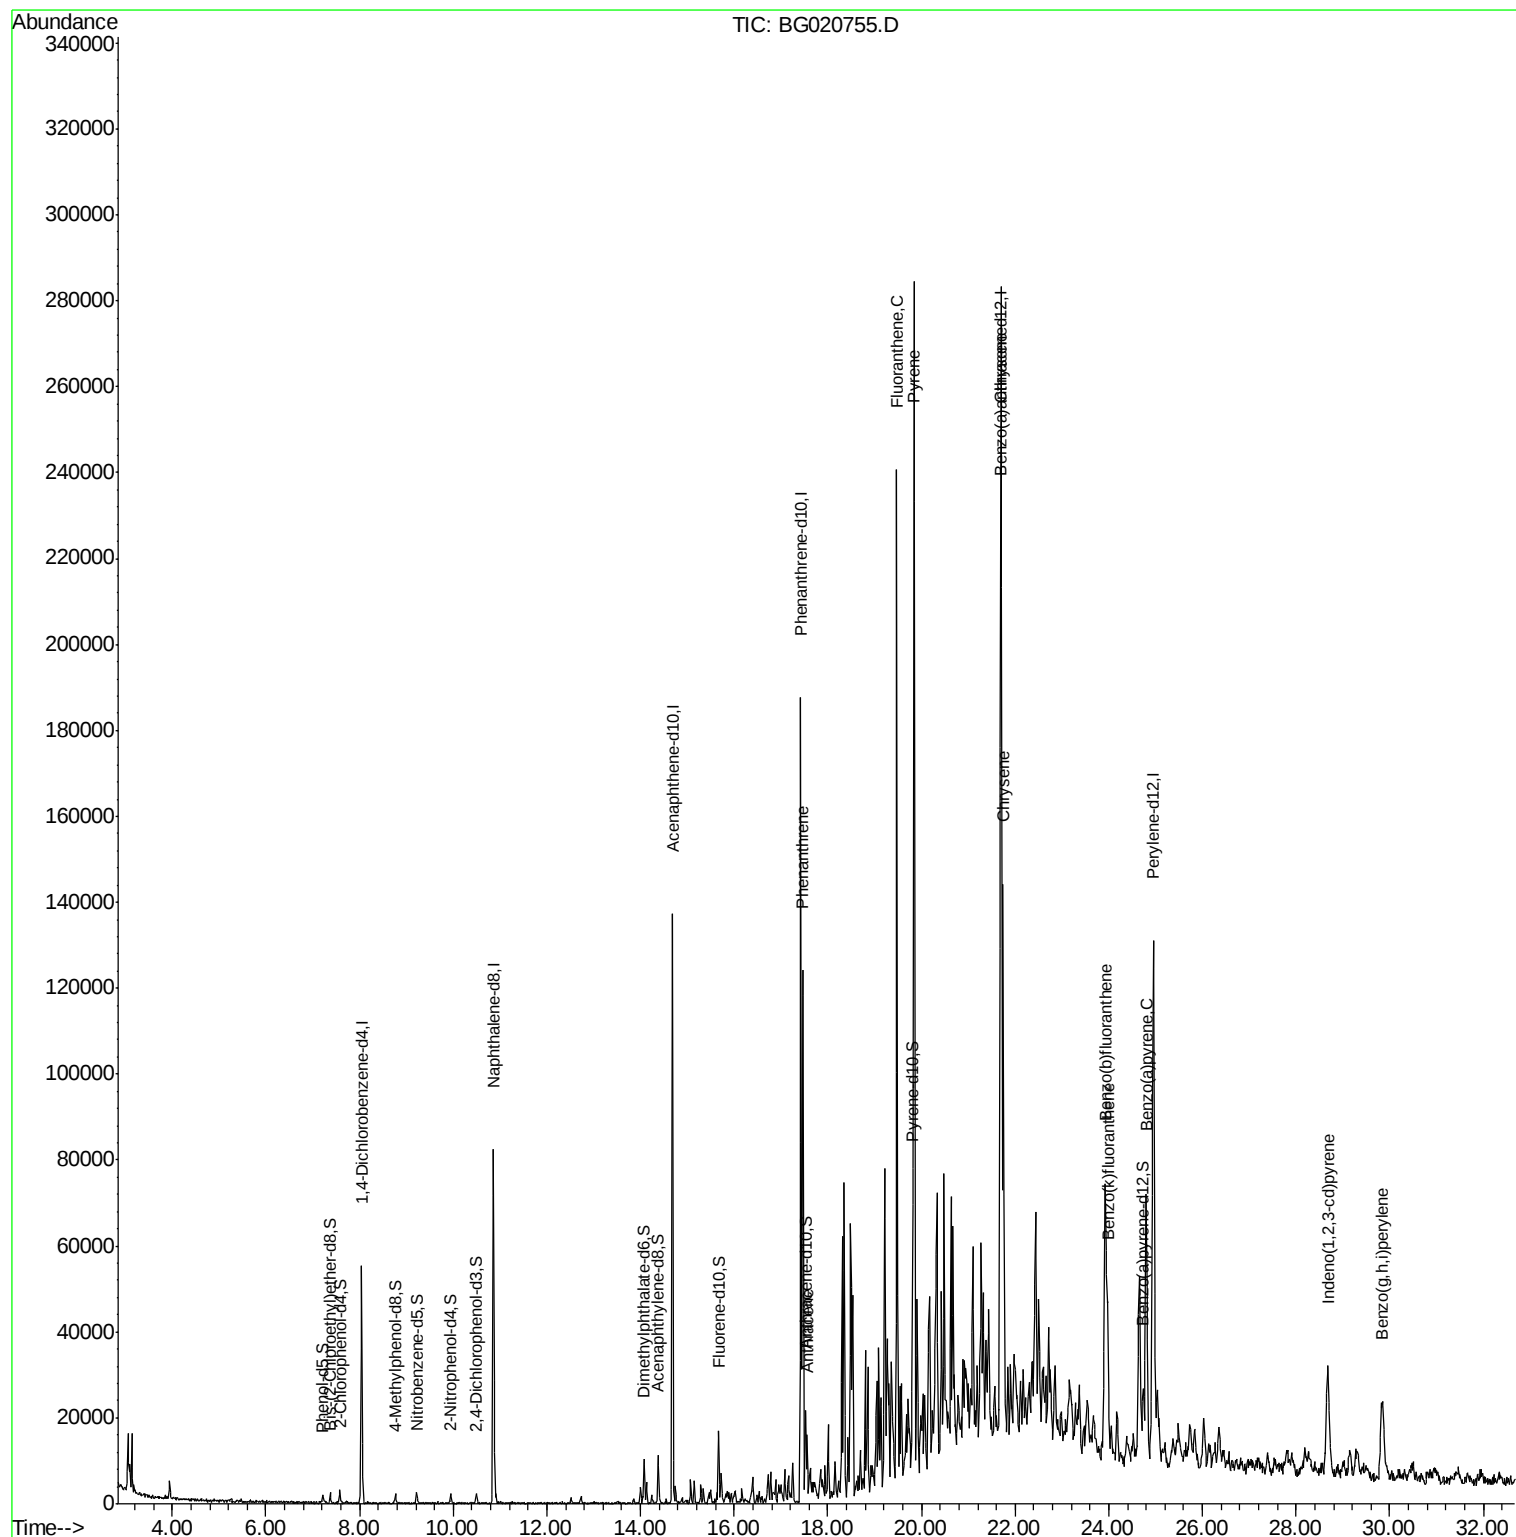

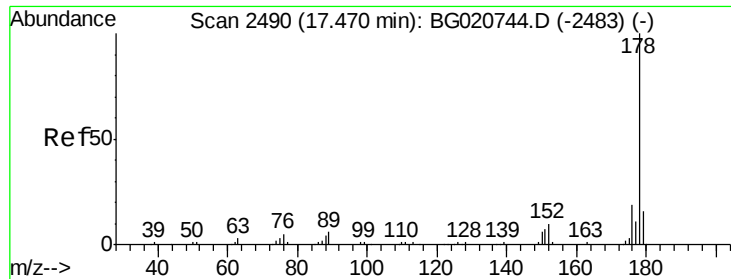

#70

Phenanthrene

Concen: 10.97 ng/ul

RT: 17.47 min Scan# 2490

Delta R.T. -0.00 min

Lab File: BG020755.D

Acq: 15 Jan 2016 16:41

Instrument :

BNA_G





ClientSampleId :

BC9F8

Tgt Ion:	178	Resp:	80597
Ion Ratio	Lower	Upper	
178	100		
179	14.6	12.3	18.5
176	18.8	15.4	23.0

Manual Integrations
APPROVED

Sohil
1/16/2016 3:03:22 AM

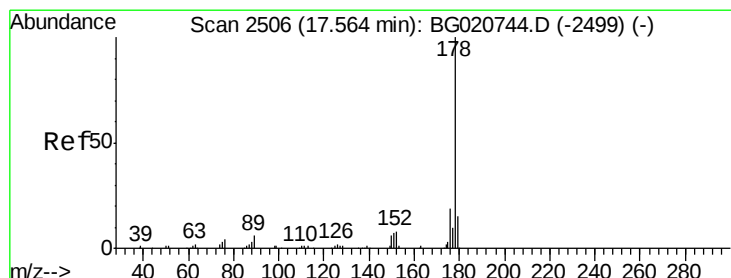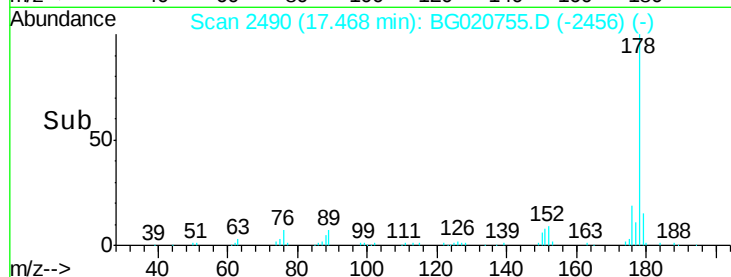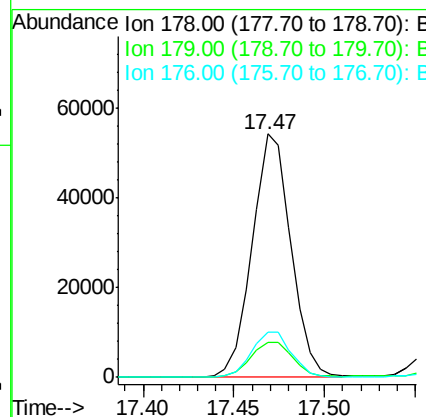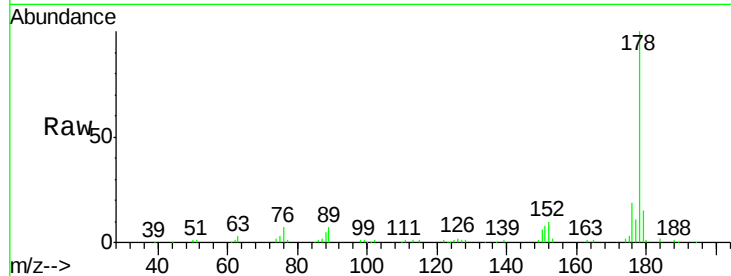

#72

Anthracene

Concen: 1.49 ng/ul




RT: 17.56 min Scan# 2506


Delta R.T. -0.00 min

Lab File: BG020755.D

Acq: 15 Jan 2016 16:41

Tgt Ion:	178	Resp:	11044
Ion Ratio	Lower	Upper	
178	100		
179	15.5	13.4	20.2
176	19.6	15.4	23.0

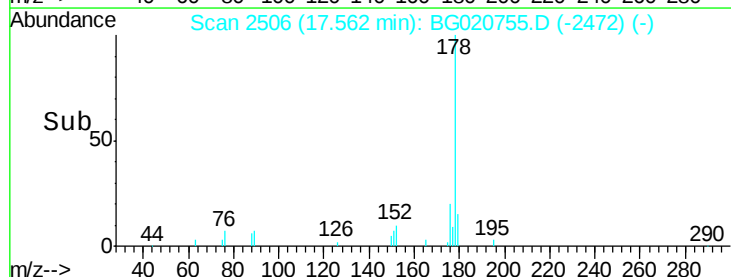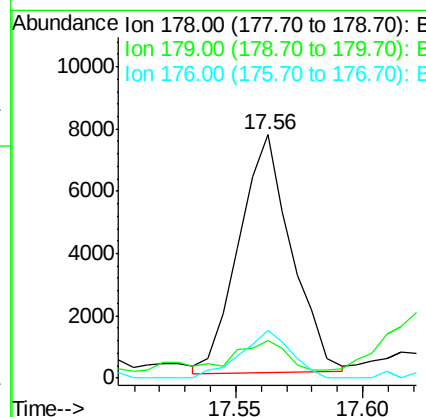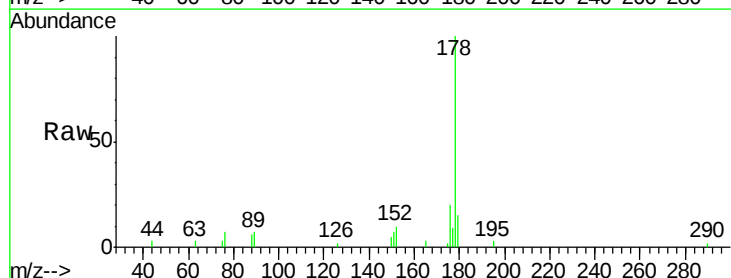

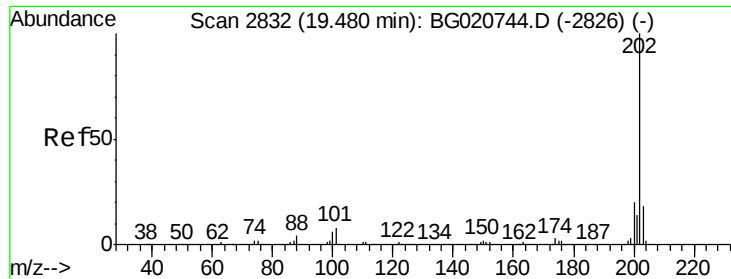





#77
Fluoranthene
 Concen: 15.75 ng/ul
 RT: 19.48 min Scan# 2832
 Delta R.T. -0.00 min
 Lab File: BG020755.D
 Acq: 15 Jan 2016 16:41

Instrument :
 BNA_G
 ClientSampleId :
 BC9F8

Tgt Ion	Ratio	Resp Lower	Resp Upper
202	100		
101	7.5	6.1	9.1
100	5.2	4.6	7.0




Manual Integrations
 APPROVED


Sohil
 1/16/2016 3:03:22 AM

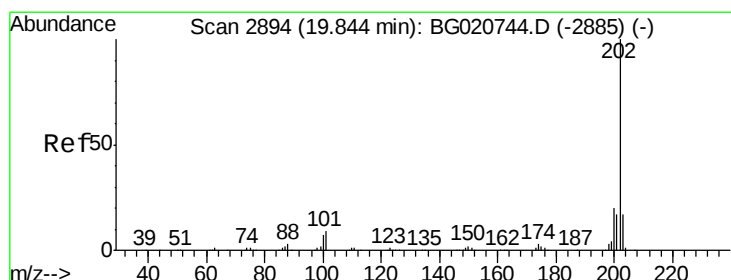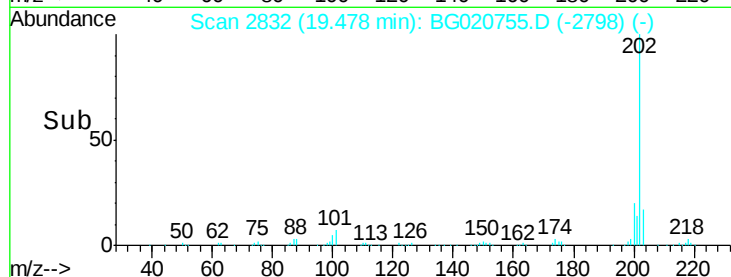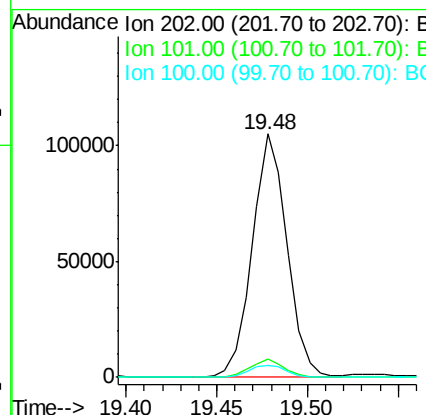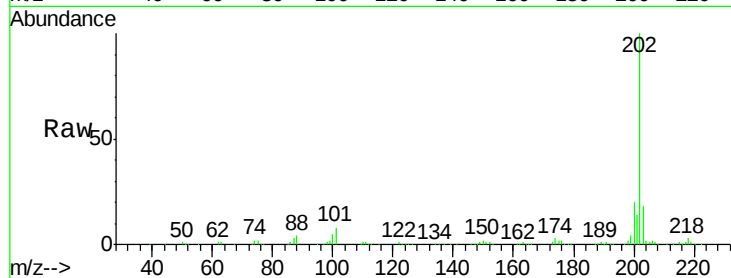

#80
Pyrene
 Concen: 19.36 ng/ul
 RT: 19.84 min Scan# 2894
 Delta R.T. -0.00 min
 Lab File: BG020755.D
 Acq: 15 Jan 2016 16:41

Tgt Ion	Ratio	Resp Lower	Resp Upper
202	100		
101	9.0	6.9	10.3
100	7.0	5.6	8.4

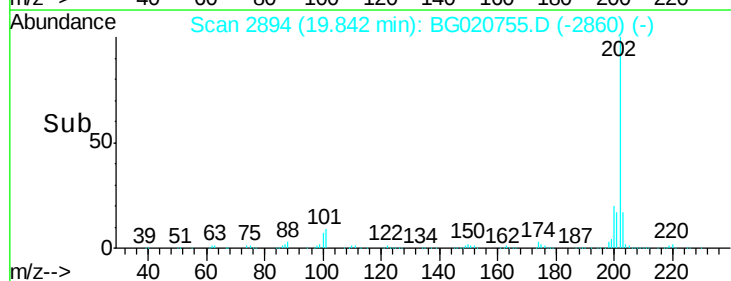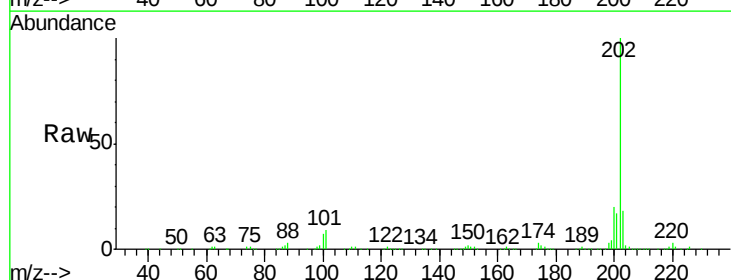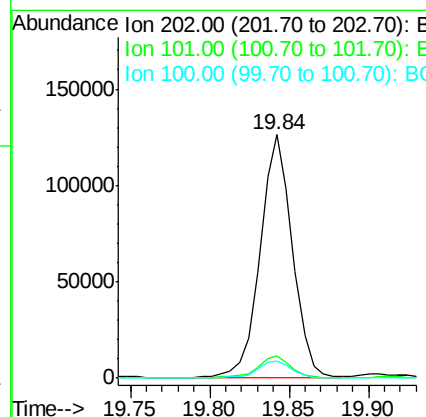

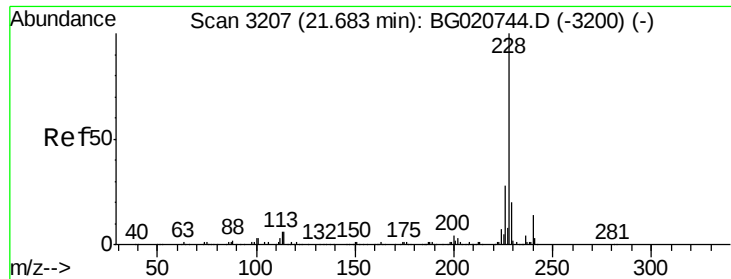

#83

Benzo(a)anthracene

Concen: 9.78 ng/ul

RT: 21.68 min Scan# 3207

Delta R.T. -0.00 min

Lab File: BG020755.D


Acq: 15 Jan 2016 16:41

Instrument :

BNA_G

ClientSampleId :



BC9F8

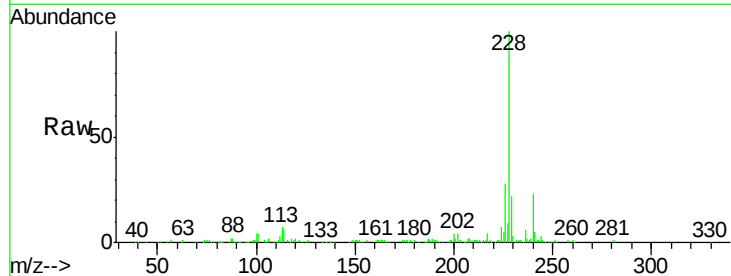

Tgt Ion	Ratio	Lower	Upper
228	100		
229	21.6	16.0	24.0
226	27.9	21.8	32.8

Manual Integrations
APPROVED

Sohil
1/16/2016 3:03:22 AM

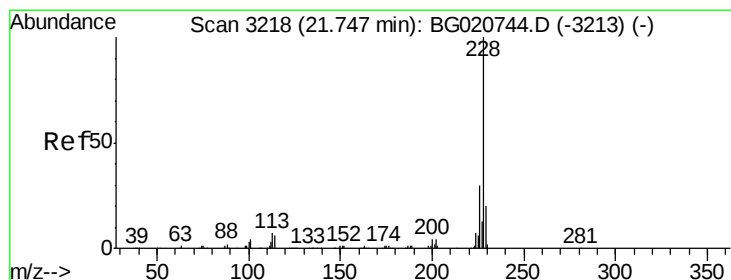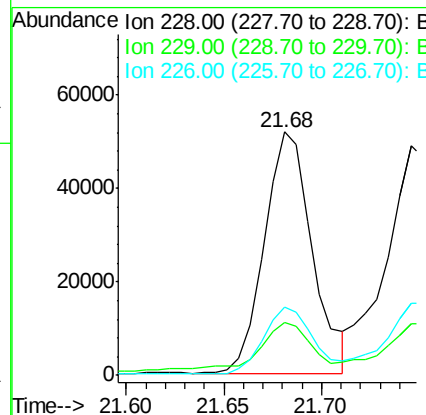

#85

Chrysene


Concen: 10.88 ng/ul

RT: 21.75 min Scan# 3218



Delta R.T. -0.00 min


Lab File: BG020755.D

Acq: 15 Jan 2016 16:41

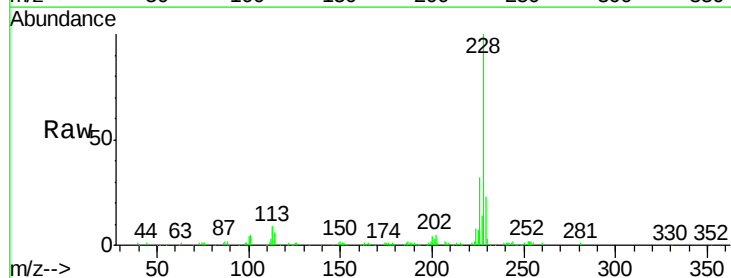

Tgt Ion	Ratio	Lower	Upper
228	100		
226	31.5	24.1	36.1
229	22.7	16.0	24.0

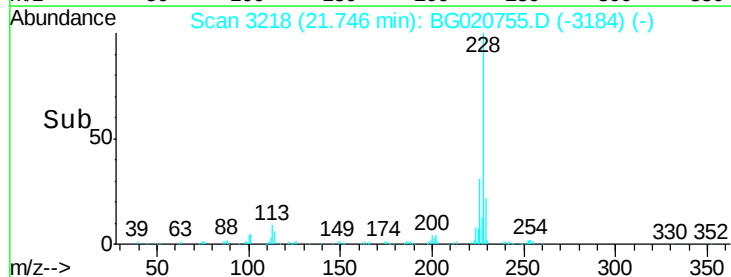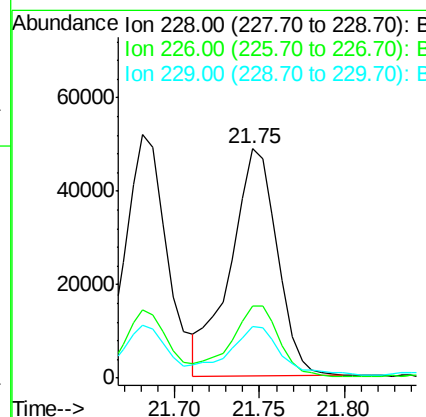

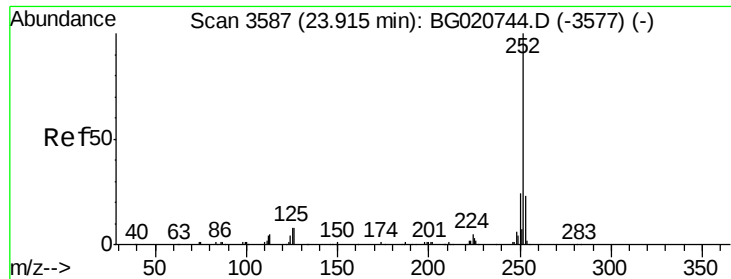





#88
Benzo(b)fluoranthene
Concen: 8.96 ng/ul
RT: 23.92 min Scan# 3588
Delta R.T. 0.00 min
Lab File: BG020755.D
Acq: 15 Jan 2016 16:41

Instrument :
BNA_G
ClientSampleId :
BC9F8

Tgt Ion	Ratio	Lower	Upper
252	100		
253	20.9	17.4	26.0
125	6.9	4.9	7.3




Manual Integrations
APPROVED


Sohil
1/16/2016 3:03:22 AM

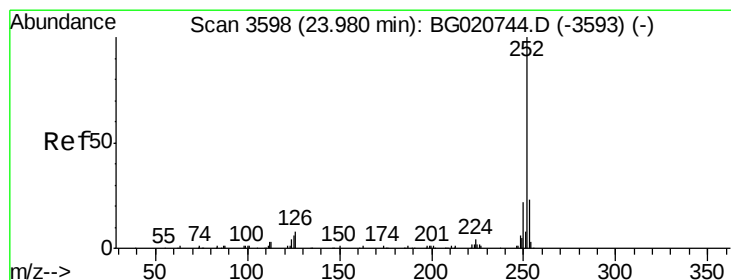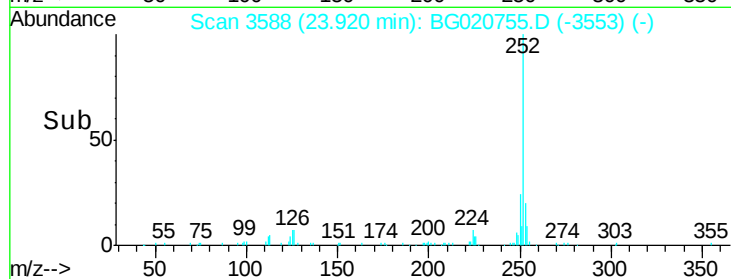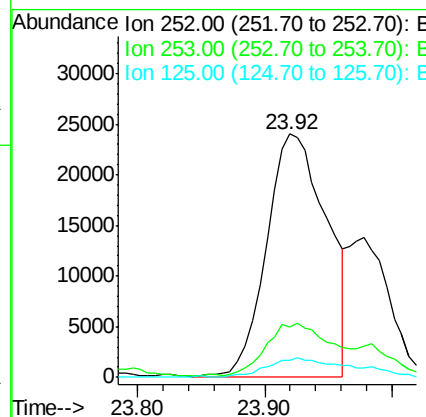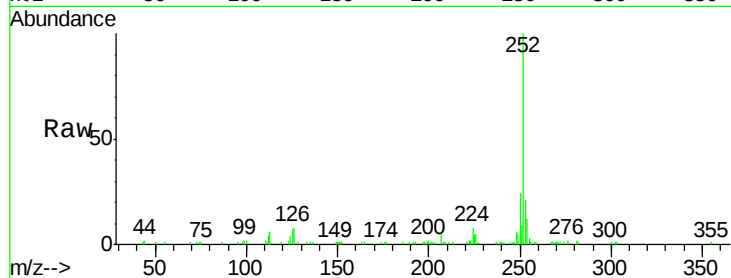

#89
Benzo(k)fluoranthene
Concen: 3.57 ng/ul m
RT: 23.98 min Scan# 3598
Delta R.T. -0.00 min
Lab File: BG020755.D
Acq: 15 Jan 2016 16:41

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.1	17.1	25.7
125	6.4	5.4	8.0

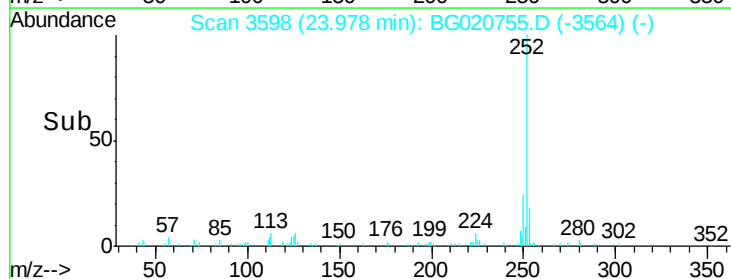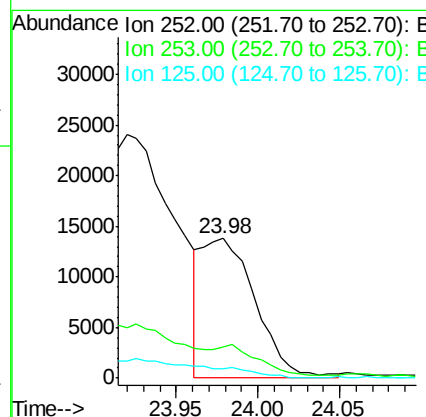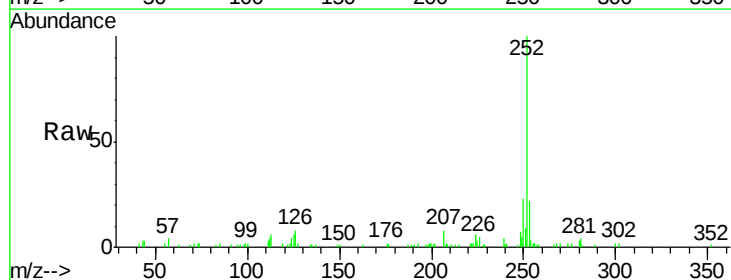

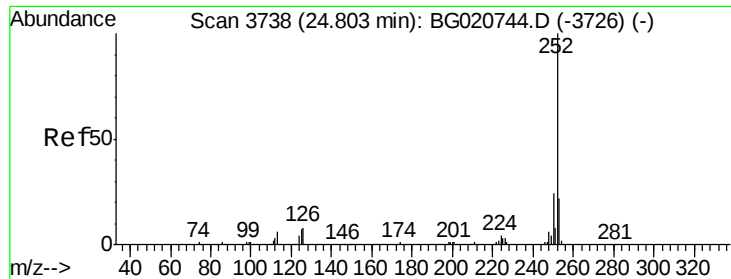

#91

Benzo(a)pyrene

Concen: 8.44 ng/ul m

RT: 24.80 min Scan# 3738

Delta R.T. -0.00 min

Lab File: BG020755.D

Acq: 15 Jan 2016 16:41

Instrument :

BNA_G





ClientSampleId :

BC9F8

Tgt Ion:	252	Resp:	71972
Ion Ratio	Lower	Upper	
252	100		
253	24.3	17.2	25.8
125	8.9	5.8	8.6#

Manual Integrations
APPROVED

Sohil
1/16/2016 3:03:22 AM

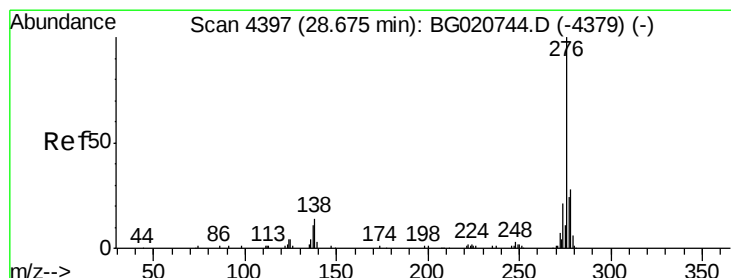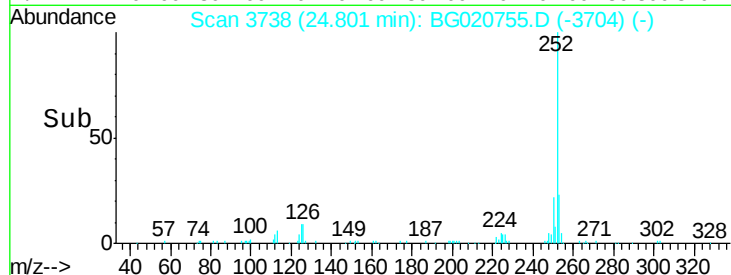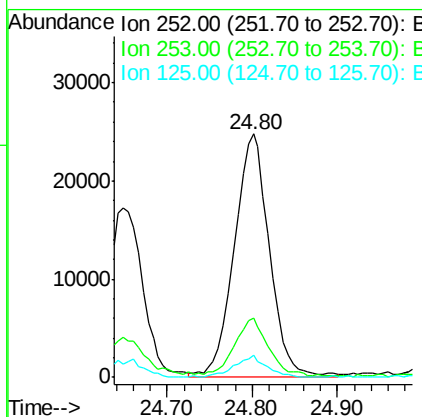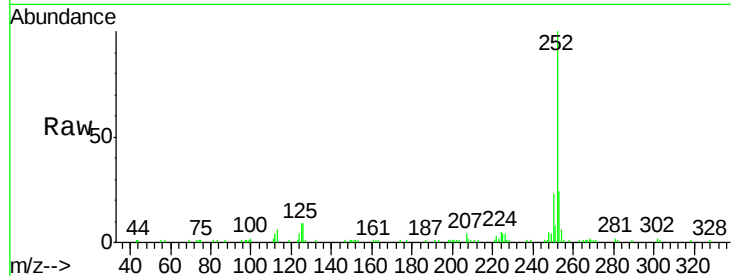

#92

Indeno(1,2,3-cd)pyrene

Concen: 3.95 ng/ul




RT: 28.68 min Scan# 4398


Delta R.T. 0.00 min

Lab File: BG020755.D

Acq: 15 Jan 2016 16:41

Tgt Ion:	276	Resp:	39761
Ion Ratio	Lower	Upper	
276	100		
138	13.8	10.9	16.3
277	24.2	18.9	28.3

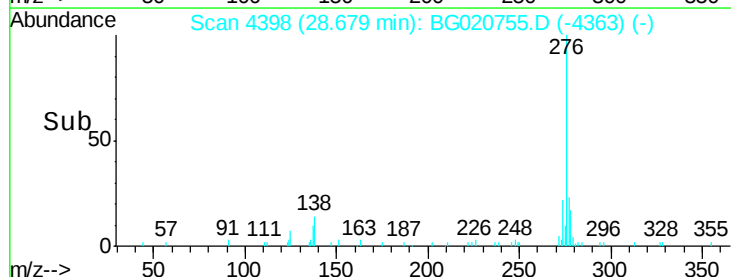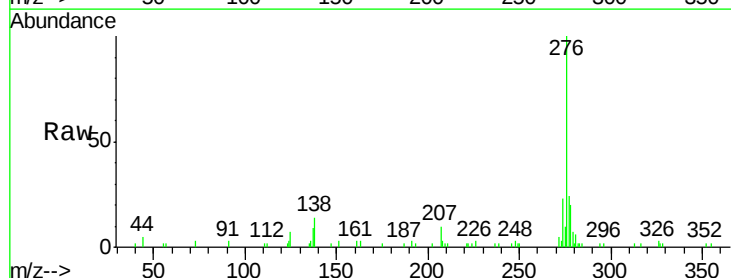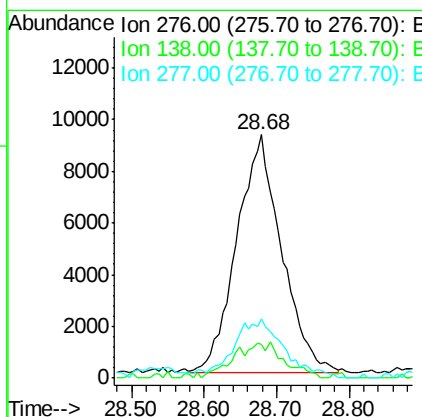

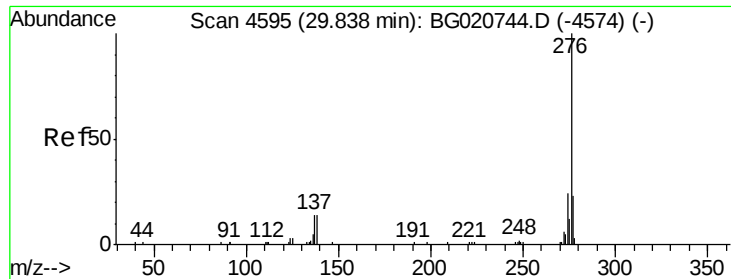

#94

Benzo(g,h,i)perylene

Concen: 5.21 ng/ul m

RT: 29.84 min Scan# 4595

Delta R.T. -0.00 min

Lab File: BG020755.D


Acq: 15 Jan 2016 16:41

Instrument :

BNA_G

ClientSampleId :

BC9F8

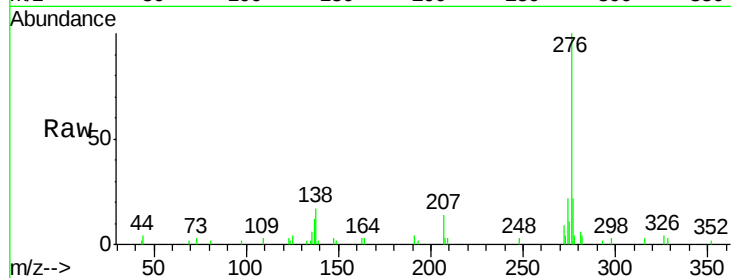

Tgt Ion:	276	Resp:	43249
Ion Ratio	Lower	Upper	
276	100		
138	17.0	11.2	16.8#
277	21.5	19.0	28.6

Manual Integrations
APPROVED

Sohil
1/16/2016 3:03:22 AM

