
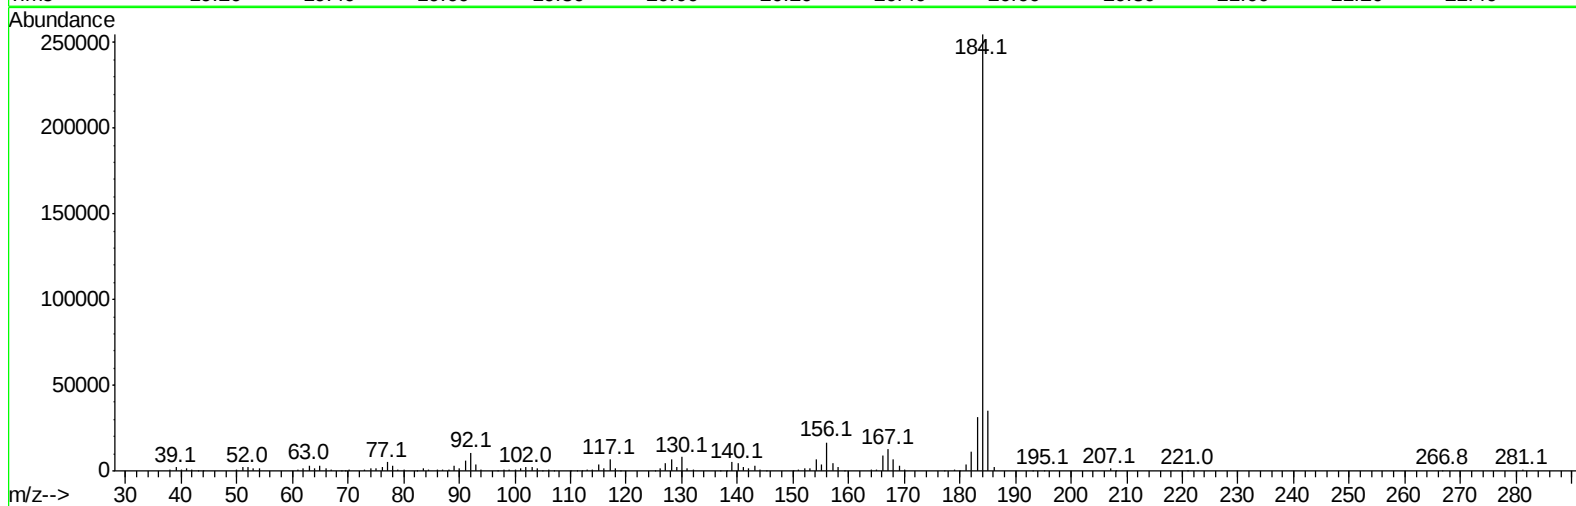


Data Path : U:\HPCHEM1\BNA G\DATA\BG011518\
Data File : BG032033.D
Acq On : 15 Jan 2018 14:10
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 16 06:51:41 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 15 10:05:15 2018
Response via : Initial Calibration

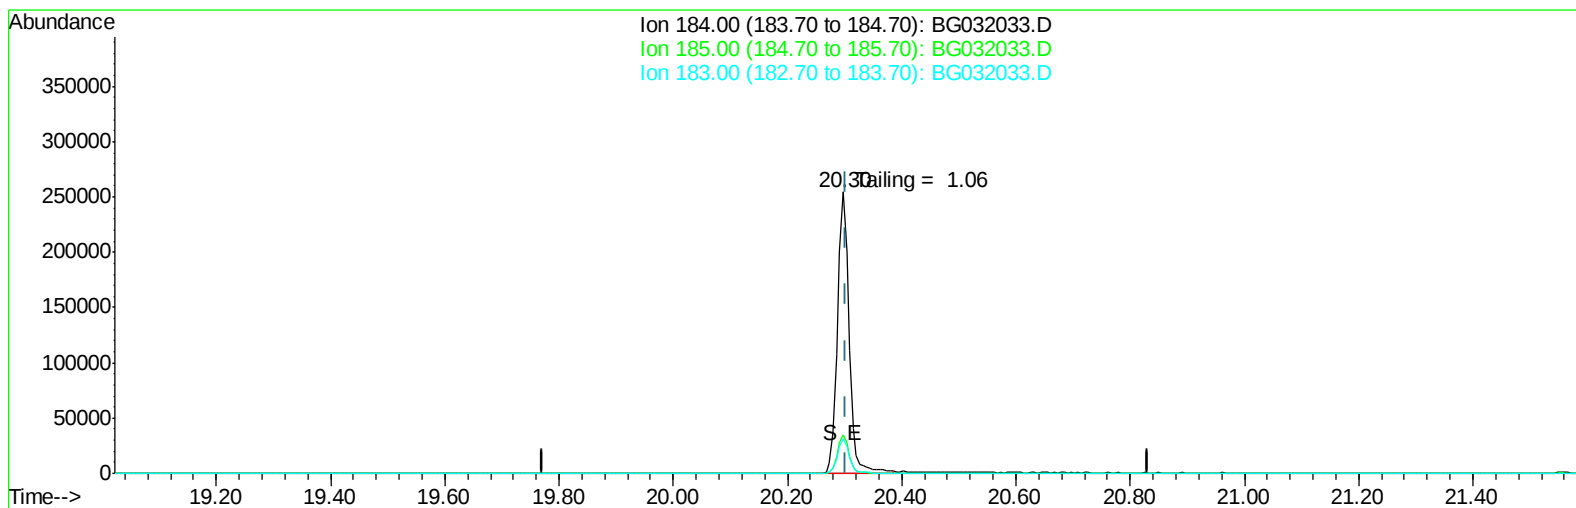

TIC: BG032033.D

(76) Benzidine



20.297min (-0.005) 0.00ng

response 362640

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	13.83
183.00	13.30	12.42
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA G\DATA\BG011518\
Data File : BG032033.D
Acq On : 15 Jan 2018 14:10
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 16 06:51:41 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 15 10:05:15 2018
Response via : Initial Calibration

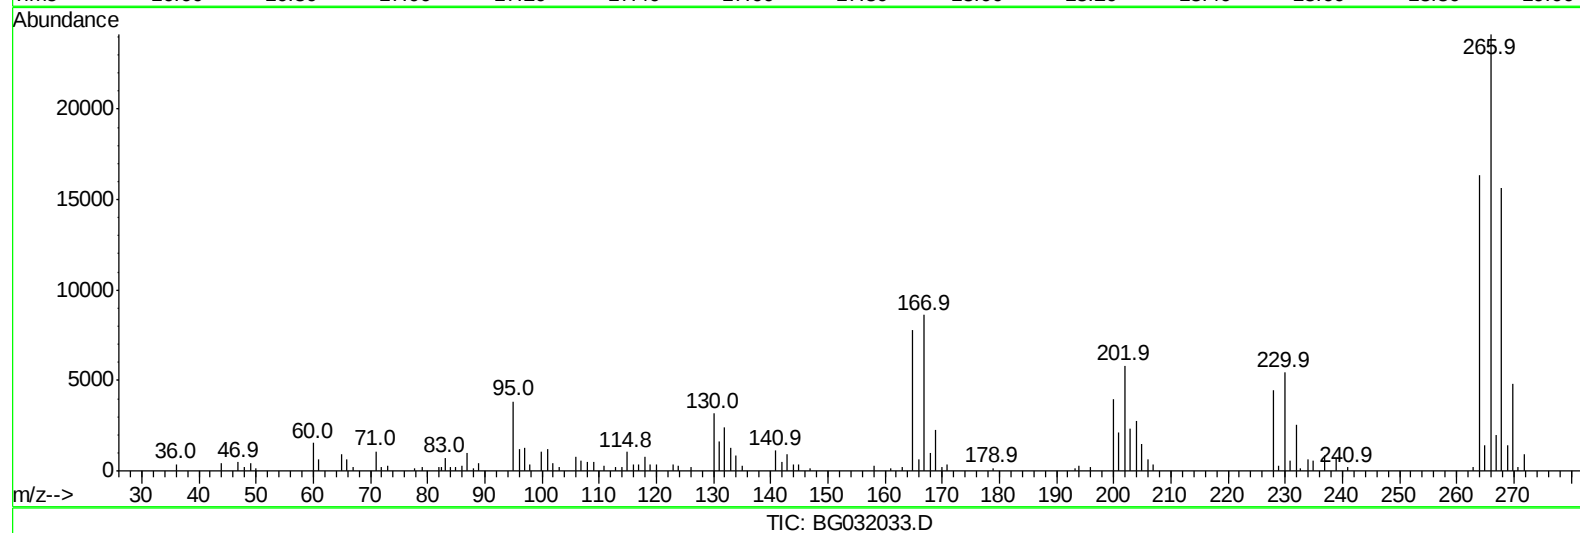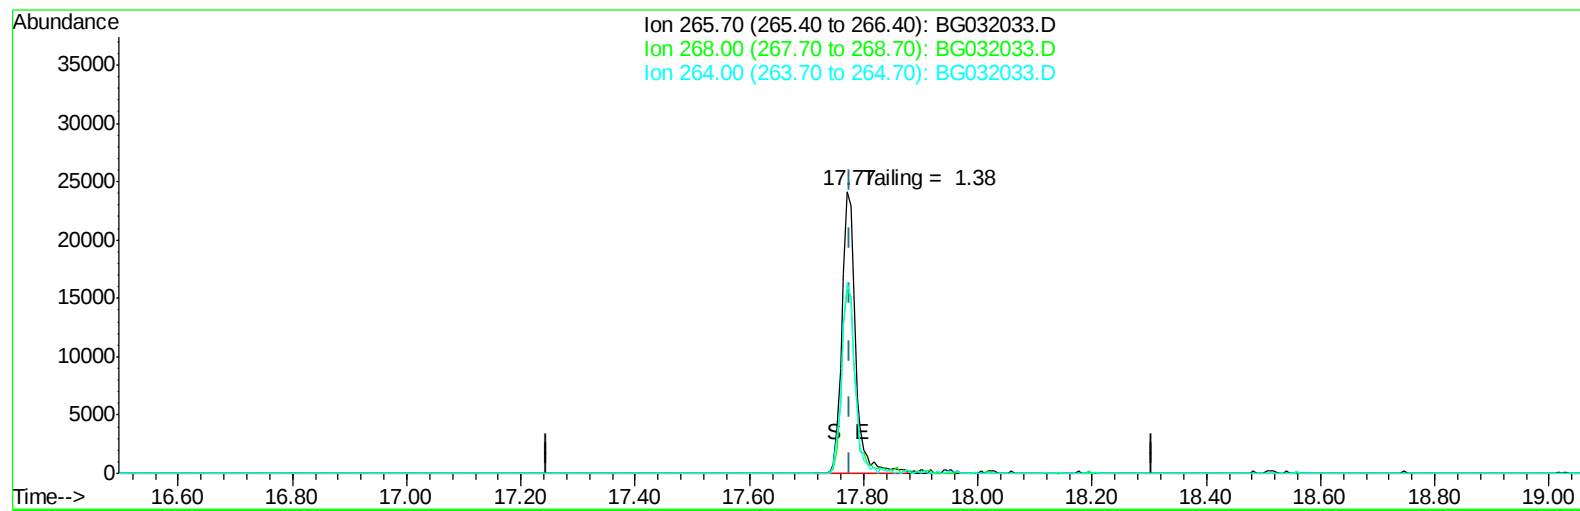

TIC: BG032033.D

(69) Pentachlorophenol (C)

17.771min (-0.005) 10807.74ng

response 40235

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.96
264.00	62.00	67.63
0.00	0.00	0.00