
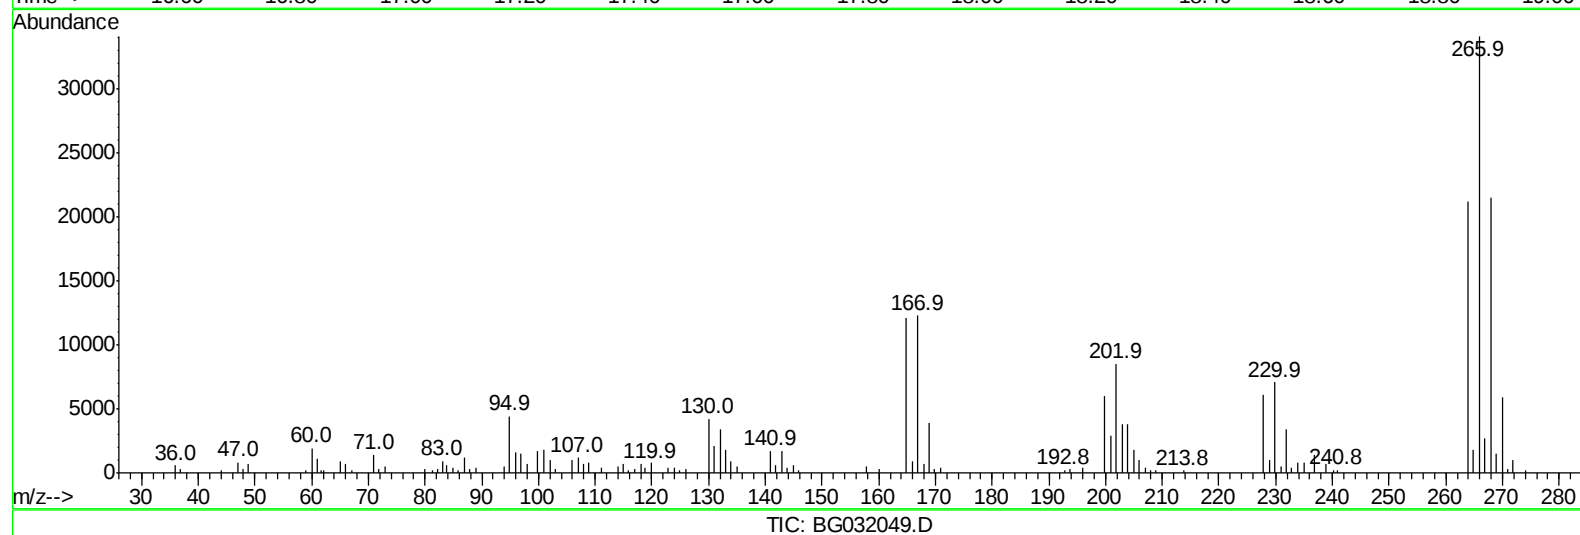


Data Path : U:\HPCHEM1\BNA G\DATA\BG011518\
Data File : BG032049.D
Acq On : 16 Jan 2018 2:21
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 16 06:52:56 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 15 10:05:15 2018
Response via : Initial Calibration

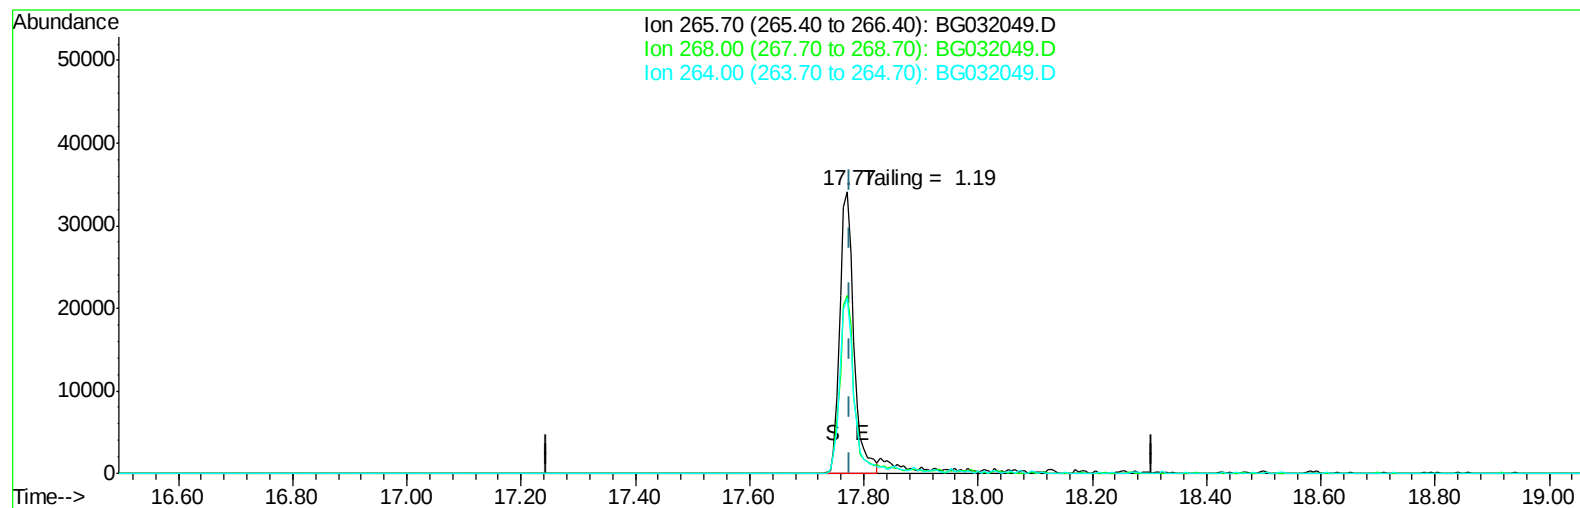

(69) Pentachlorophenol (C)



17.770min (-0.006) 18037.94ng

response 58077

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.12
264.00	62.00	62.23
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA G\DATA\BG011518\
Data File : BG032049.D
Acq On : 16 Jan 2018 2:21
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 16 06:52:56 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 15 10:05:15 2018
Response via : Initial Calibration

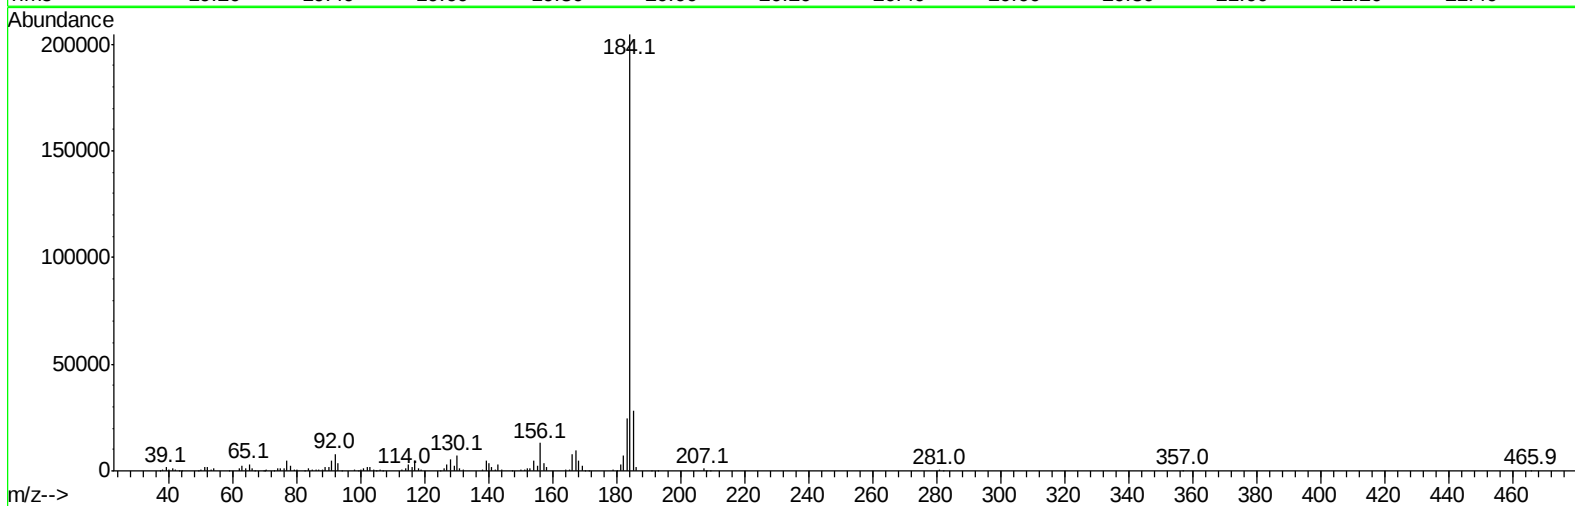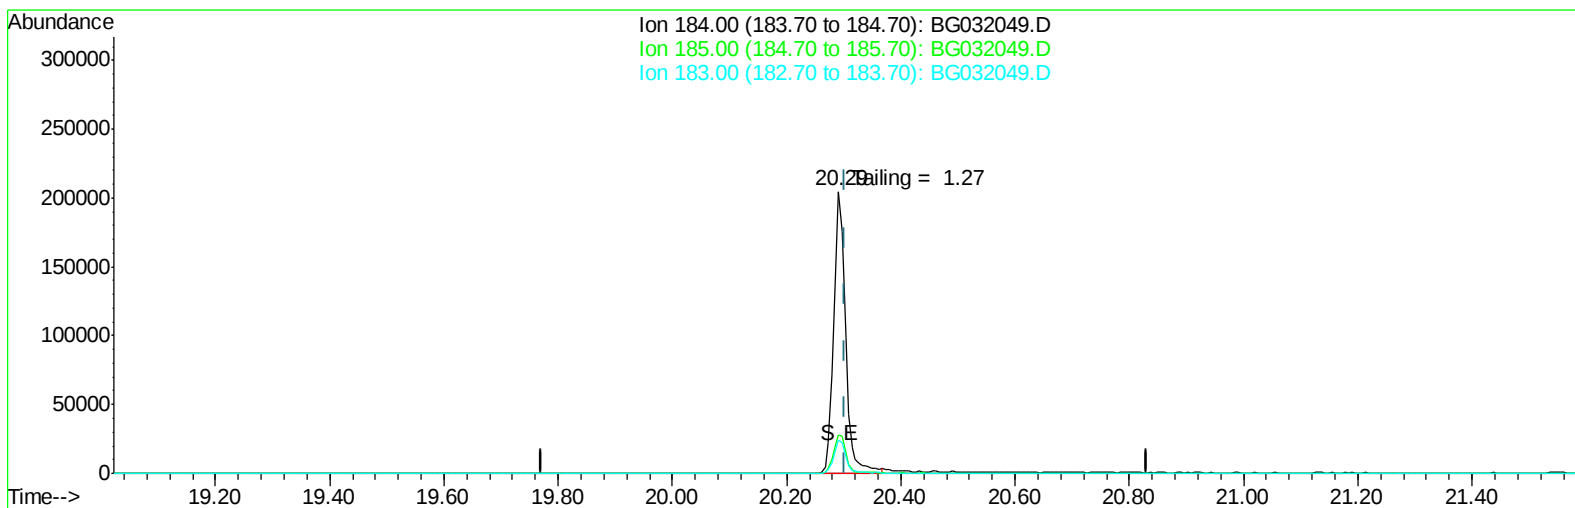

TIC: BG032049.D

(76) Benzidine

20.291min (-0.012) 192880.14ng

response 294215

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	13.83
183.00	13.30	11.91
0.00	0.00	0.00