

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_G\DATA\BG011518\
 Data File : BG032060.D
 Acq On : 16 Jan 2018 9:13
 Operator : SJ/JU
 Sample : J1112-08
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 ENV-106-1(MW)-DUP

Quant Time: Jan 16 09:56:36 2018
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG011218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 15 10:05:15 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.77	152	42904	20.00	ng	0.00
21) Naphthalene-d8	11.65	136	166815	20.00	ng	-0.01
38) Acenaphthene-d10	15.40	164	121663	20.00	ng	0.00
63) Phenanthrene-d10	18.13	188	330721	20.00	ng	-0.01
75) Chrysene-d12	22.46	240	400395	20.00	ng	-0.02
86) Perylene-d12	26.18	264	407252	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	6.19	112	117216	49.97	ng	0.00
7) Phenol-d6	7.87	99	90713	30.70	ng	0.00
23) Nitrobenzene-d5	9.96	82	309897	125.68	ng	-0.01
41) 2,4,6-Tribromophenol	16.87	330	261930	130.10	ng	0.00
44) 2-Fluorobiphenyl	14.03	172	1123402	114.49	ng	0.00
78) Terphenyl-d14	20.67	244	2017515	111.26	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_G\DATA\BG011518\
Data File : BG032060.D
Acq On : 16 Jan 2018 9:13
Operator : SJ/JU
Sample : J1112-08
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
ENV-106-1(MW)-DUP

Quant Time: Jan 16 09:56:36 2018
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 15 10:05:15 2018
Response via : Initial Calibration

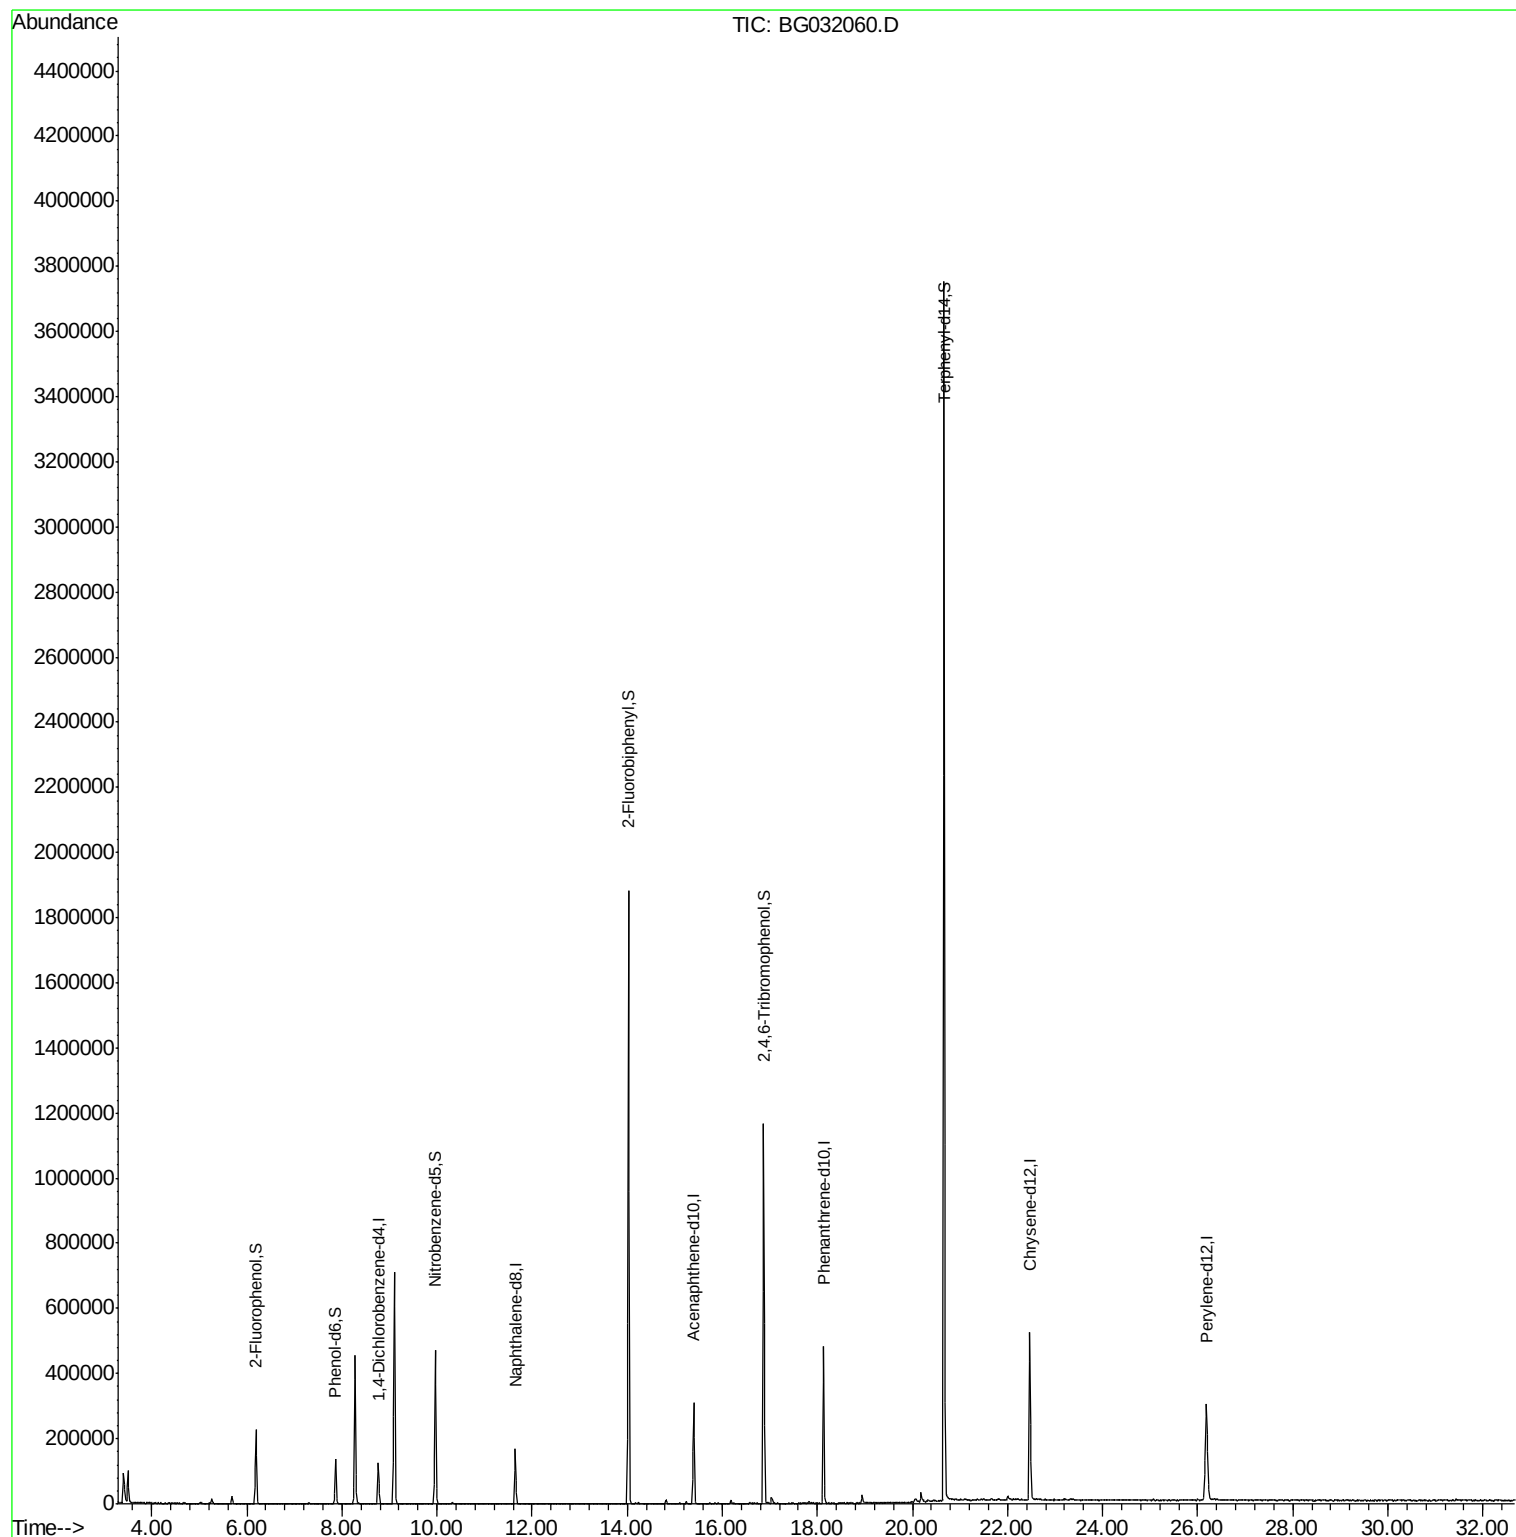

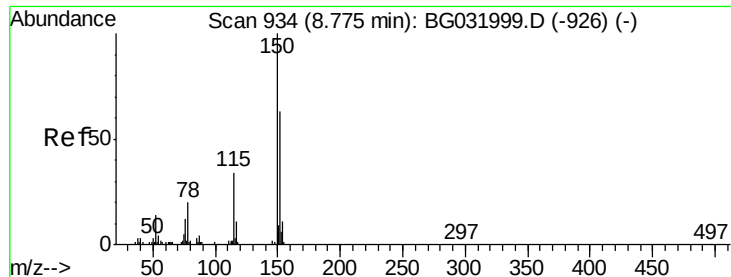


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.77 min Scan# 933
Delta R.T. -0.01 min
Lab File: BG032060.D
Acq: 16 Jan 2018 9:13

Instrument :
BNA_G
ClientSampleId :
ENV-106-1(MW)-DUP

Tgt Ion:152 Resp: 42904
Ion Ratio Lower Upper
152 100
150 157.1 126.6 189.8
115 53.2 53.0 79.4

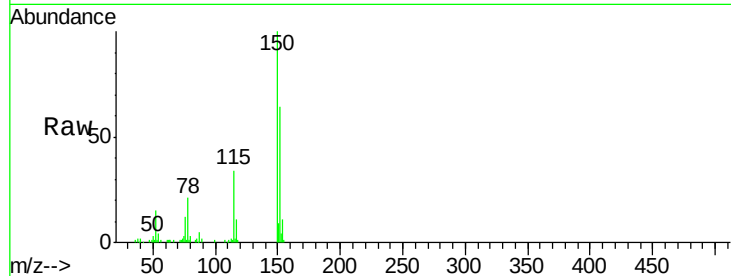


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

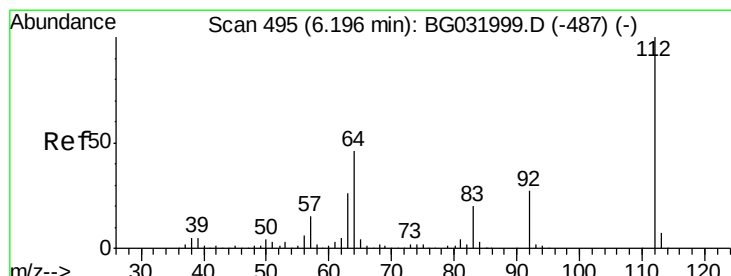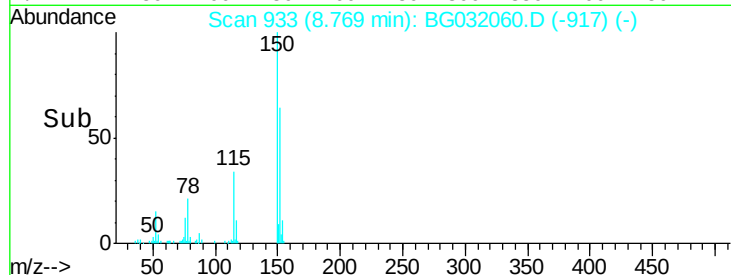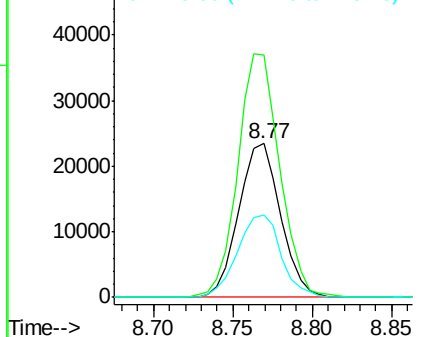



#5


2-Fluorophenol
Concen: 49.967 ng
RT: 6.19 min Scan# 494
Delta R.T. -0.01 min
Lab File: BG032060.D
Acq: 16 Jan 2018 9:13

Tgt Ion:112 Resp: 117216
Ion Ratio Lower Upper
112 100
64 52.8 56.3 84.5#
63 28.3 30.1 45.1#

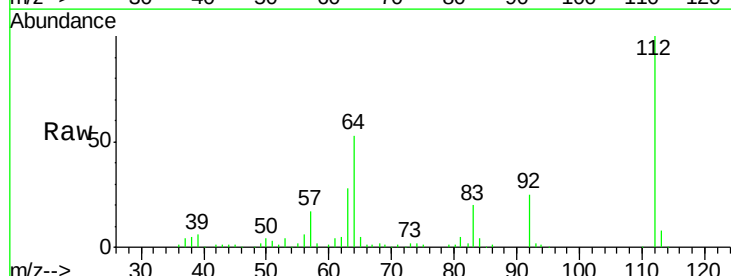

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

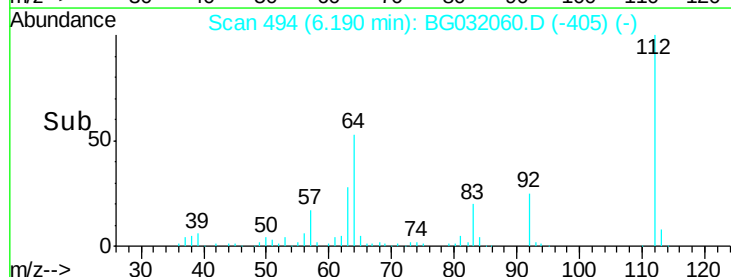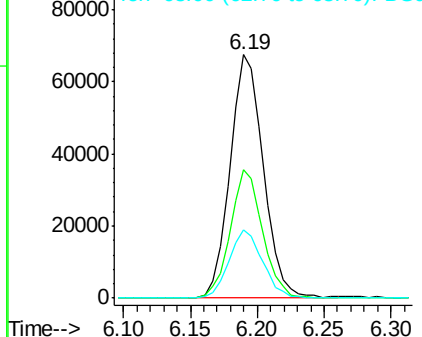

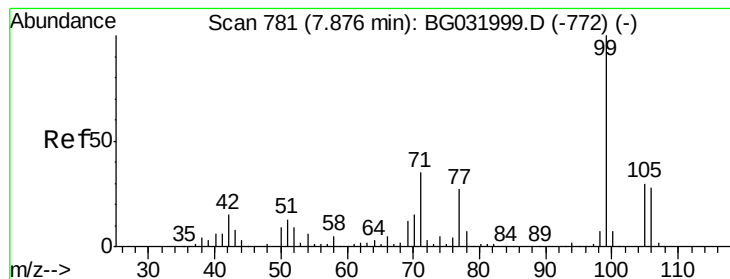

#7

Phenol-d6

Concen: 30.704 ng

RT: 7.87 min Scan# 780

Delta R.T. -0.01 min

Lab File: BG032060.D

Acq: 16 Jan 2018 9:13

Instrument :

BNA_G

ClientSampleId :

ENV-106-1(MW)-DUP


Tgt Ion: 99 Resp: 90713

Ion Ratio Lower Upper




99 100

42 16.8 14.1 21.1

71 38.2 26.1 39.1

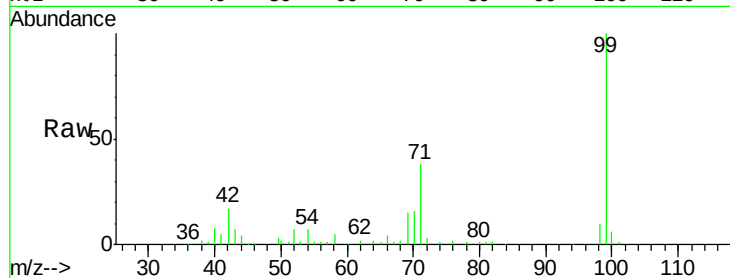

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

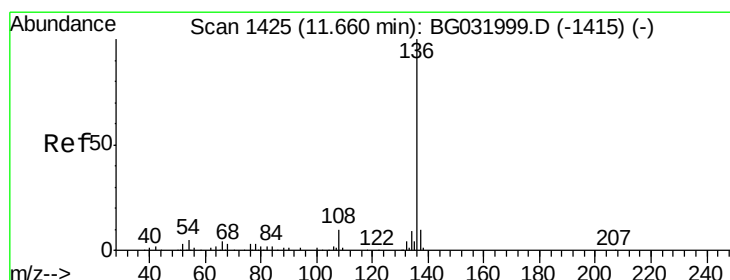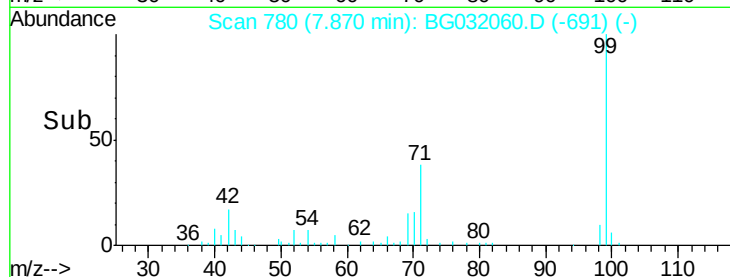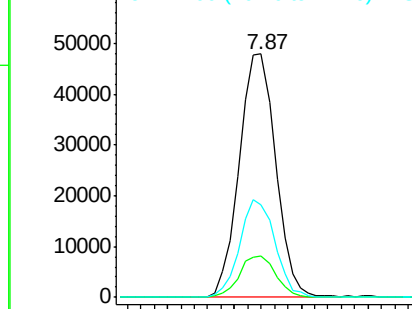

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.65 min Scan# 1423

Delta R.T. -0.01 min

Lab File: BG032060.D

Acq: 16 Jan 2018 9:13

Tgt Ion: 136 Resp: 166815


Ion Ratio Lower Upper

136 100



137 11.0 9.2 13.8


54 5.8 10.3 15.5#

68 3.8 4.5 6.7#

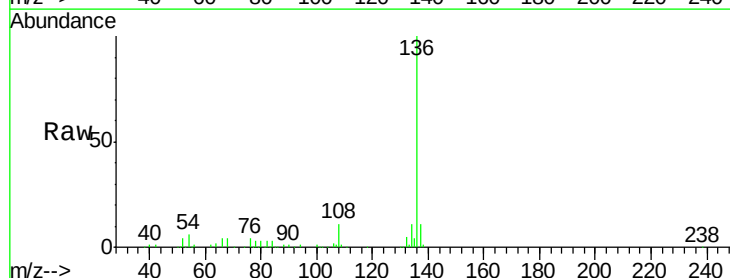

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



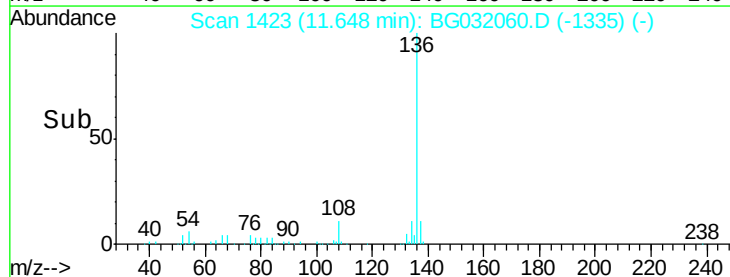
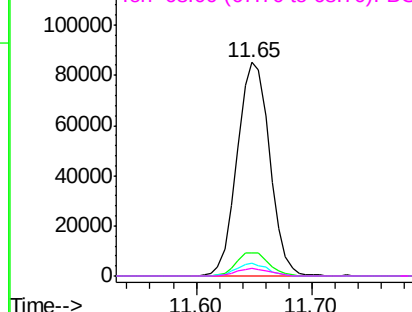


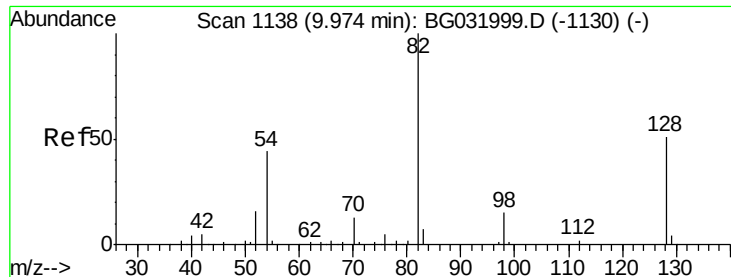

#23
Nitrobenzene-d5
Concen: 125.683 ng
RT: 9.96 min Scan# 1136
Delta R.T. -0.01 min
Lab File: BG032060.D
Acq: 16 Jan 2018 9:13




Instrument :
BNA_G
ClientSampleId :
ENV-106-1(MW)-DUP


Tgt Ion: 82 Resp: 309897
Ion Ratio Lower Upper
82 100
128 46.7 29.7 44.5#
54 47.0 43.1 64.7

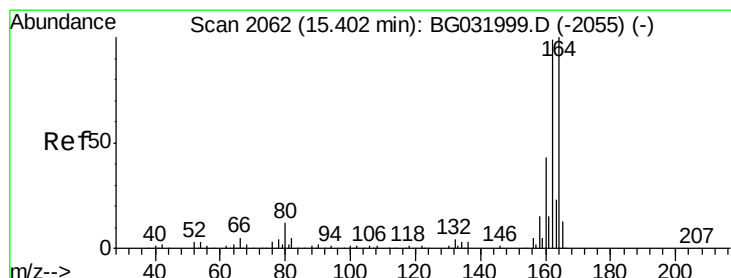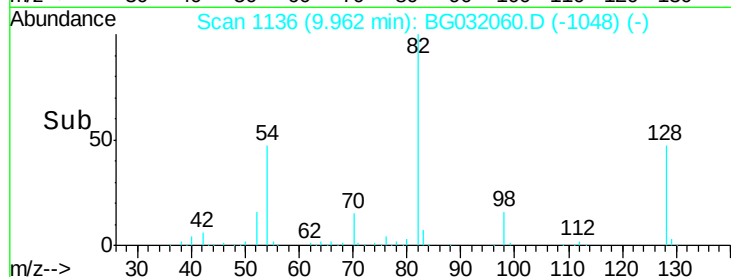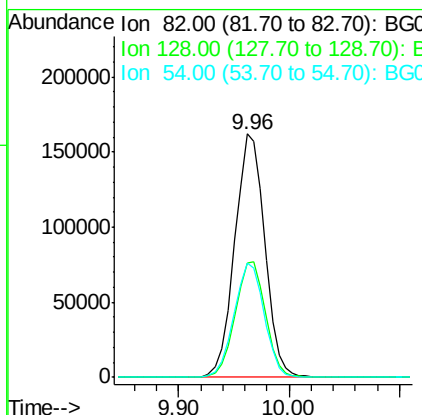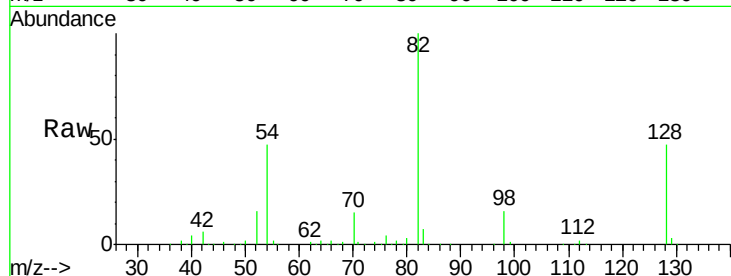

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 15.40 min Scan# 2061
Delta R.T. -0.01 min
Lab File: BG032060.D
Acq: 16 Jan 2018 9:13

Tgt Ion: 164 Resp: 121663
Ion Ratio Lower Upper
164 100
162 102.7 78.8 118.2
160 42.4 35.4 53.0


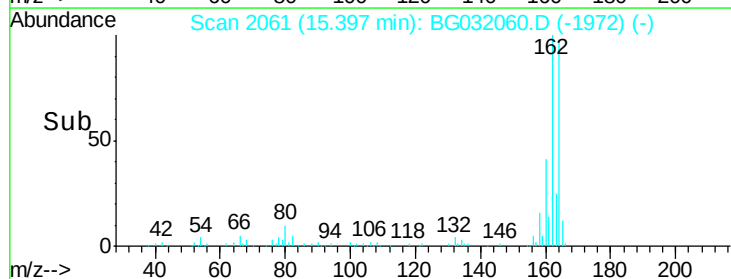
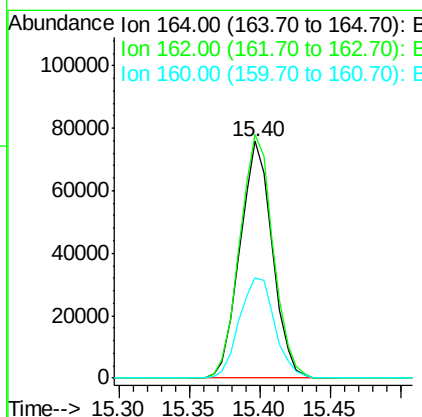
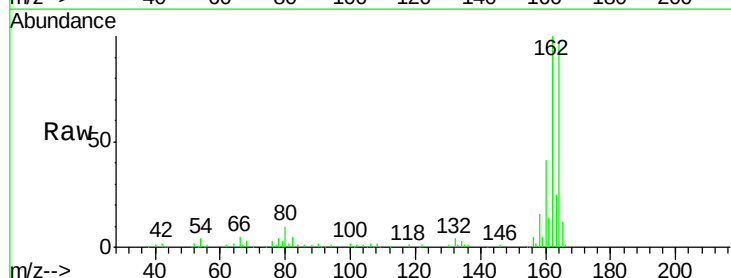


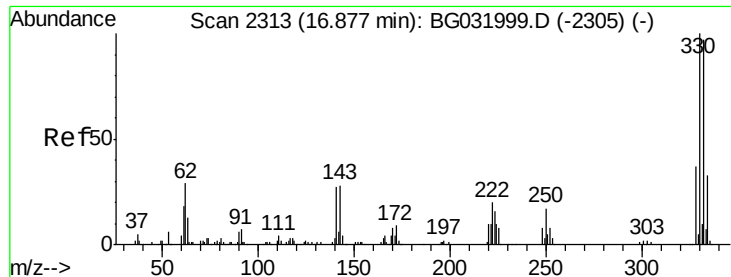

#41
 2,4,6-Tribromophenol
 Concen: 130.104 ng
 RT: 16.87 min Scan# 2312
 Delta R.T. -0.01 min
 Lab File: BG032060.D
 Acq: 16 Jan 2018 9:13




Instrument :
 BNA_G
 ClientSampleId :
 ENV-106-1(MW)-DUP


Tgt Ion:330 Resp: 261930
 Ion Ratio Lower Upper
 330 100
 332 96.4 77.0 115.6
 141 28.6 25.2 37.8

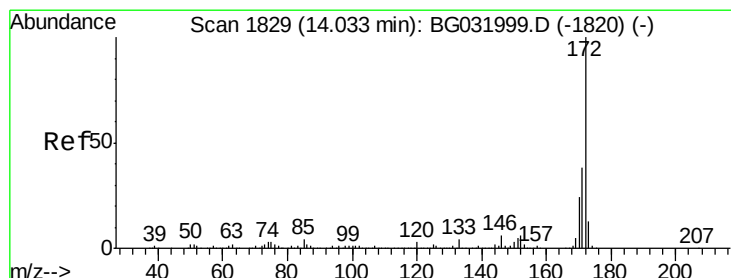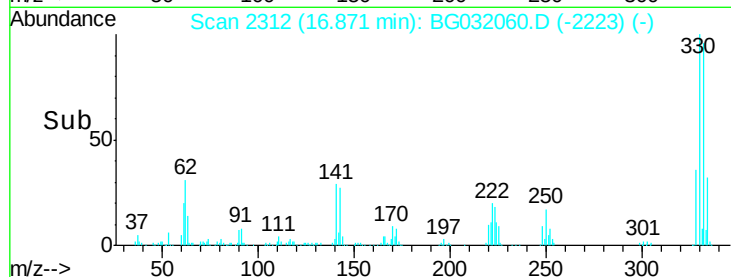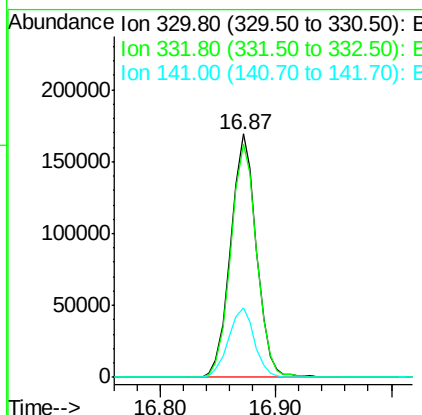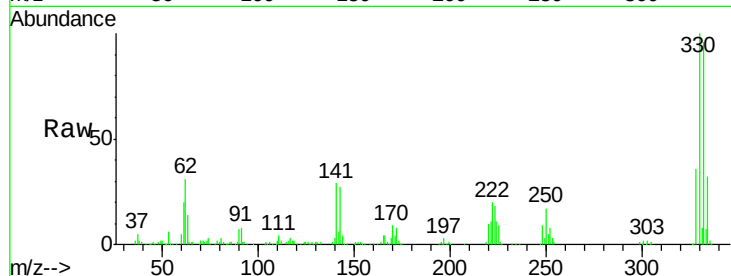

#44
 2-Fluorobiphenyl
 Concen: 114.494 ng
 RT: 14.03 min Scan# 1828
 Delta R.T. -0.01 min
 Lab File: BG032060.D
 Acq: 16 Jan 2018 9:13

Tgt Ion:172 Resp: 1123402
 Ion Ratio Lower Upper
 172 100
 171 37.8 30.0 45.0
 170 24.2 19.5 29.3


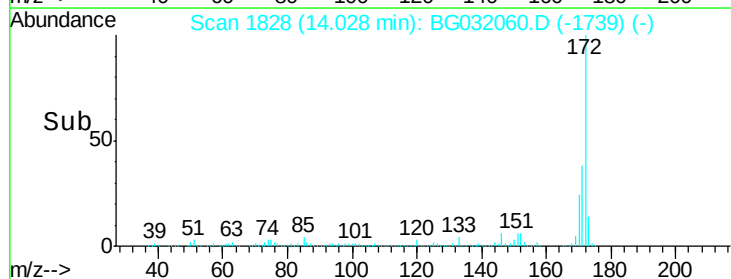
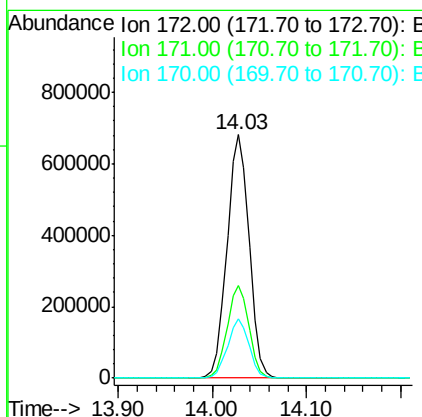
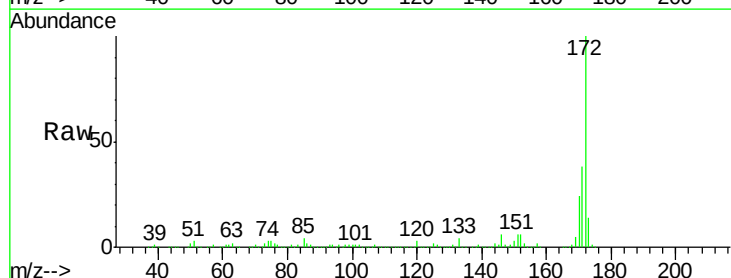


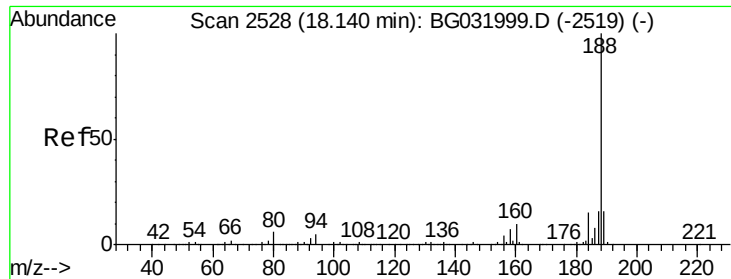

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 18.13 min Scan# 2526
Delta R.T. -0.01 min
Lab File: BG032060.D
Acq: 16 Jan 2018 9:13




Instrument :
BNA_G
ClientSampleId :
ENV-106-1(MW)-DUP


Tgt Ion:188 Resp: 330721
Ion Ratio Lower Upper
188 100
94 5.0 6.9 10.3#
80 5.4 7.7 11.5#

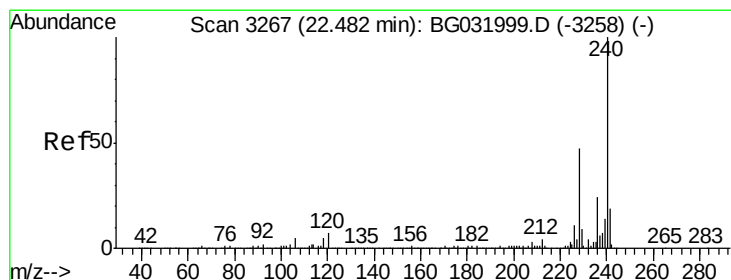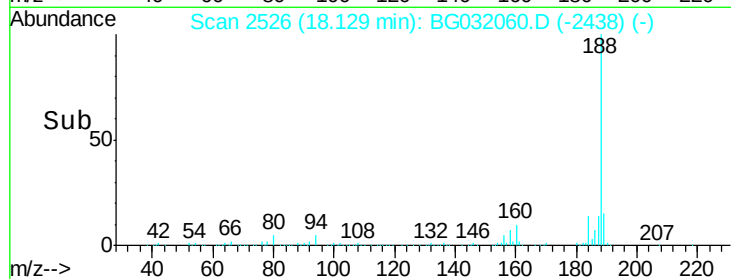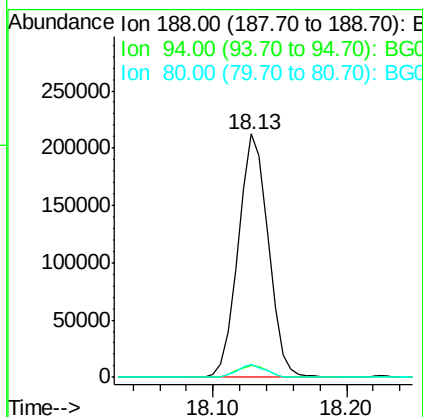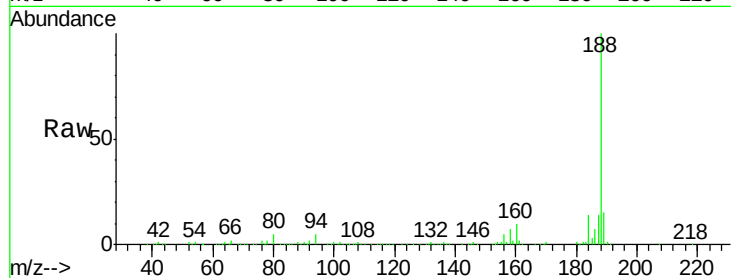

#75
Chrysene-d12
Concen: 20.000 ng
RT: 22.46 min Scan# 3264
Delta R.T. -0.02 min
Lab File: BG032060.D
Acq: 16 Jan 2018 9:13

Tgt Ion:240 Resp: 400395
Ion Ratio Lower Upper
240 100
120 4.4 6.8 10.2#
236 25.7 20.9 31.3

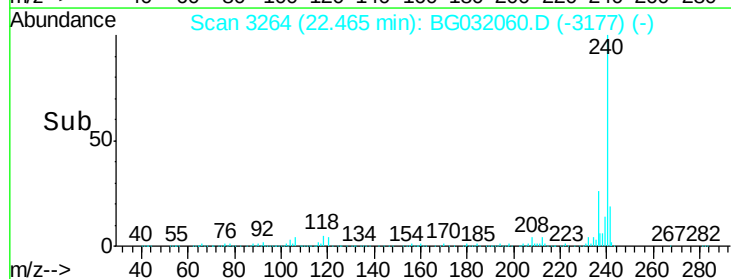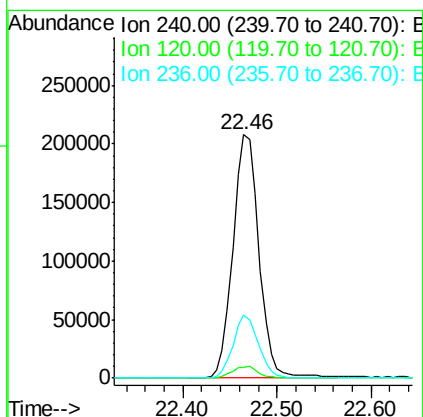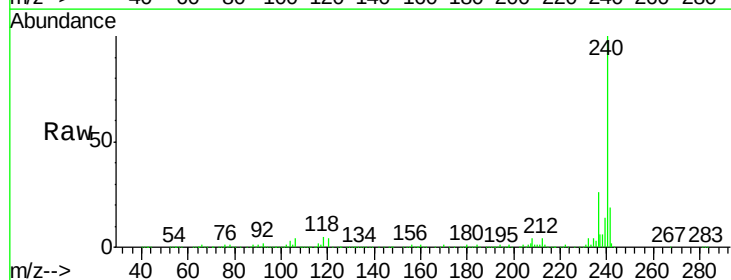

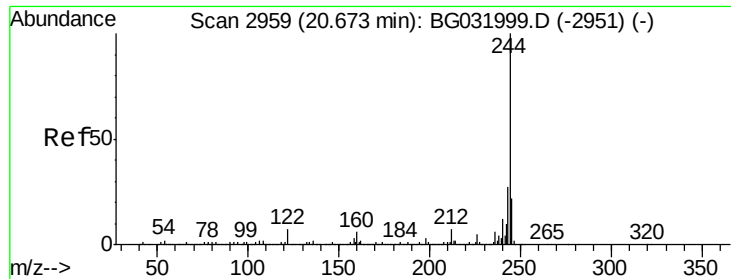

#78

Terphenyl-d14

Concen: 111.259 ng

RT: 20.67 min Scan# 2958

Delta R.T. -0.01 min

Lab File: BG032060.D

Acq: 16 Jan 2018 9:13

Instrument :

BNA_G

ClientSampleId :

ENV-106-1(MW)-DUP


Tgt Ion:244 Resp: 2017515

Ion Ratio Lower Upper

244 100

212 8.2 5.8 8.8




122 6.5 7.0 10.4#

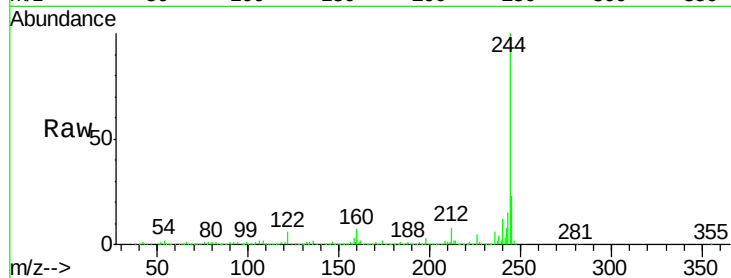

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

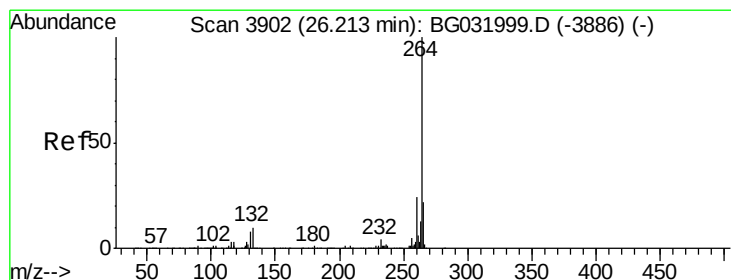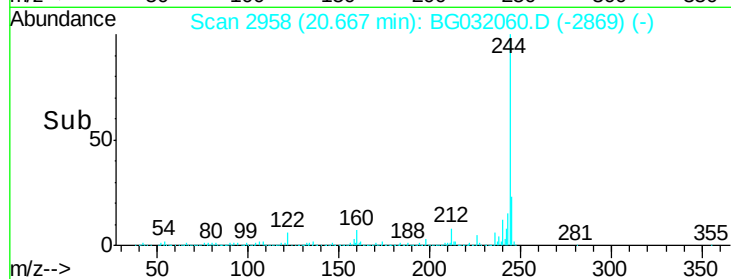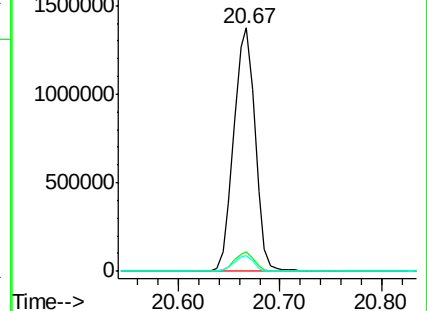

#86

Perylene-d12

Concen: 20.000 ng

RT: 26.18 min Scan# 3897

Delta R.T. -0.03 min

Lab File: BG032060.D

Acq: 16 Jan 2018 9:13


Tgt Ion:264 Resp: 407252

Ion Ratio Lower Upper

264 100

260 22.4 17.4 26.0

265 21.5 17.7 26.5

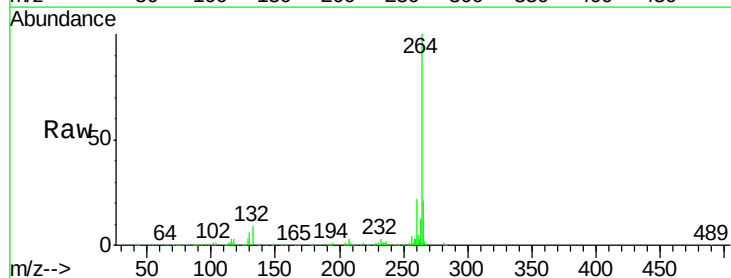

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

