


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_G\Data\BG011518\
 Data File : BG032033.D
 Acq On : 15 Jan 2018 14:10
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG011218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 15 10:05:15 2018

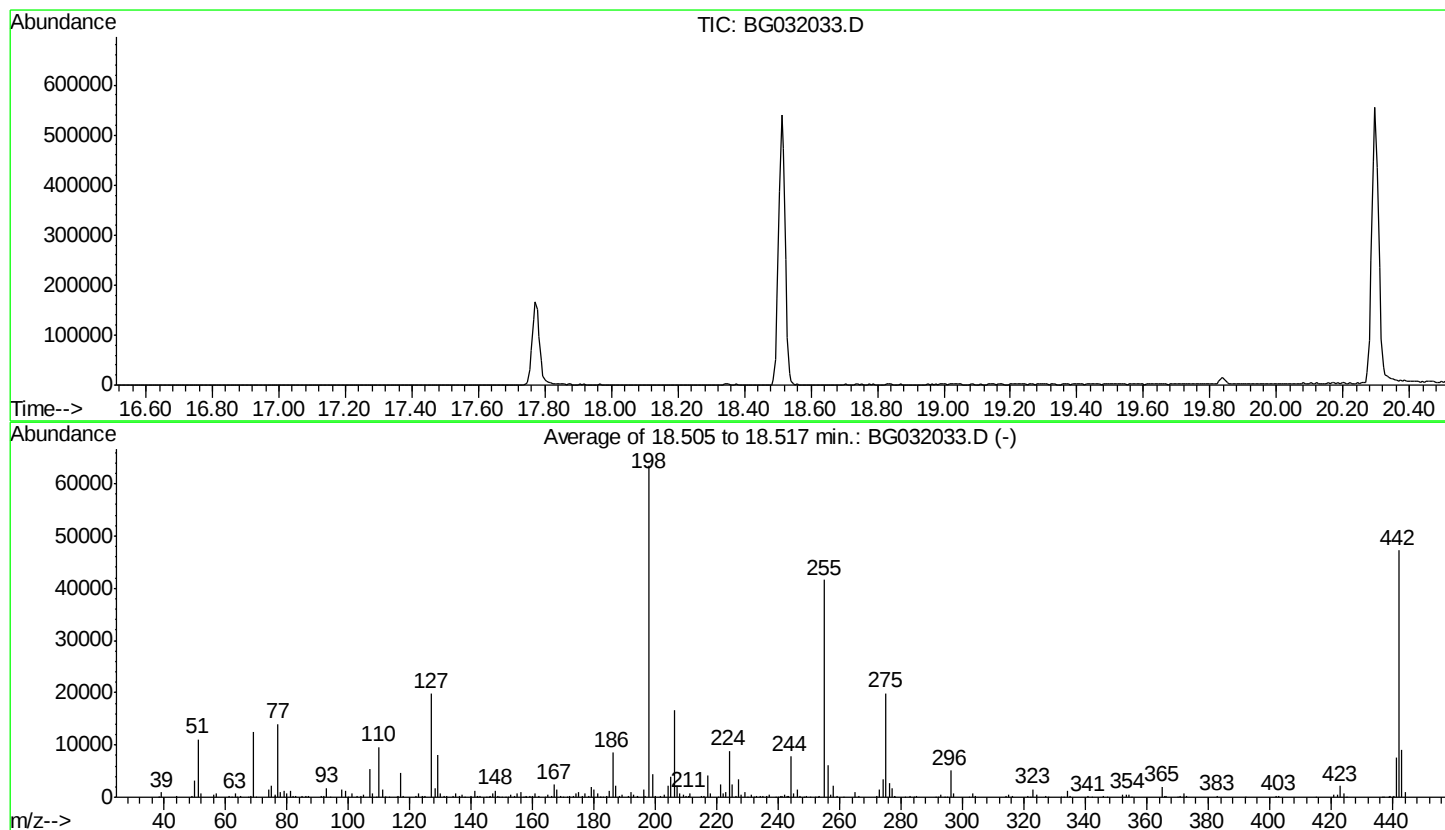

AutoFind: Scans 2590, 2591, 2592; Background Corrected with Scan 2584

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	17.4	11029	PASS
68	69	0.00	2	1.2	152	PASS
69	198	0.00	100	19.8	12558	PASS
70	69	0.00	2	0.5	66	PASS
127	198	10	80	31.2	19765	PASS
197	198	0.00	2	0.4	230	PASS
198	198	100	100	100.0	63442	PASS
199	198	5	9	6.9	4367	PASS
275	198	10	60	31.4	19895	PASS
365	198	1	100	3.3	2072	PASS
441	442	0.01	24	15.9	7499	PASS
442	198	50	100	74.4	47197	PASS
443	442	15	24	19.3	9100	PASS